

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011723\
 Data File : PL080368.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jan 2023 13:52
 Operator : AR\AJ
 Sample : PB150300BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB150300BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/18/2023
 Supervised By : Ankita Jodhani 01/18/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 20:40:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 12 01:47:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.360	2.688	39497623	39341457	19.772	17.590
2) SA Decachlor...	8.801	7.845	34721941	45740725	23.534m	20.349

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011723\
Data File : PL080368.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jan 2023 13:52
Operator : AR\AJ
Sample : PB150300BL
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
PB150300BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/18/2023
Supervised By : Ankita Jodhani 01/18/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 20:40:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011223.M
Quant Title : GC Extractables
QLast Update : Thu Jan 12 01:47:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

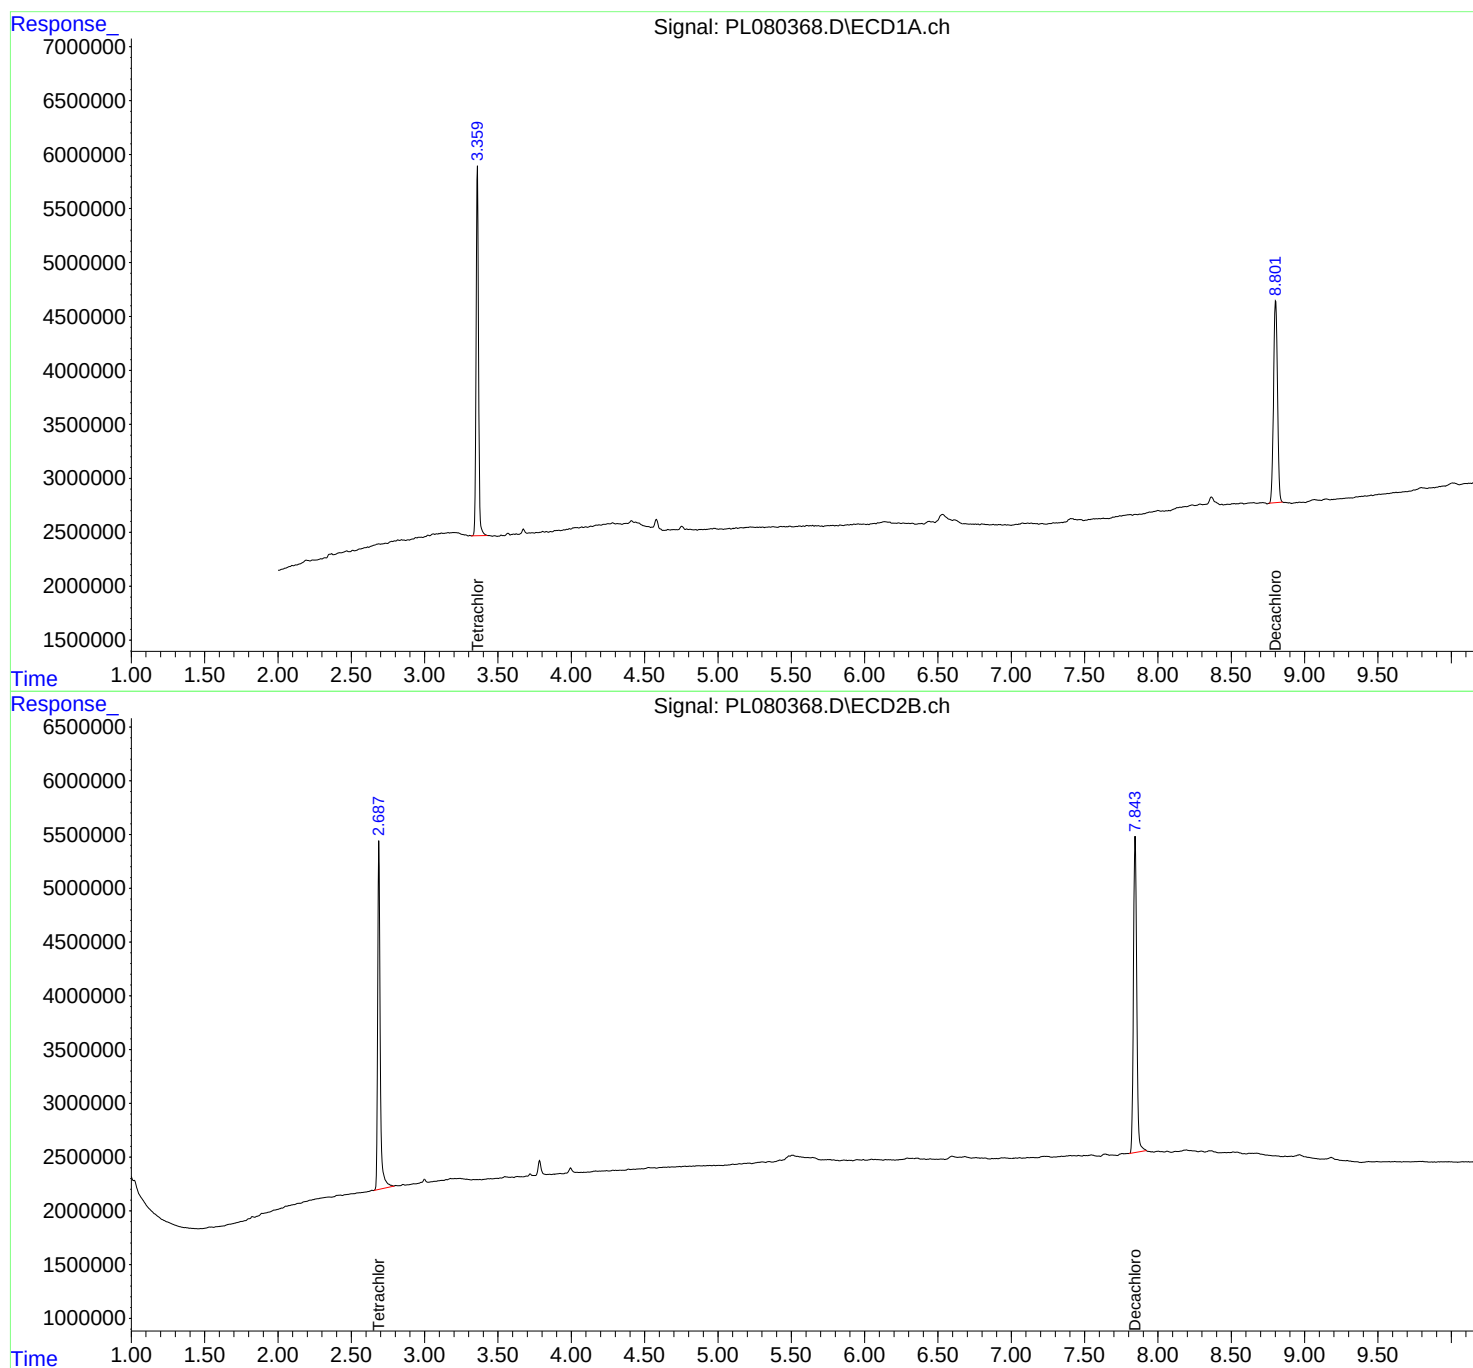

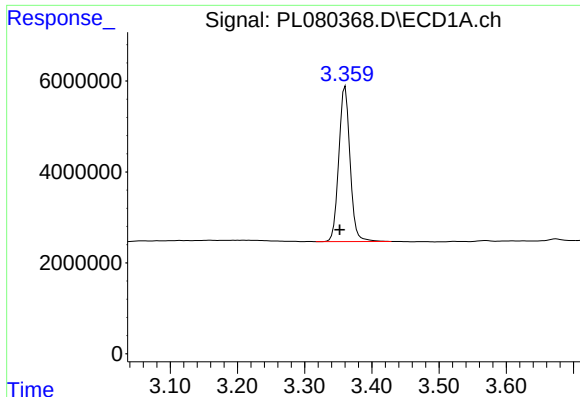


#1 Tetrachloro-m-xylene

R.T.: 3.360 min
Delta R.T.: 0.008 min
Response: 39497623
Conc: 19.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB150300BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/18/2023
Supervised By :Ankita Jodhani 01/18/2023

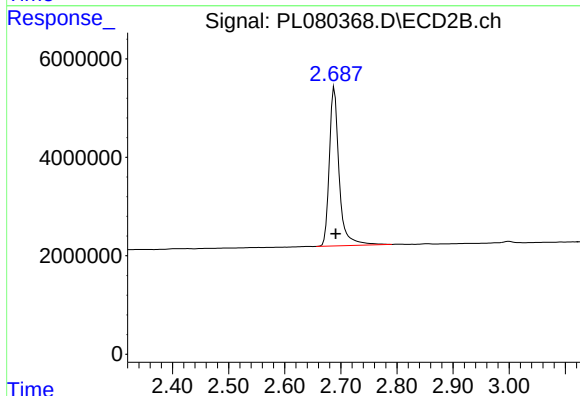


#1 Tetrachloro-m-xylene

R.T.: 2.688 min
Delta R.T.: -0.002 min
Response: 39341457
Conc: 17.59 ng/ml

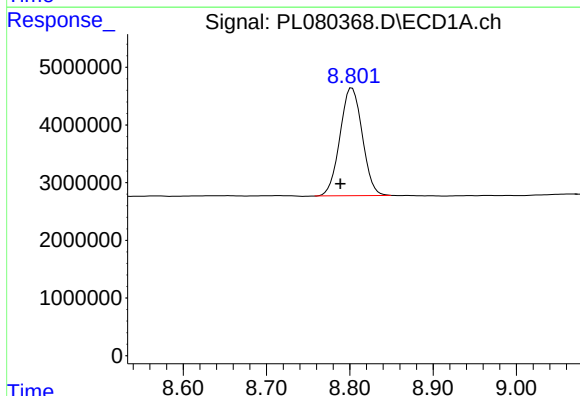

#28 Decachlorobiphenyl

R.T.: 8.801 min
Delta R.T.: 0.013 min
Response: 34721941
Conc: 23.53 ng/ml m

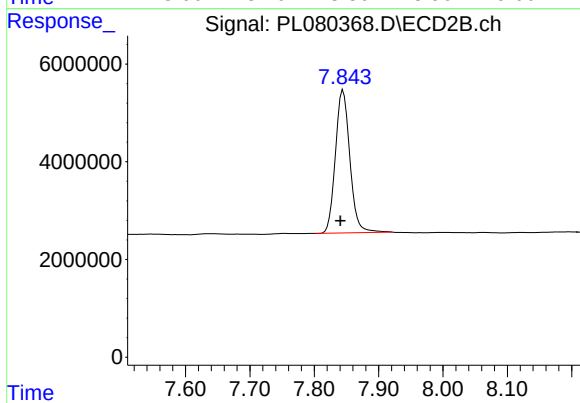

#28 Decachlorobiphenyl

R.T.: 7.845 min
Delta R.T.: 0.004 min
Response: 45740725
Conc: 20.35 ng/ml