

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011819\
 Data File : PL044053.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2019 11:41
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 03:12:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011819.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 19 02:56:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
15) B	Endosulfa...	6.110f	0.000	23163636	0	4.069	N.D. #
16) A	4,4'-DDD	0.000	6.800f	0	10537085	N.D.	5.212 #
27)	Chlordane-5	6.110	0.000	23163636	0	103.140	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011819\
Data File : PL044053.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2019 11:41
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 03:12:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011819.M
Quant Title : GC Extractables
QLast Update : Sat Jan 19 02:56:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

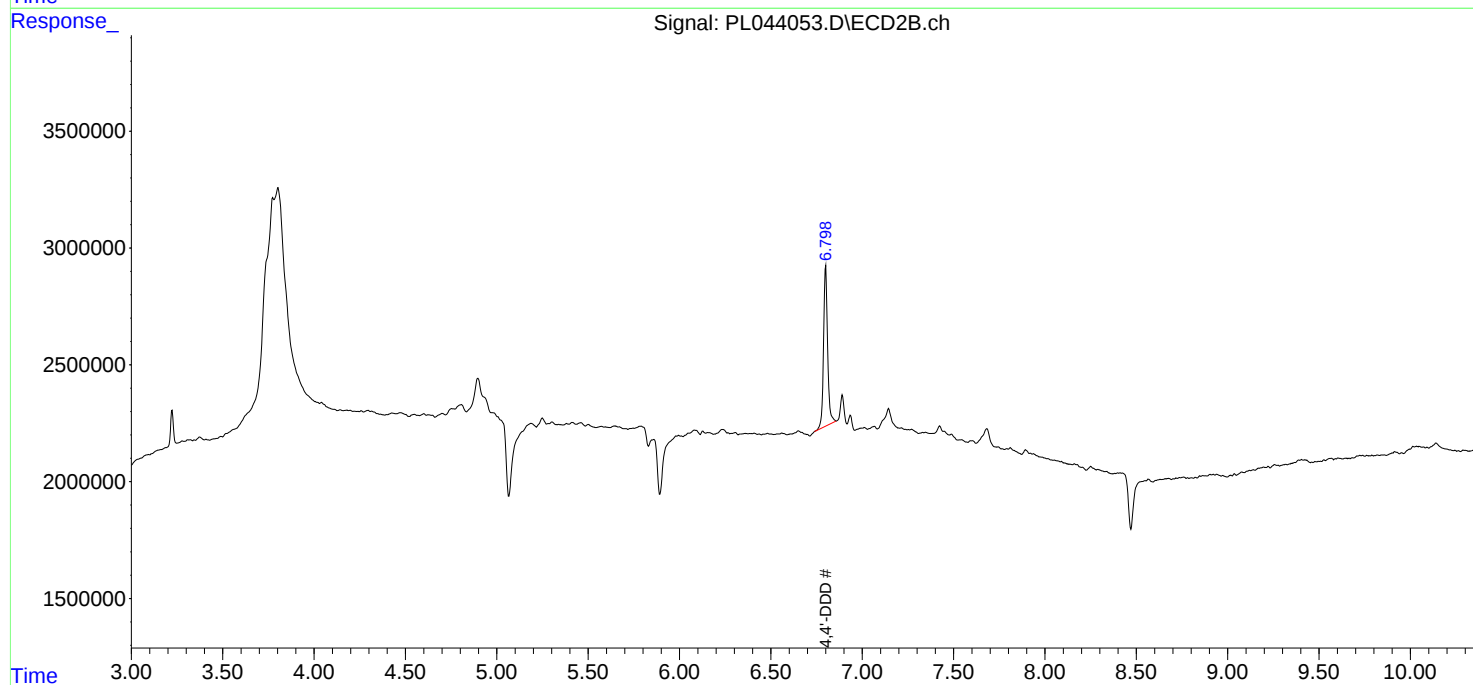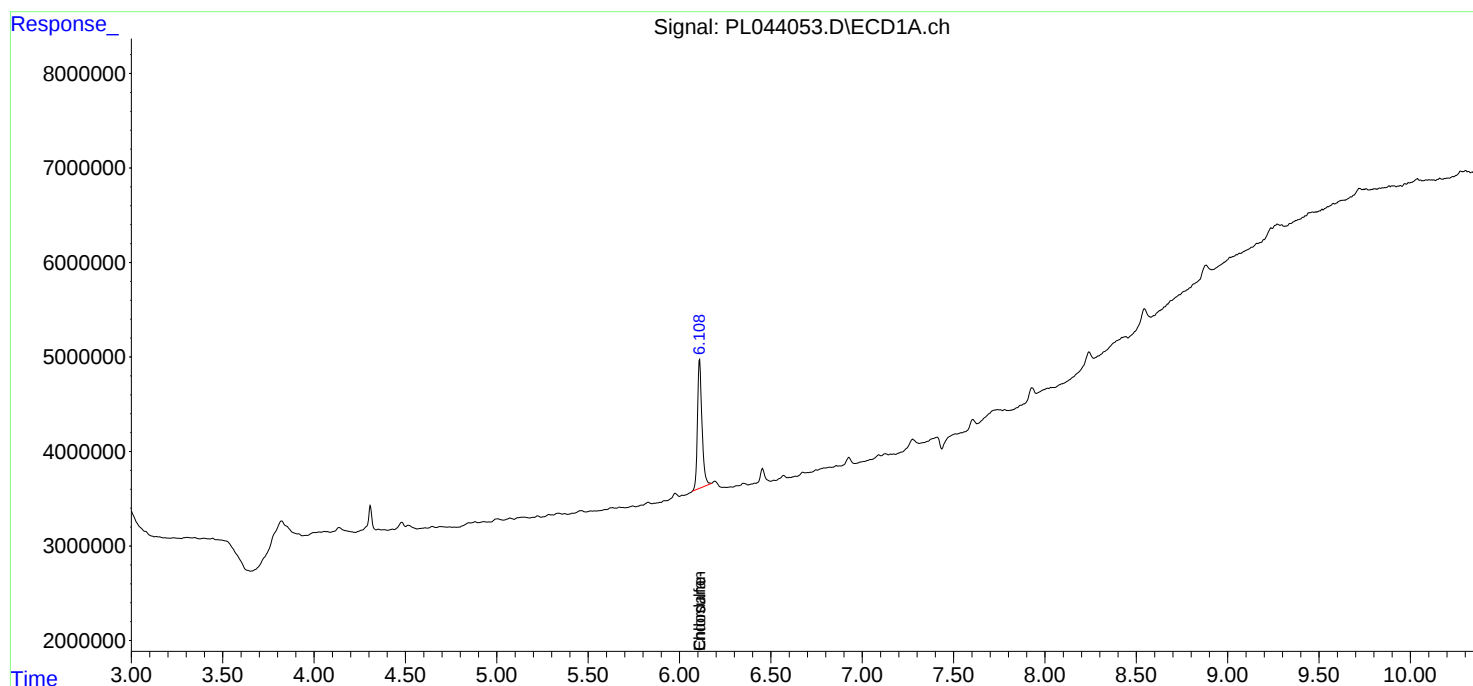


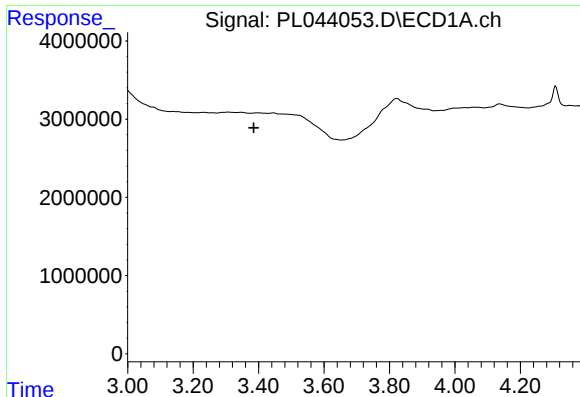

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.385 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

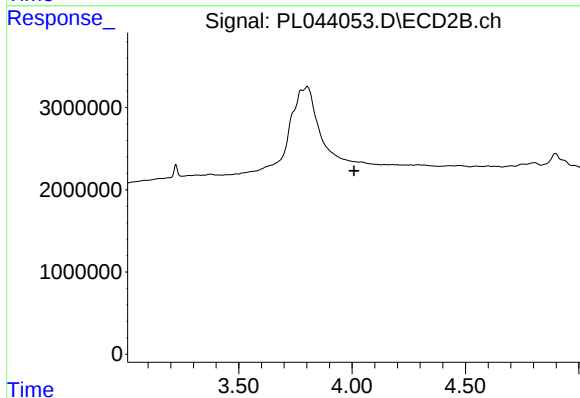


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.008 min
Response: 0
Conc: N.D.

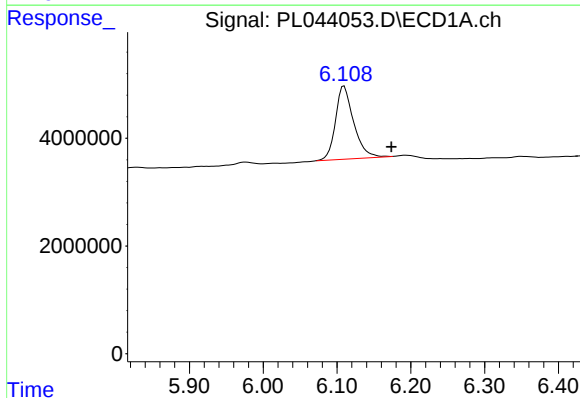


#15 Endosulfan II

R.T.: 6.110 min
Delta R.T.: -0.064 min
Response: 23163636
Conc: 4.07 ng/ml

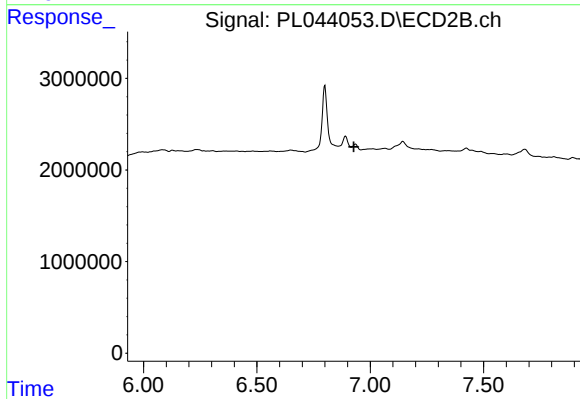

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.927 min
Response: 0
Conc: N.D.

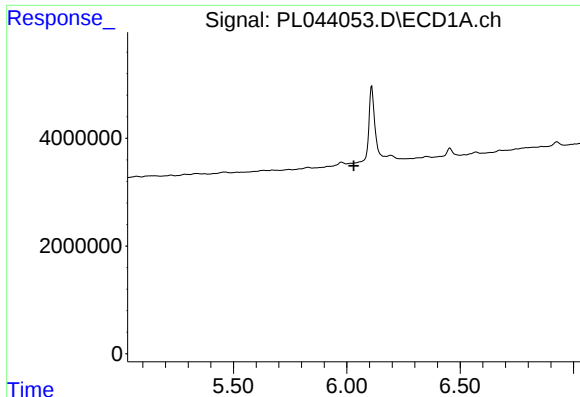

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.031 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

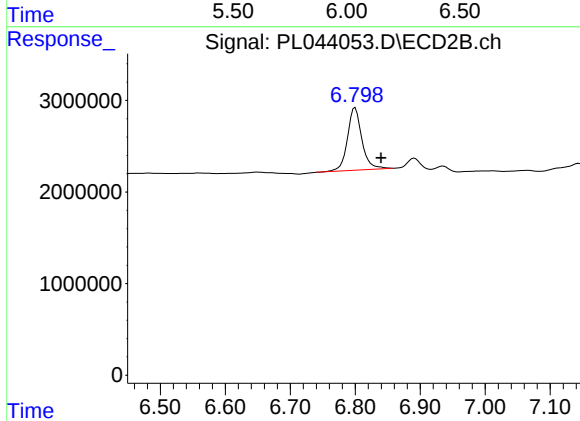


#16 4,4'-DDD

R.T.: 6.800 min
Delta R.T.: -0.040 min
Response: 10537085
Conc: 5.21 ng/ml

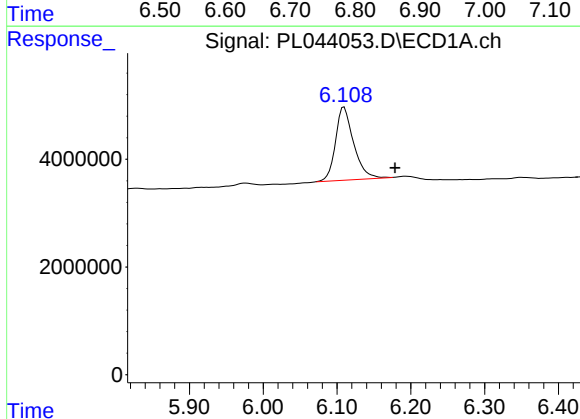


#27 Chlordane-5

R.T.: 6.110 min
Delta R.T.: -0.069 min
Response: 23163636
Conc: 103.14 ng/ml

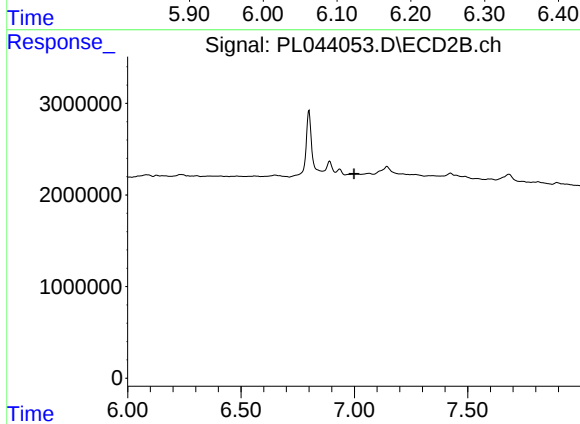

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.998 min
Response: 0
Conc: N.D.

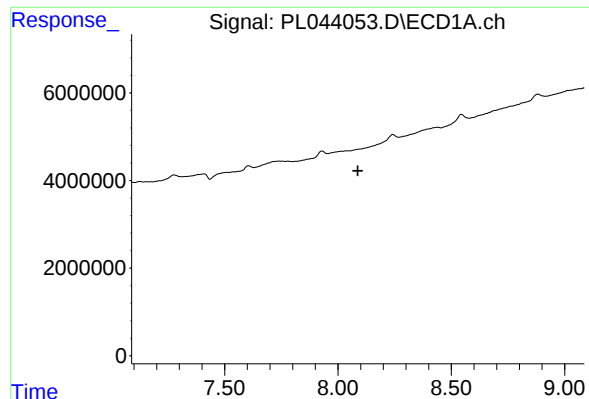

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

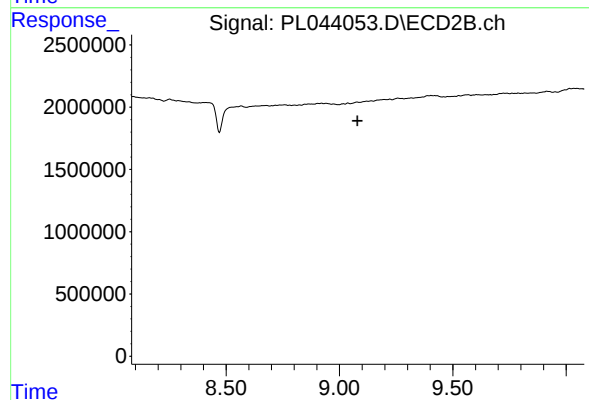

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.080 min
Response: 0
Conc: N.D.