

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011819\
 Data File : PL044078.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2019 17:48
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 03:15:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011819.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 19 02:56:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.384	4.008	149.3E6	57675109	27.442	24.473
28)	SA Decachlor...	8.087	9.080	150.4E6	46838166	25.450	20.686
Target Compounds							
15)	B Endosulfa...	6.109f	0.000	20920308	0	3.675	N.D. #
27)	Chlordane-5	6.109	0.000	20920308	0	93.151	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011819\
Data File : PL044078.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2019 17:48
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 03:15:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011819.M
Quant Title : GC Extractables
QLast Update : Sat Jan 19 02:56:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

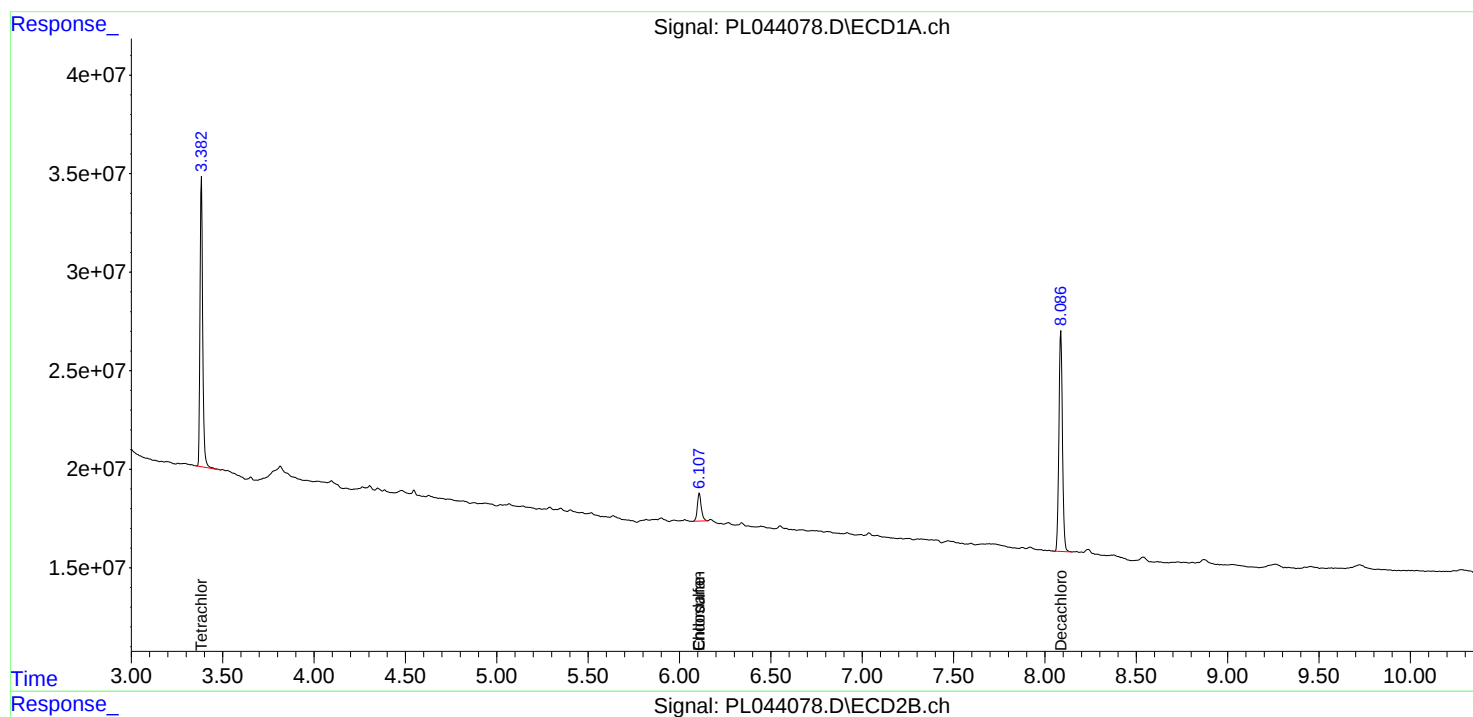


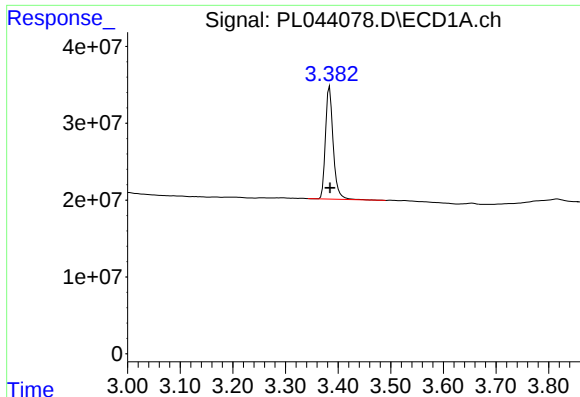

#1 Tetrachloro-m-xylene


R.T.: 3.384 min
Delta R.T.: -0.001 min
Response: 149314592
Conc: 27.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

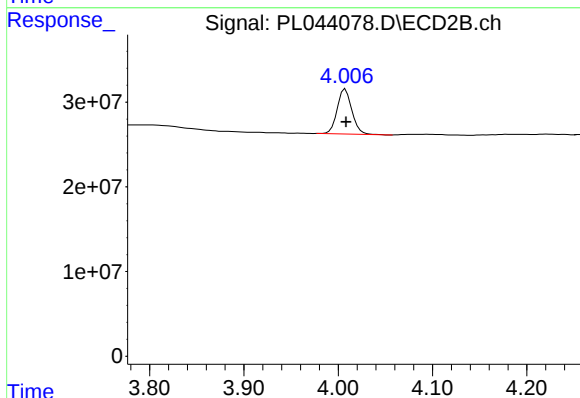


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 57675109
Conc: 24.47 ng/ml

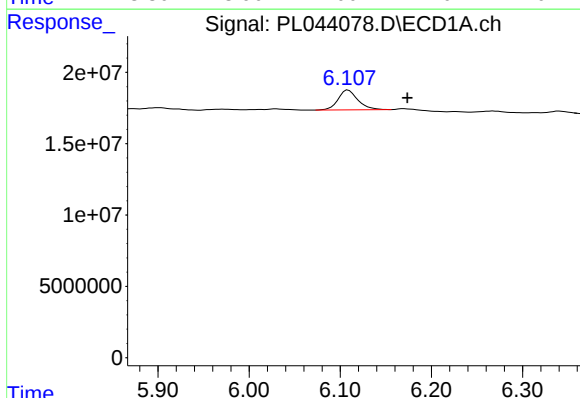


#15 Endosulfan II

R.T.: 6.109 min
Delta R.T.: -0.065 min
Response: 20920308
Conc: 3.67 ng/ml

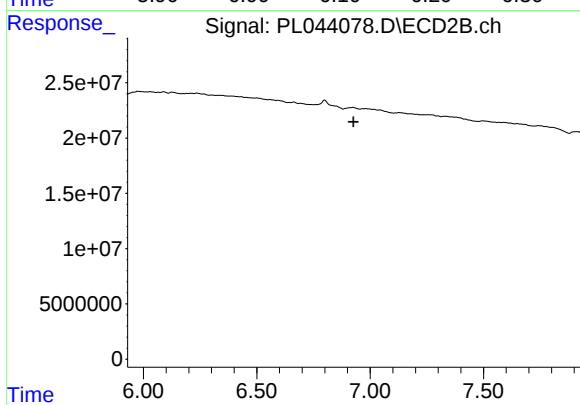

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.927 min
Response: 0
Conc: N.D.

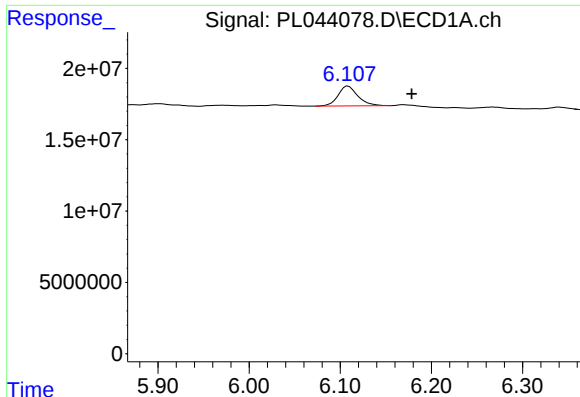

#27 Chlordane-5


R.T.: 6.109 min
Delta R.T.: -0.070 min
Response: 20920308
Conc: 93.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

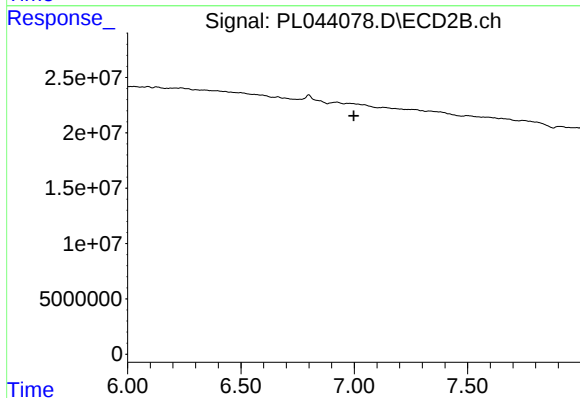


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.998 min
Response: 0
Conc: N.D.

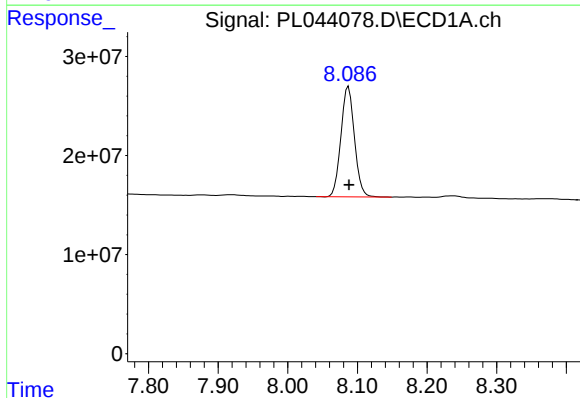

#28 Decachlorobiphenyl

R.T.: 8.087 min
Delta R.T.: 0.000 min
Response: 150416901
Conc: 25.45 ng/ml

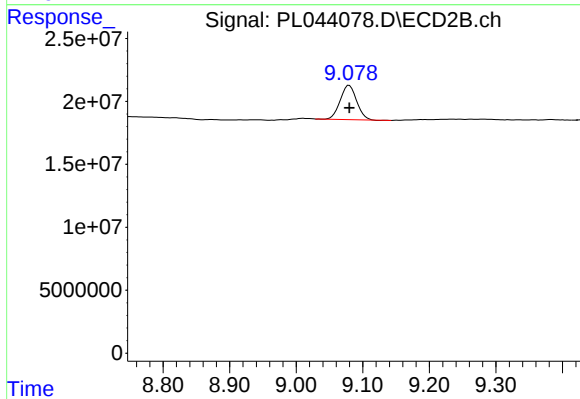

#28 Decachlorobiphenyl

R.T.: 9.080 min
Delta R.T.: 0.000 min
Response: 46838166
Conc: 20.69 ng/ml