

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011820\
 Data File : PL055841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2020 06:41
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 00:31:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 10 00:58:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	3.967	174.5E6	52223075	18.884	19.713
28)	SA Decachlor...	8.234	8.955	173.4E6	39429632	19.741	18.965
Target Compounds							
9)	A Endosulfan I	5.546	0.000	13014020	0	1.053	N.D. #
14)	MA Endrin	0.000	6.628	0	6686819	N.D.	2.965 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011820\
Data File : PL055841.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2020 06:41
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 00:31:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
Quant Title : GC Extractables
QLast Update : Fri Jan 10 00:58:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

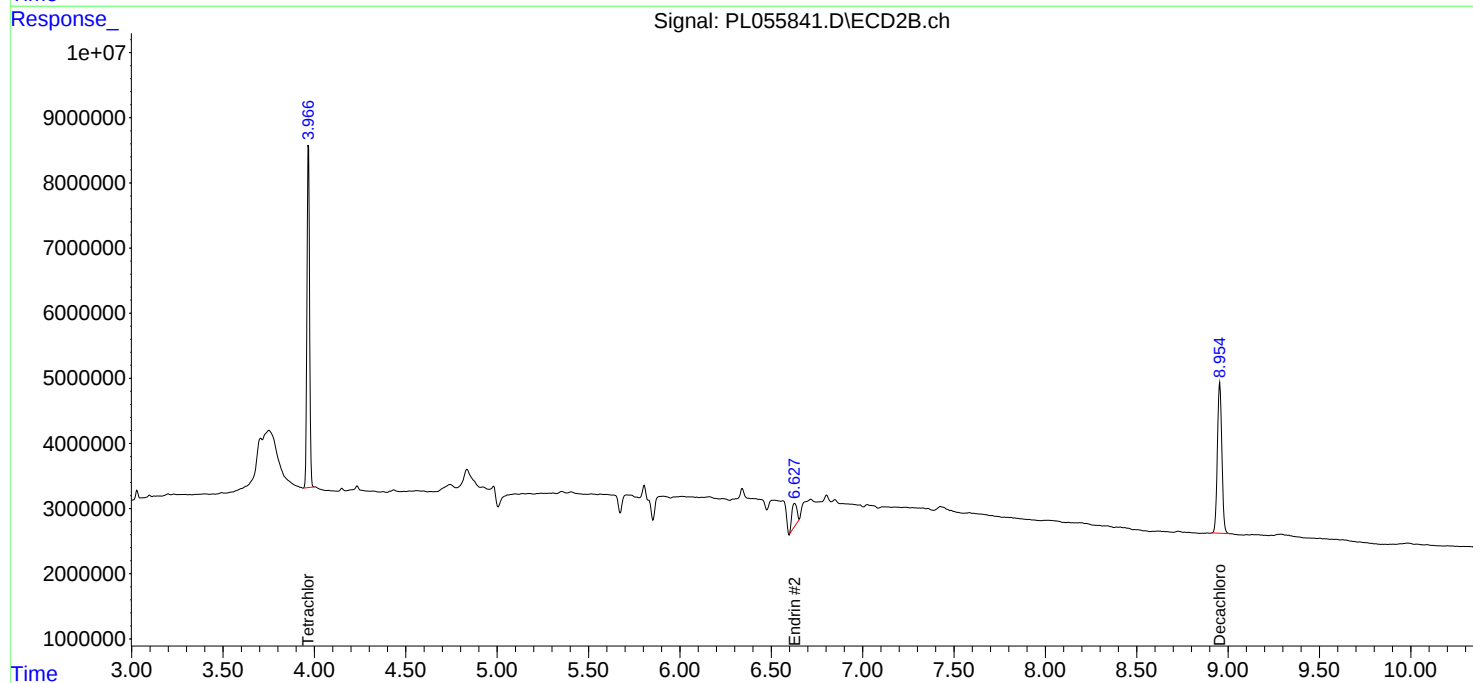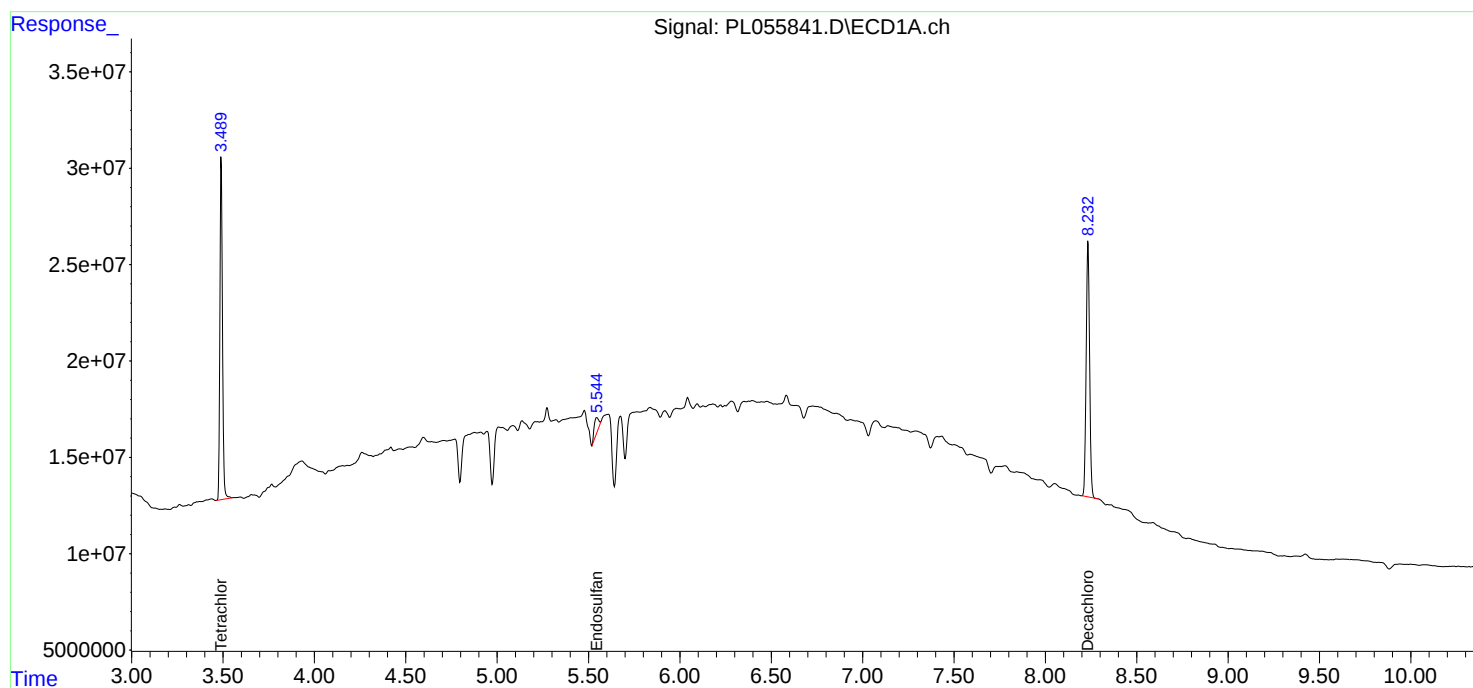


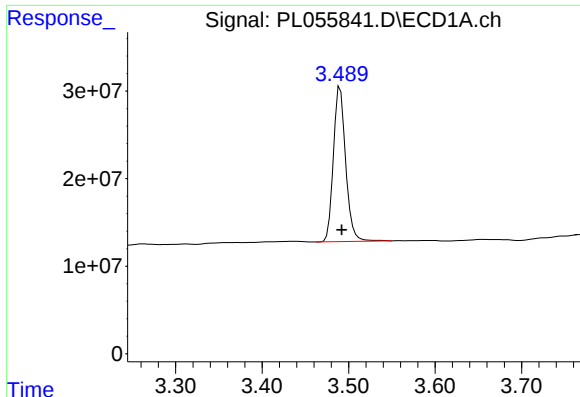

#1 Tetrachloro-m-xylene


R.T.: 3.490 min
Delta R.T.: -0.002 min
Response: 174497566
Conc: 18.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

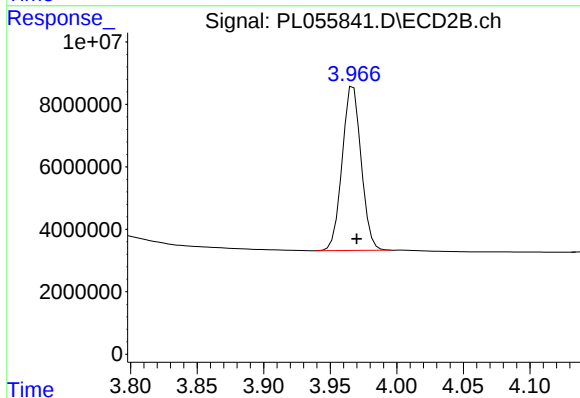


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: -0.002 min
Response: 52223075
Conc: 19.71 ng/ml

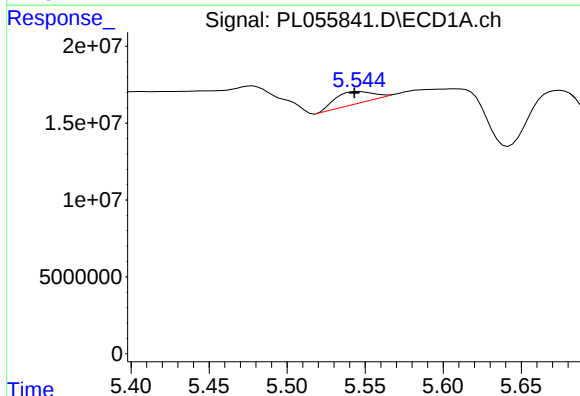


#9 Endosulfan I

R.T.: 5.546 min
Delta R.T.: 0.003 min
Response: 13014020
Conc: 1.05 ng/ml

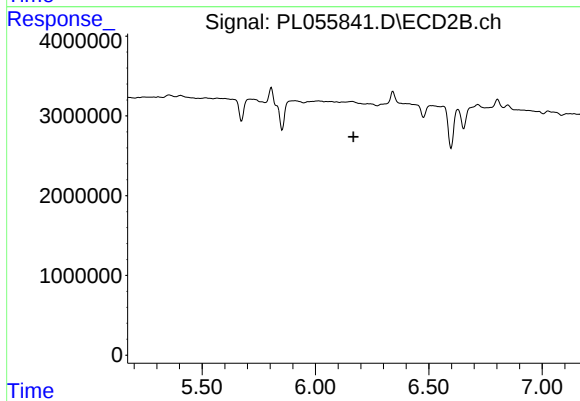

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.168 min
Response: 0
Conc: N.D.

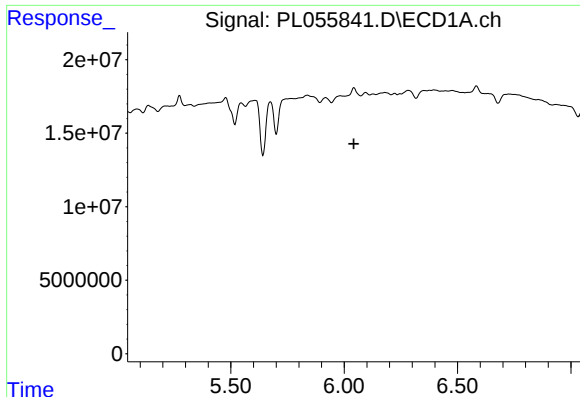

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

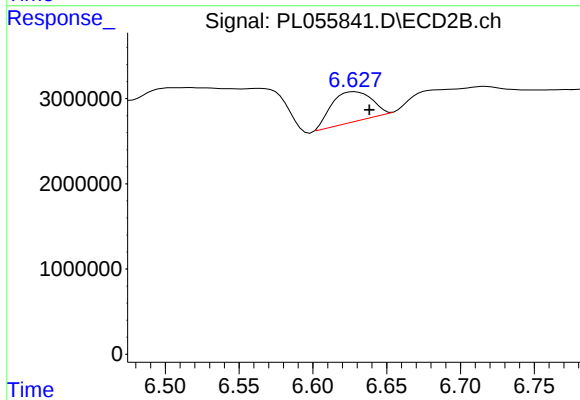


#14 Endrin

R.T.: 6.628 min
Delta R.T.: -0.010 min
Response: 6686819
Conc: 2.97 ng/ml

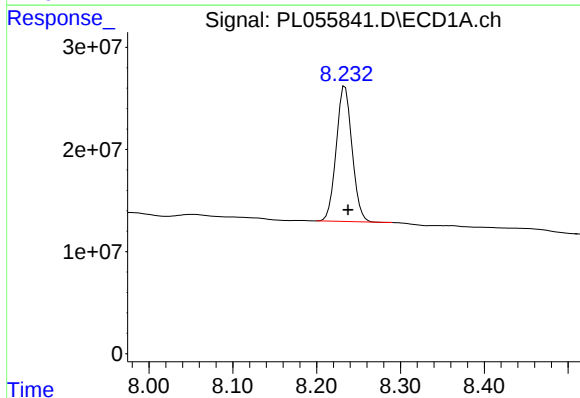

#28 Decachlorobiphenyl

R.T.: 8.234 min
Delta R.T.: -0.004 min
Response: 173363095
Conc: 19.74 ng/ml

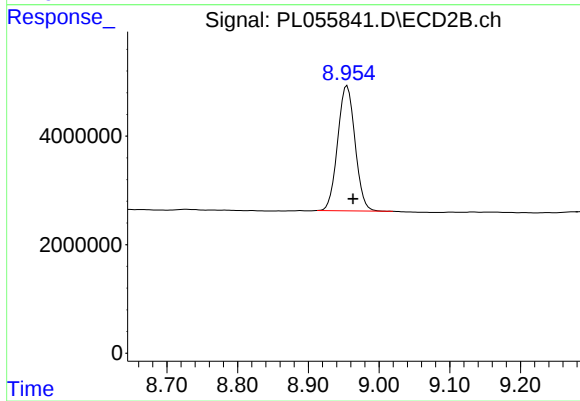

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: -0.008 min
Response: 39429632
Conc: 18.97 ng/ml