

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011820\
 Data File : PL055846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2020 07:52
 Operator : AJ\MA
 Sample : L1155-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 00:32:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 10 00:58:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	3.967	122.9E6	36629910	13.299	13.827
28)	SA Decachlor...	8.234	8.955	132.3E6	32652034	15.069	15.705
Target Compounds							
24)	Chlordane-2	4.863	0.000	1696507	0	4.171	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011820\
Data File : PL055846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2020 07:52
Operator : AJ\MA
Sample : L1155-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 00:32:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
Quant Title : GC Extractables
QLast Update : Fri Jan 10 00:58:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

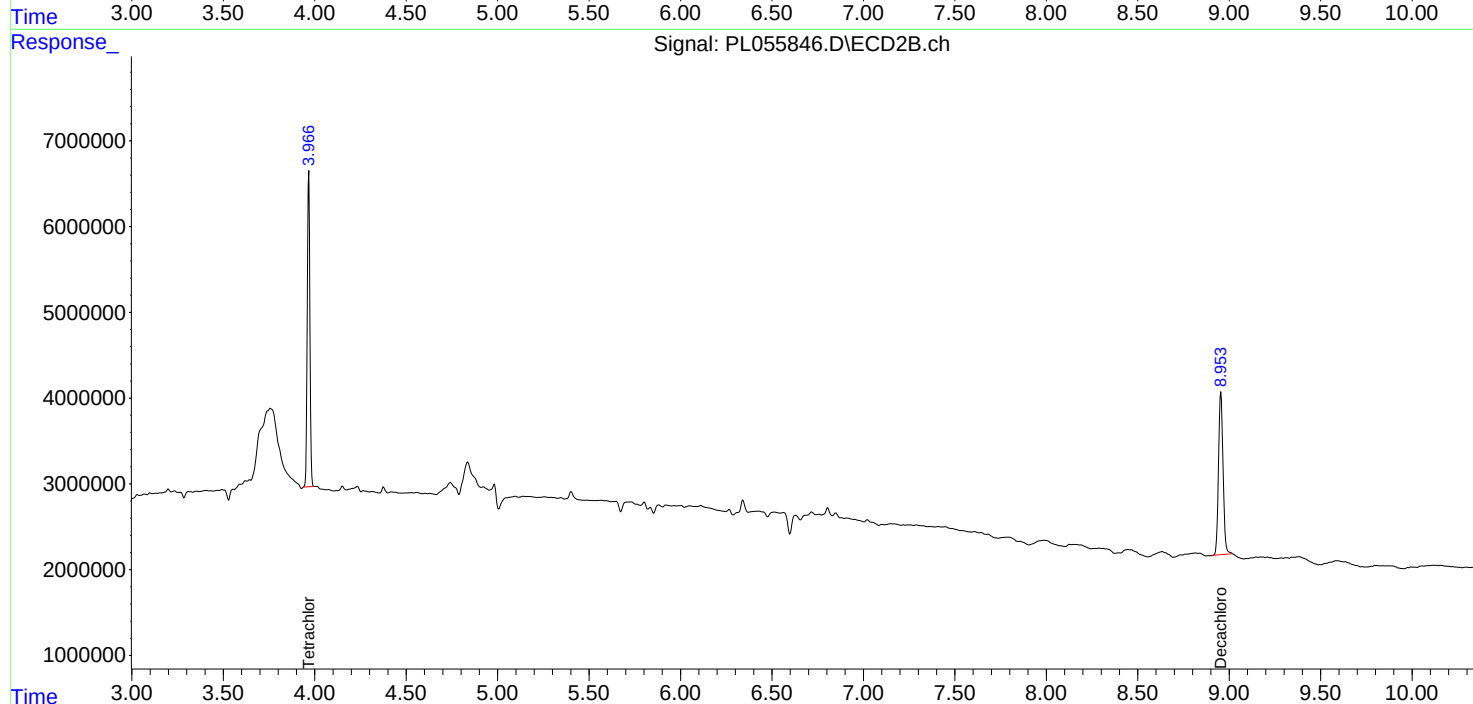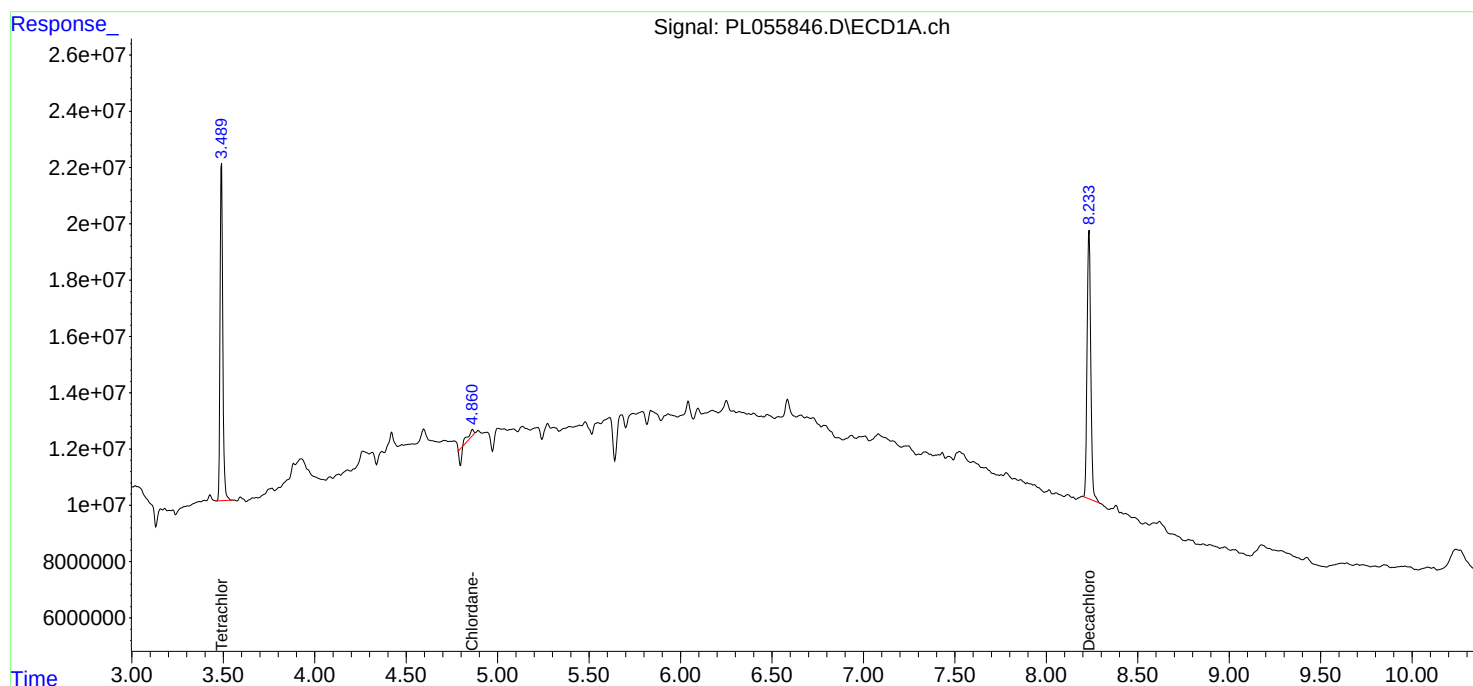


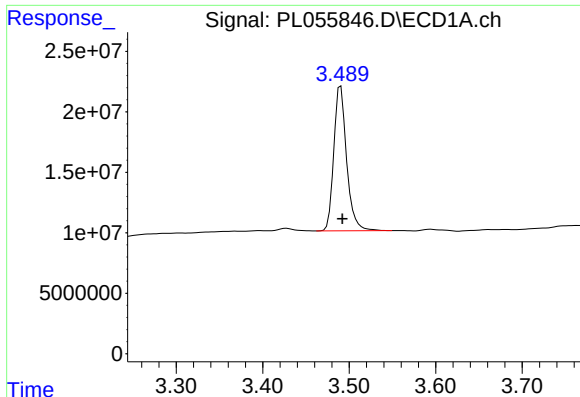

#1 Tetrachloro-m-xylene


R.T.: 3.490 min
Delta R.T.: -0.002 min
Response: 122890427
Conc: 13.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

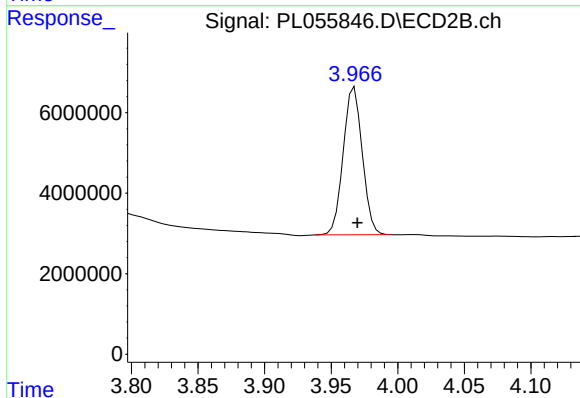


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: -0.002 min
Response: 36629910
Conc: 13.83 ng/ml

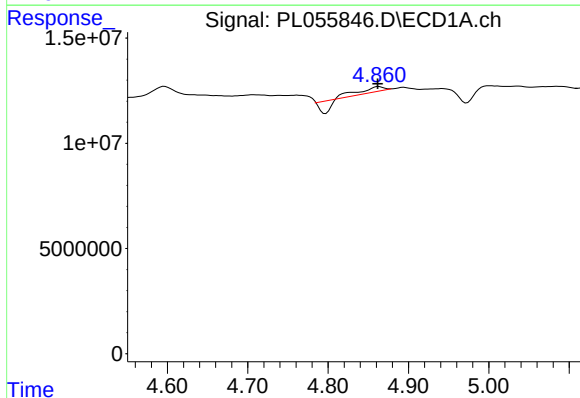


#24 Chlordane-2

R.T.: 4.863 min
Delta R.T.: 0.002 min
Response: 1696507
Conc: 4.17 ng/ml

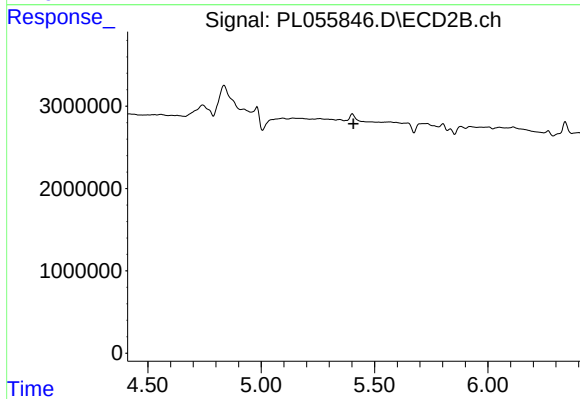

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.407 min
Response: 0
Conc: N.D.

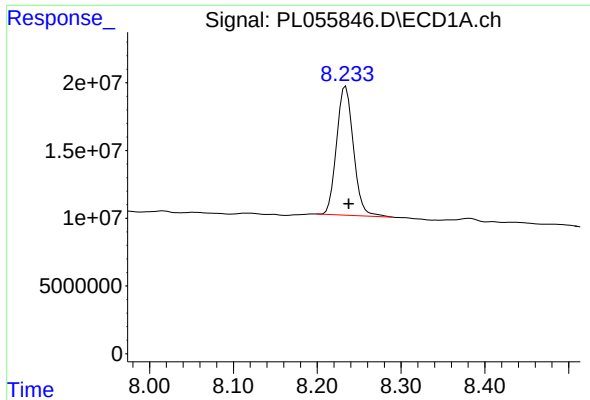

#28 Decachlorobiphenyl

R.T.: 8.234 min
Delta R.T.: -0.004 min
Response: 132330492
Conc: 15.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

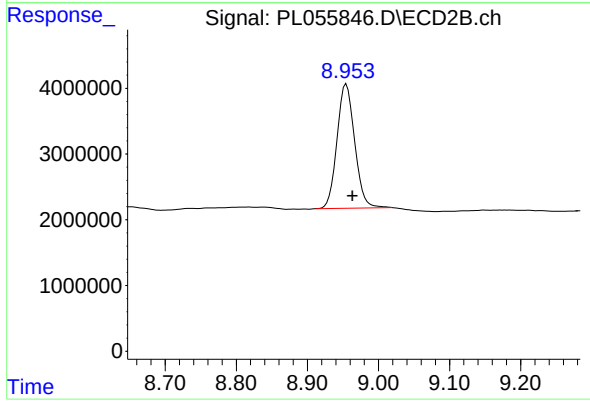

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: -0.008 min
Response: 32652034
Conc: 15.71 ng/ml