

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011820\
 Data File : PL055856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2020 10:13
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 00:33:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 10 00:58:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	3.968	178.1E6	53729006	19.278	20.282
28)	SA Decachlor...	8.235	8.954	179.2E6	40683146	20.412	19.568
Target Compounds							
9)	A Endosulfan I	5.547	0.000	10835084	0	0.877	N.D. #
14)	MA Endrin	0.000	6.629	0	6080834	N.D.	2.697 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011820\
Data File : PL055856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2020 10:13
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 00:33:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011020.M
Quant Title : GC Extractables
QLast Update : Fri Jan 10 00:58:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

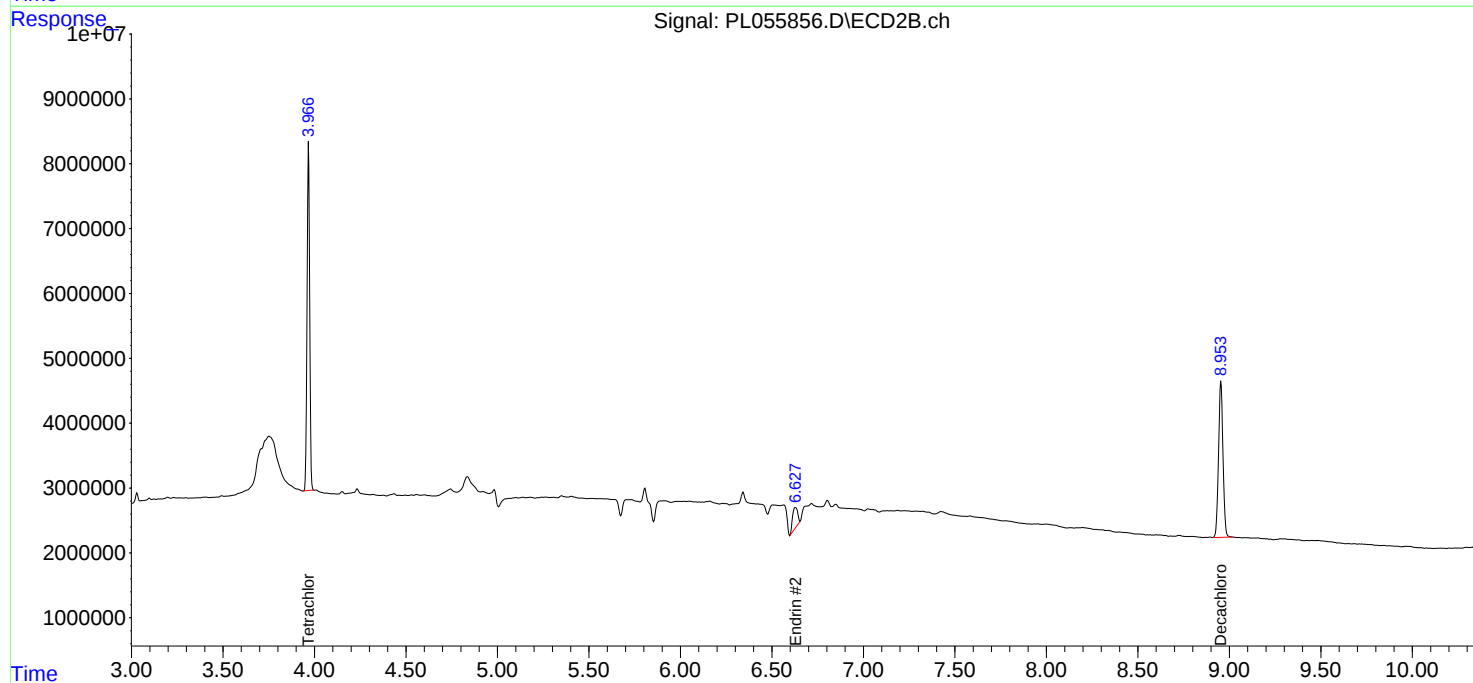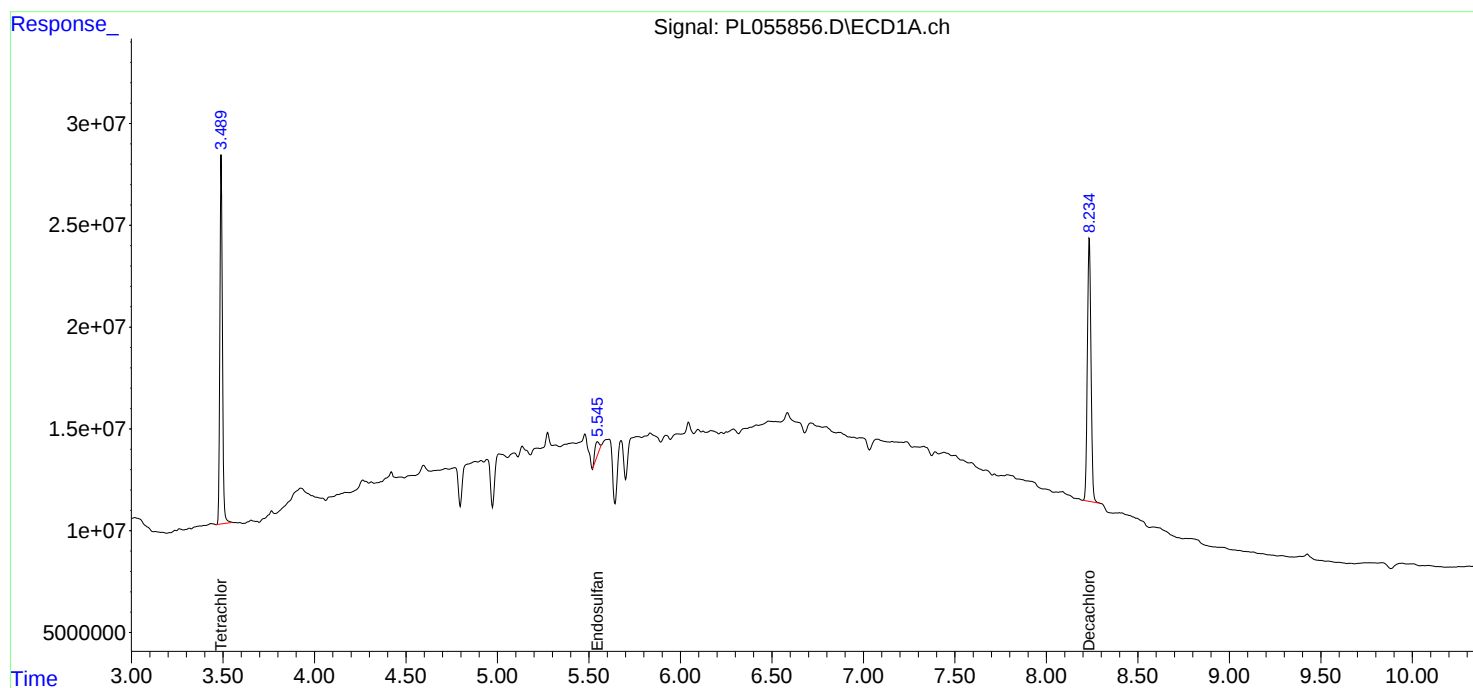


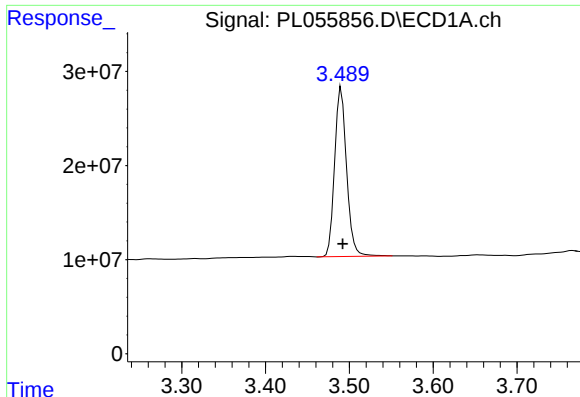

#1 Tetrachloro-m-xylene


R.T.: 3.490 min
Delta R.T.: -0.002 min
Response: 178145001
Conc: 19.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

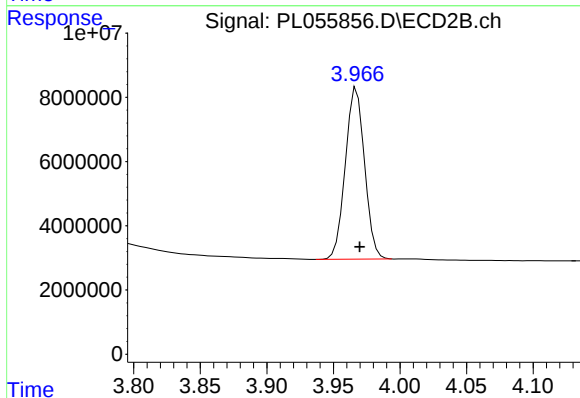


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: -0.002 min
Response: 53729006
Conc: 20.28 ng/ml

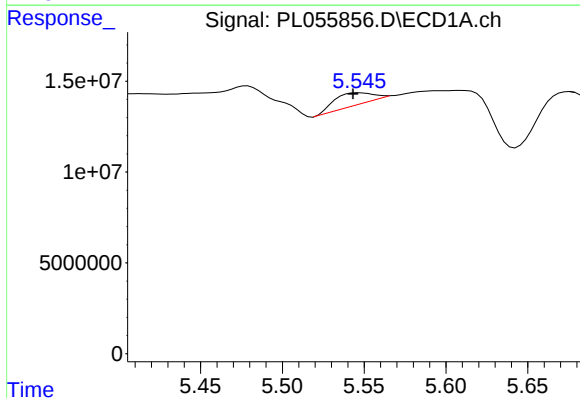


#9 Endosulfan I

R.T.: 5.547 min
Delta R.T.: 0.004 min
Response: 10835084
Conc: 0.88 ng/ml

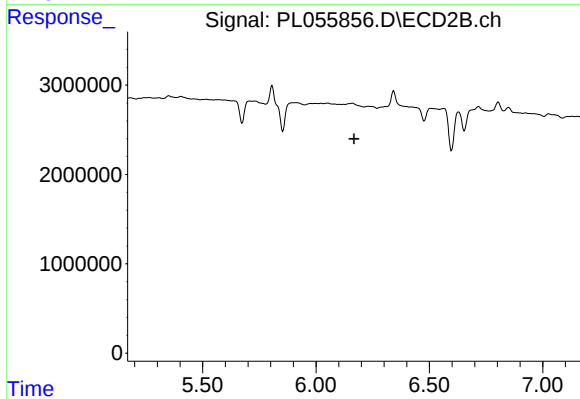

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.168 min
Response: 0
Conc: N.D.

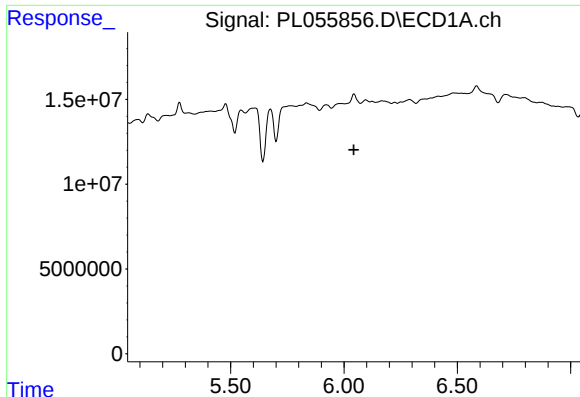

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

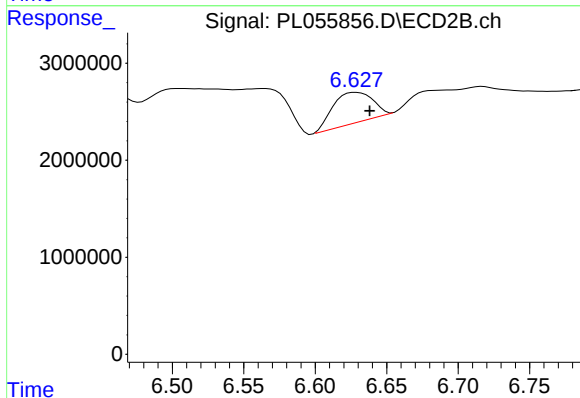


#14 Endrin

R.T.: 6.629 min
Delta R.T.: -0.010 min
Response: 6080834
Conc: 2.70 ng/ml

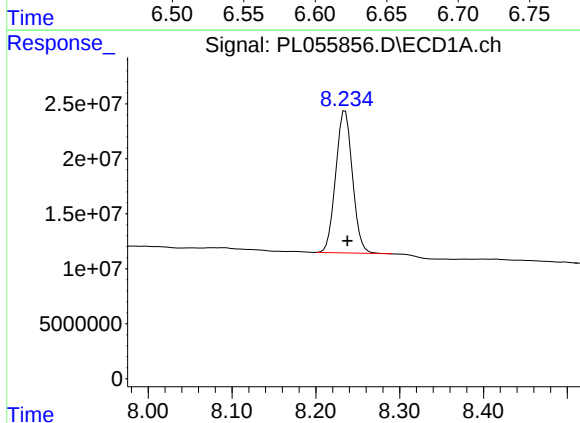

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: -0.003 min
Response: 179249078
Conc: 20.41 ng/ml

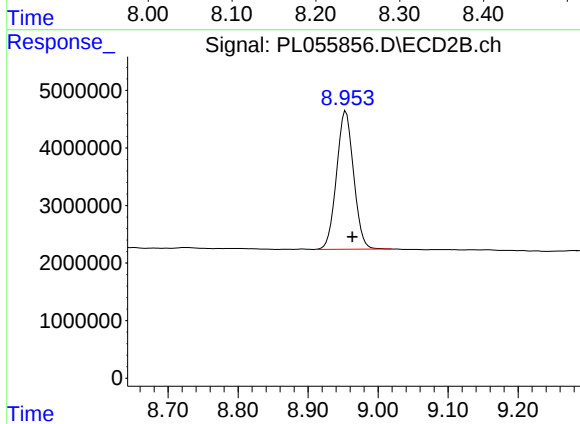

#28 Decachlorobiphenyl

R.T.: 8.954 min
Delta R.T.: -0.009 min
Response: 40683146
Conc: 19.57 ng/ml