

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011821\
 Data File : PL064176.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2021 11:21
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 12:45:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 12:33:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.122	365.9E6	254.0E6	95.616	96.705
28)	SA Decachlor...	8.170	9.285	277.3E6	207.8E6	90.818	91.588
Target Compounds							
23)	Chlordane-1	4.298	5.136	108.2E6	98533582	941.053	924.261
24)	Chlordane-2	4.797	5.612	124.9E6	105.1E6	897.754	876.649
25)	Chlordane-3	5.362	6.268	382.7E6	389.9E6	958.941	960.021
26)	Chlordane-4	5.420	6.341	312.6E6	467.2E6	942.727	944.958
27)	Chlordane-5	6.250	7.161	129.7E6	76578891	946.309	1004.179


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011821\
Data File : PL064176.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2021 11:21
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 12:45:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 12:33:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

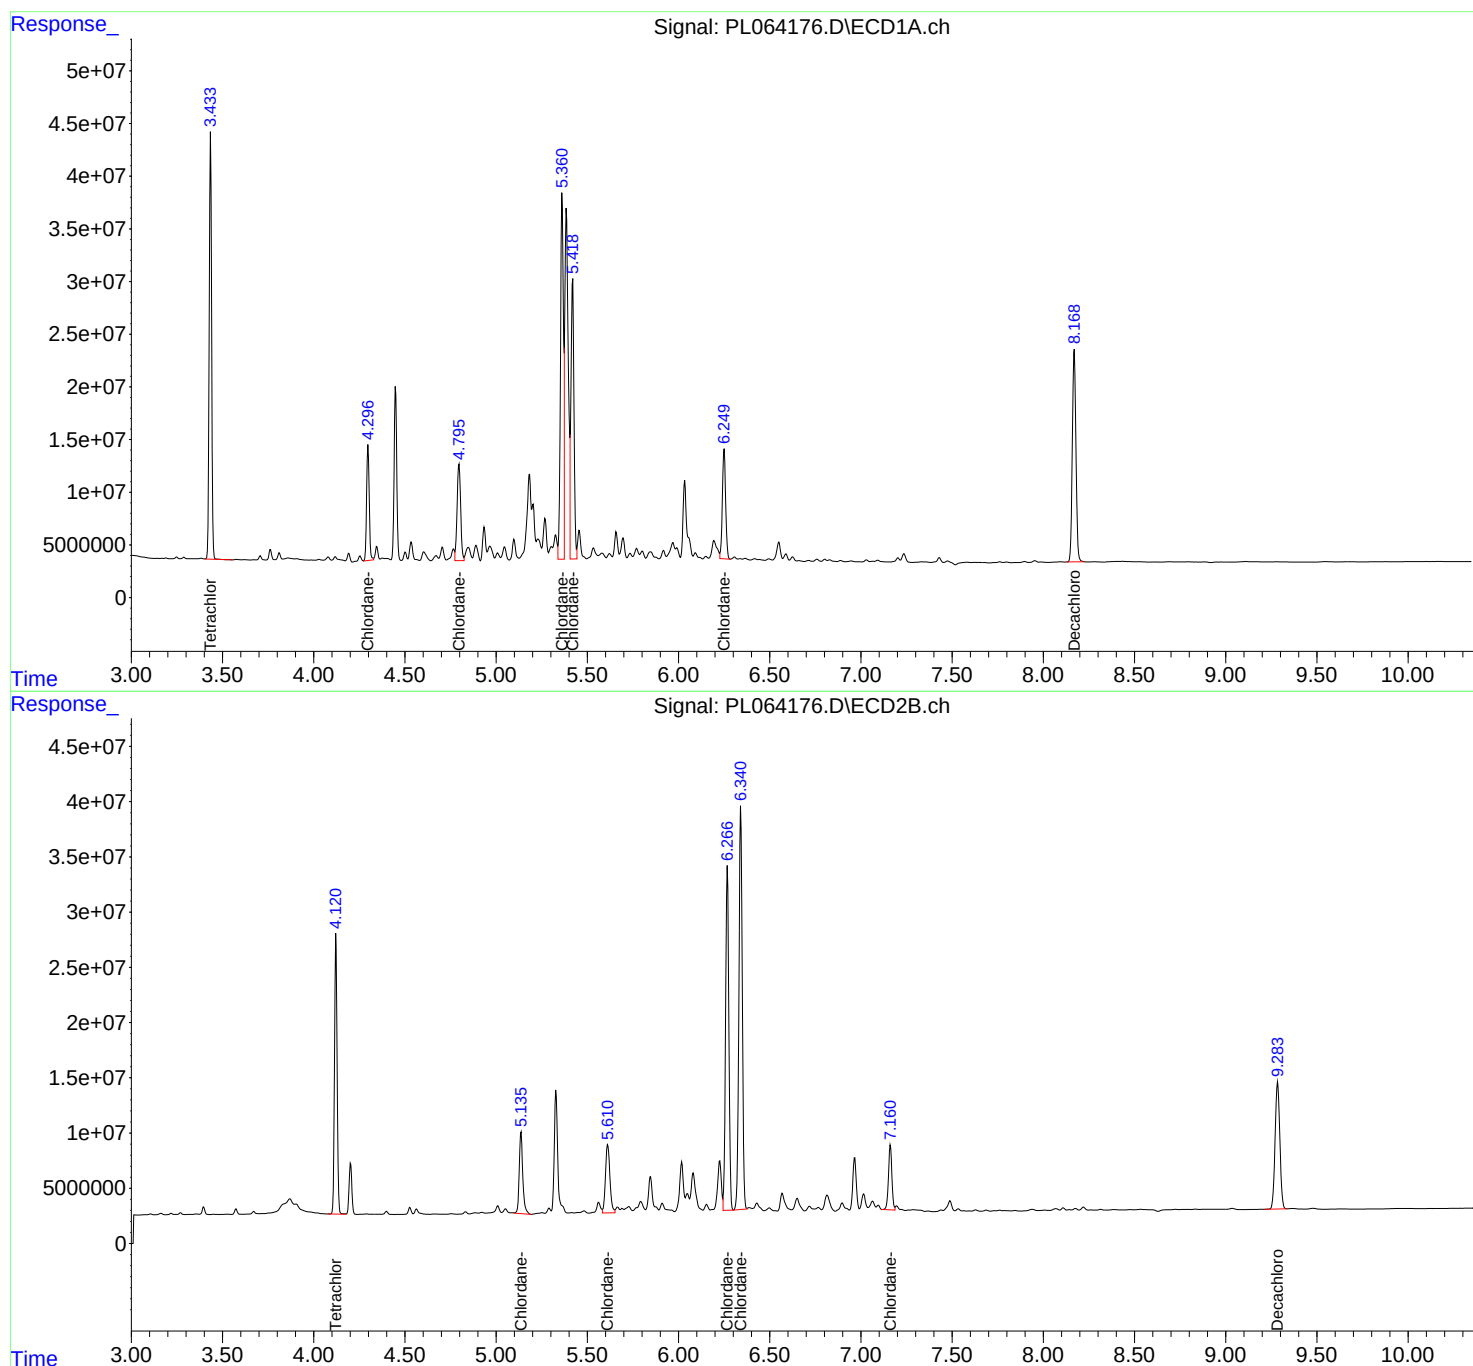


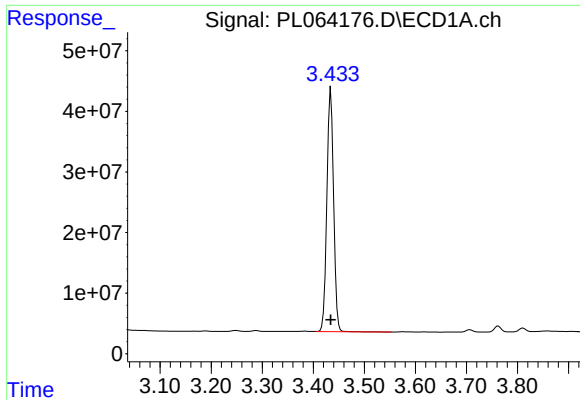

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 365933369
Conc: 95.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

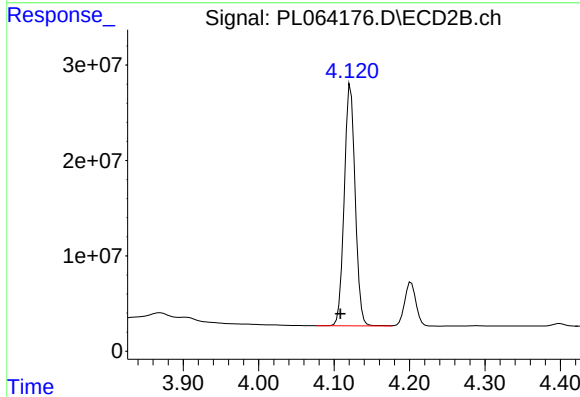


#1 Tetrachloro-m-xylene

R.T.: 4.122 min
Delta R.T.: 0.014 min
Response: 253953152
Conc: 96.71 ng/ml

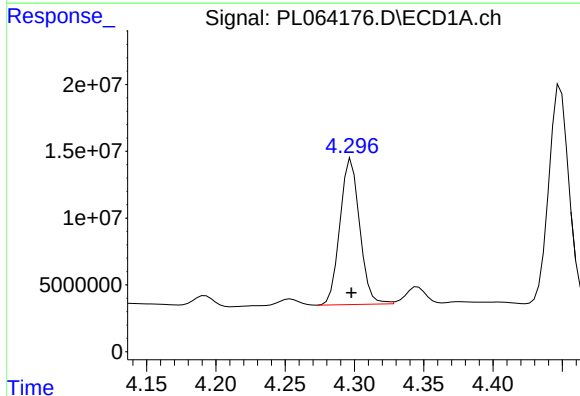


#23 Chlordane-1

R.T.: 4.298 min
Delta R.T.: 0.000 min
Response: 108175490
Conc: 941.05 ng/ml

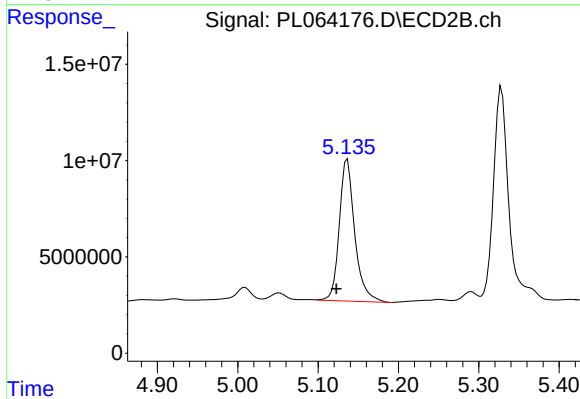

#23 Chlordane-1


R.T.: 5.136 min
Delta R.T.: 0.014 min
Response: 98533582
Conc: 924.26 ng/ml

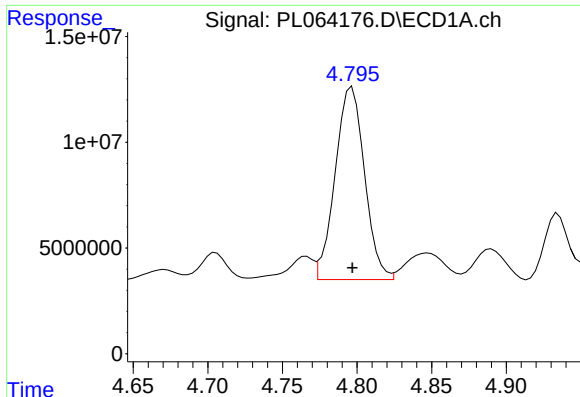

#24 Chlordane-2


R.T.: 4.797 min
Delta R.T.: 0.000 min
Response: 124932731
Conc: 897.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

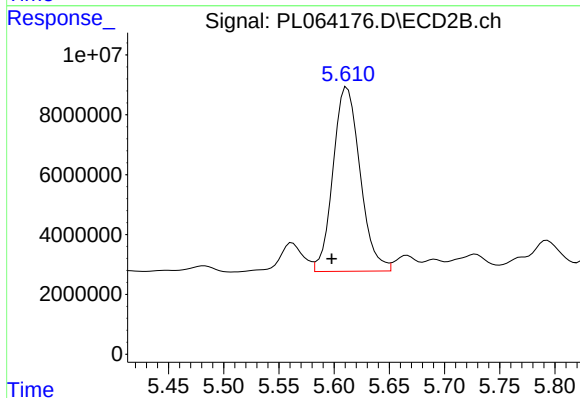


#24 Chlordane-2

R.T.: 5.612 min
Delta R.T.: 0.014 min
Response: 105106729
Conc: 876.65 ng/ml

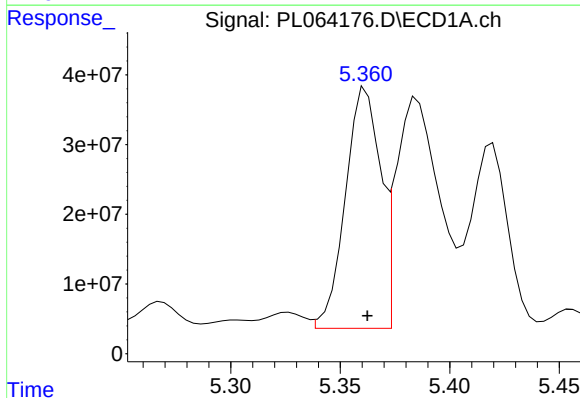


#25 Chlordane-3

R.T.: 5.362 min
Delta R.T.: 0.000 min
Response: 382730444
Conc: 958.94 ng/ml

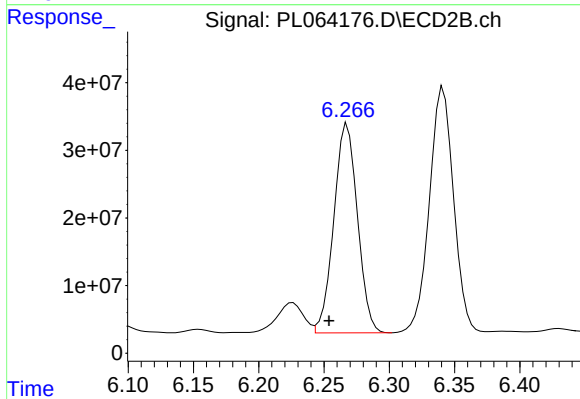

#25 Chlordane-3


R.T.: 6.268 min
Delta R.T.: 0.014 min
Response: 389923740
Conc: 960.02 ng/ml

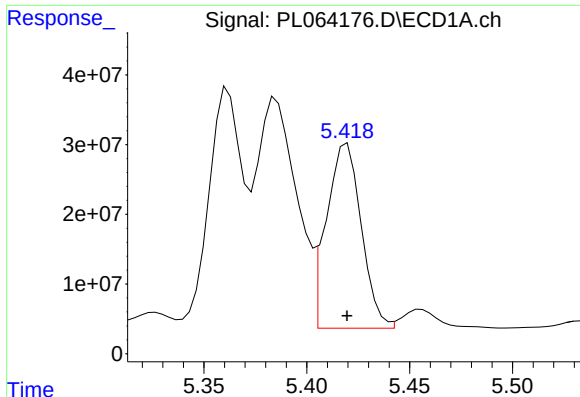

#26 Chlordane-4


R.T.: 5.420 min
Delta R.T.: 0.000 min
Response: 312583636
Conc: 942.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

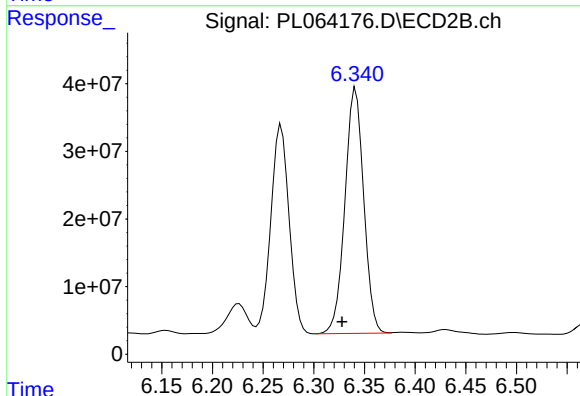


#26 Chlordane-4

R.T.: 6.341 min
Delta R.T.: 0.014 min
Response: 467246742
Conc: 944.96 ng/ml

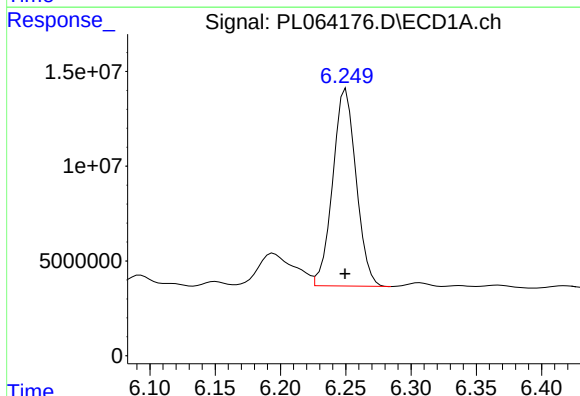


#27 Chlordane-5

R.T.: 6.250 min
Delta R.T.: 0.000 min
Response: 129716094
Conc: 946.31 ng/ml

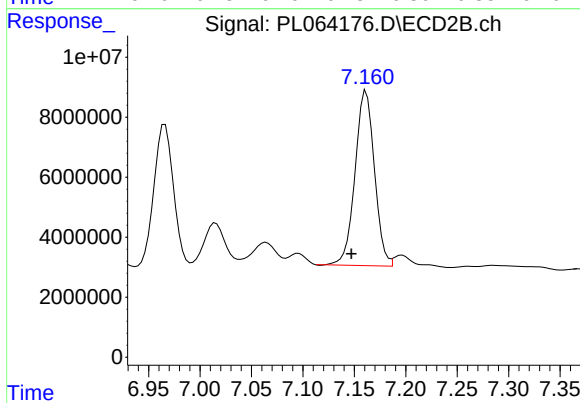

#27 Chlordane-5


R.T.: 7.161 min
Delta R.T.: 0.014 min
Response: 76578891
Conc: 1004.18 ng/ml

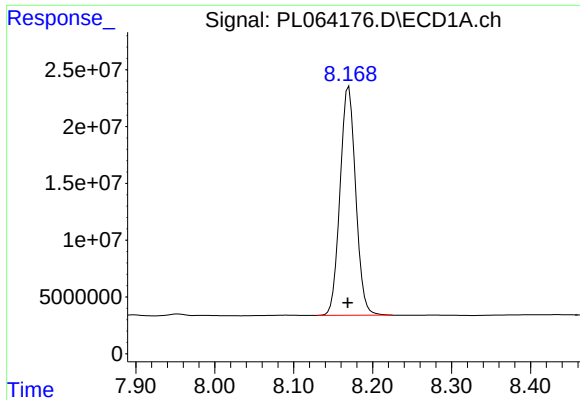

#28 Decachlorobiphenyl

R.T.: 8.170 min
Delta R.T.: 0.001 min
Response: 277296370
Conc: 90.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

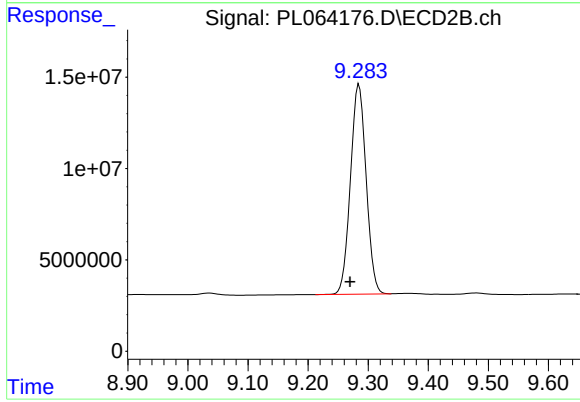

#28 Decachlorobiphenyl

R.T.: 9.285 min
Delta R.T.: 0.014 min
Response: 207758412
Conc: 91.59 ng/ml