

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011821\
 Data File : PL064177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2021 11:35
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 12:36:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 12:33:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.108	286.3E6	195.6E6	74.802	74.492
28)	SA Decachlor...	8.169	9.271	218.0E6	163.7E6	71.406	72.169
Target Compounds							
23)	Chlordane-1	4.297	5.123	84411965	77327312	734.327	725.343
24)	Chlordane-2	4.796	5.598	98895300	84975165	710.651	708.740
25)	Chlordane-3	5.362	6.254	296.8E6	304.0E6	743.699	748.379
26)	Chlordane-4	5.420	6.328	243.4E6	366.0E6	733.963	740.140
27)	Chlordane-5	6.249	7.148	100.5E6	55321151	733.377	725.426


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011821\
Data File : PL064177.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2021 11:35
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 12:36:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 12:33:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

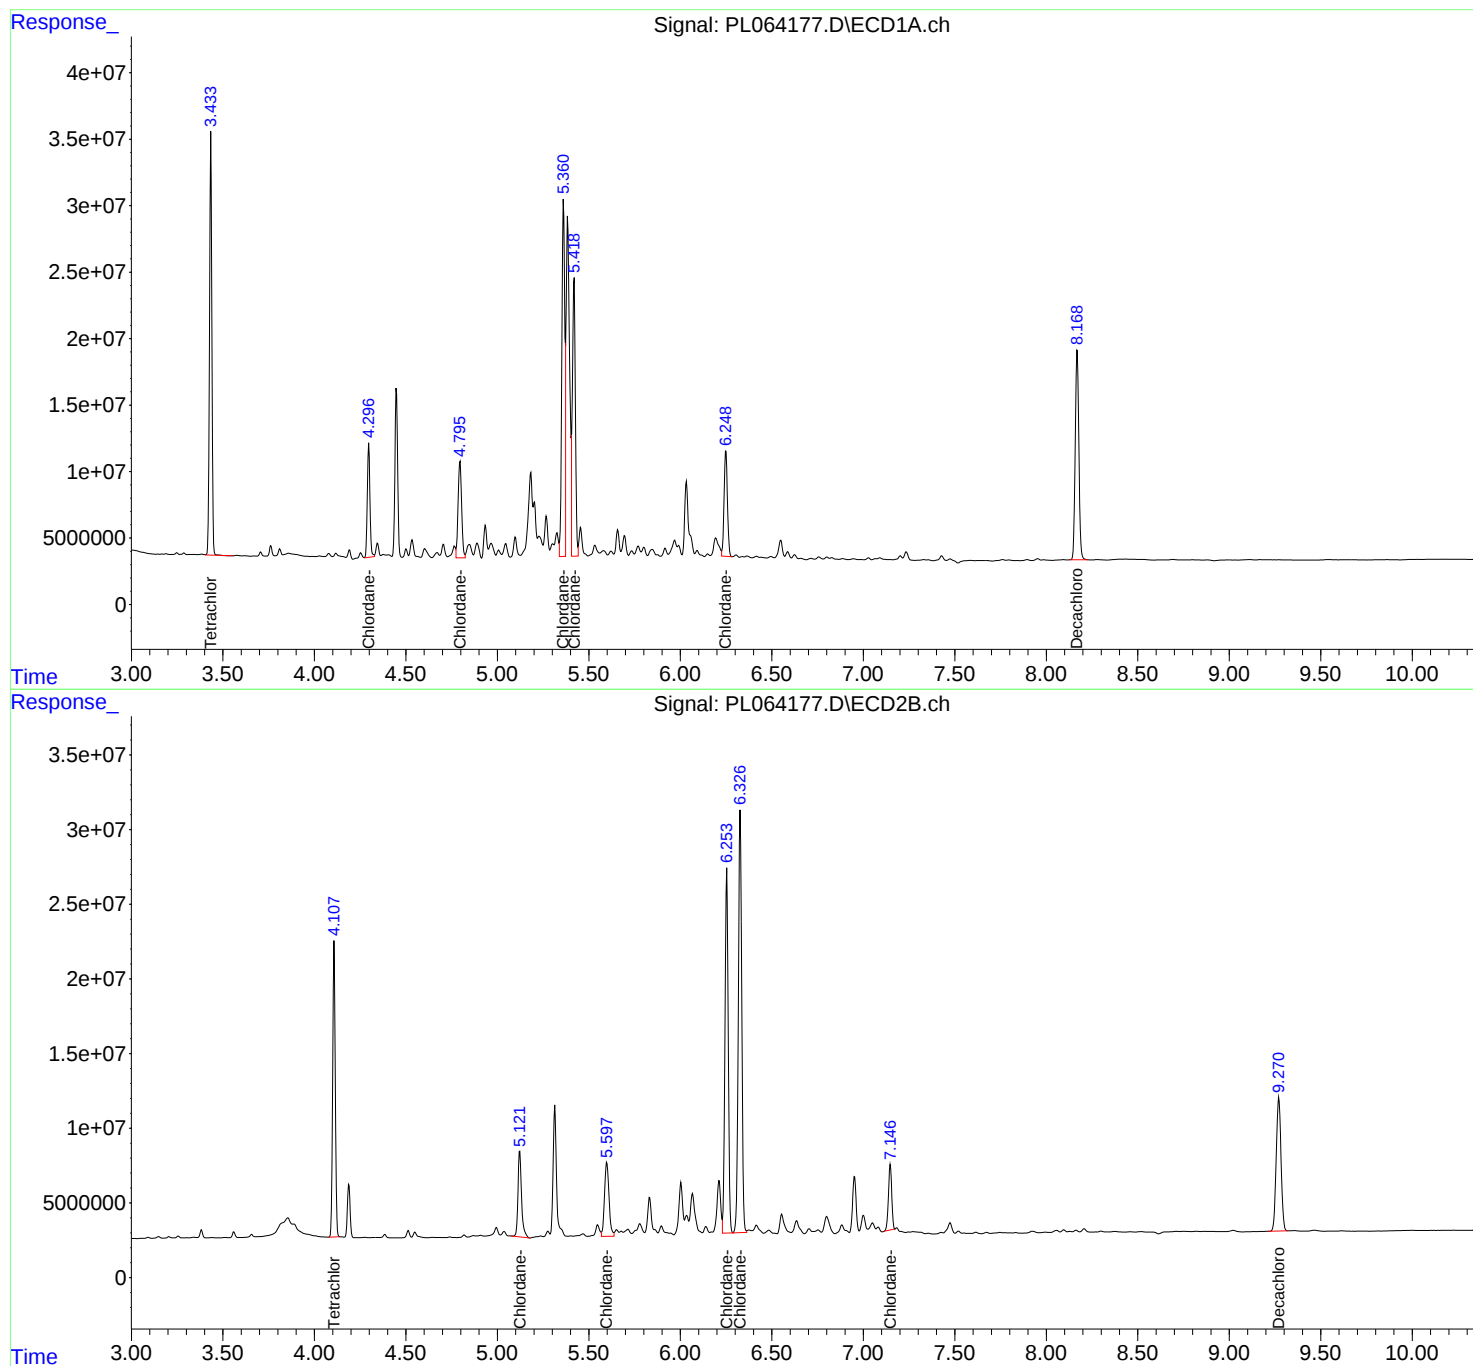


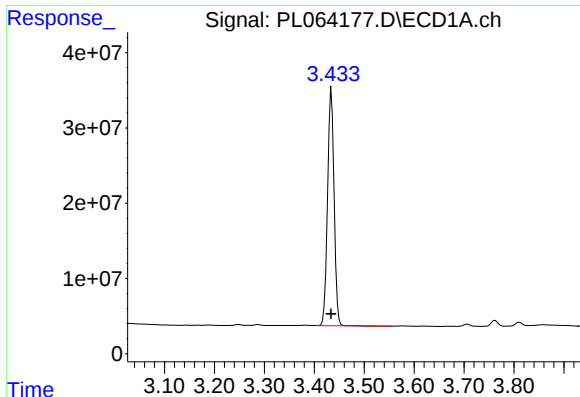

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 286276209
Conc: 74.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

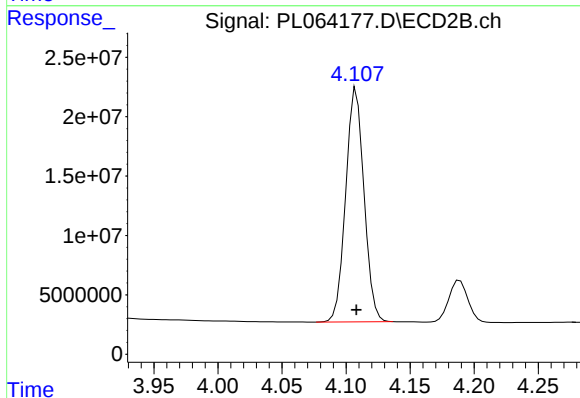


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 195620363
Conc: 74.49 ng/ml

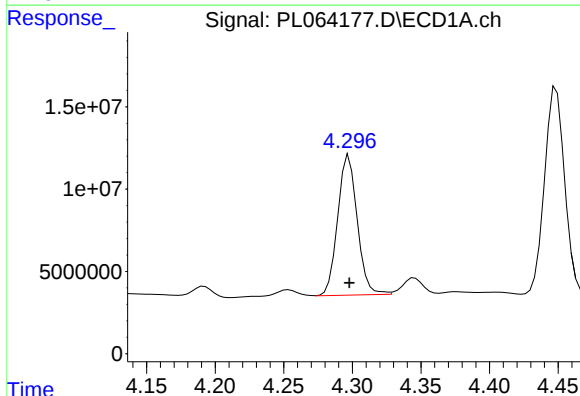


#23 Chlordane-1

R.T.: 4.297 min
Delta R.T.: 0.000 min
Response: 84411965
Conc: 734.33 ng/ml

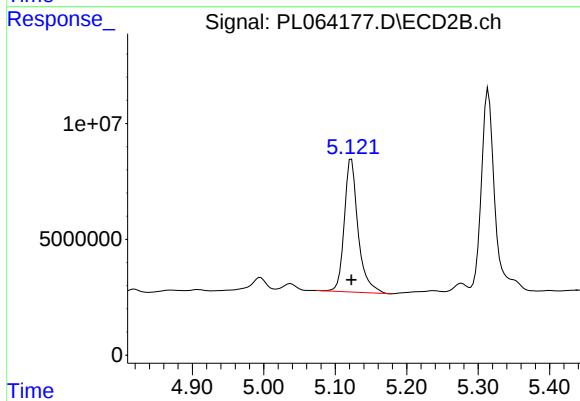

#23 Chlordane-1


R.T.: 5.123 min
Delta R.T.: 0.000 min
Response: 77327312
Conc: 725.34 ng/ml

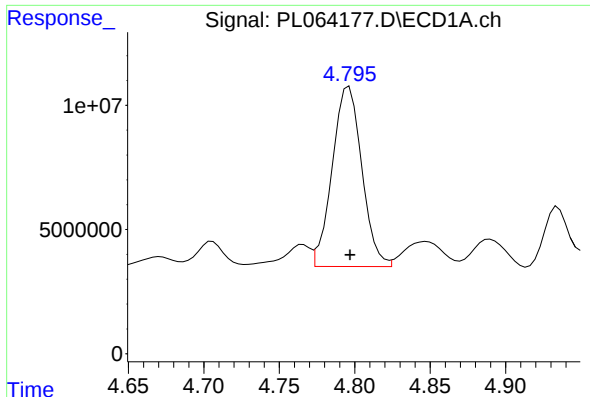

#24 Chlordane-2


R.T.: 4.796 min
Delta R.T.: 0.000 min
Response: 98895300
Conc: 710.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

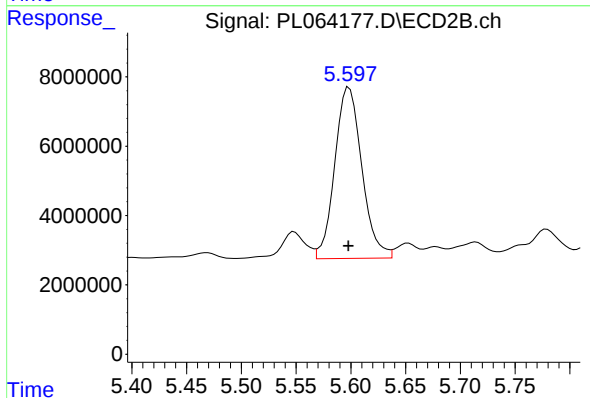


#24 Chlordane-2

R.T.: 5.598 min
Delta R.T.: 0.000 min
Response: 84975165
Conc: 708.74 ng/ml

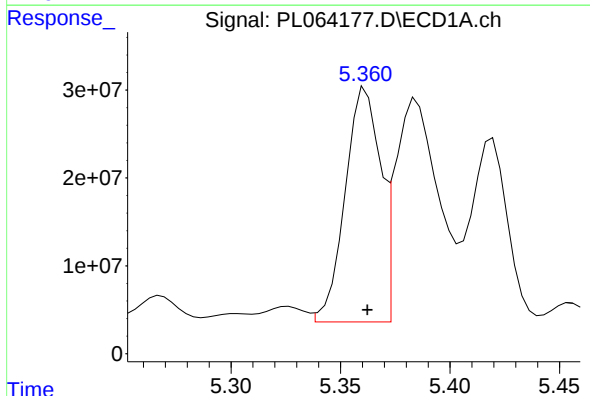


#25 Chlordane-3

R.T.: 5.362 min
Delta R.T.: 0.000 min
Response: 296823487
Conc: 743.70 ng/ml

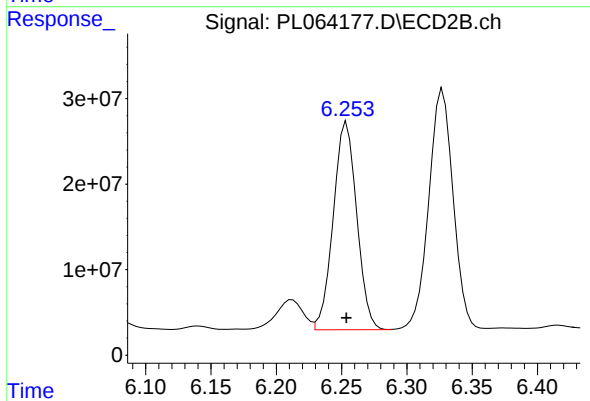

#25 Chlordane-3


R.T.: 6.254 min
Delta R.T.: 0.000 min
Response: 303962756
Conc: 748.38 ng/ml

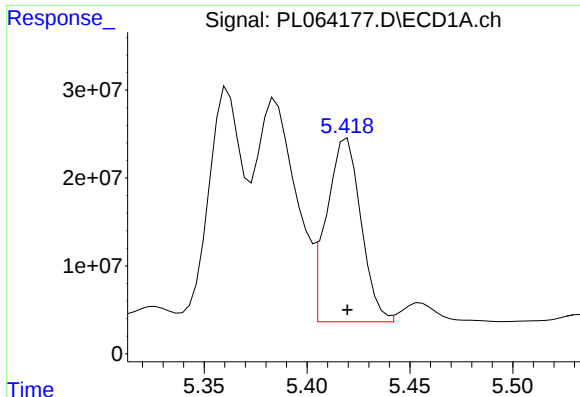

#26 Chlordane-4


R.T.: 5.420 min
Delta R.T.: 0.000 min
Response: 243362850
Conc: 733.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

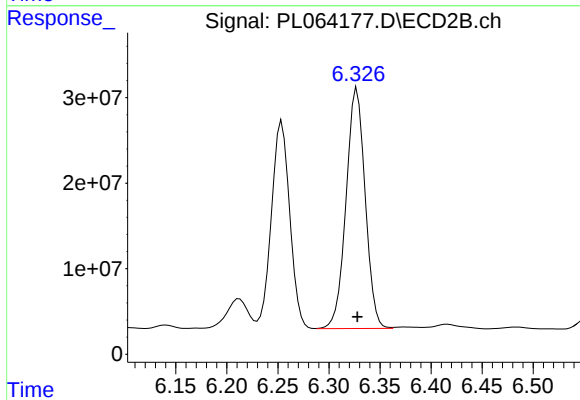


#26 Chlordane-4

R.T.: 6.328 min
Delta R.T.: 0.000 min
Response: 365971701
Conc: 740.14 ng/ml

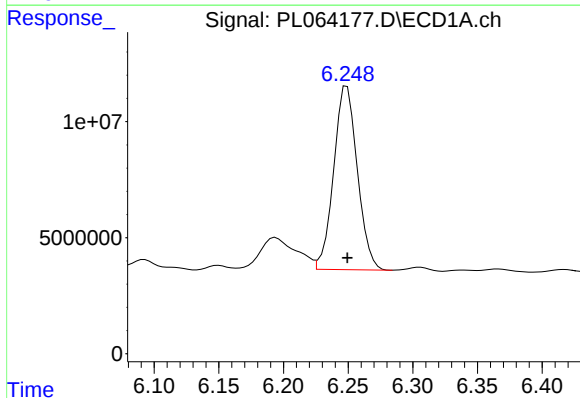


#27 Chlordane-5

R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 100528282
Conc: 733.38 ng/ml

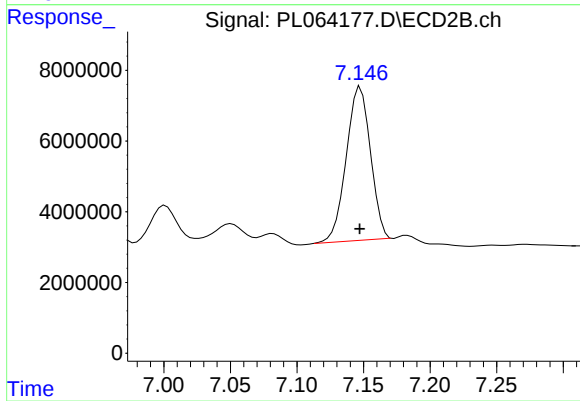

#27 Chlordane-5


R.T.: 7.148 min
Delta R.T.: 0.000 min
Response: 55321151
Conc: 725.43 ng/ml

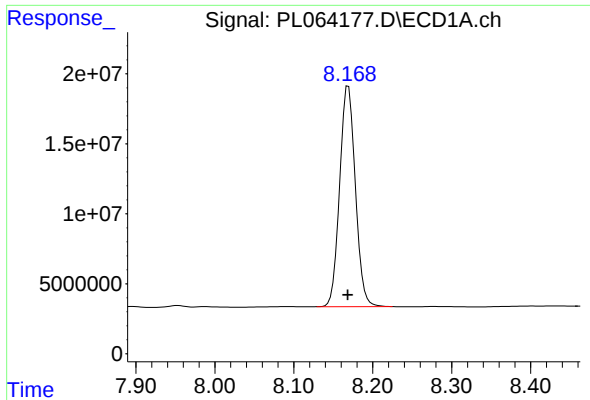

#28 Decachlorobiphenyl

R.T.: 8.169 min
Delta R.T.: 0.000 min
Response: 218024457
Conc: 71.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

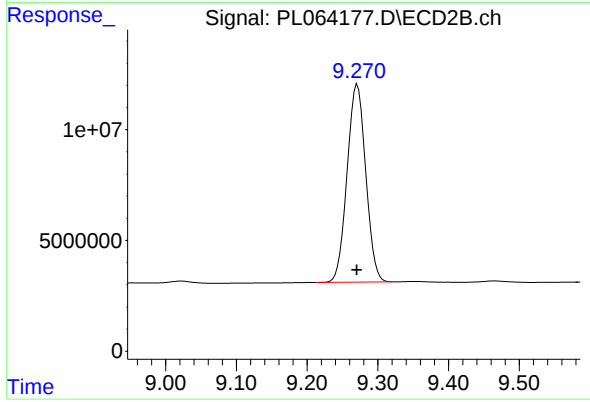

#28 Decachlorobiphenyl

R.T.: 9.271 min
Delta R.T.: 0.000 min
Response: 163708763
Conc: 72.17 ng/ml