

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011821\
 Data File : PL064178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2021 11:49
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 12:36:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 12:33:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.108	191.4E6	131.3E6	50.000	50.000
28)	SA Decachlor...	8.168	9.270	152.7E6	113.4E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.298	5.123	57475751	53303991	500.000	500.000
24)	Chlordane-2	4.797	5.598	69580738	59948011	500.000	500.000
25)	Chlordane-3	5.362	6.254	199.6E6	203.1E6	500.000	500.000
26)	Chlordane-4	5.420	6.328	165.8E6	247.2E6	500.000	500.000
27)	Chlordane-5	6.249	7.147	68537912	38130099	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011821\
Data File : PL064178.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2021 11:49
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 12:36:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 12:33:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

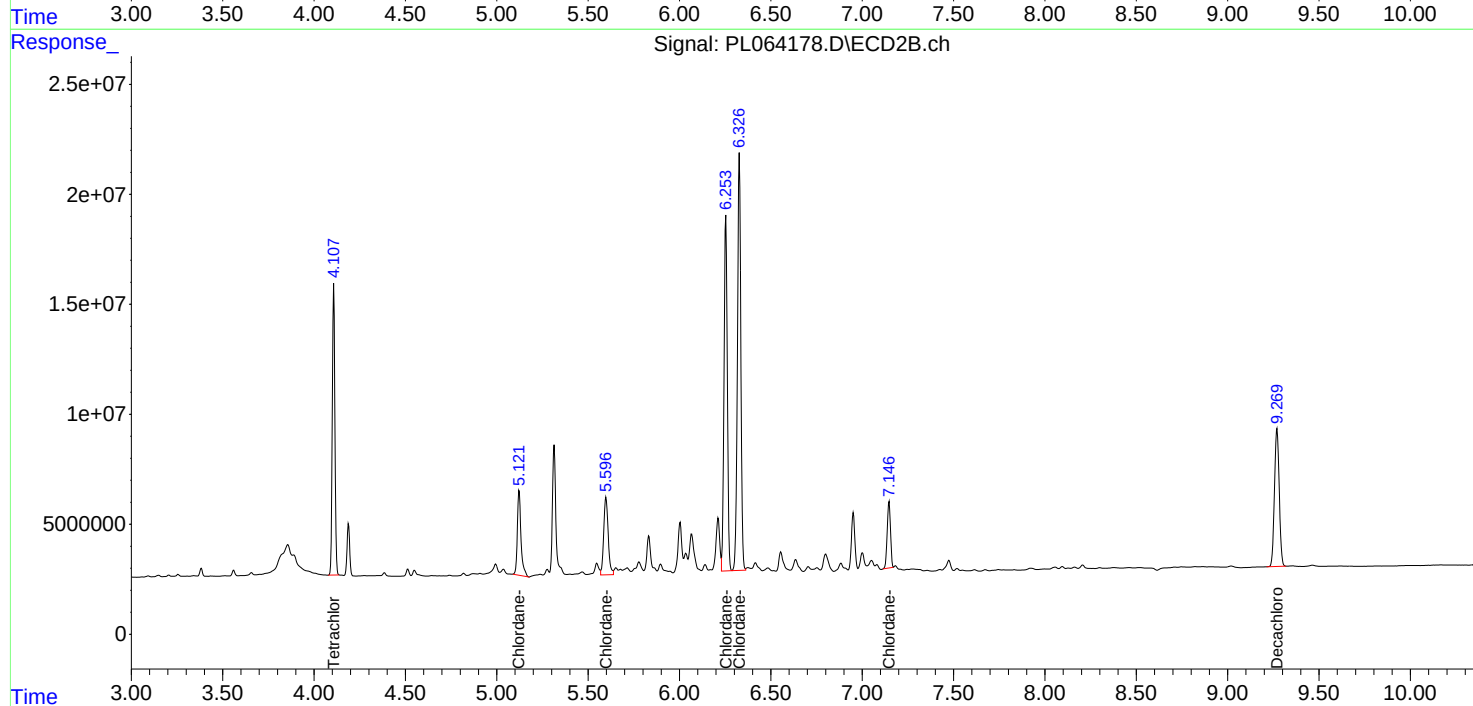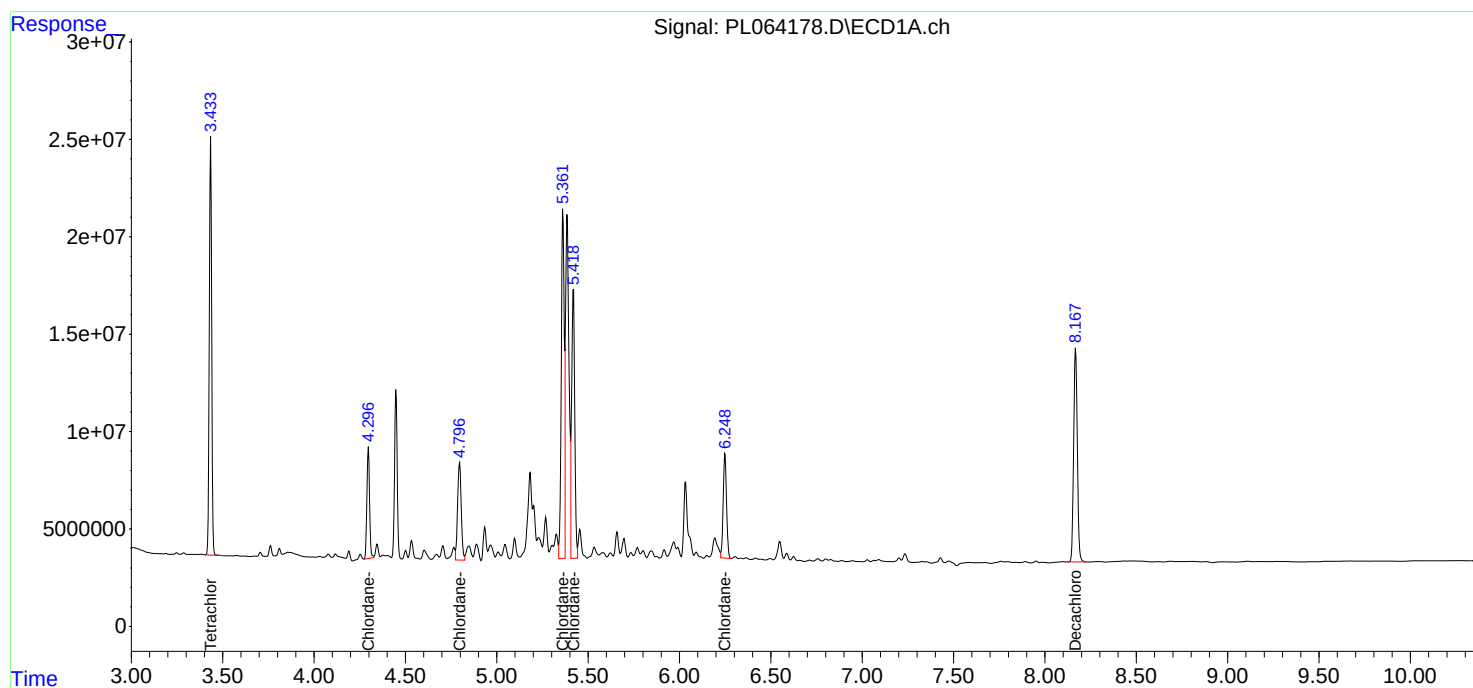


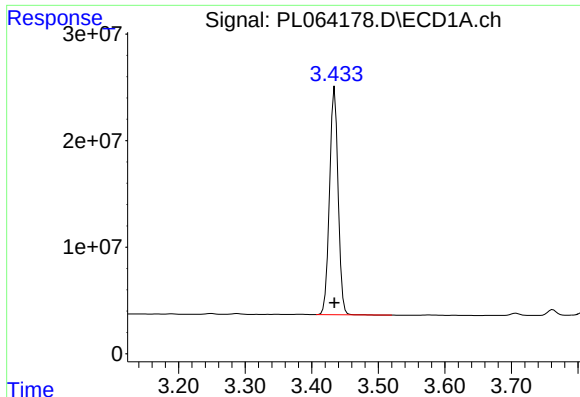

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 191356314
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

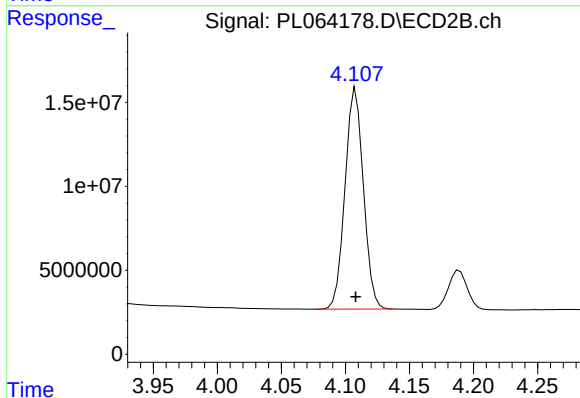


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 131302944
Conc: 50.00 ng/ml

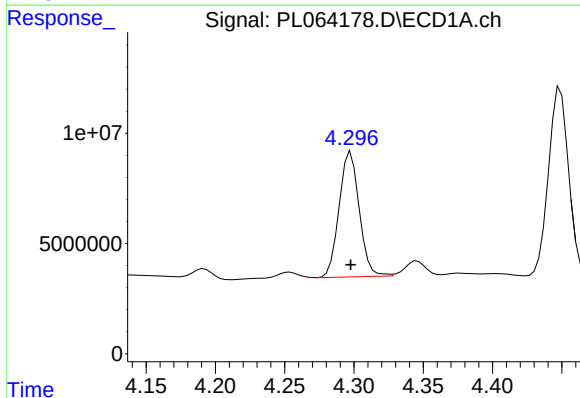


#23 Chlordane-1

R.T.: 4.298 min
Delta R.T.: 0.000 min
Response: 57475751
Conc: 500.00 ng/ml

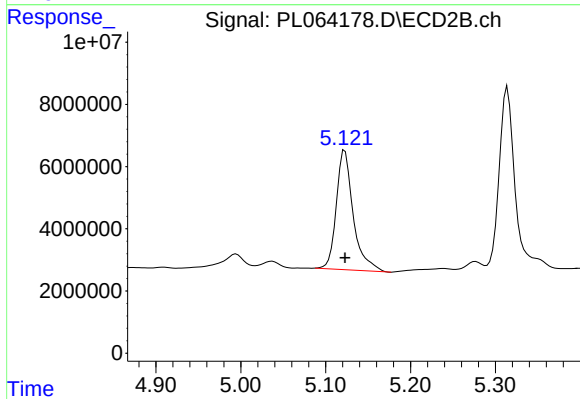

#23 Chlordane-1


R.T.: 5.123 min
Delta R.T.: 0.000 min
Response: 53303991
Conc: 500.00 ng/ml

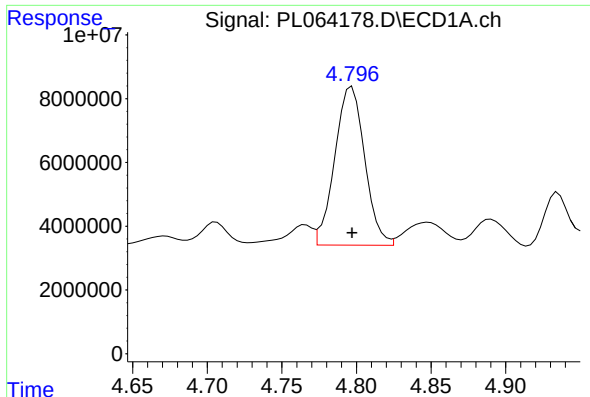

#24 Chlordane-2


R.T.: 4.797 min
Delta R.T.: 0.000 min
Response: 69580738
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

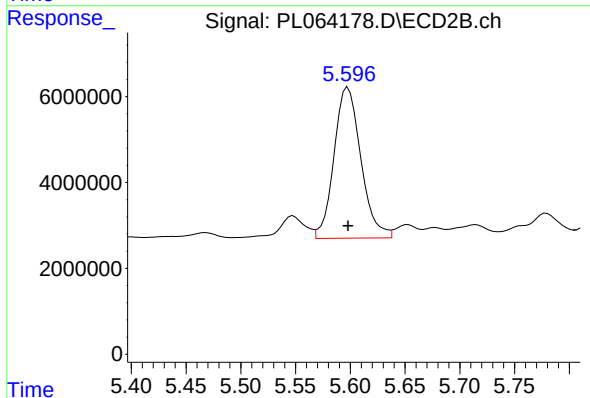


#24 Chlordane-2

R.T.: 5.598 min
Delta R.T.: 0.000 min
Response: 59948011
Conc: 500.00 ng/ml

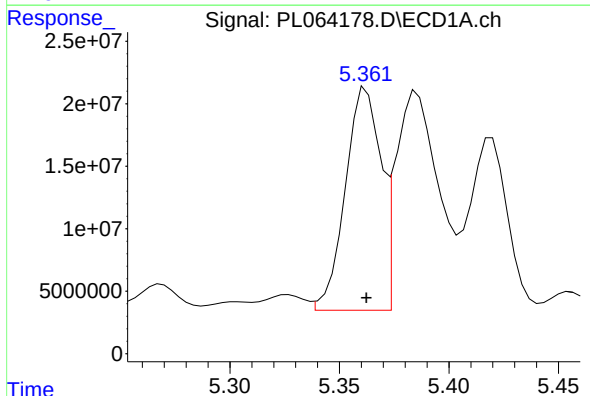


#25 Chlordane-3

R.T.: 5.362 min
Delta R.T.: 0.000 min
Response: 199559002
Conc: 500.00 ng/ml

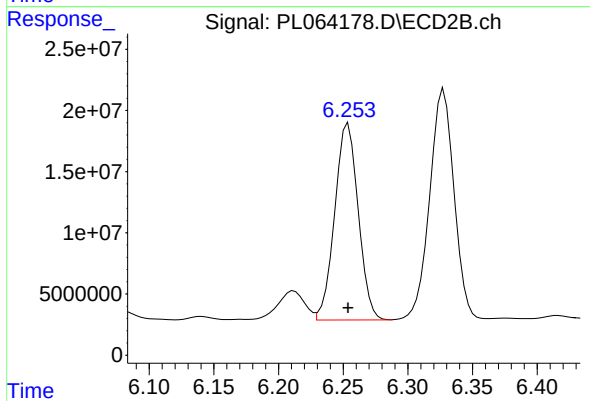

#25 Chlordane-3


R.T.: 6.254 min
Delta R.T.: 0.000 min
Response: 203080898
Conc: 500.00 ng/ml

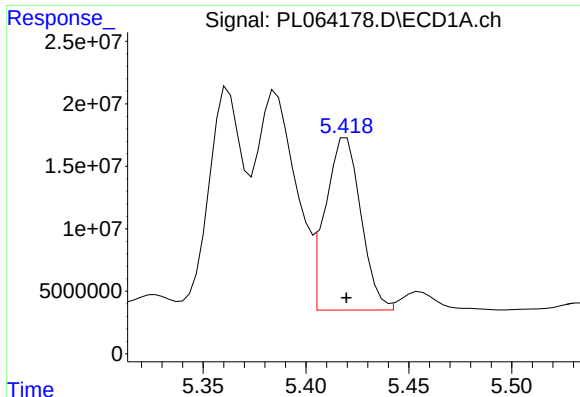

#26 Chlordane-4


R.T.: 5.420 min
Delta R.T.: 0.000 min
Response: 165786933
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

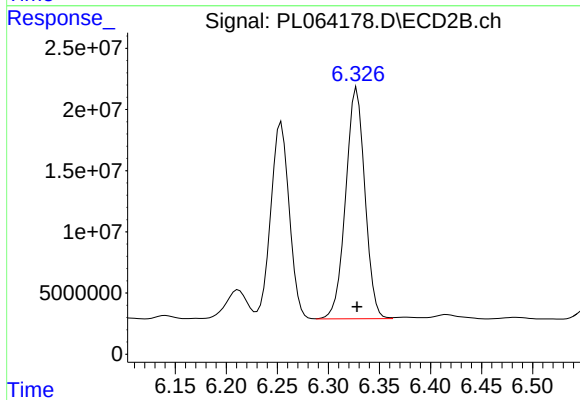


#26 Chlordane-4

R.T.: 6.328 min
Delta R.T.: 0.000 min
Response: 247231412
Conc: 500.00 ng/ml

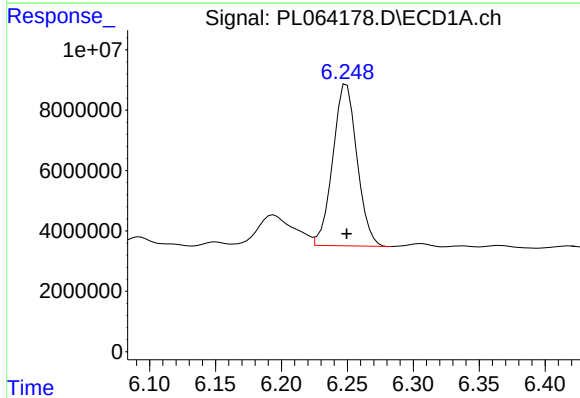


#27 Chlordane-5

R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 68537912
Conc: 500.00 ng/ml

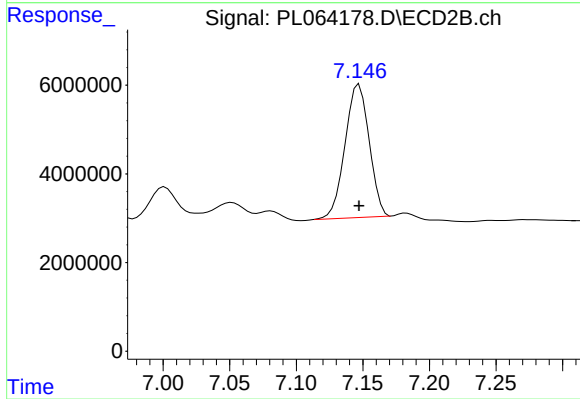

#27 Chlordane-5


R.T.: 7.147 min
Delta R.T.: 0.000 min
Response: 38130099
Conc: 500.00 ng/ml

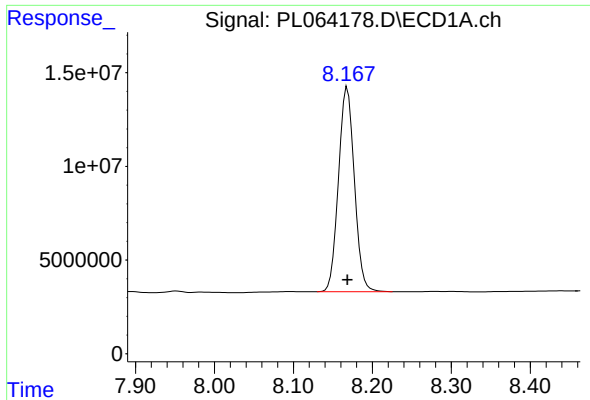

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 152666083
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

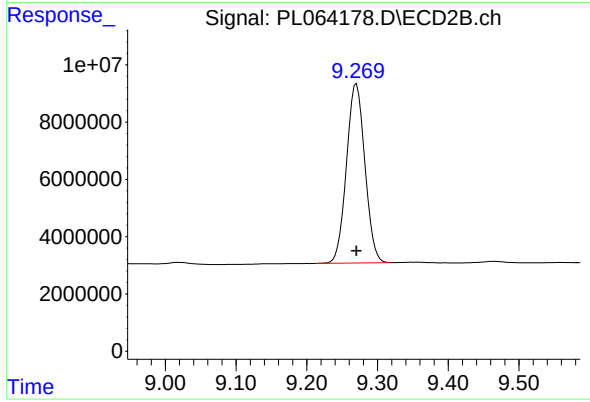

#28 Decachlorobiphenyl

R.T.: 9.270 min
Delta R.T.: 0.000 min
Response: 113420686
Conc: 50.00 ng/ml