

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011821\
 Data File : PL064181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2021 12:32
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL011821

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 13:22:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 12:47:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.108	183.4E6	127.7E6	48.260	48.741
28)	SA Decachlor...	8.169	9.272	152.7E6	114.1E6	47.693	48.393
Target Compounds							
23)	Chlordane-1	4.297	5.122	56057833	52030030	481.361	465.891
24)	Chlordane-2	4.796	5.597	67597212	58747293	480.302	463.382
25)	Chlordane-3	5.361	6.254	192.6E6	200.2E6	481.984	495.042
26)	Chlordane-4	5.419	6.328	161.0E6	243.8E6	489.469	493.262
27)	Chlordane-5	6.249	7.148	67232965	39814998	479.780	521.283



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011821\
Data File : PL064181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2021 12:32
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL011821

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 13:22:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 12:47:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

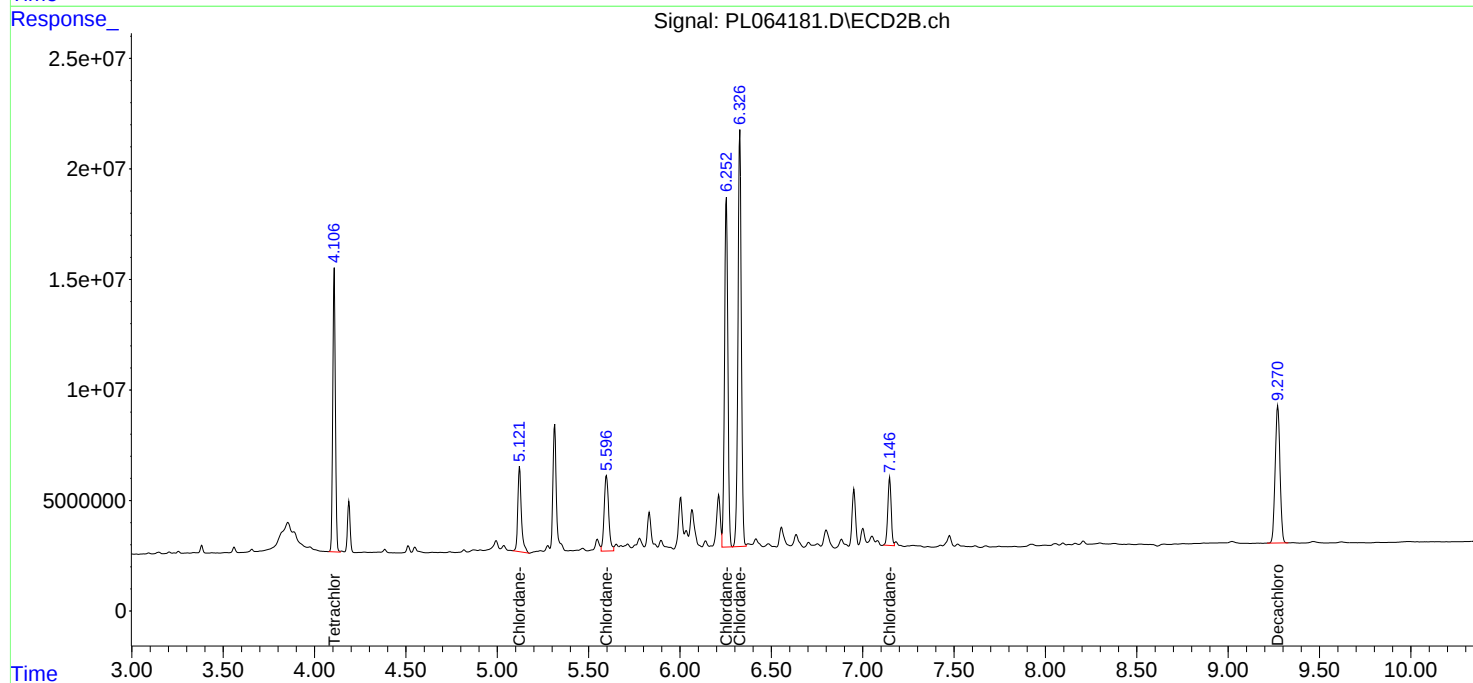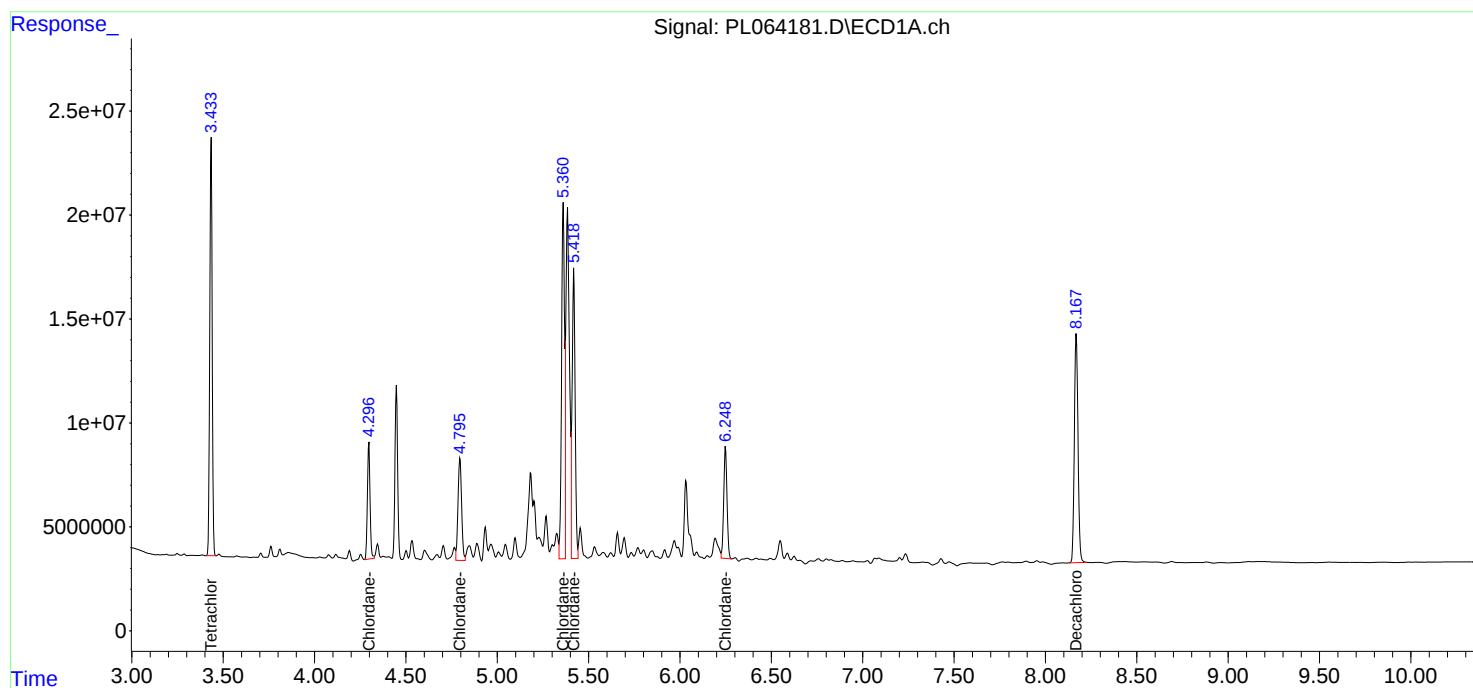


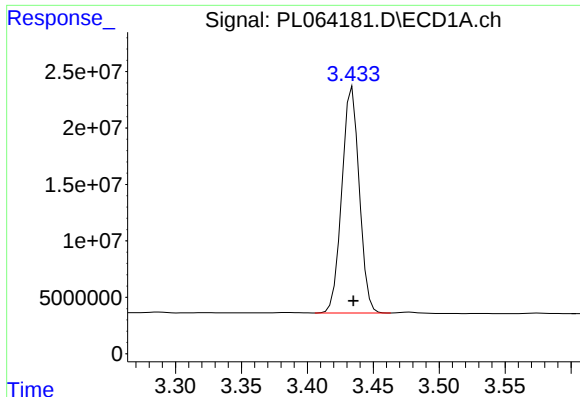

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 183448356
Conc: 48.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL011821

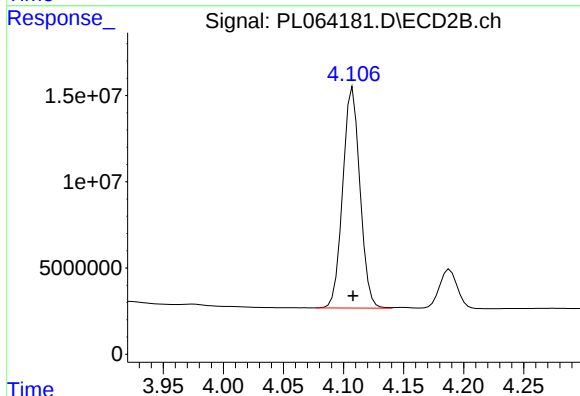


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 127676846
Conc: 48.74 ng/ml

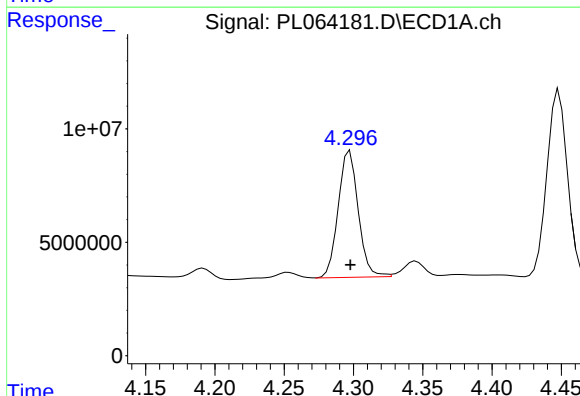


#23 Chlordane-1

R.T.: 4.297 min
Delta R.T.: 0.000 min
Response: 56057833
Conc: 481.36 ng/ml

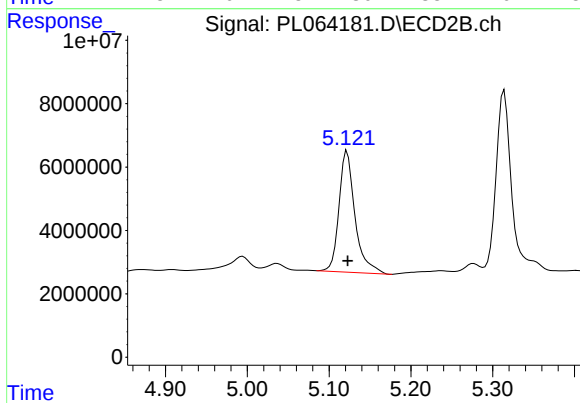

#23 Chlordane-1


R.T.: 5.122 min
Delta R.T.: 0.000 min
Response: 52030030
Conc: 465.89 ng/ml

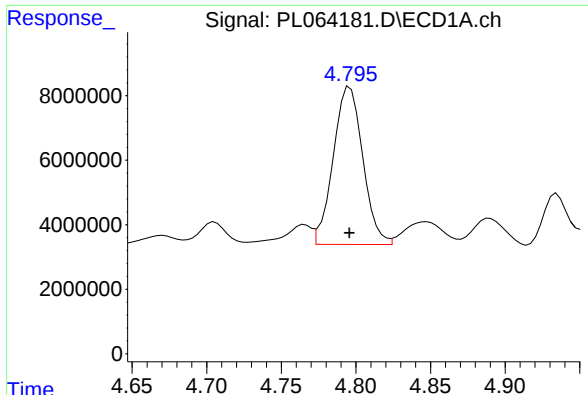

#24 Chlordane-2


R.T.: 4.796 min
Delta R.T.: 0.000 min
Response: 67597212
Conc: 480.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL011821

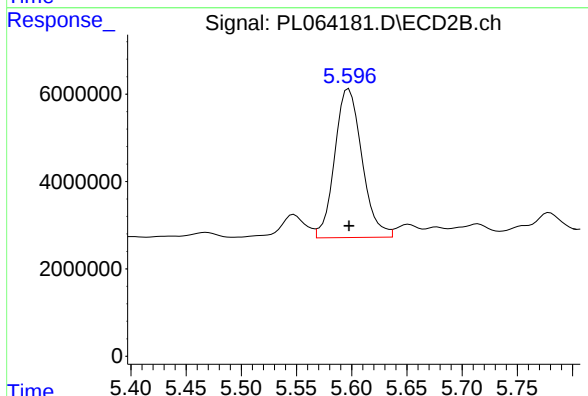


#24 Chlordane-2

R.T.: 5.597 min
Delta R.T.: 0.000 min
Response: 58747293
Conc: 463.38 ng/ml

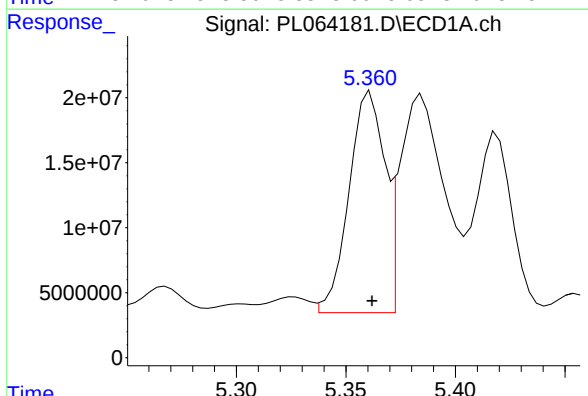


#25 Chlordane-3

R.T.: 5.361 min
Delta R.T.: 0.000 min
Response: 192579361
Conc: 481.98 ng/ml

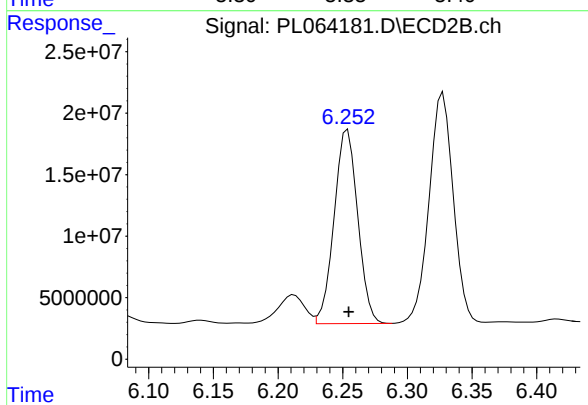

#25 Chlordane-3


R.T.: 6.254 min
Delta R.T.: 0.000 min
Response: 200163711
Conc: 495.04 ng/ml

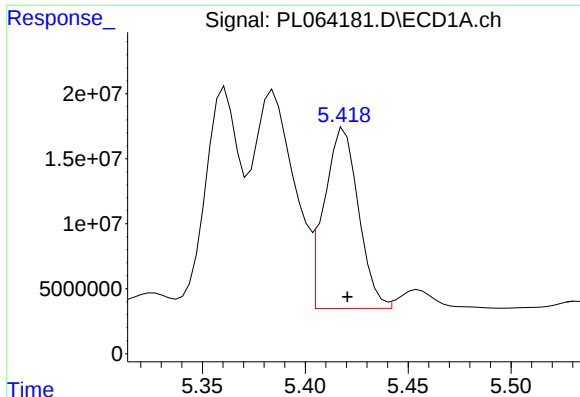

#26 Chlordane-4


R.T.: 5.419 min
Delta R.T.: -0.001 min
Response: 161049644
Conc: 489.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL011821

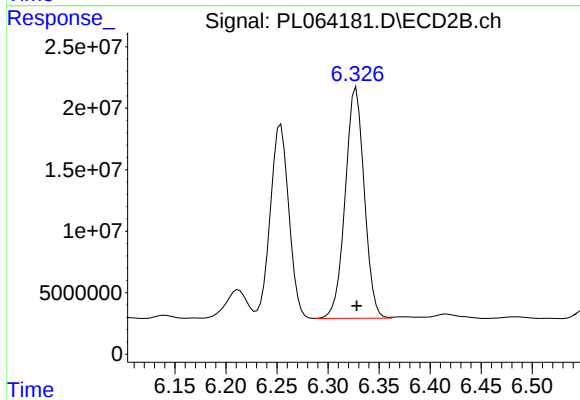


#26 Chlordane-4

R.T.: 6.328 min
Delta R.T.: 0.000 min
Response: 243812541
Conc: 493.26 ng/ml

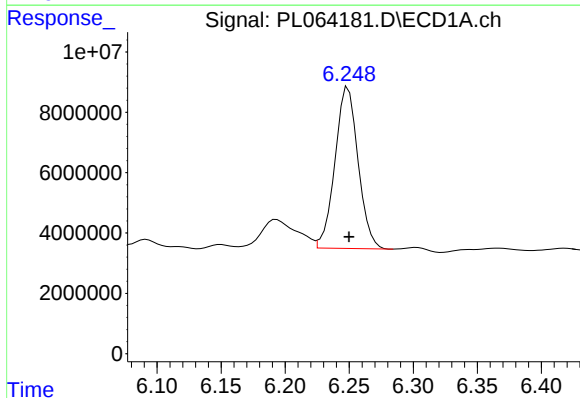


#27 Chlordane-5

R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 67232965
Conc: 479.78 ng/ml

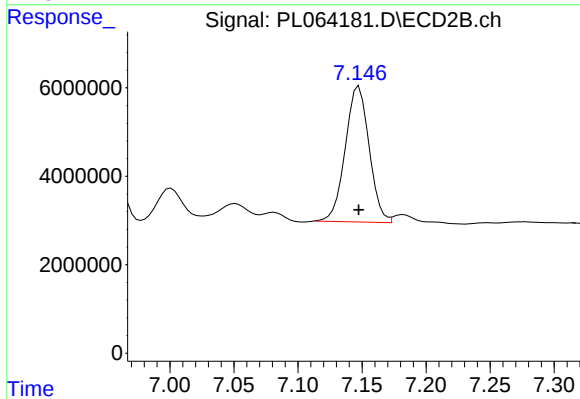

#27 Chlordane-5


R.T.: 7.148 min
Delta R.T.: 0.000 min
Response: 39814998
Conc: 521.28 ng/ml

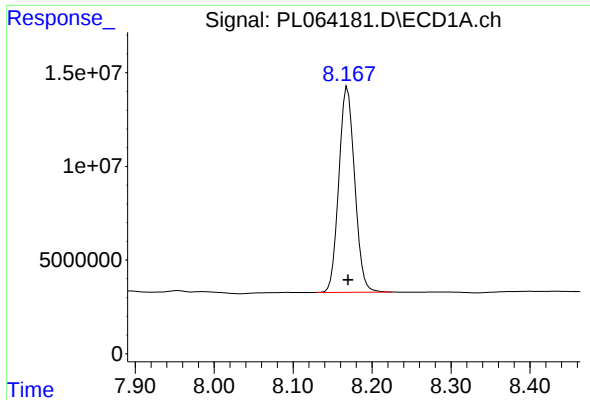

#28 Decachlorobiphenyl

R.T.: 8.169 min
Delta R.T.: 0.000 min
Response: 152680365
Conc: 47.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL011821

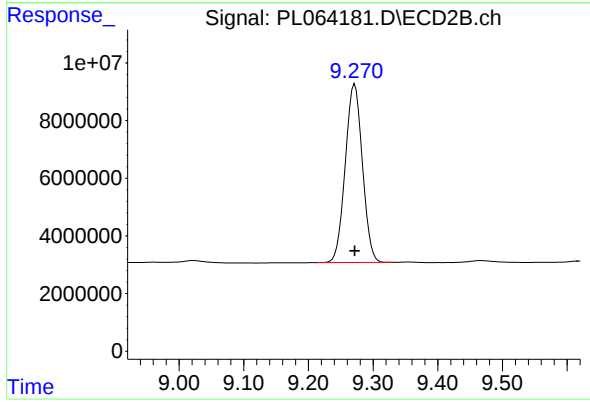

#28 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: 0.000 min
Response: 114071343
Conc: 48.39 ng/ml