

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011821\
 Data File : PL064193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2021 16:24
 Operator : AR\AJ
 Sample : M1146-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 520-Z

Manual Integrations
 APPROVED

Ankita
 1/19/2021 12:10:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 07:58:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	4.107	63491057	71857291	21.174m	28.108 #
28)	SA Decachlor...	8.169	9.270	56728187	42961762	18.587	18.101
Target Compounds							
13)	MA Dieldrin	5.713	6.641	2213191	1707064	0.595	0.607

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011821\
Data File : PL064193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2021 16:24
Operator : AR\AJ
Sample : M1146-02
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
520-Z


Manual Integrations
APPROVED

Ankita
1/19/2021 12:10:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 07:58:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

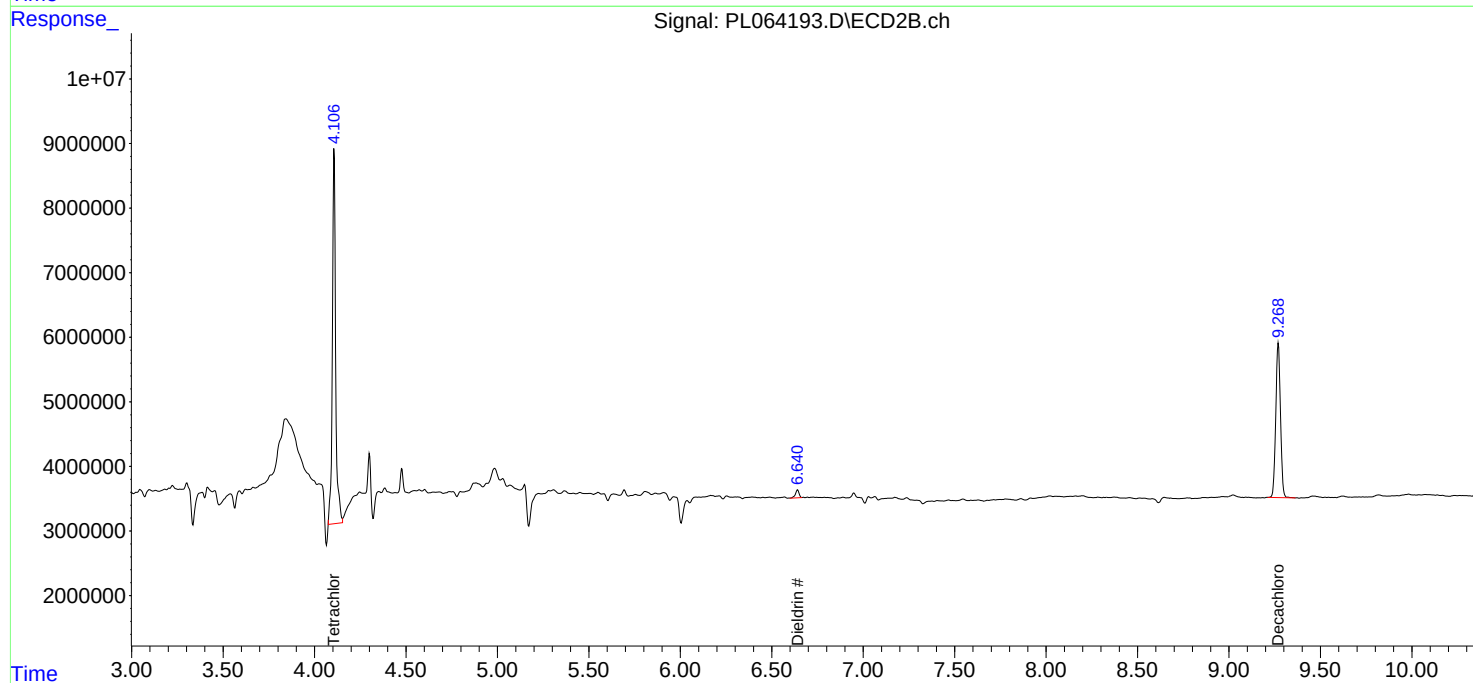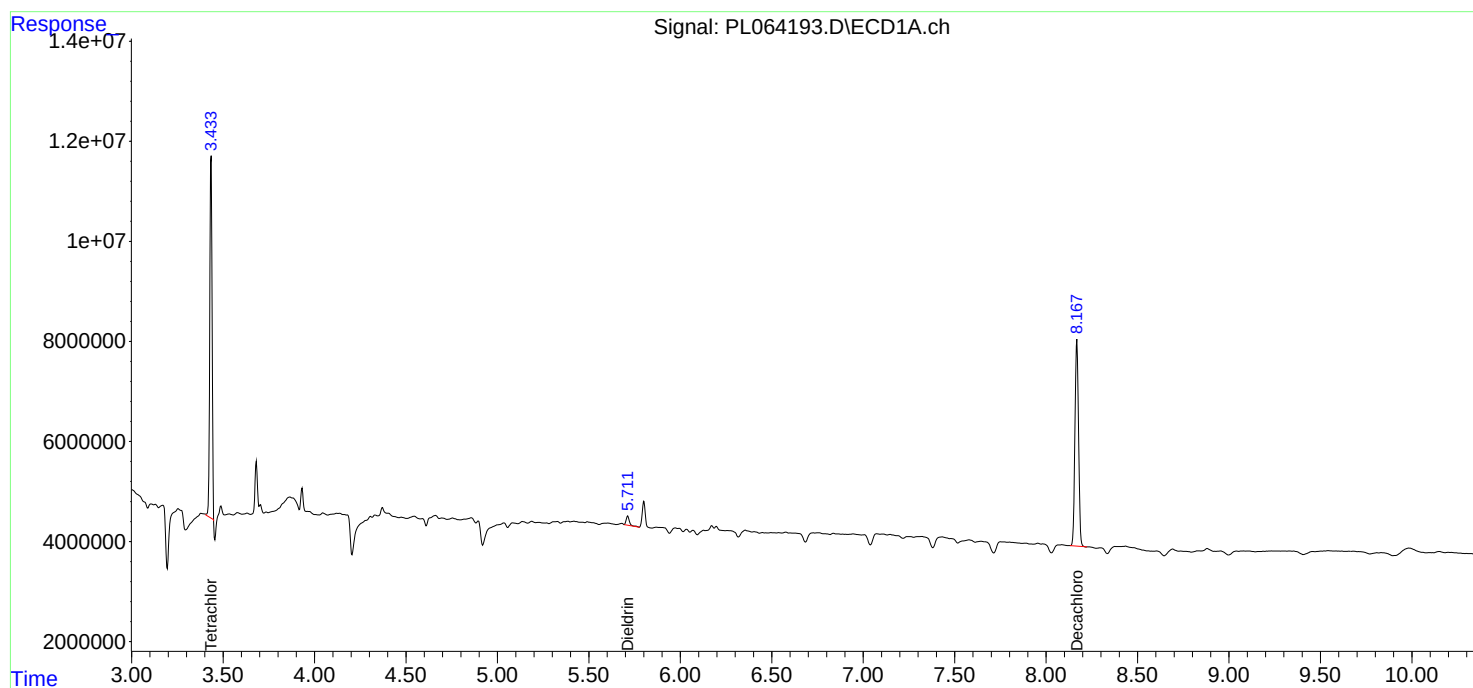

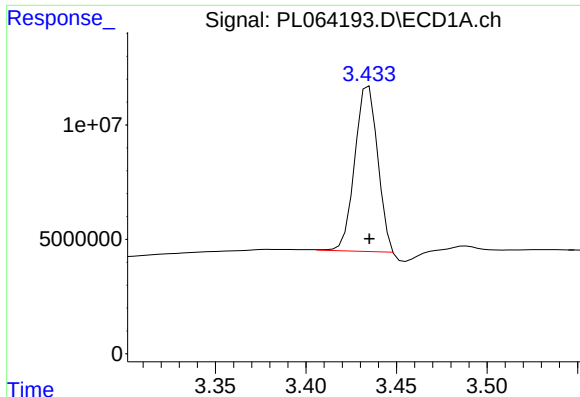


#1 Tetrachloro-m-xylene

R.T.: 3.433 min
Delta R.T.: -0.002 min
Response: 63491057
Conc: 21.17 ng/ml m

Instrument :
ECD_L
ClientSampleId :
520-Z


Manual Integrations
APPROVED

Ankita
1/19/2021 12:10:53 PM

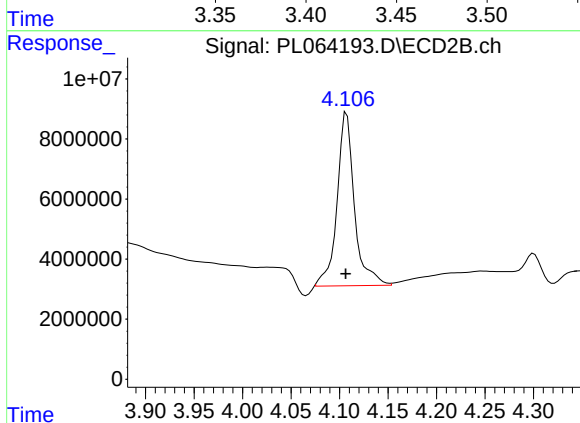


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.001 min
Response: 71857291
Conc: 28.11 ng/ml

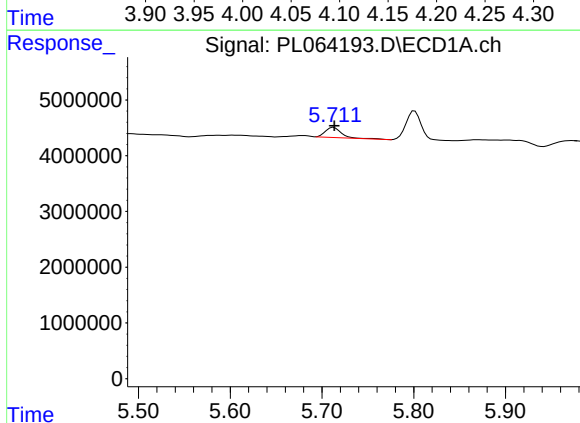


#13 Dieldrin

R.T.: 5.713 min
Delta R.T.: 0.000 min
Response: 2213191
Conc: 0.60 ng/ml

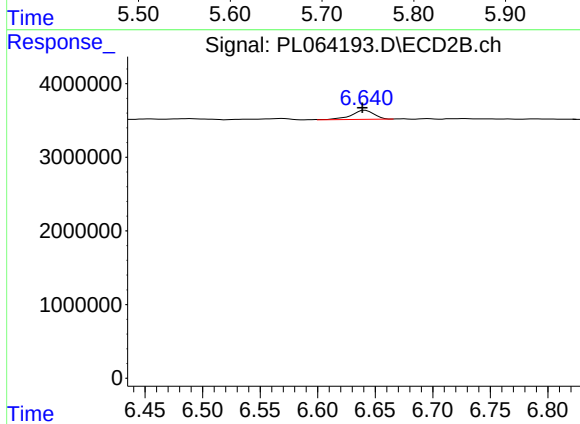

#13 Dieldrin

R.T.: 6.641 min
Delta R.T.: 0.002 min
Response: 1707064
Conc: 0.61 ng/ml

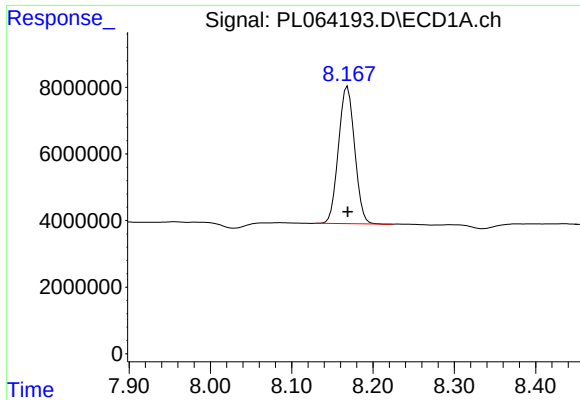


#28 Decachlorobiphenyl

R.T.: 8.169 min
Delta R.T.: 0.000 min
Response: 56728187
Conc: 18.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
520-Z

Manual Integrations
APPROVED

Ankita
1/19/2021 12:10:53 PM

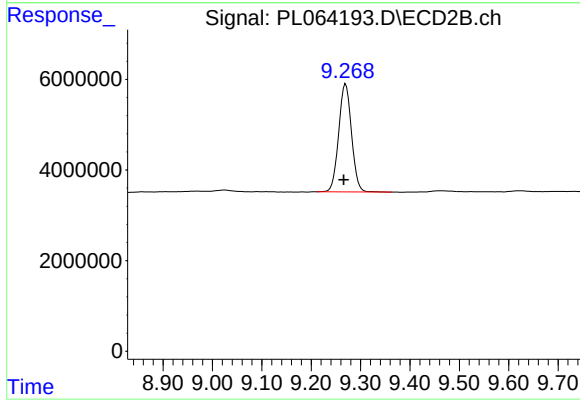

#28 Decachlorobiphenyl

R.T.: 9.270 min
Delta R.T.: 0.004 min
Response: 42961762
Conc: 18.10 ng/ml