

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011821\
 Data File : PL064197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2021 17:21
 Operator : AR\AJ
 Sample : M1160-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BASIN-2

Manual Integrations
 APPROVED

Ankita
 1/19/2021 12:10:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 08:00:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.107	65435679	51043456	21.823	19.967
28)	SA Decachlor...	8.168	9.270	60190328	45656169	19.721	19.237
Target Compounds							
12)	B 4,4'-DDE	5.584	6.481	5294510	2911824	1.503	1.093m#
17)	MA 4,4'-DDT	6.338	7.278	3770357	2582822	1.263m	1.140m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011821\
Data File : PL064197.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2021 17:21
Operator : AR\AJ
Sample : M1160-05
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BASIN-2


Manual Integrations
APPROVED

Ankita
1/19/2021 12:10:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 08:00:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

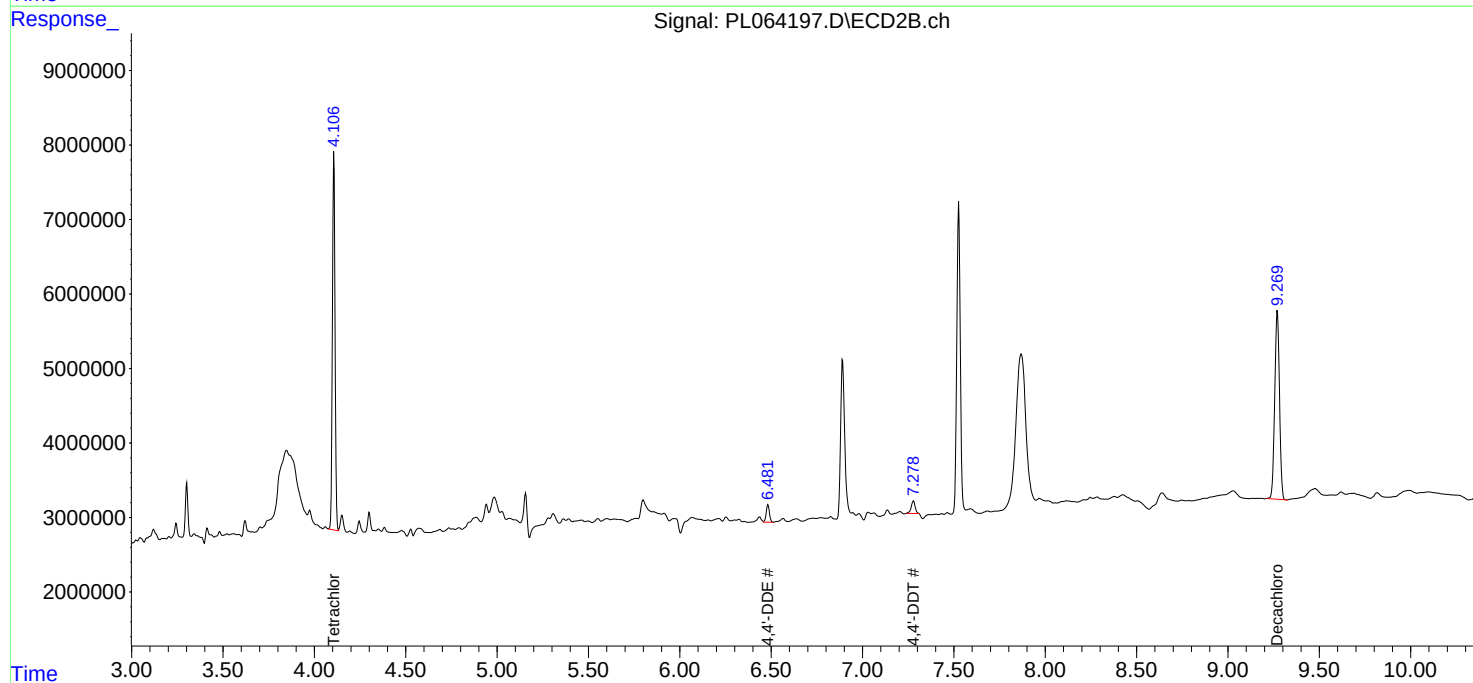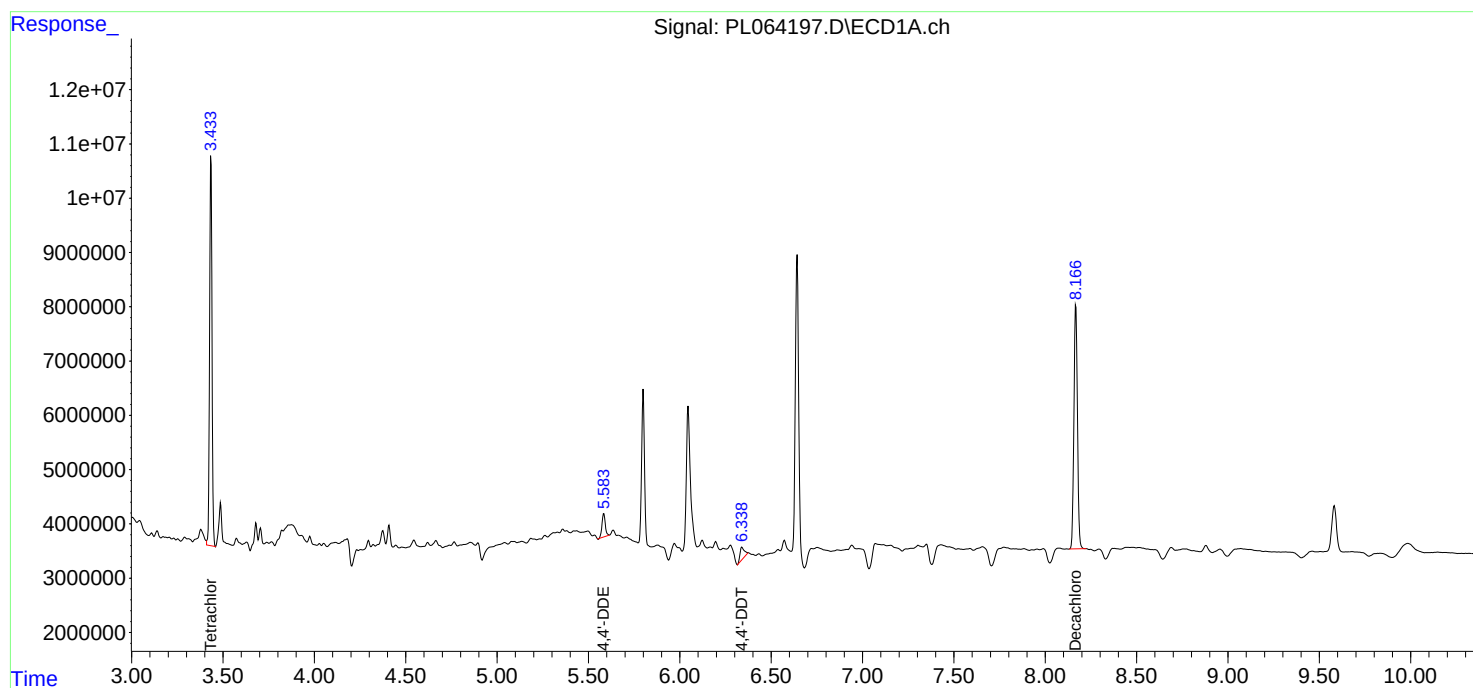

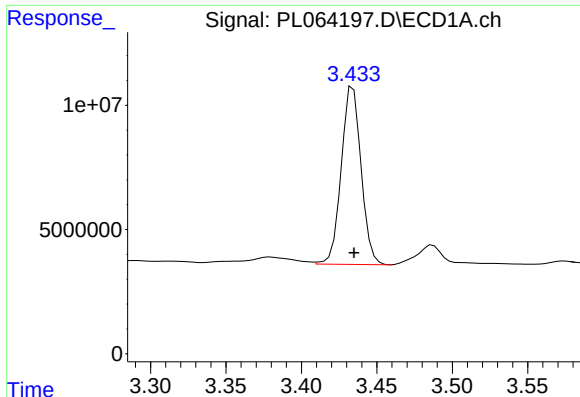


#1 Tetrachloro-m-xylene

R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 65435679
Conc: 21.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
BASIN-2


Manual Integrations
APPROVED

Ankita
1/19/2021 12:10:55 PM

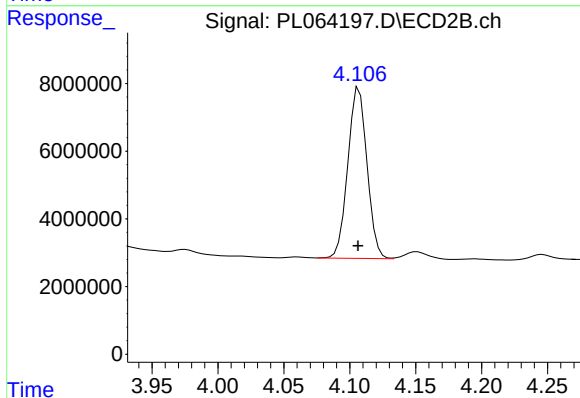


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 51043456
Conc: 19.97 ng/ml

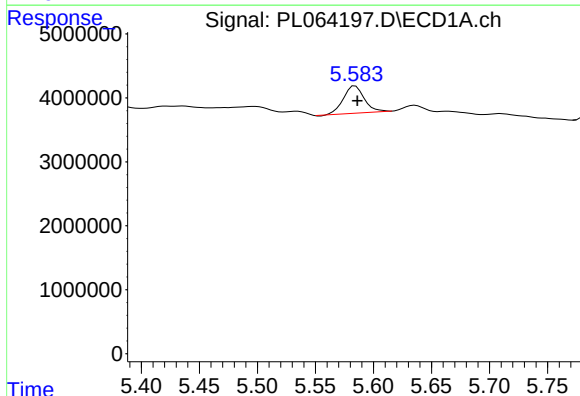


#12 4,4'-DDE

R.T.: 5.584 min
Delta R.T.: -0.002 min
Response: 5294510
Conc: 1.50 ng/ml

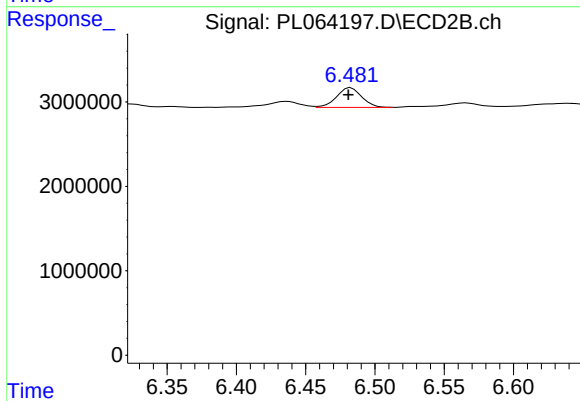

#12 4,4'-DDE

R.T.: 6.481 min
Delta R.T.: 0.000 min
Response: 2911824
Conc: 1.09 ng/ml m

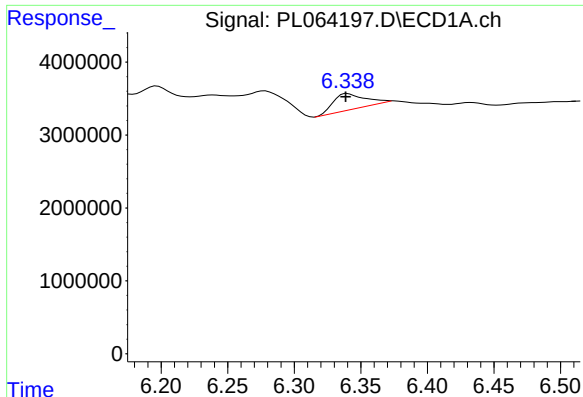


#17 4,4'-DDT

R.T.: 6.338 min
Delta R.T.: 0.000 min
Response: 3770357
Conc: 1.26 ng/ml m

Instrument :
ECD_L
ClientSampleId :
BASIN-2


Manual Integrations
APPROVED

Ankita
1/19/2021 12:10:55 PM

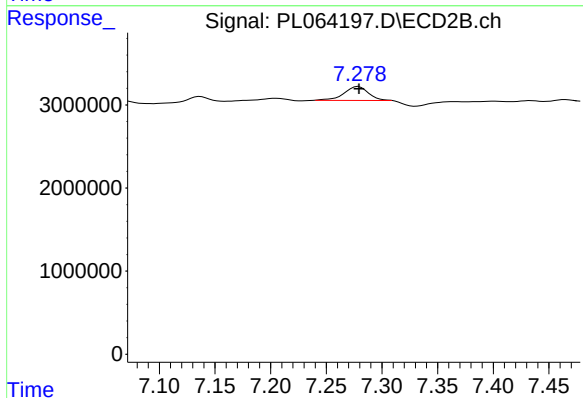


#17 4,4'-DDT

R.T.: 7.278 min
Delta R.T.: -0.002 min
Response: 2582822
Conc: 1.14 ng/ml m

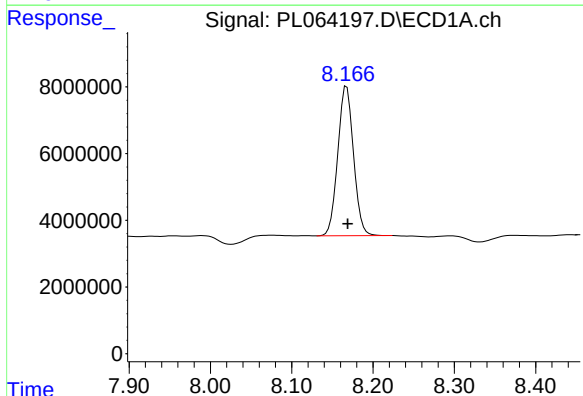

#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: -0.001 min
Response: 60190328
Conc: 19.72 ng/ml

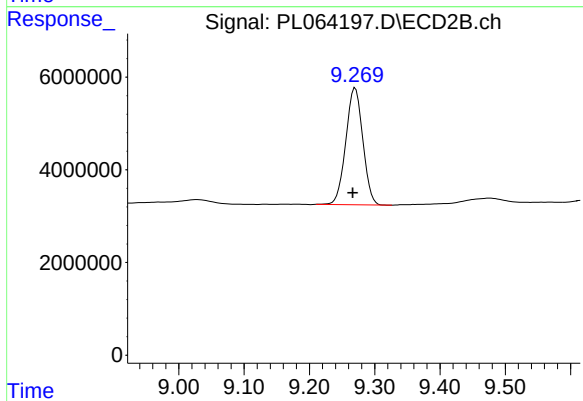

#28 Decachlorobiphenyl

R.T.: 9.270 min
Delta R.T.: 0.004 min
Response: 45656169
Conc: 19.24 ng/ml