

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011822\
 Data File : PL072040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2022 08:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 04:16:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.565	5.495	9459565	28450361	17.039	17.517
28)	SA Decachlor...	10.327	11.393	15905338	27761911	17.903	17.206
Target Compounds							
4)	MA Heptachlor	0.000	7.137f	0	305946	N.D.	0.132 #
6)	B beta-BHC	6.045f	6.740	218695	1564951	0.662	1.581 #
7)	B delta-BHC	0.000	7.022f	0	341584	N.D.	0.139 #
9)	A Endosulfan I	0.000	8.338f	0	31883	N.D.	0.018 #
10)	B gamma-Chl...	0.000	8.253f	0	280722	N.D.	0.139 #
11)	B alpha-Chl...	0.000	8.322	0	68619	N.D.	0.035 #
15)	B Endosulfa...	0.000	9.154f	0	329643	N.D.	0.192 #
20)	A Methoxychlor	0.000	9.861	0	581175	N.D.	0.702 #
25)	Chlordane-3	0.000	8.253f	0	280722	N.D.	1.010 #
26)	Chlordane-4	0.000	8.322	0	68619	N.D.	0.207 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011822\
Data File : PL072040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2022 08:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 04:16:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

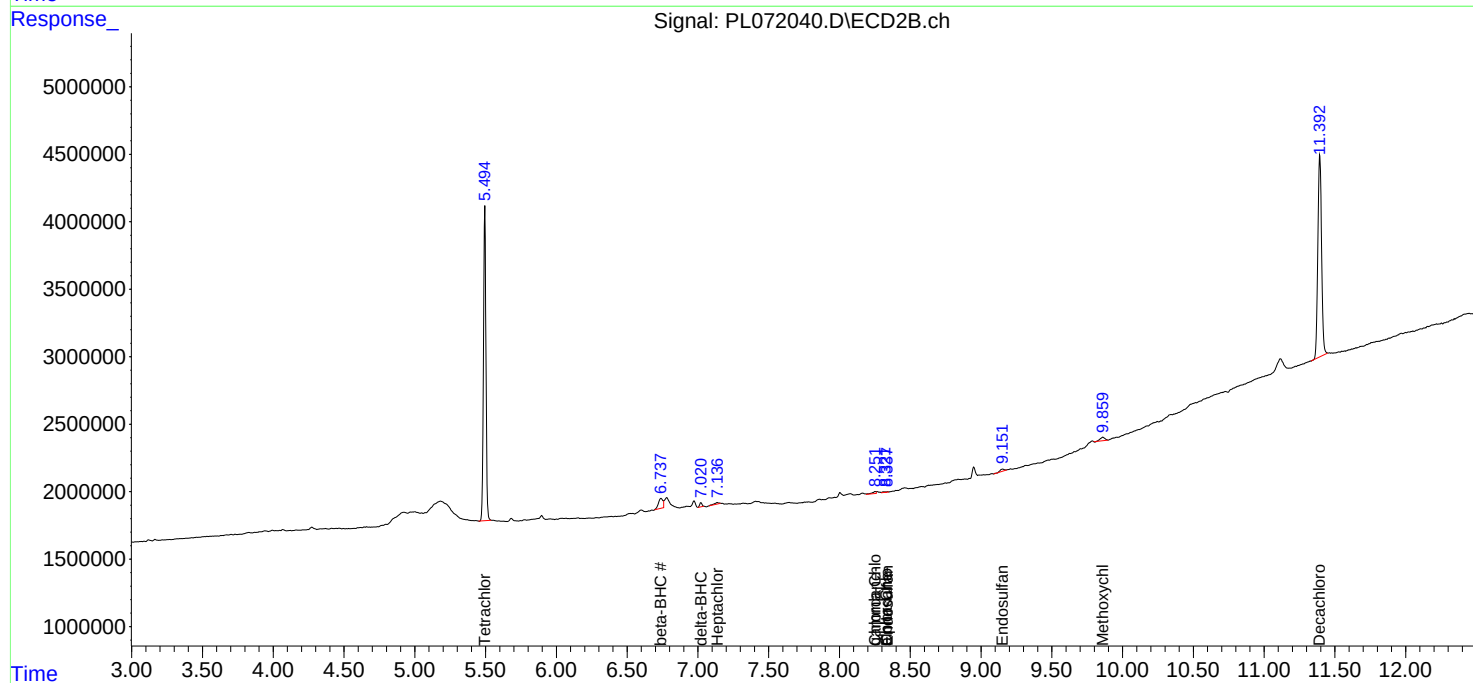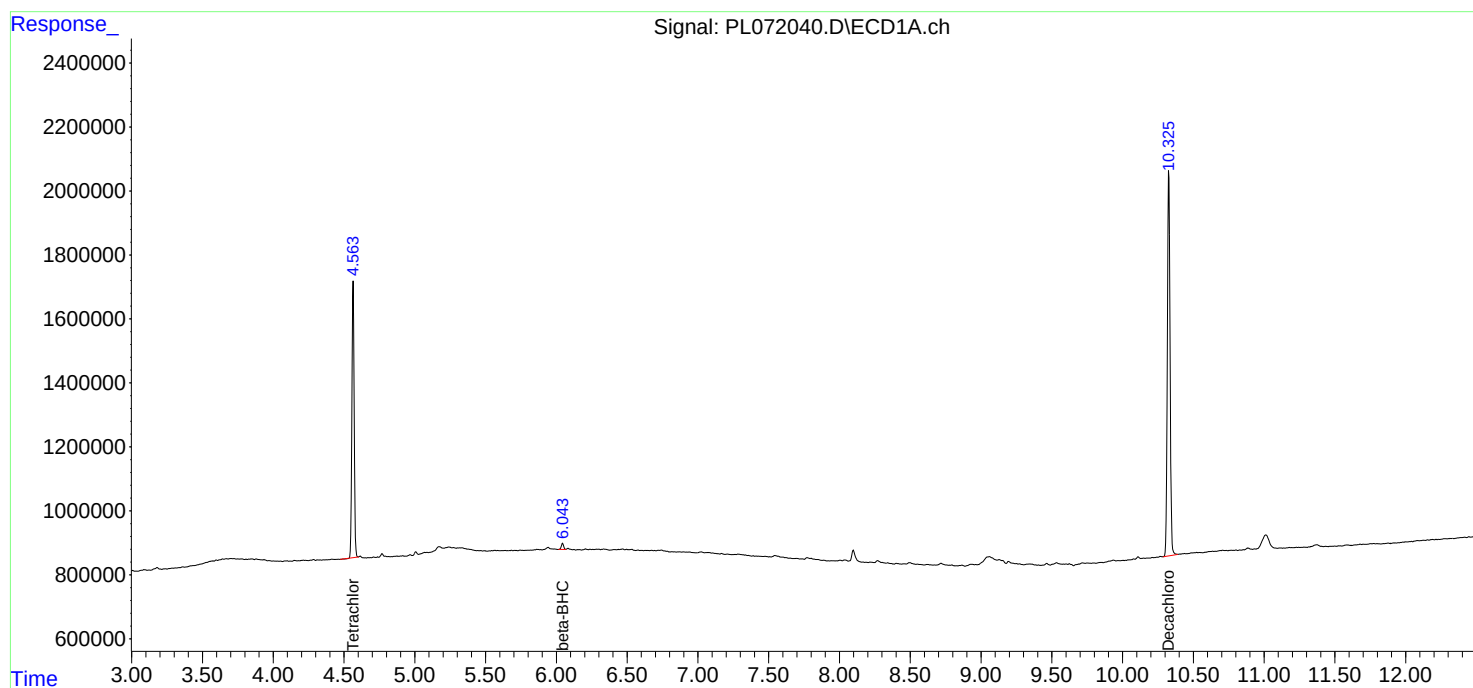


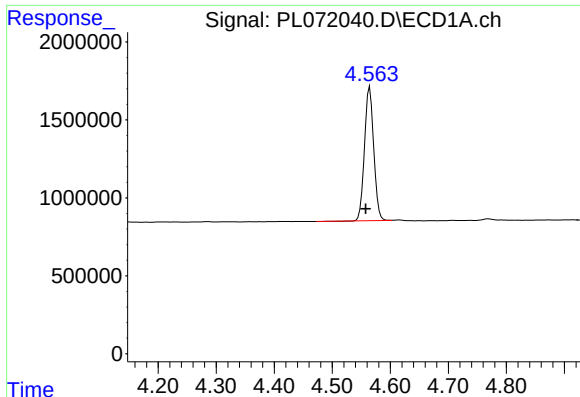

#1 Tetrachloro-m-xylene


R.T.: 4.565 min
Delta R.T.: 0.007 min
Response: 9459565
Conc: 17.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

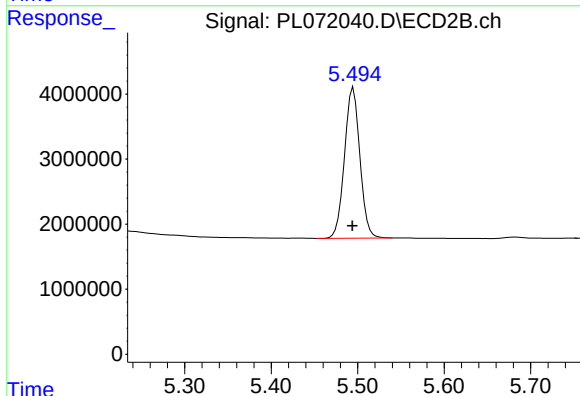


#1 Tetrachloro-m-xylene

R.T.: 5.495 min
Delta R.T.: 0.000 min
Response: 28450361
Conc: 17.52 ng/ml

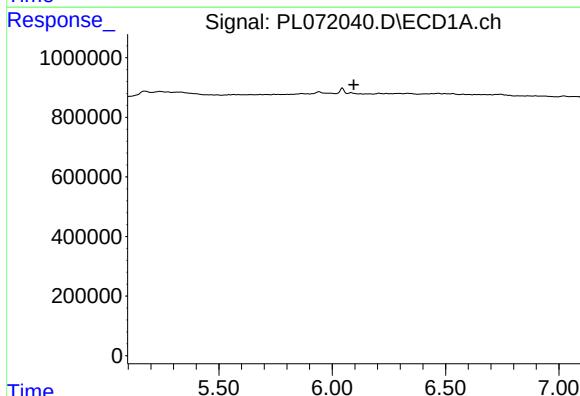


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 6.095 min
Response: 0
Conc: N.D.

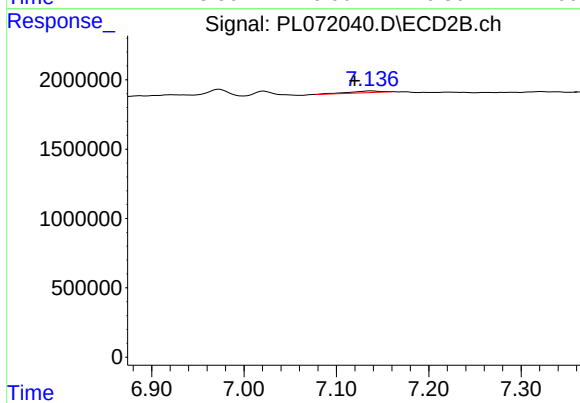

#4 Heptachlor


R.T.: 7.137 min
Delta R.T.: 0.017 min
Response: 305946
Conc: 0.13 ng/ml

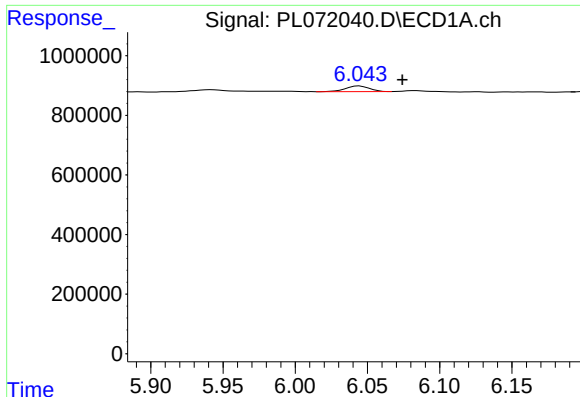

#6 beta-BHC


R.T.: 6.045 min
Delta R.T.: -0.030 min
Response: 218695
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

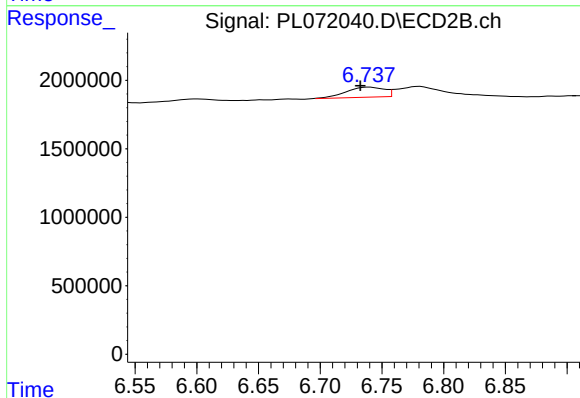


#6 beta-BHC

R.T.: 6.740 min
Delta R.T.: 0.007 min
Response: 1564951
Conc: 1.58 ng/ml

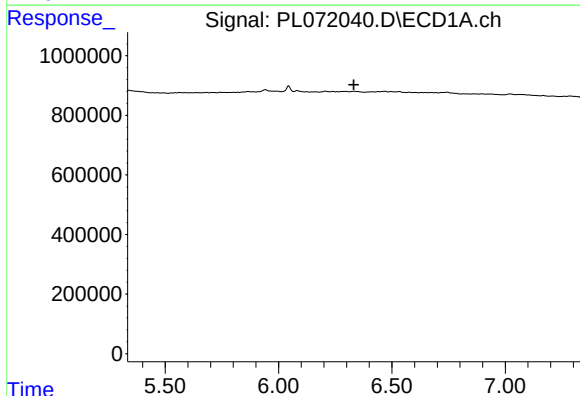


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

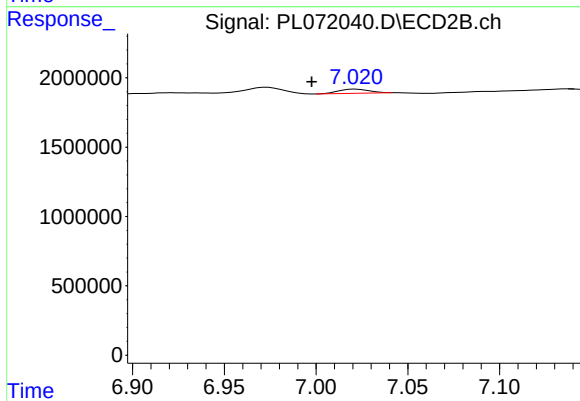

#7 delta-BHC


R.T.: 7.022 min
Delta R.T.: 0.024 min
Response: 341584
Conc: 0.14 ng/ml

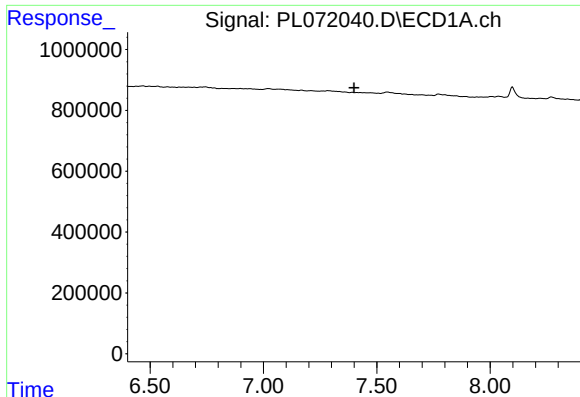

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

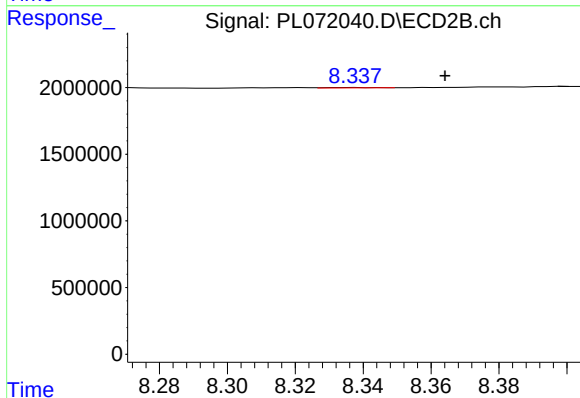


#9 Endosulfan I

R.T.: 8.338 min
Delta R.T.: -0.026 min
Response: 31883
Conc: 0.02 ng/ml

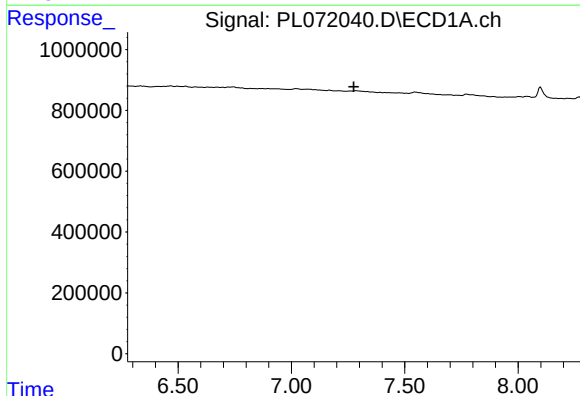


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

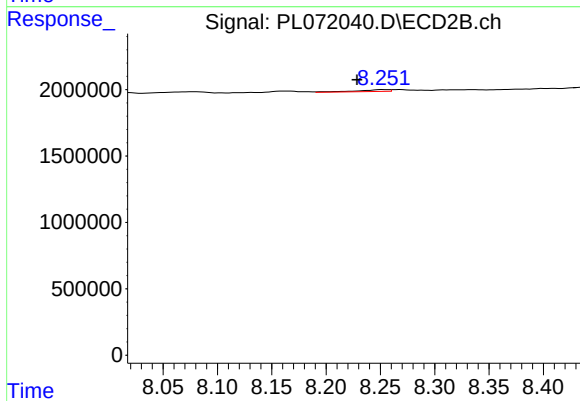

#10 gamma-Chlordane


R.T.: 8.253 min
Delta R.T.: 0.024 min
Response: 280722
Conc: 0.14 ng/ml

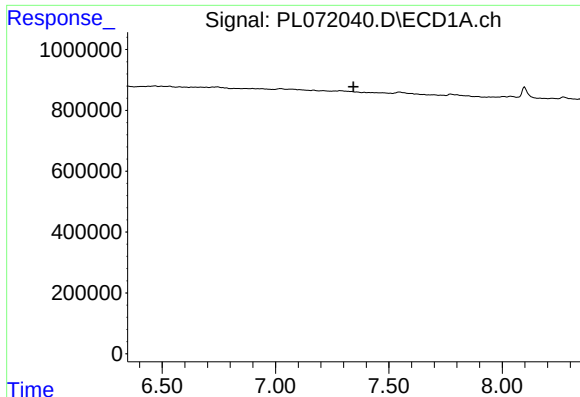

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

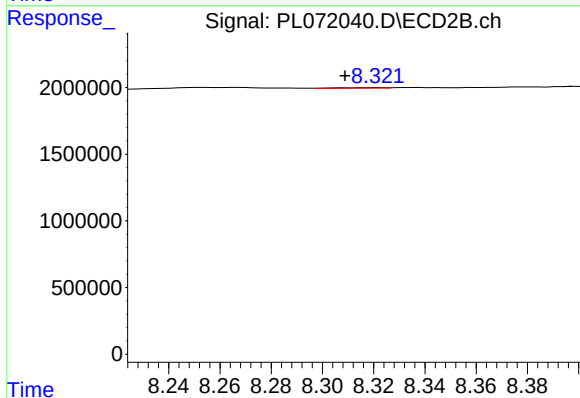


#11 alpha-Chlordane

R.T.: 8.322 min
Delta R.T.: 0.013 min
Response: 68619
Conc: 0.03 ng/ml

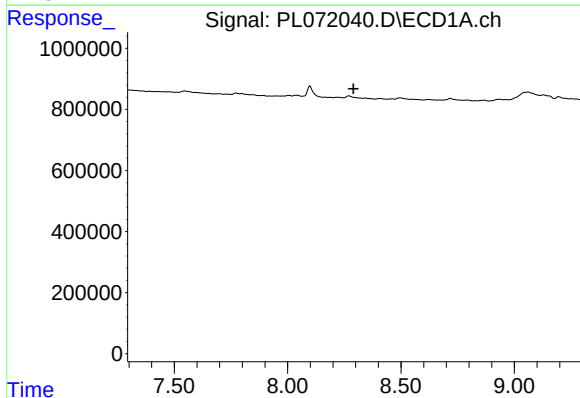


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

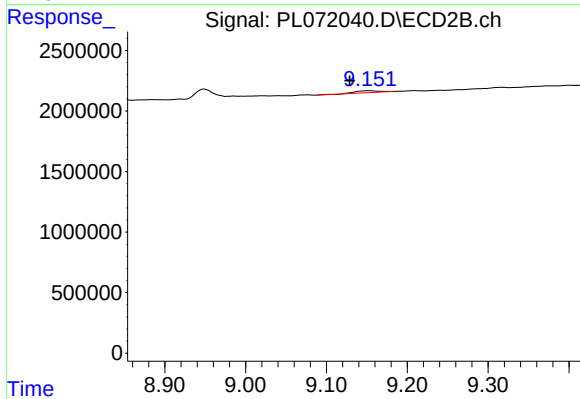

#15 Endosulfan II


R.T.: 9.154 min
Delta R.T.: 0.025 min
Response: 329643
Conc: 0.19 ng/ml

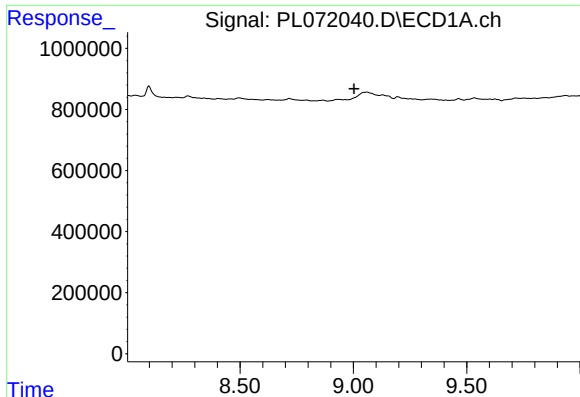

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

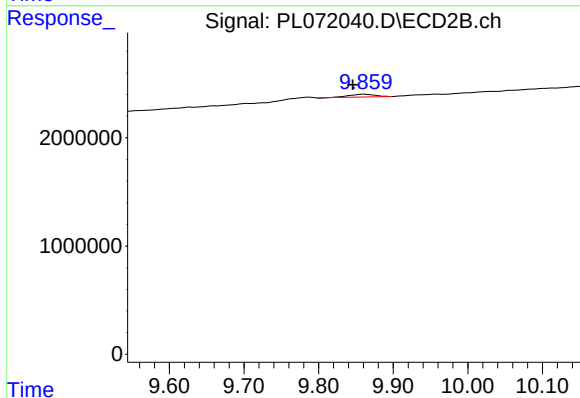


#20 Methoxychlor

R.T.: 9.861 min
Delta R.T.: 0.015 min
Response: 581175
Conc: 0.70 ng/ml

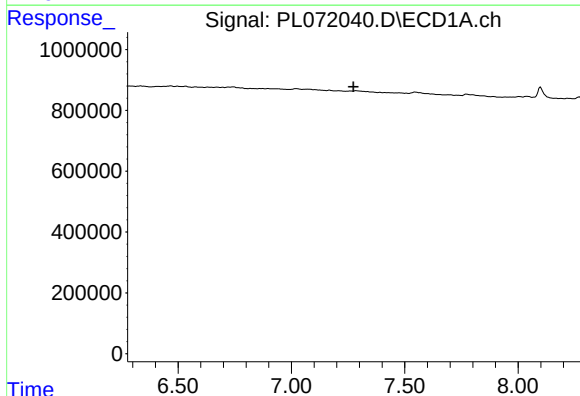


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

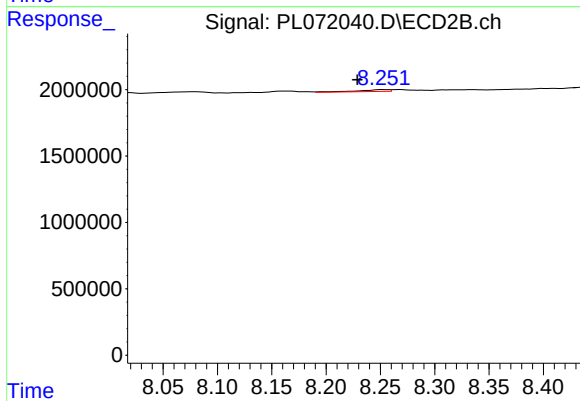

#25 Chlordane-3


R.T.: 8.253 min
Delta R.T.: 0.024 min
Response: 280722
Conc: 1.01 ng/ml

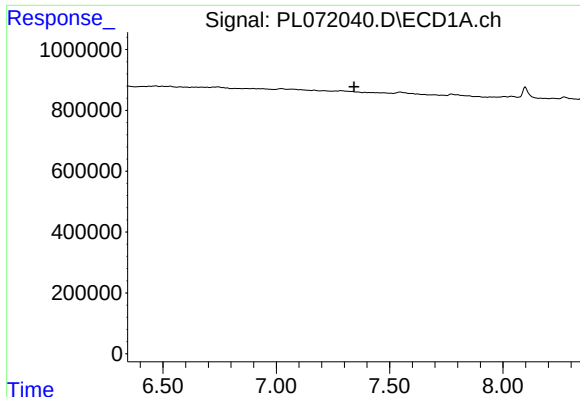

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

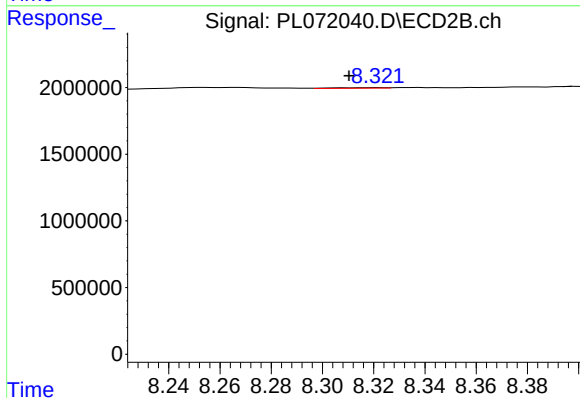


#26 Chlordane-4

R.T.: 8.322 min
Delta R.T.: 0.012 min
Response: 68619
Conc: 0.21 ng/ml

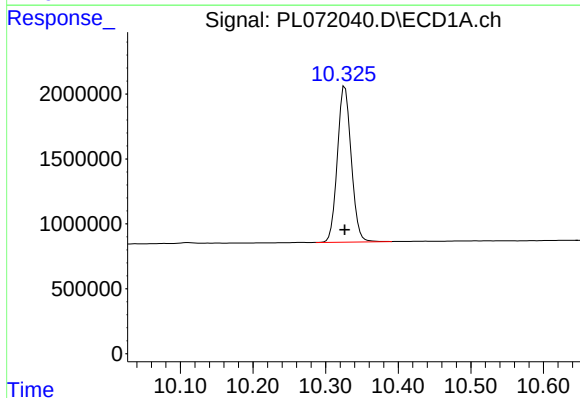

#28 Decachlorobiphenyl

R.T.: 10.327 min
Delta R.T.: 0.000 min
Response: 15905338
Conc: 17.90 ng/ml

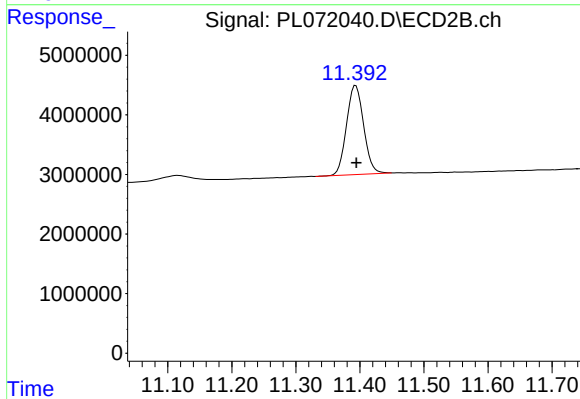

#28 Decachlorobiphenyl

R.T.: 11.393 min
Delta R.T.: -0.001 min
Response: 27761911
Conc: 17.21 ng/ml