

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011822\
 Data File : PL072056.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2022 14:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 04:21:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	10078336	29110096	18.153	17.924
28)	SA Decachlor...	10.321	11.386	15889802	29895321	17.885	18.528
Target Compounds							
7)	B delta-BHC	0.000	7.017f	0	763633	N.D.	0.310 #
8)	B Heptachlo...	0.000	7.931f	0	173778	N.D.	0.087 #
9)	A Endosulfan I	0.000	8.357	0	43529	N.D.	0.024 #
10)	B gamma-Chl...	0.000	8.235	0	153504	N.D.	0.076 #
11)	B alpha-Chl...	0.000	8.325f	0	141447	N.D.	0.071 #
13)	MA Dieldrin	0.000	8.682f	0	101864	N.D.	0.052 #
15)	B Endosulfa...	0.000	9.149f	0	128991	N.D.	0.075 #
16)	A 4,4'-DDD	0.000	9.039	0	117754	N.D.	0.082 #
25)	Chlordane-3	0.000	8.235	0	153504	N.D.	0.553 #
26)	Chlordane-4	0.000	8.325	0	141447	N.D.	0.426 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011822\
Data File : PL072056.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2022 14:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 04:21:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

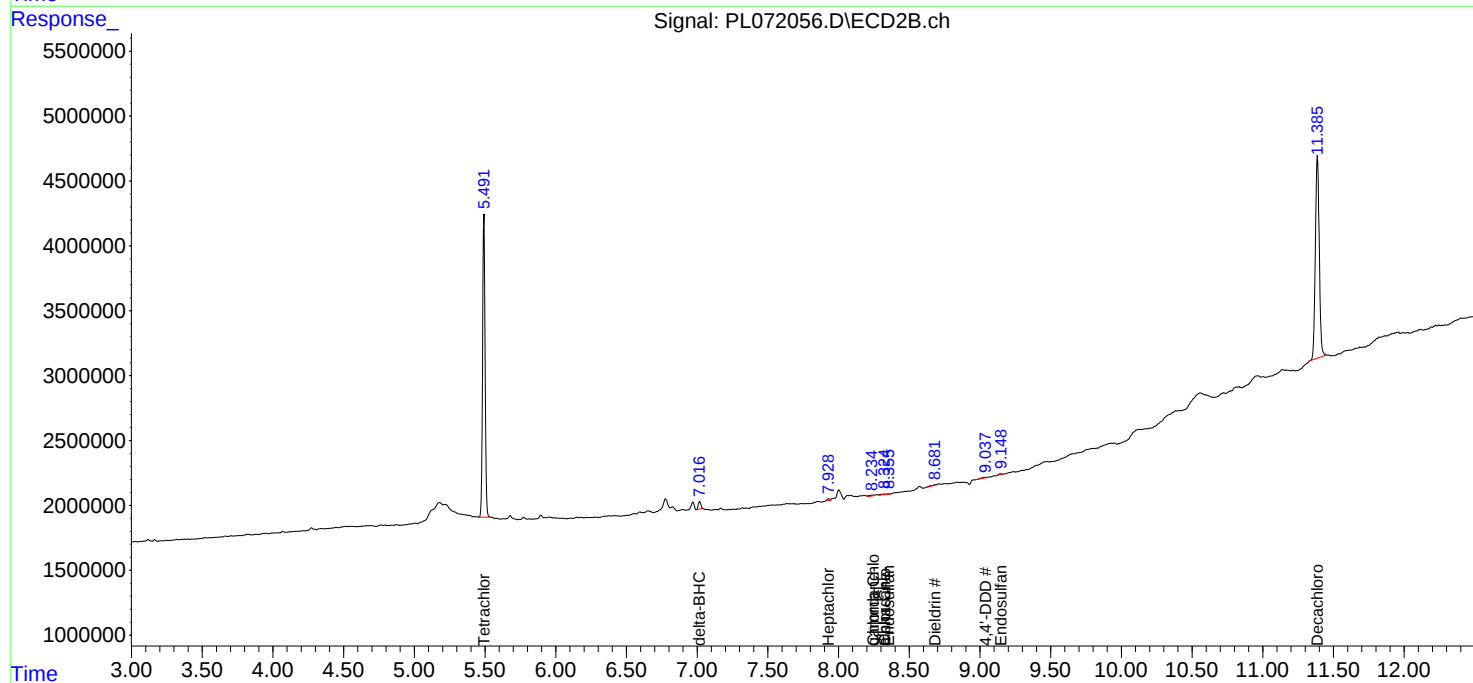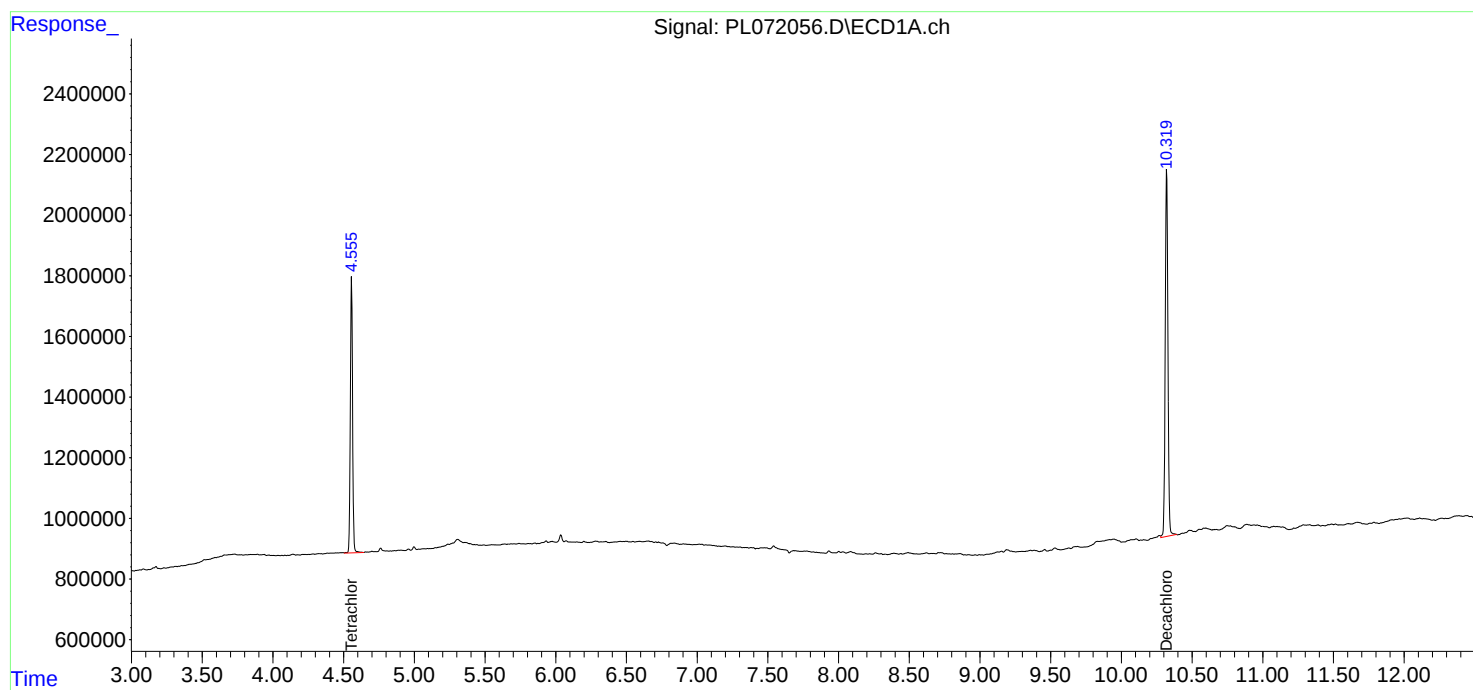


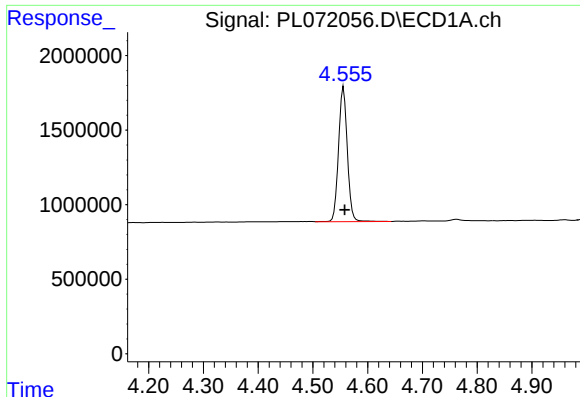

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 10078336
Conc: 18.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

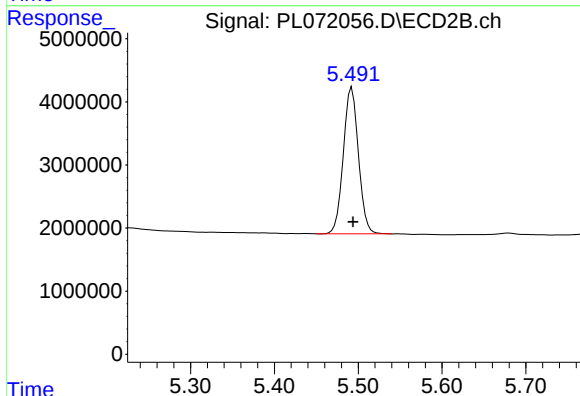


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 29110096
Conc: 17.92 ng/ml

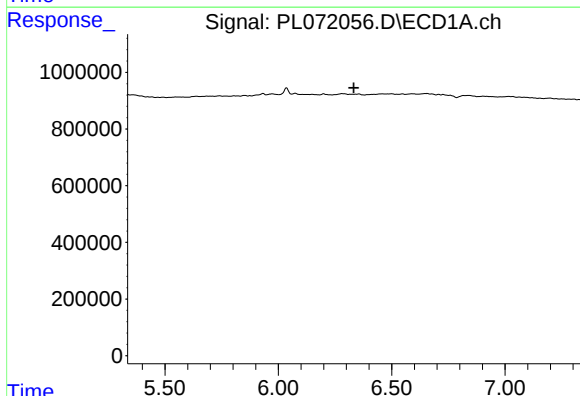


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

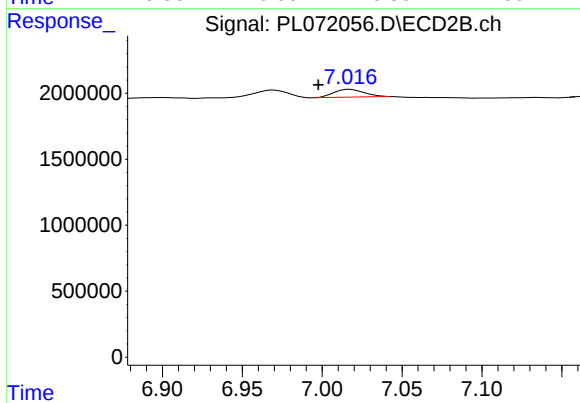

#7 delta-BHC


R.T.: 7.017 min
Delta R.T.: 0.020 min
Response: 763633
Conc: 0.31 ng/ml

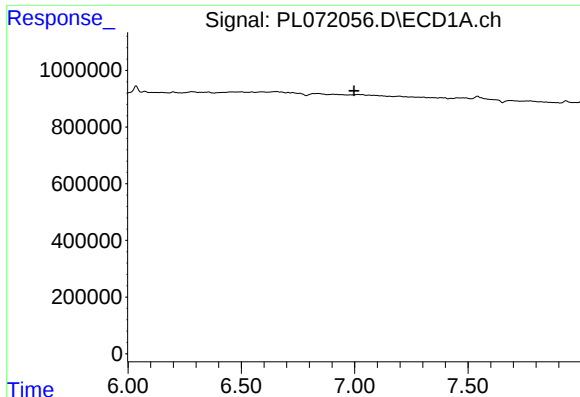

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.998 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

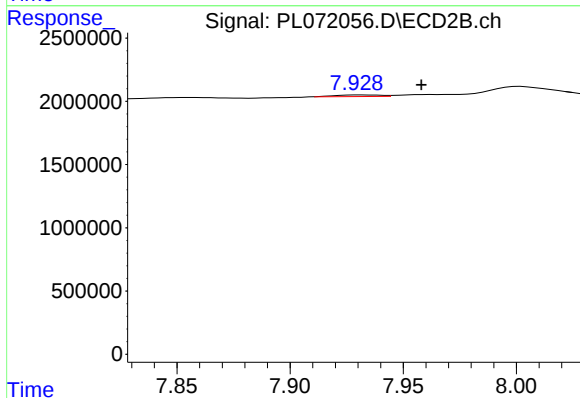


#8 Heptachlor epoxide

R.T.: 7.931 min
Delta R.T.: -0.027 min
Response: 173778
Conc: 0.09 ng/ml

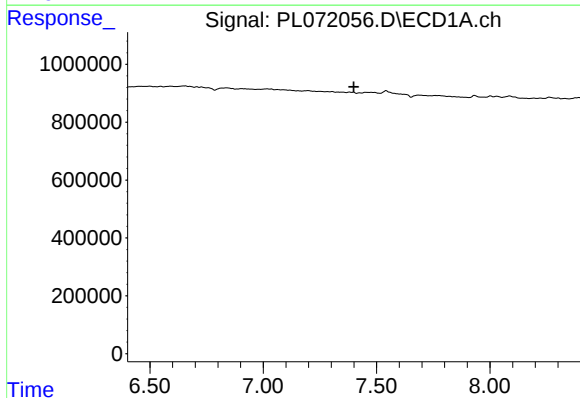


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

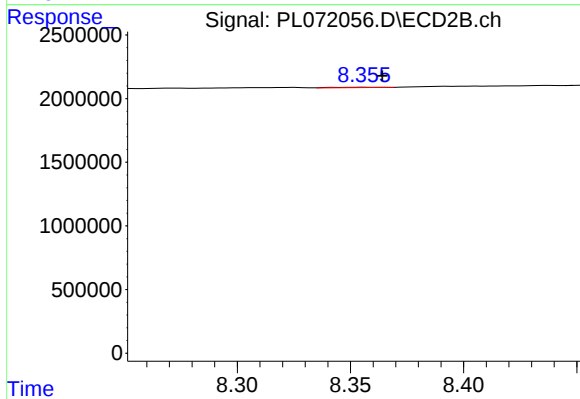

#9 Endosulfan I


R.T.: 8.357 min
Delta R.T.: -0.007 min
Response: 43529
Conc: 0.02 ng/ml

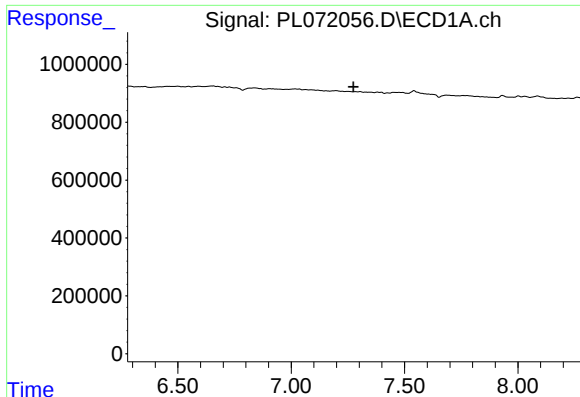

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

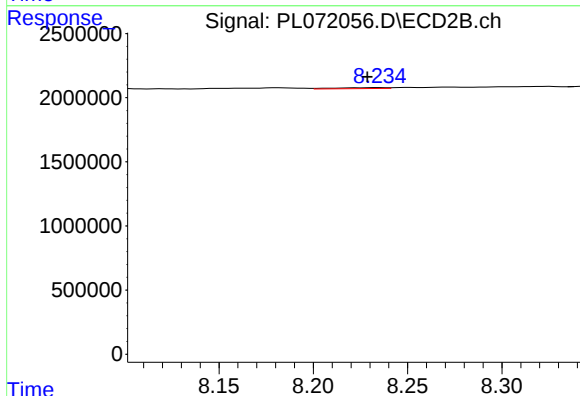


#10 gamma-Chlordane

R.T.: 8.235 min
Delta R.T.: 0.007 min
Response: 153504
Conc: 0.08 ng/ml

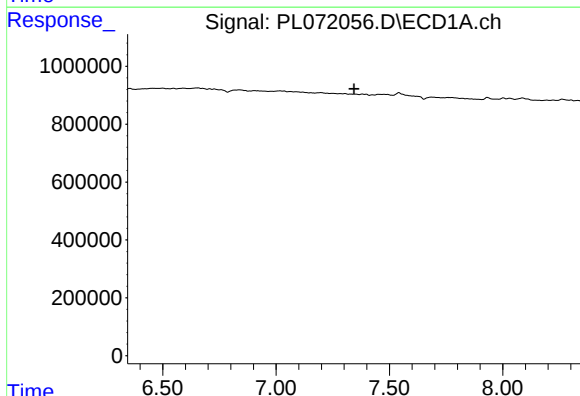


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

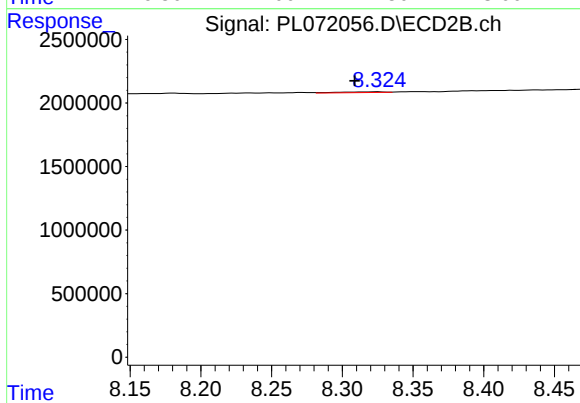

#11 alpha-Chlordane


R.T.: 8.325 min
Delta R.T.: 0.016 min
Response: 141447
Conc: 0.07 ng/ml

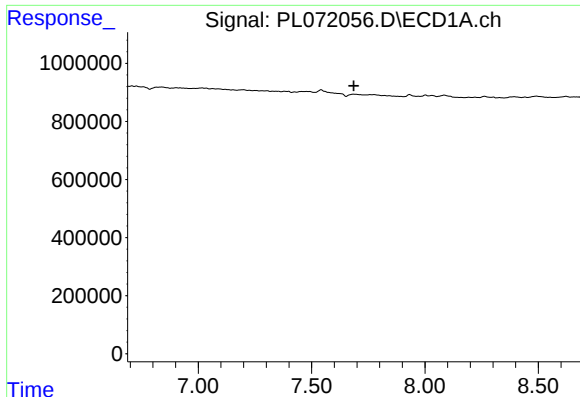

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.686 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

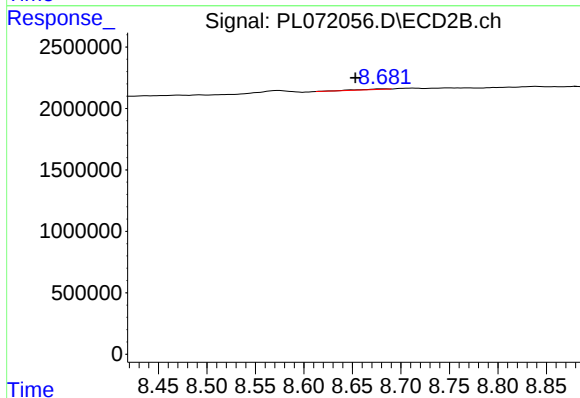


#13 Dieldrin

R.T.: 8.682 min
Delta R.T.: 0.029 min
Response: 101864
Conc: 0.05 ng/ml

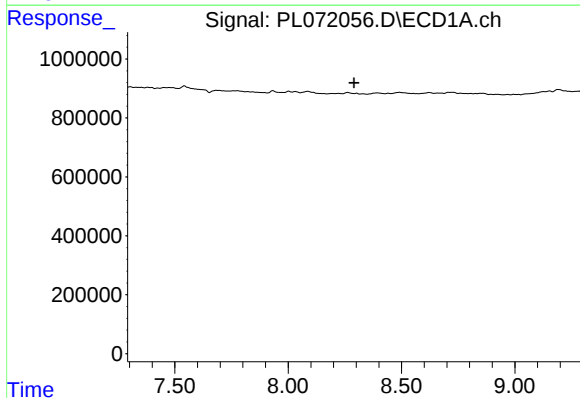


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

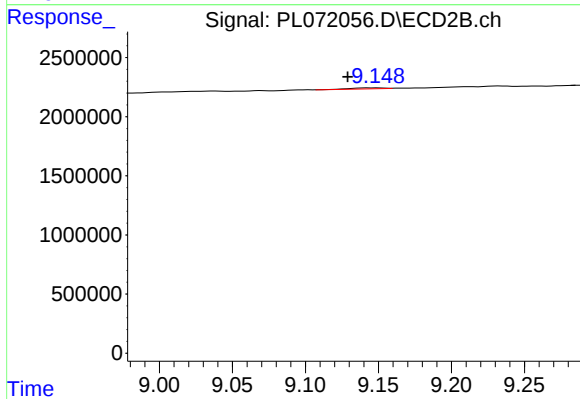

#15 Endosulfan II


R.T.: 9.149 min
Delta R.T.: 0.020 min
Response: 128991
Conc: 0.08 ng/ml

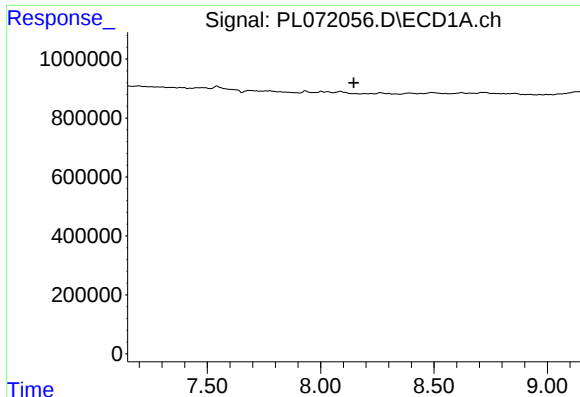

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

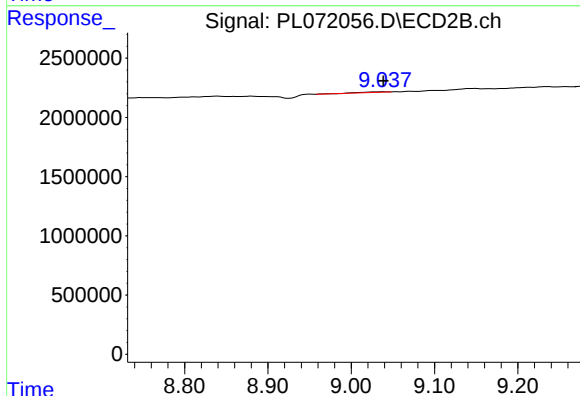


#16 4,4'-DDD

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 117754
Conc: 0.08 ng/ml

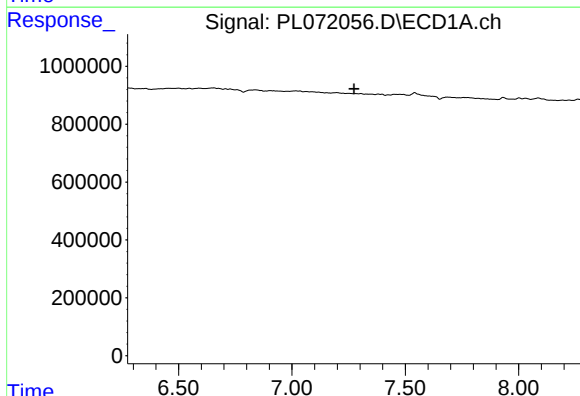


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

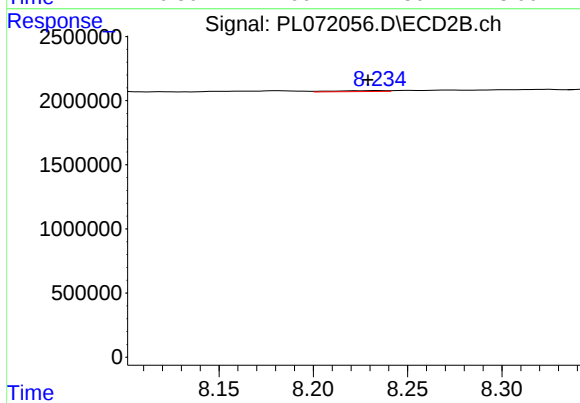

#25 Chlordane-3


R.T.: 8.235 min
Delta R.T.: 0.006 min
Response: 153504
Conc: 0.55 ng/ml

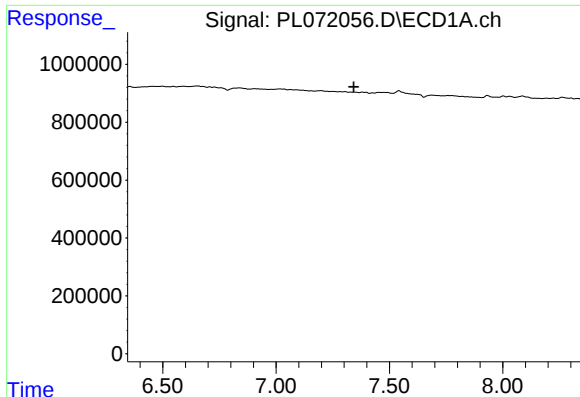

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

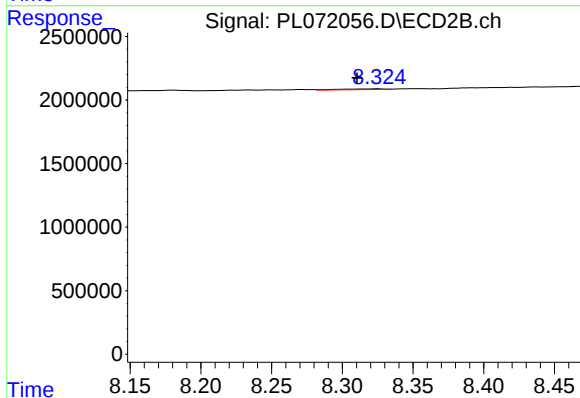


#26 Chlordane-4

R.T.: 8.325 min
Delta R.T.: 0.015 min
Response: 141447
Conc: 0.43 ng/ml

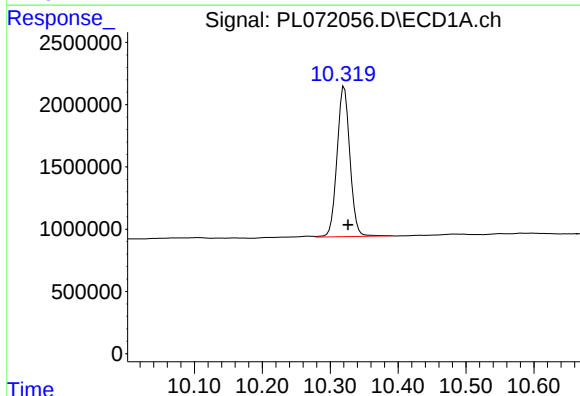

#28 Decachlorobiphenyl

R.T.: 10.321 min
Delta R.T.: -0.006 min
Response: 15889802
Conc: 17.89 ng/ml

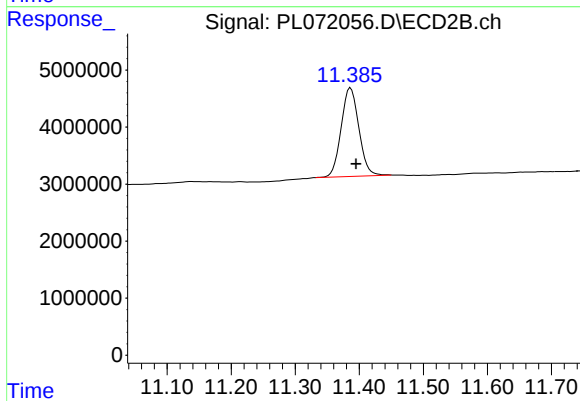

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: -0.008 min
Response: 29895321
Conc: 18.53 ng/ml