

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011822\
 Data File : PL072065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2022 17:23
 Operator : AR\AJ
 Sample : N1154-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 04:24:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.492	6031356	17127712	10.864	10.546
28)	SA Decachlor...	10.319	11.386	8957376	16009147	10.082	9.922
Target Compounds							
7)	B delta-BHC	0.000	7.017f	0	894726	N.D.	0.364 #
9)	A Endosulfan I	0.000	8.392f	0	35219	N.D.	0.019 #
12)	B 4,4'-DDE	7.543f	0.000	281981	0	0.391	N.D. #
15)	B Endosulfa...	0.000	9.148f	0	389611	N.D.	0.227 #
27)	Chlordane-5	0.000	9.201	0	85560	N.D.	1.402 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011822\
Data File : PL072065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2022 17:23
Operator : AR\AJ
Sample : N1154-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 04:24:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

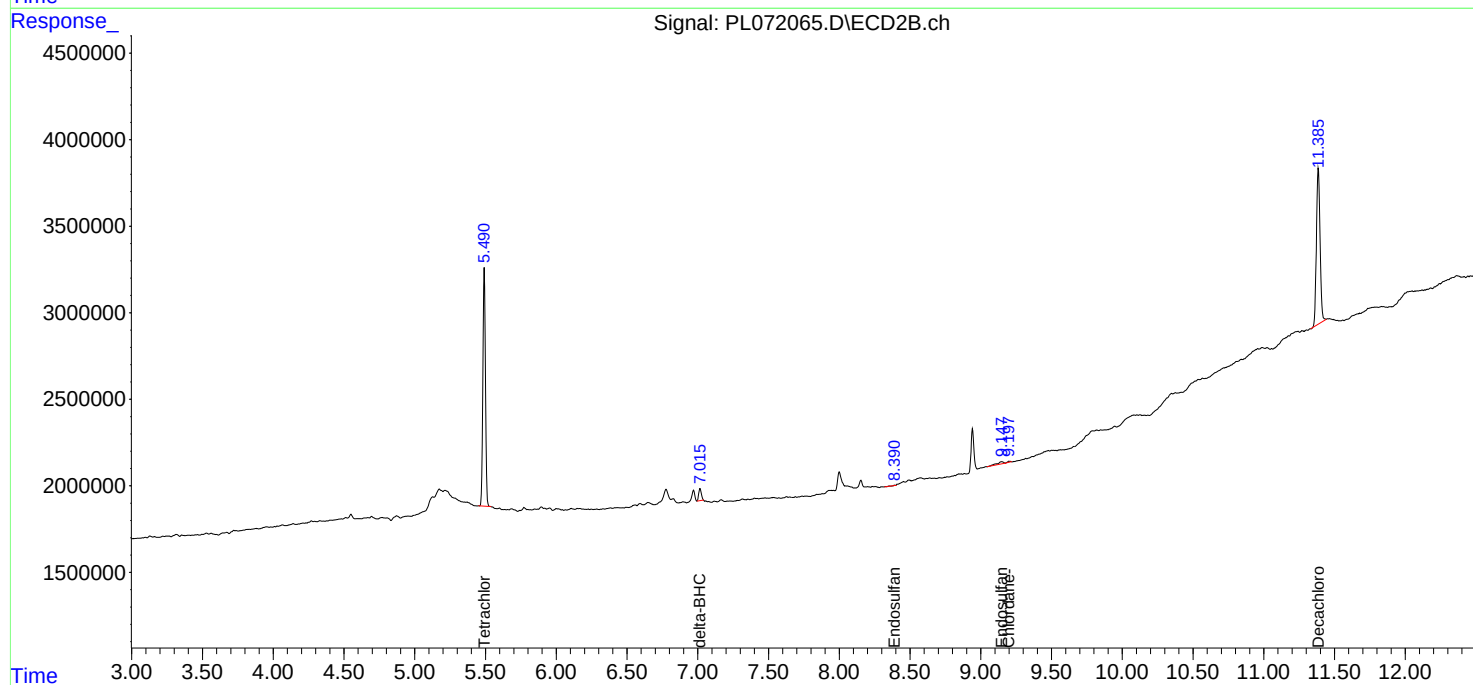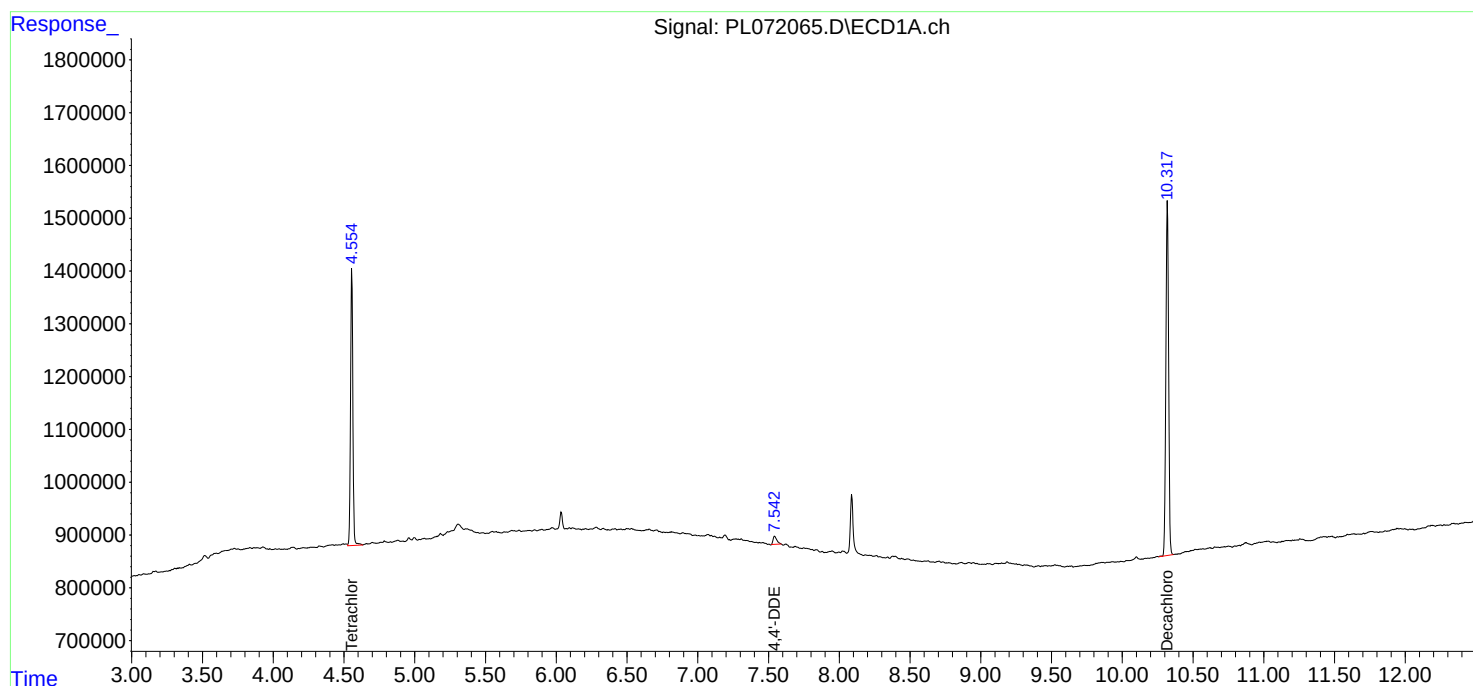


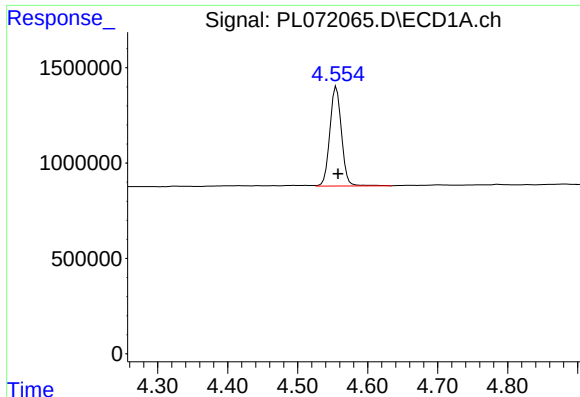

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 6031356
Conc: 10.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

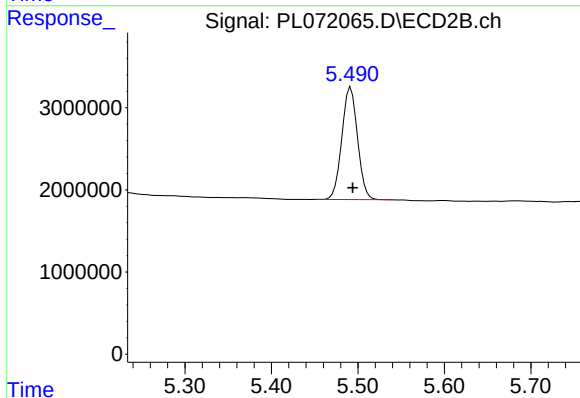


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 17127712
Conc: 10.55 ng/ml

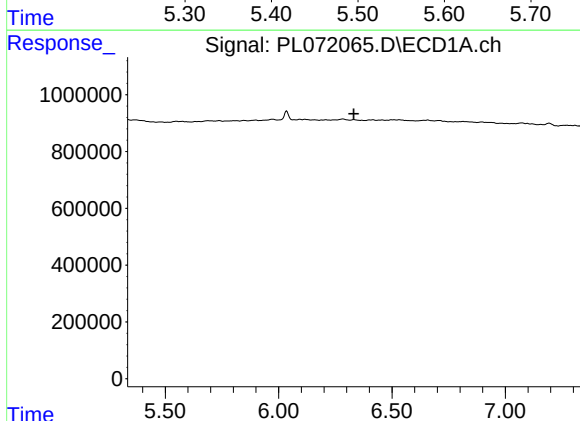


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

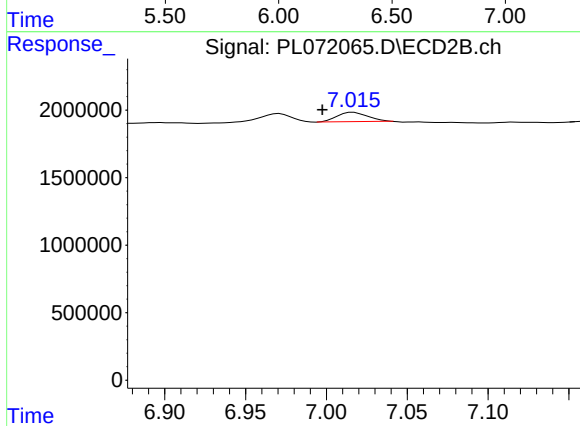

#7 delta-BHC


R.T.: 7.017 min
Delta R.T.: 0.019 min
Response: 894726
Conc: 0.36 ng/ml

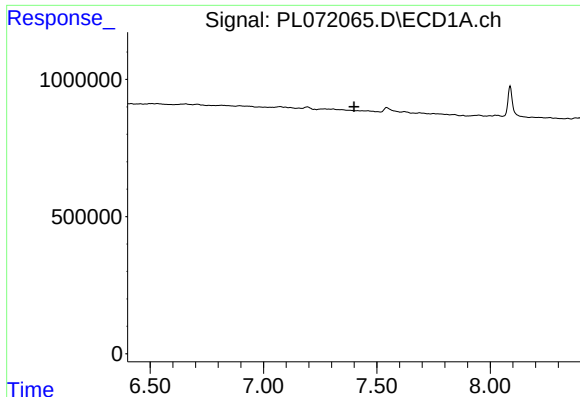

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

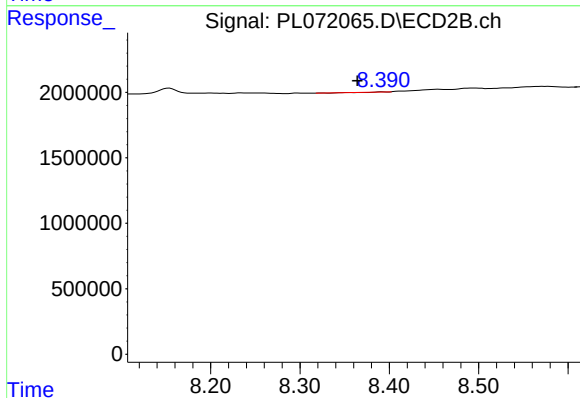


#9 Endosulfan I

R.T.: 8.392 min
Delta R.T.: 0.028 min
Response: 35219
Conc: 0.02 ng/ml

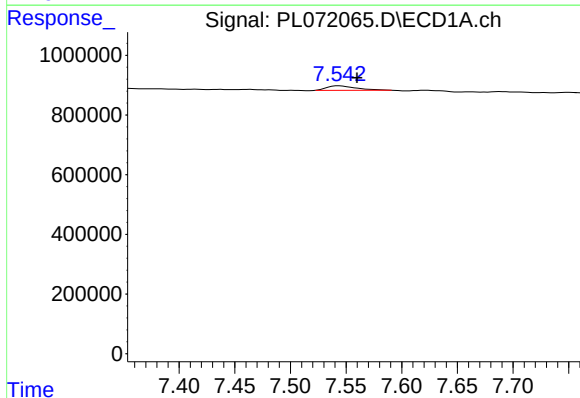


#12 4,4'-DDE

R.T.: 7.543 min
Delta R.T.: -0.017 min
Response: 281981
Conc: 0.39 ng/ml

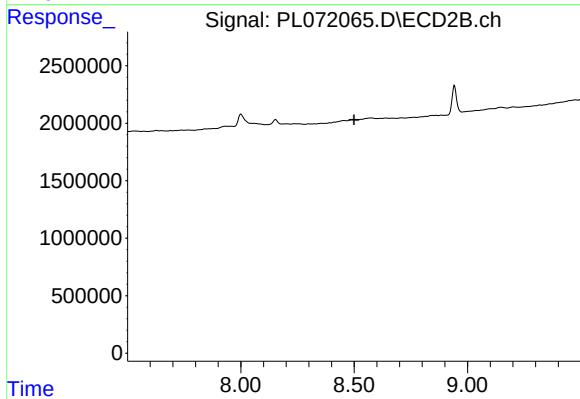

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 8.499 min
Response: 0
Conc: N.D.

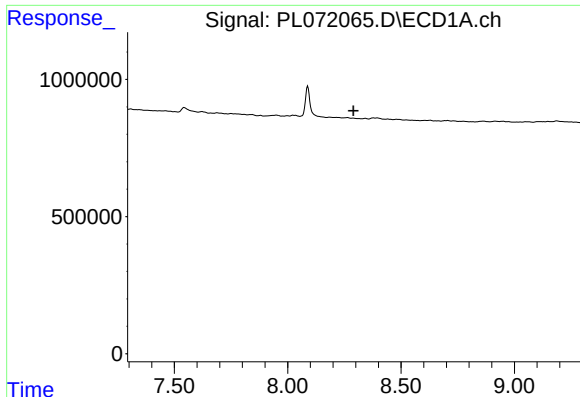

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

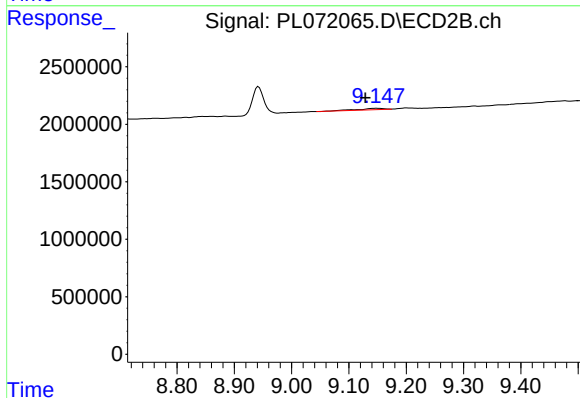


#15 Endosulfan II

R.T.: 9.148 min
Delta R.T.: 0.019 min
Response: 389611
Conc: 0.23 ng/ml

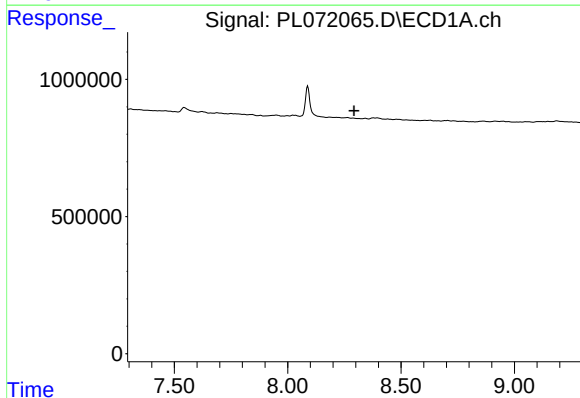


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 8.293 min
Response: 0
Conc: N.D.

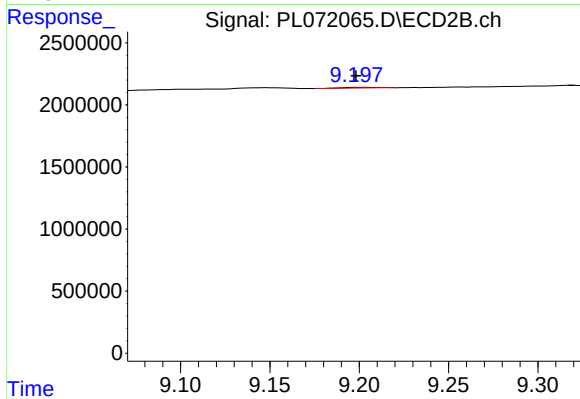

#27 Chlordane-5


R.T.: 9.201 min
Delta R.T.: 0.003 min
Response: 85560
Conc: 1.40 ng/ml

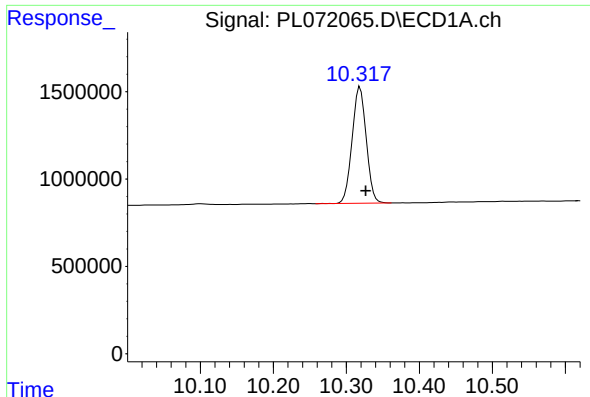

#28 Decachlorobiphenyl

R.T.: 10.319 min
Delta R.T.: -0.008 min
Response: 8957376
Conc: 10.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

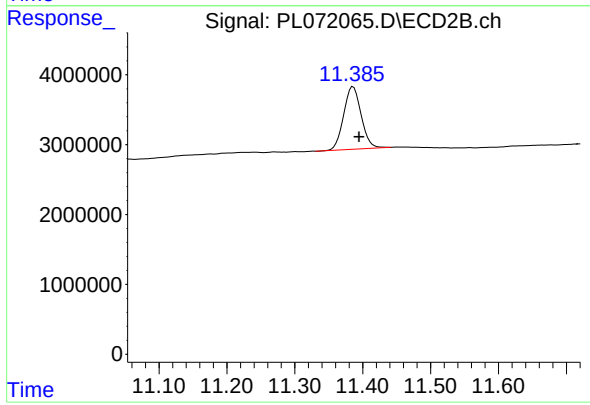

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: -0.009 min
Response: 16009147
Conc: 9.92 ng/ml