

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011822\
 Data File : PL072066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2022 17:39
 Operator : AR\AJ
 Sample : N1154-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 04:24:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	5817082	16494240	10.478	10.156
28)	SA Decachlor...	10.318	11.386	8736380	16458257	9.833	10.200
Target Compounds							
7)	B delta-BHC	0.000	7.016f	0	1046221	N.D.	0.425 #
15)	B Endosulfa...	0.000	9.148f	0	295447	N.D.	0.172 #
16)	A 4,4'-DDD	0.000	9.037	0	76936	N.D.	0.054 #
17)	MA 4,4'-DDT	0.000	9.333f	0	106899	N.D.	0.068 #
27)	Chlordane-5	0.000	9.206	0	64223	N.D.	1.053 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011822\
Data File : PL072066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2022 17:39
Operator : AR\AJ
Sample : N1154-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 04:24:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

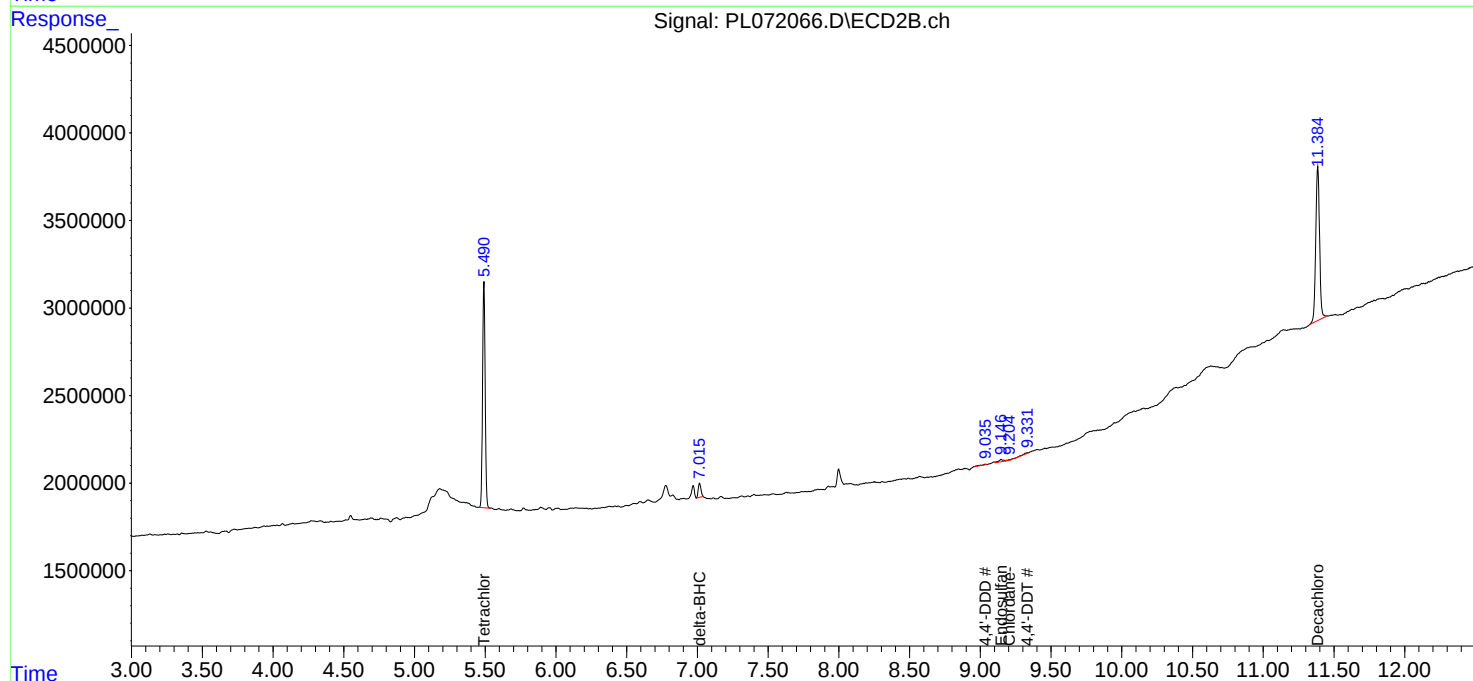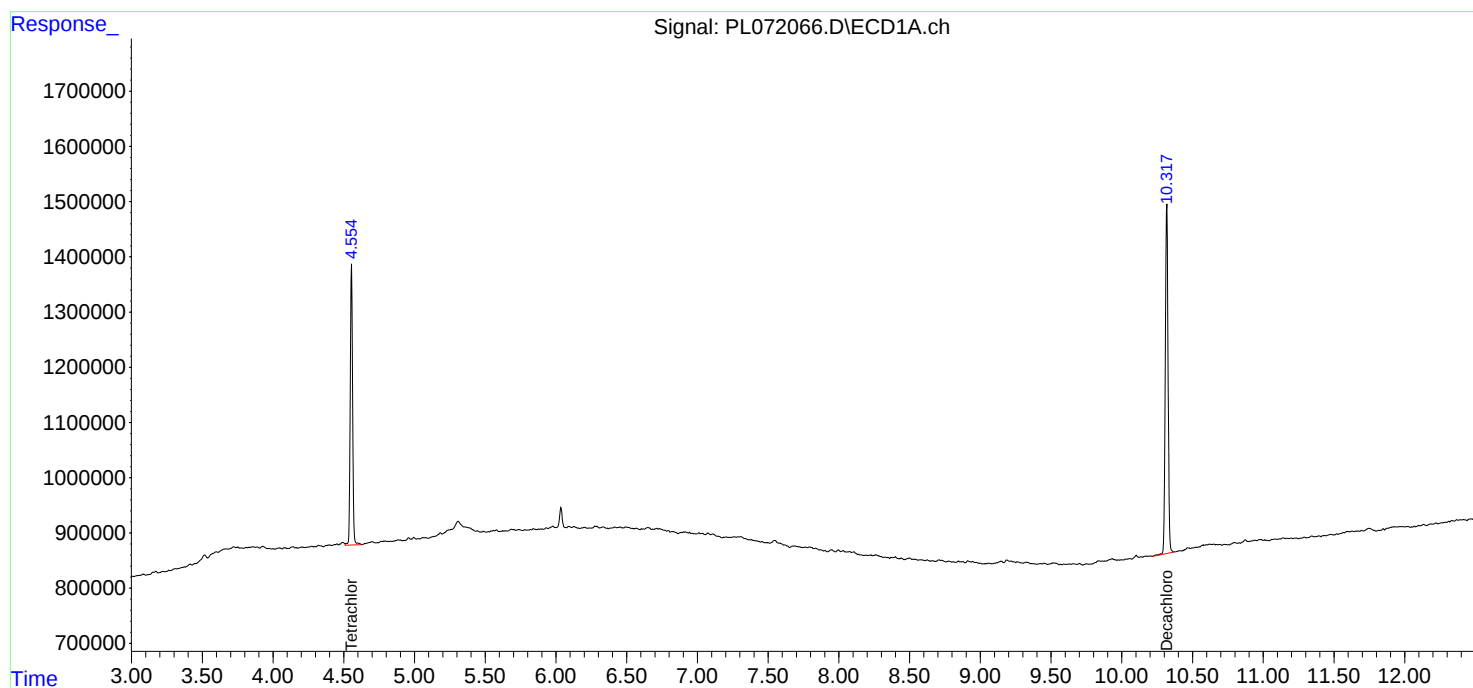


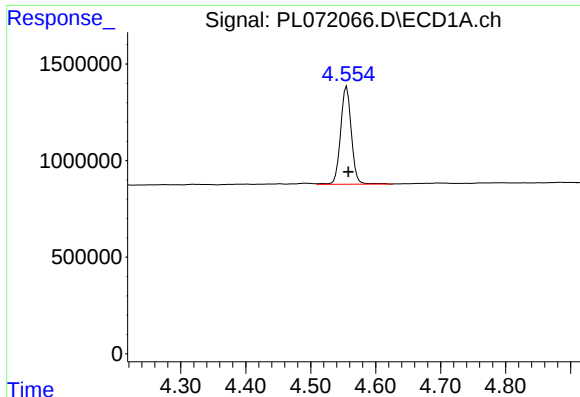

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 5817082
Conc: 10.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

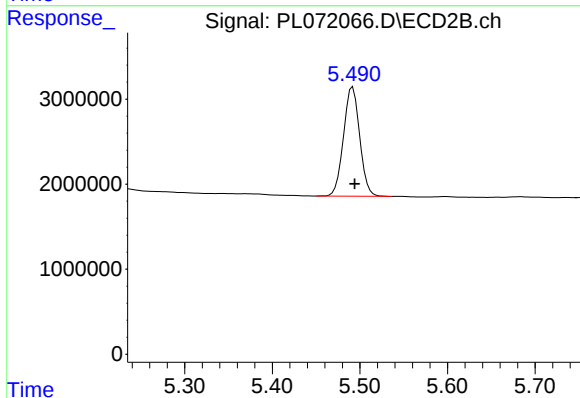


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 16494240
Conc: 10.16 ng/ml

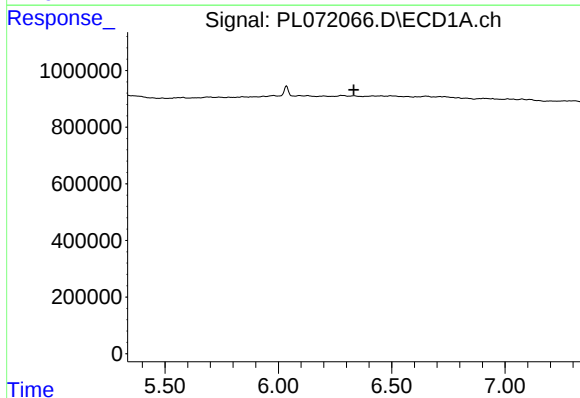


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

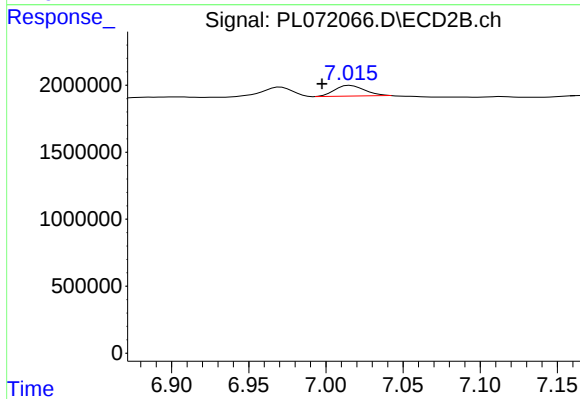

#7 delta-BHC


R.T.: 7.016 min
Delta R.T.: 0.018 min
Response: 1046221
Conc: 0.43 ng/ml

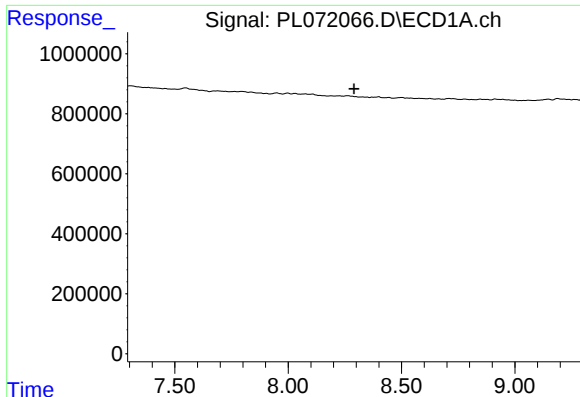

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

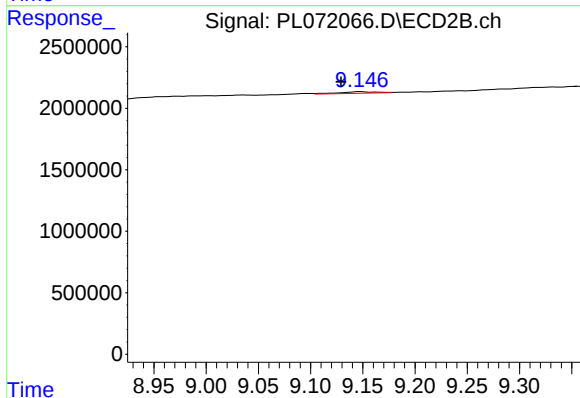


#15 Endosulfan II

R.T.: 9.148 min
Delta R.T.: 0.019 min
Response: 295447
Conc: 0.17 ng/ml

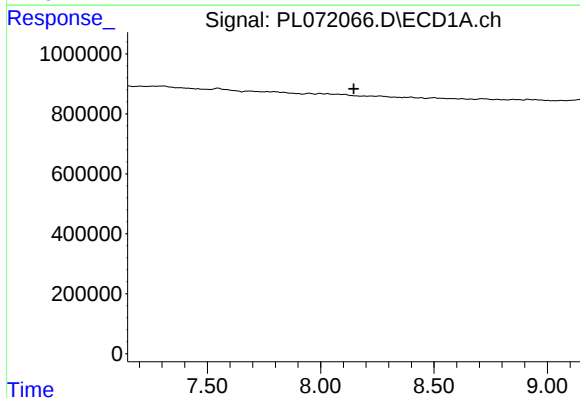


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

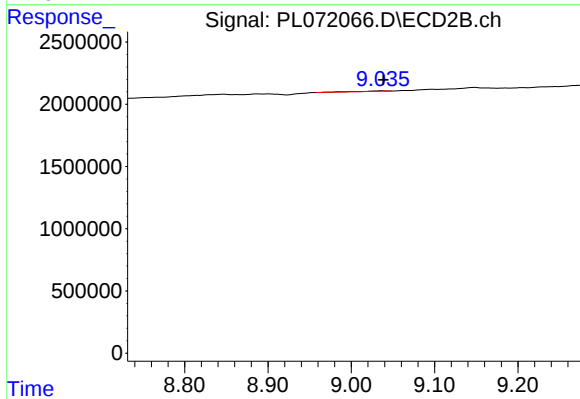

#16 4,4'-DDD


R.T.: 9.037 min
Delta R.T.: -0.002 min
Response: 76936
Conc: 0.05 ng/ml

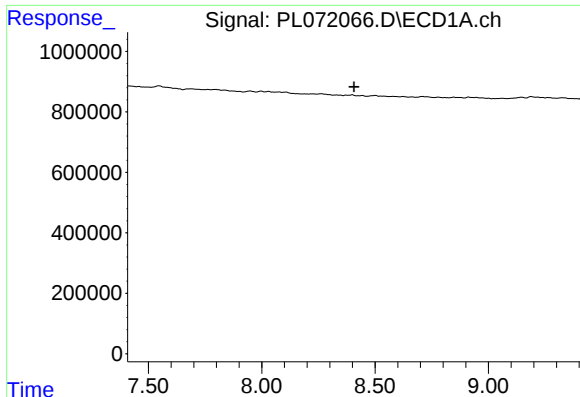

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

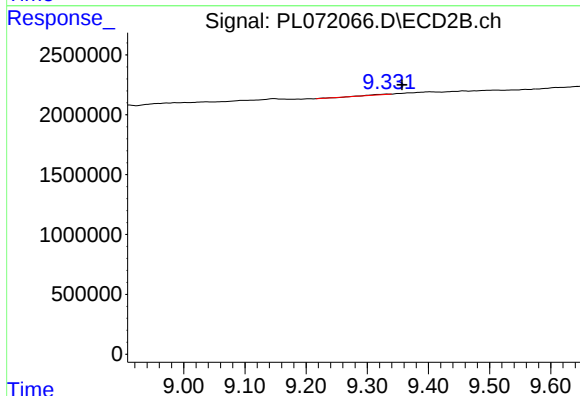


#17 4,4'-DDT

R.T.: 9.333 min
Delta R.T.: -0.024 min
Response: 106899
Conc: 0.07 ng/ml

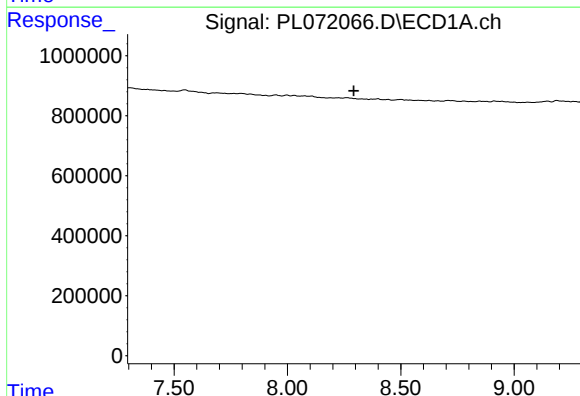


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

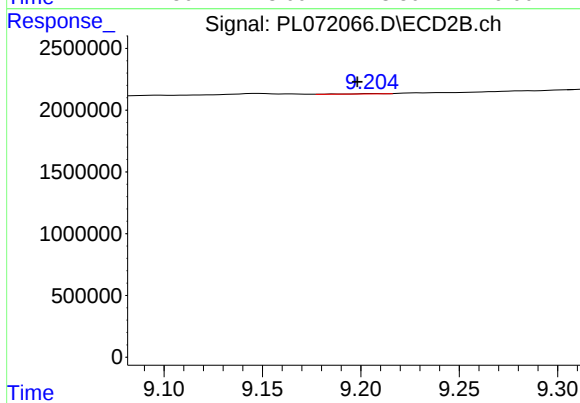

#27 Chlordane-5


R.T.: 9.206 min
Delta R.T.: 0.007 min
Response: 64223
Conc: 1.05 ng/ml

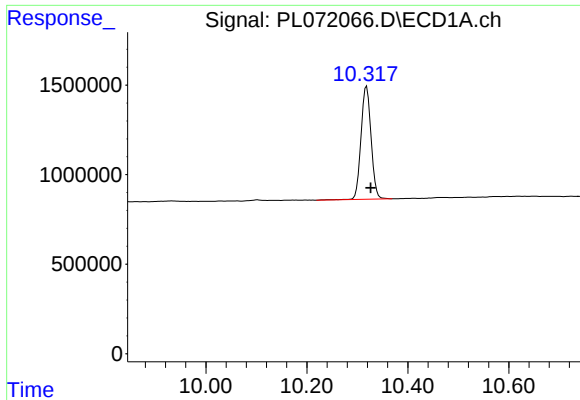

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.008 min
Response: 8736380
Conc: 9.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

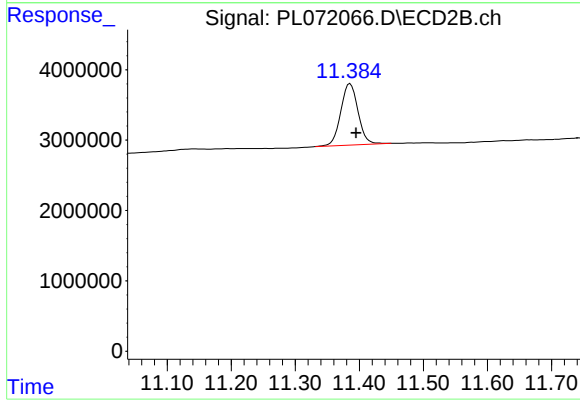

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: -0.009 min
Response: 16458257
Conc: 10.20 ng/ml