

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011822\
 Data File : PL072077.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2022 20:55
 Operator : AR\AJ
 Sample : PB142097TB
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 04:28:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	10476683	30359948	18.871	18.693
28)	SA Decachlor...	10.319	11.386	15765700	28701122	17.745	17.788
Target Compounds							
7)	B delta-BHC	0.000	7.016f	0	2290587	N.D.	0.931 #
10)	B gamma-Chl...	0.000	8.238	0	174149	N.D.	0.086 #
15)	B Endosulfa...	0.000	9.145f	0	1476270	N.D.	0.861 #
17)	MA 4,4'-DDT	0.000	9.365	0	209275	N.D.	0.132 #
25)	Chlordane-3	0.000	8.238	0	174149	N.D.	0.627 #
27)	Chlordane-5	0.000	9.199	0	39016	N.D.	0.639 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011822\
Data File : PL072077.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2022 20:55
Operator : AR\AJ
Sample : PB142097TB
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 04:28:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

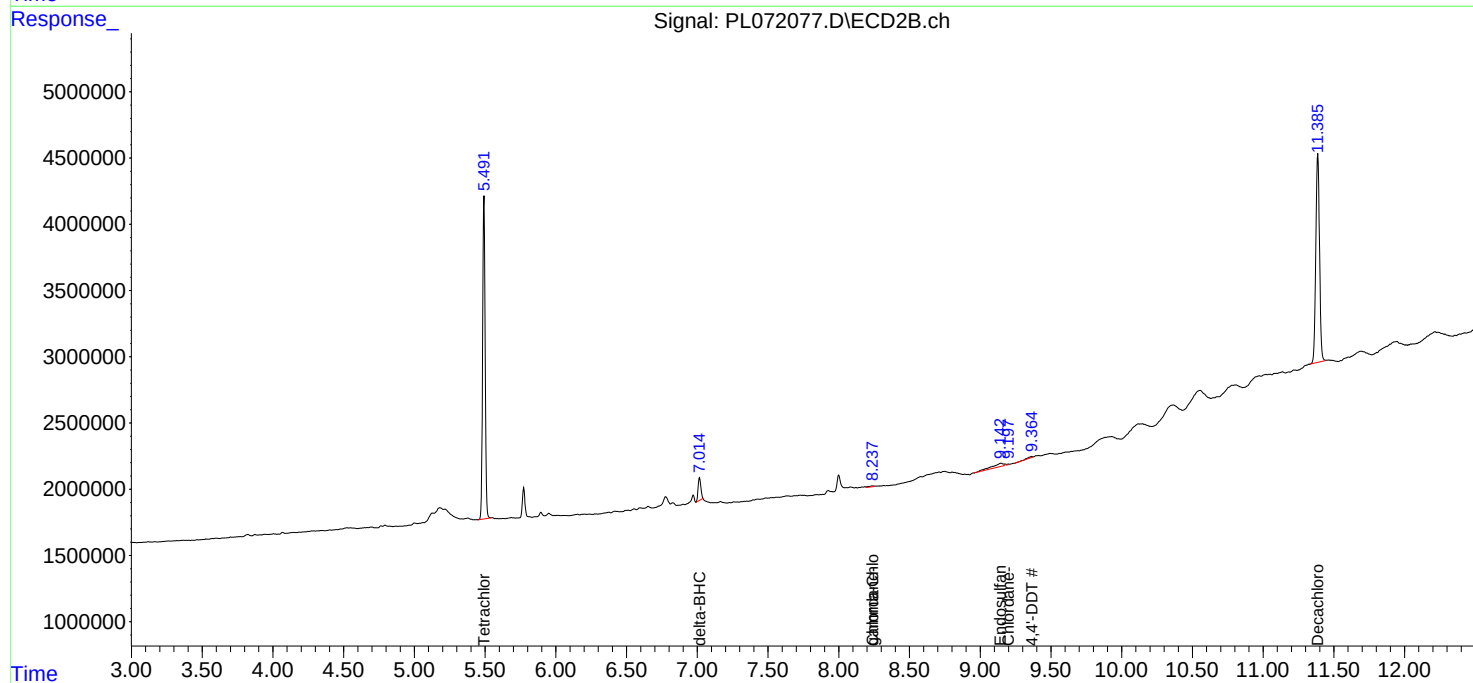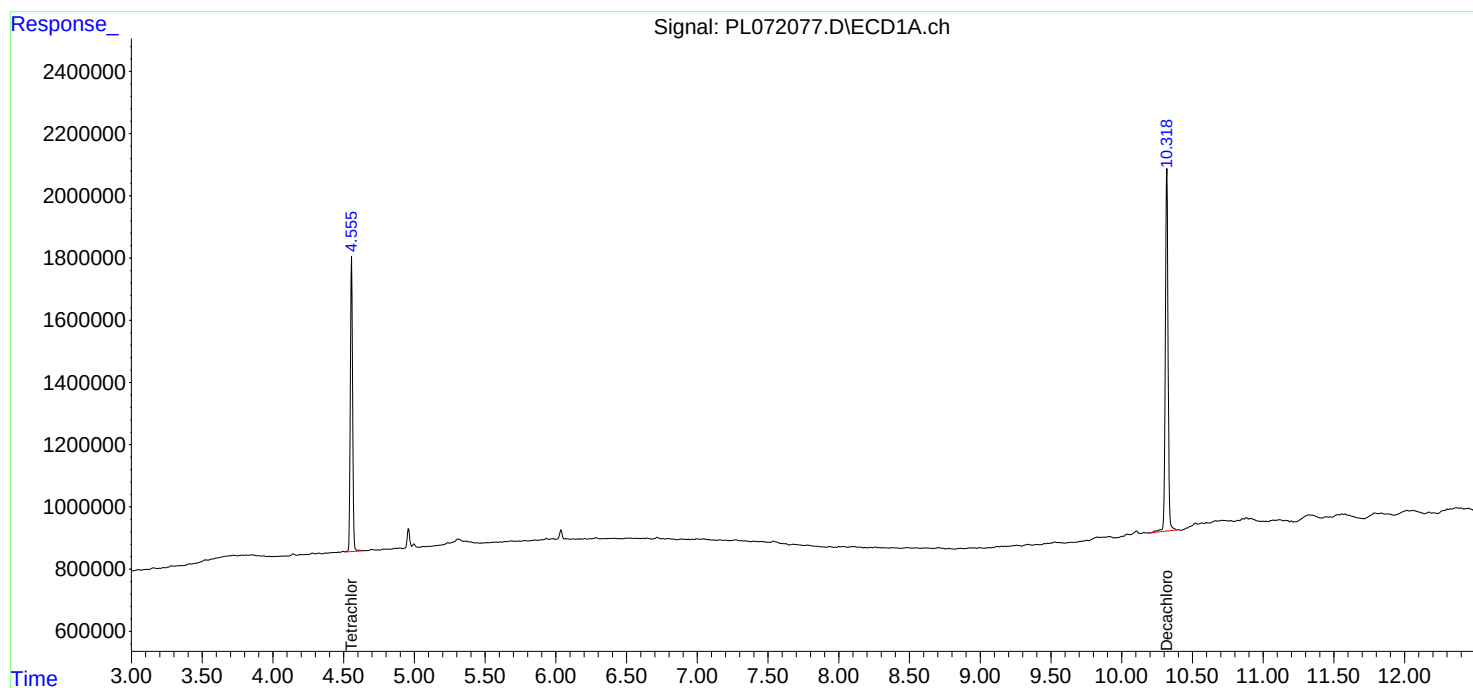


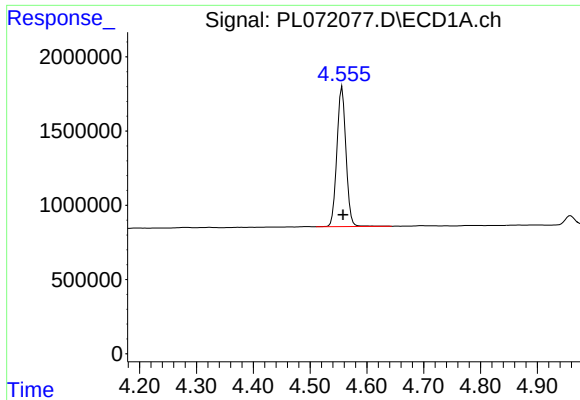

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 10476683
Conc: 18.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

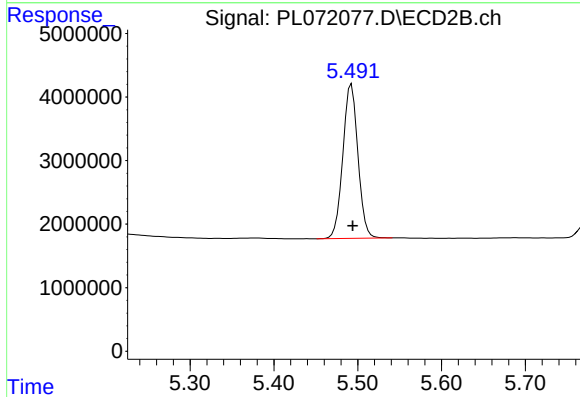


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 30359948
Conc: 18.69 ng/ml

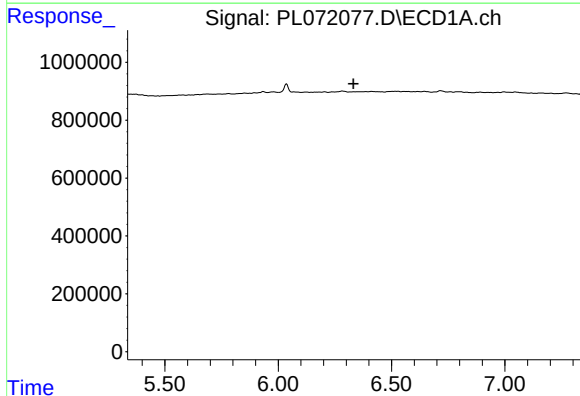


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

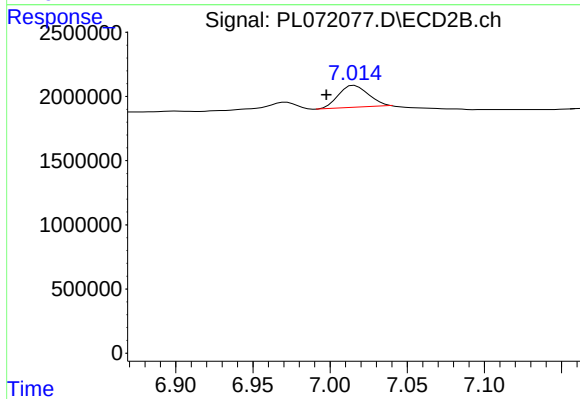

#7 delta-BHC


R.T.: 7.016 min
Delta R.T.: 0.018 min
Response: 2290587
Conc: 0.93 ng/ml

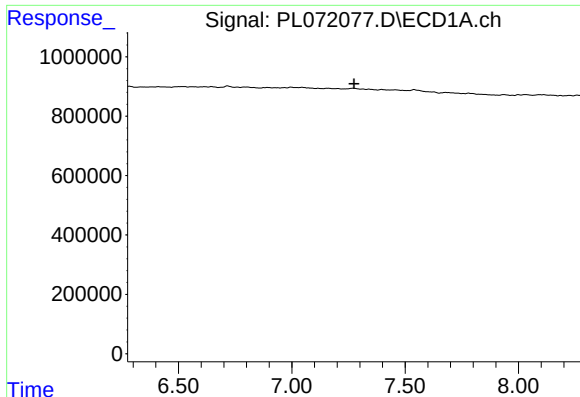

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

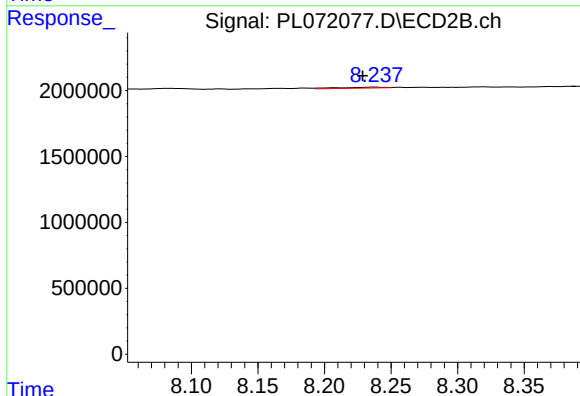


#10 gamma-Chlordane

R.T.: 8.238 min
Delta R.T.: 0.010 min
Response: 174149
Conc: 0.09 ng/ml

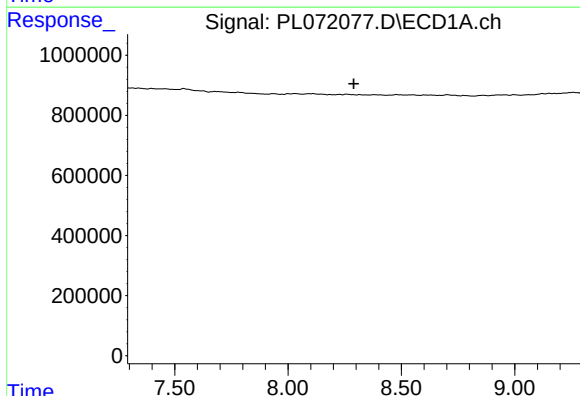


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

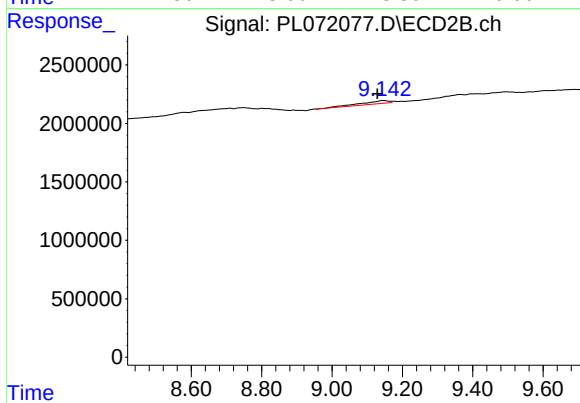

#15 Endosulfan II


R.T.: 9.145 min
Delta R.T.: 0.016 min
Response: 1476270
Conc: 0.86 ng/ml

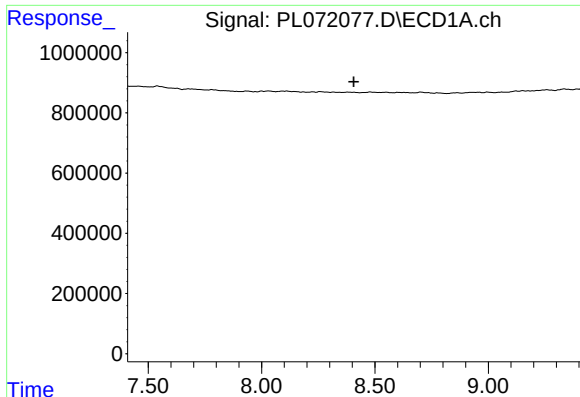

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

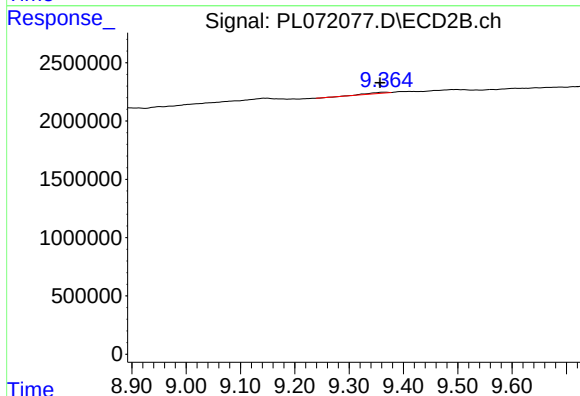


#17 4,4'-DDT

R.T.: 9.365 min
Delta R.T.: 0.008 min
Response: 209275
Conc: 0.13 ng/ml

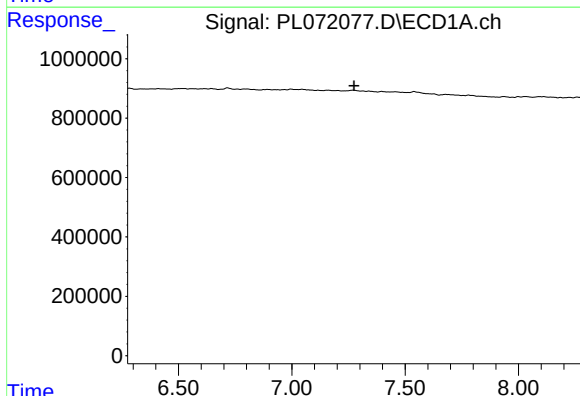


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

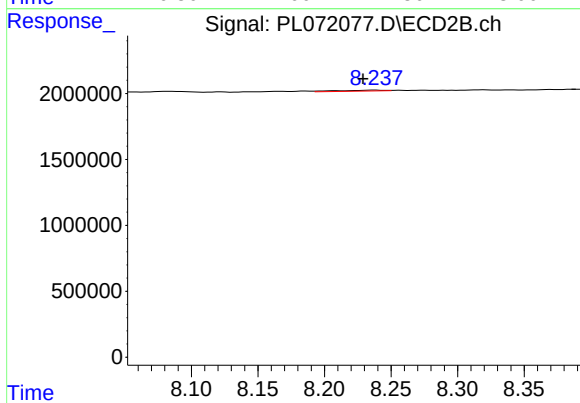

#25 Chlordane-3


R.T.: 8.238 min
Delta R.T.: 0.009 min
Response: 174149
Conc: 0.63 ng/ml

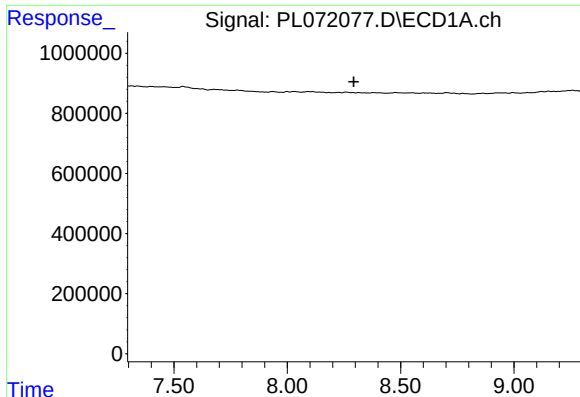

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

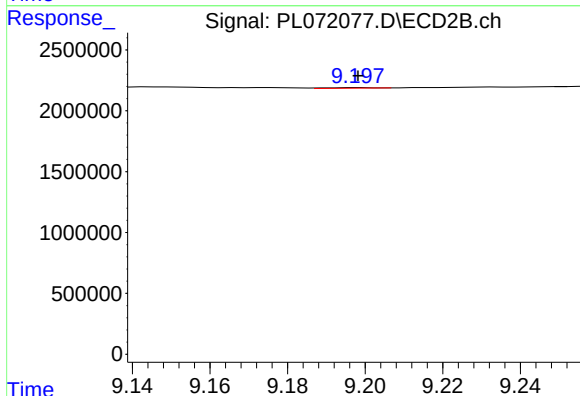


#27 Chlordane-5

R.T.: 9.199 min
Delta R.T.: 0.000 min
Response: 39016
Conc: 0.64 ng/ml

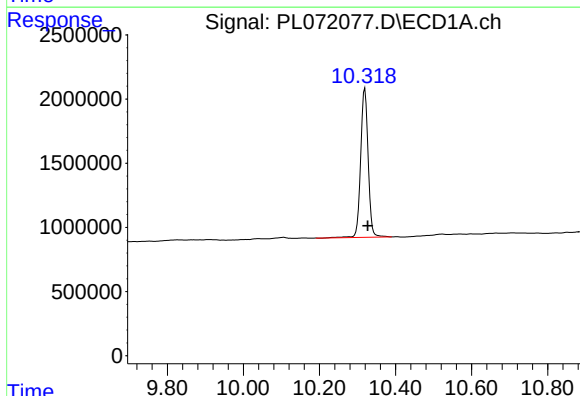

#28 Decachlorobiphenyl

R.T.: 10.319 min
Delta R.T.: -0.007 min
Response: 15765700
Conc: 17.75 ng/ml

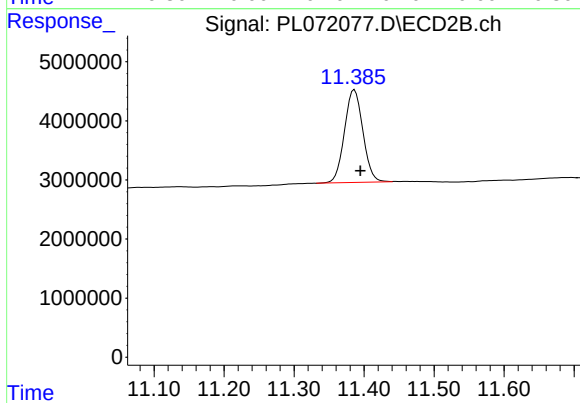

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: -0.008 min
Response: 28701122
Conc: 17.79 ng/ml