

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011822\
 Data File : PL072091.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jan 2022 00:42
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 04:32:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.493	10157425	29607166	18.295	18.230
28)	SA Decachlor...	10.319	11.386	15610724	28877816	17.571	17.898
Target Compounds							
7)	B delta-BHC	0.000	7.019f	0	158717	N.D.	0.065 #
9)	A Endosulfan I	0.000	8.353	0	19360	N.D.	0.011 #
11)	B alpha-Chl...	0.000	8.300	0	184327	N.D.	0.093 #
14)	MA Endrin	8.000f	0.000	747577	0	1.067	N.D. #
15)	B Endosulfa...	0.000	9.146f	0	342080	N.D.	0.199 #
16)	A 4,4'-DDD	0.000	9.039	0	199970	N.D.	0.140 #
19)	B Endosulfa...	0.000	9.529f	0	69585	N.D.	0.045 #
26)	Chlordane-4	0.000	8.320	0	151168	N.D.	0.455 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011822\
Data File : PL072091.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jan 2022 00:42
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 04:32:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

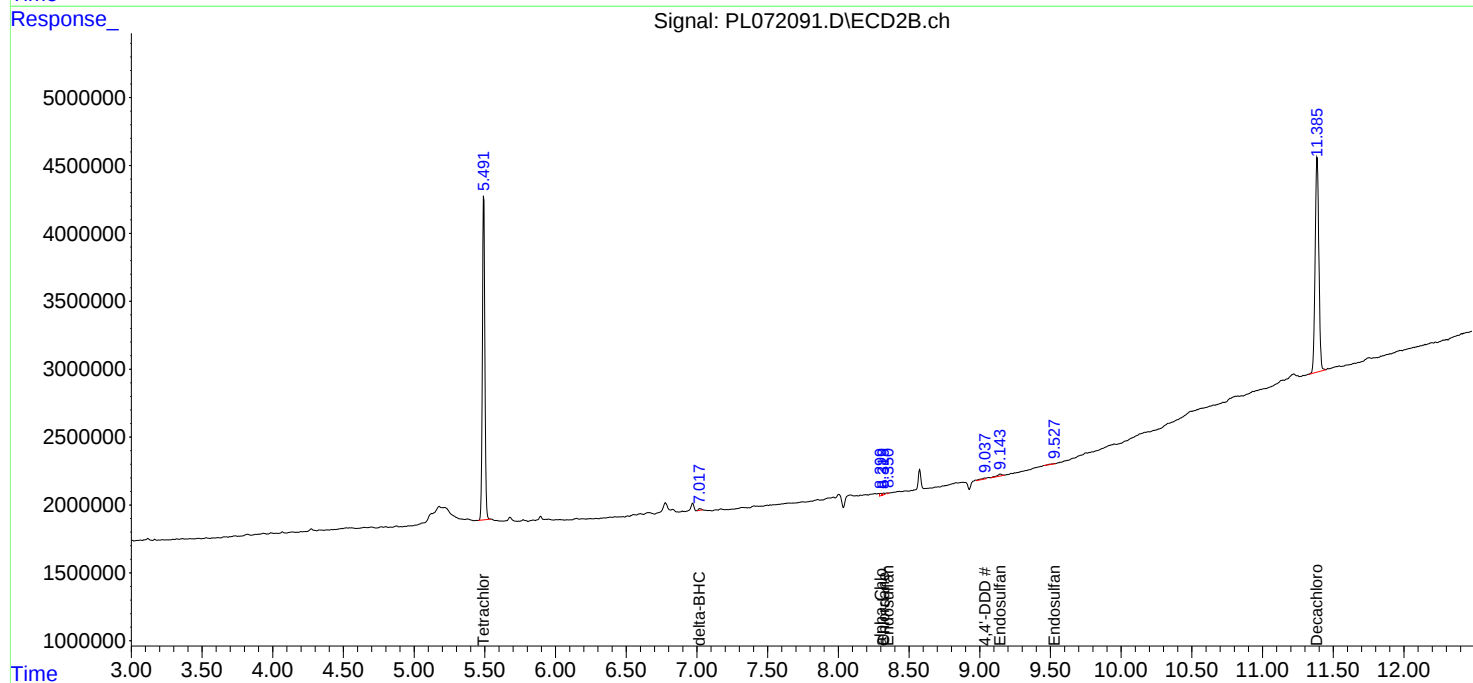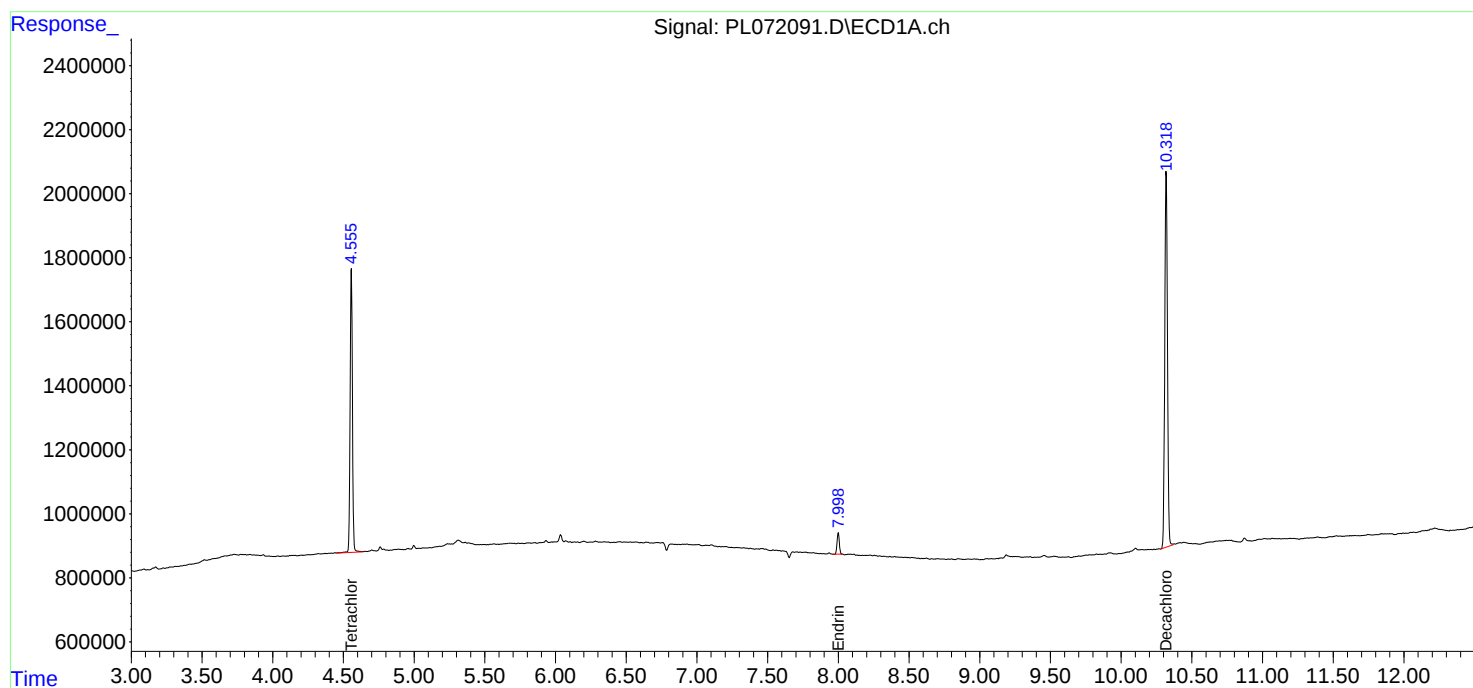


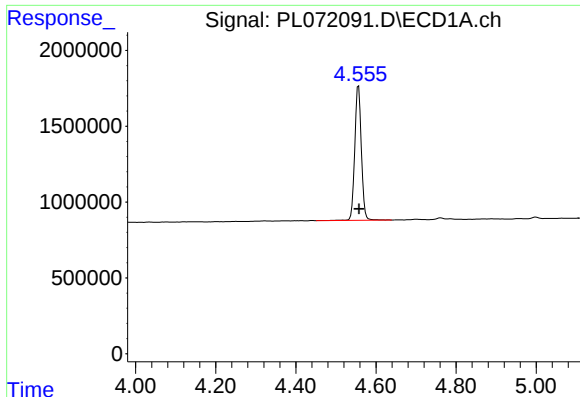

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 10157425
Conc: 18.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

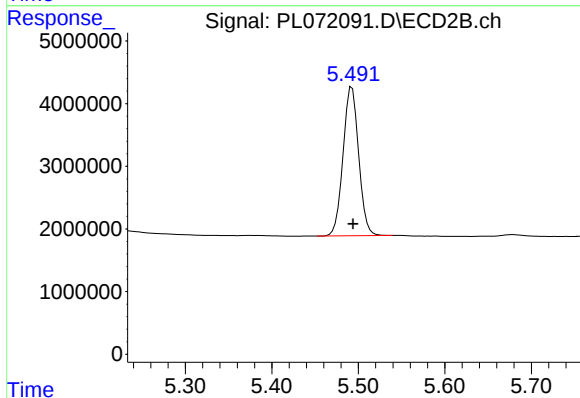


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: -0.001 min
Response: 29607166
Conc: 18.23 ng/ml

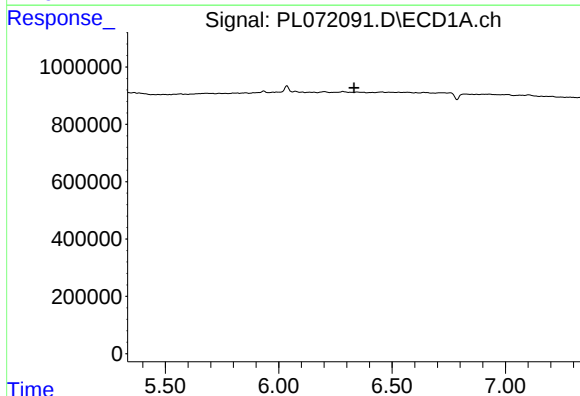


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

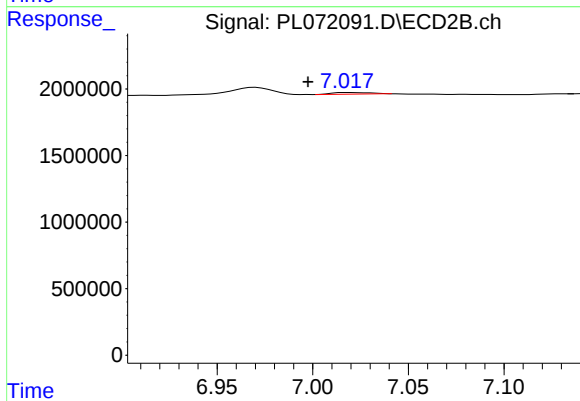

#7 delta-BHC


R.T.: 7.019 min
Delta R.T.: 0.021 min
Response: 158717
Conc: 0.06 ng/ml

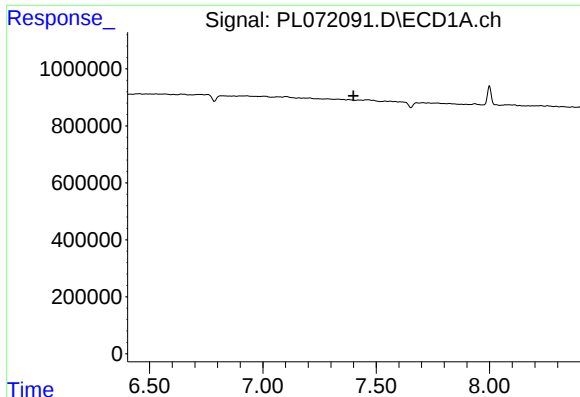

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

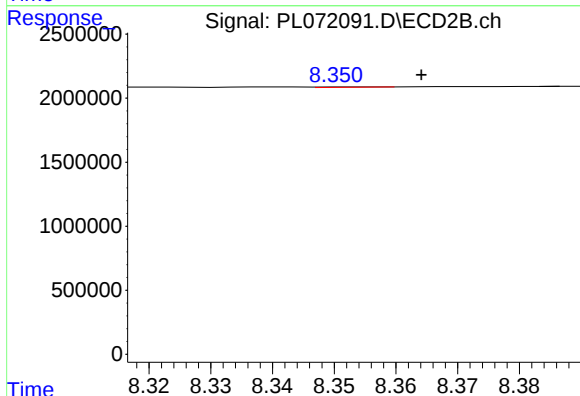


#9 Endosulfan I

R.T.: 8.353 min
Delta R.T.: -0.011 min
Response: 19360
Conc: 0.01 ng/ml

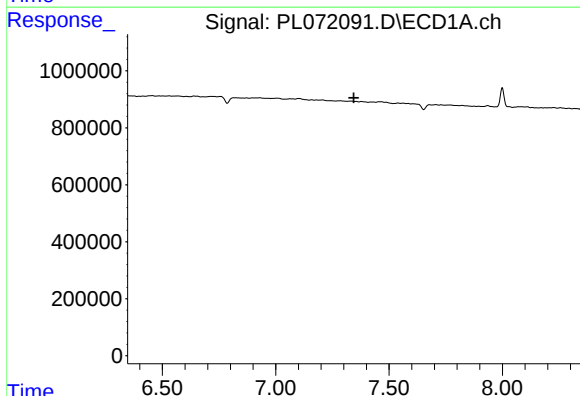


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

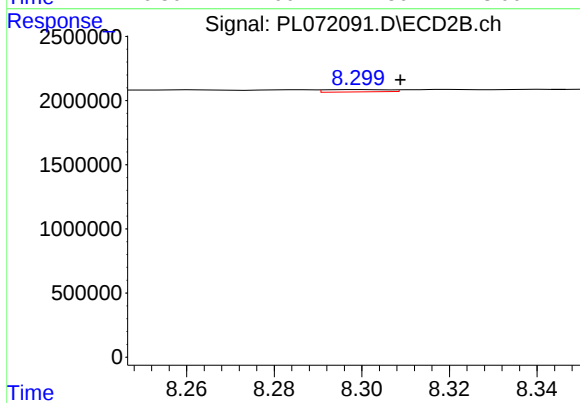

#11 alpha-Chlordane


R.T.: 8.300 min
Delta R.T.: -0.009 min
Response: 184327
Conc: 0.09 ng/ml

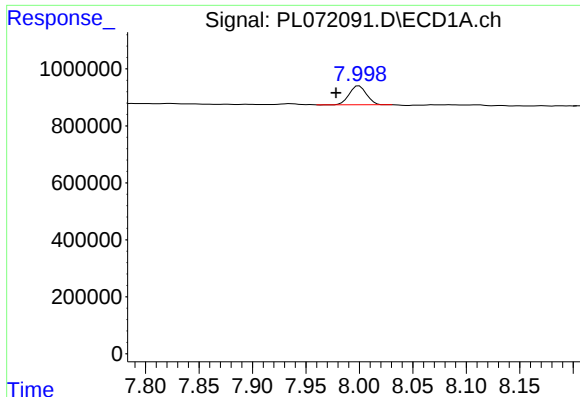

#14 Endrin


R.T.: 8.000 min
Delta R.T.: 0.022 min
Response: 747577
Conc: 1.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

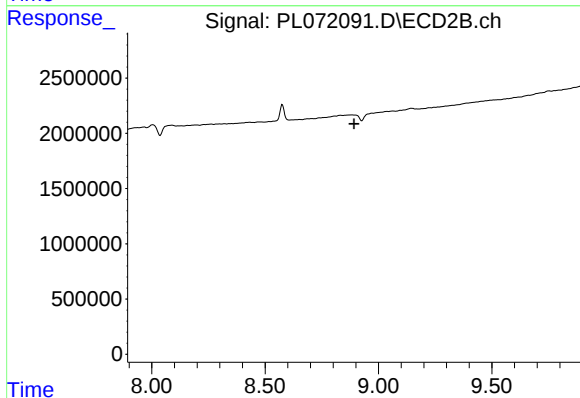


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.893 min
Response: 0
Conc: N.D.

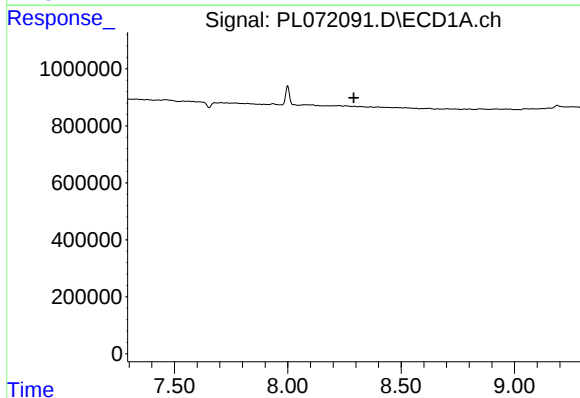


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.291 min
Response: 0
Conc: N.D.

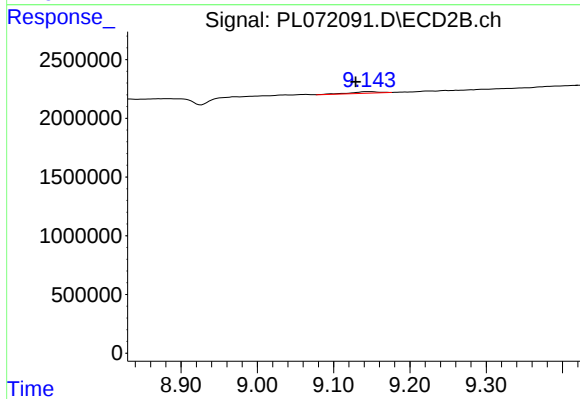

#15 Endosulfan II


R.T.: 9.146 min
Delta R.T.: 0.017 min
Response: 342080
Conc: 0.20 ng/ml

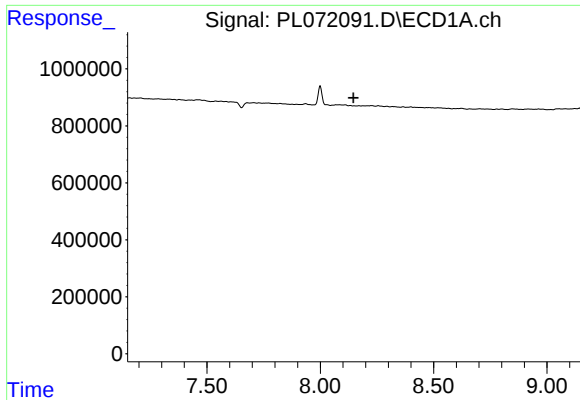

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

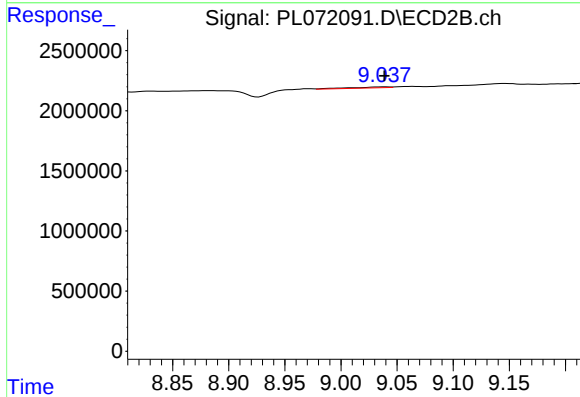


#16 4,4'-DDD

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 199970
Conc: 0.14 ng/ml

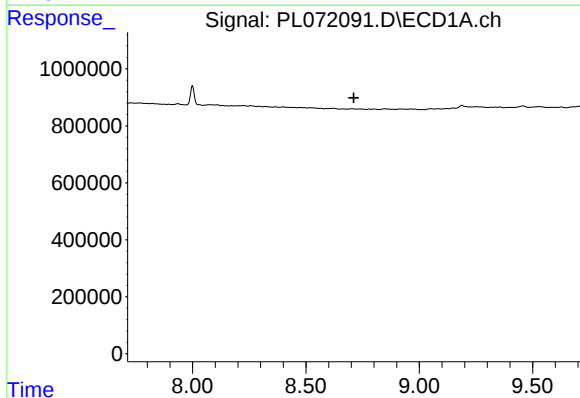


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

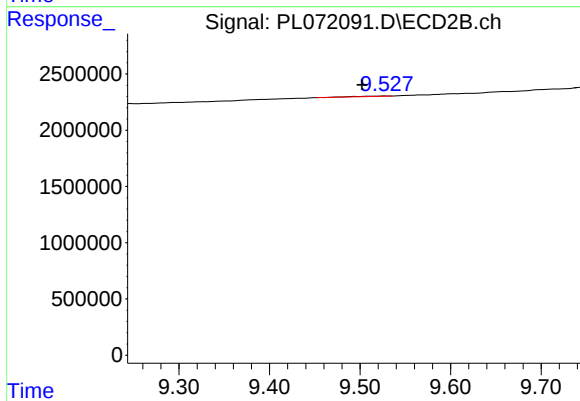

#19 Endosulfan Sulfate


R.T.: 9.529 min
Delta R.T.: 0.027 min
Response: 69585
Conc: 0.04 ng/ml

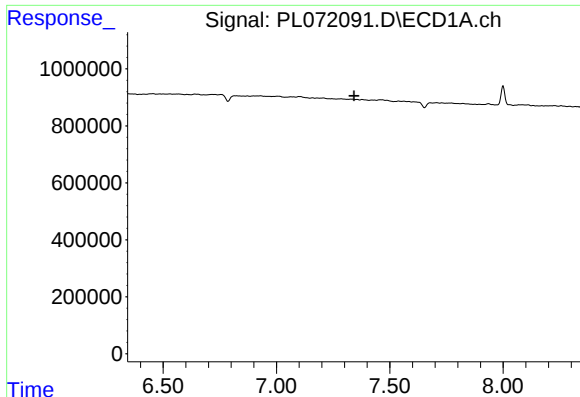

#26 Chlorine-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

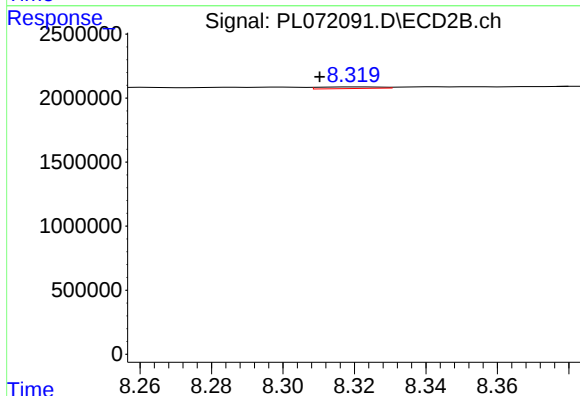


#26 Chlorine-4

R.T.: 8.320 min
Delta R.T.: 0.010 min
Response: 151168
Conc: 0.46 ng/ml

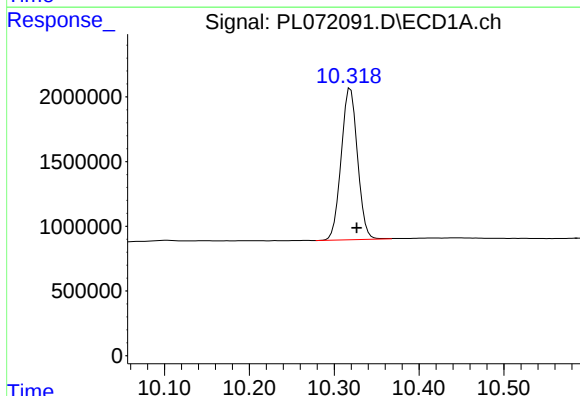

#28 Decachlorobiphenyl

R.T.: 10.319 min
Delta R.T.: -0.007 min
Response: 15610724
Conc: 17.57 ng/ml

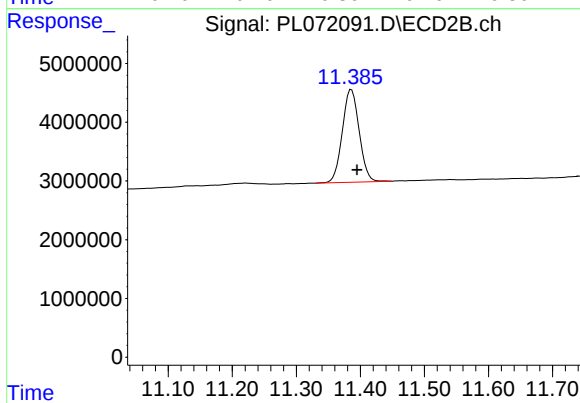

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: -0.009 min
Response: 28877816
Conc: 17.90 ng/ml