

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011921\
 Data File : PL064233.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jan 2021 17:39
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 05:41:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.434	4.108	59057524	47857204	19.696	18.720
28) SA Decachlor...	8.166	9.267	45816797	36958856	15.012	15.572
Target Compounds						
14) MA Endrin	0.000	6.886f	0	1181658	N.D.	0.517 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011921\
Data File : PL064233.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jan 2021 17:39
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 05:41:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

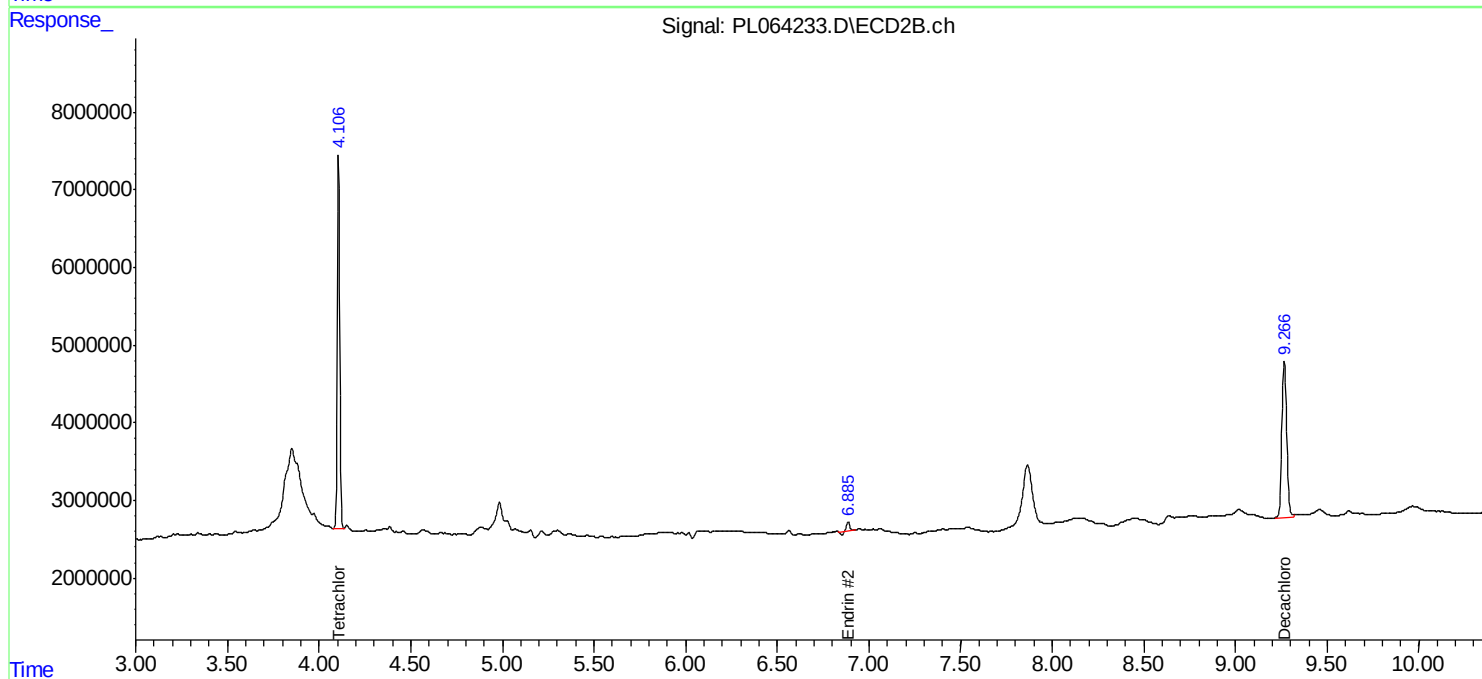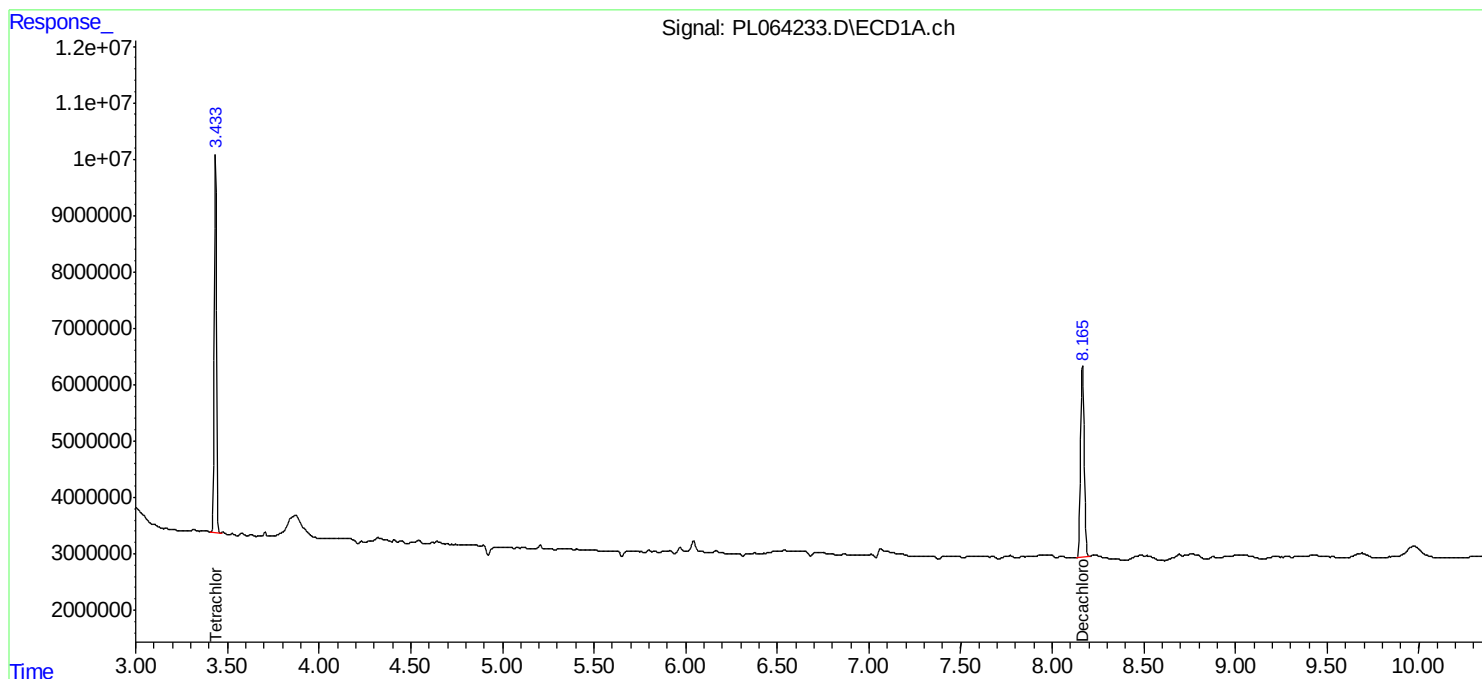


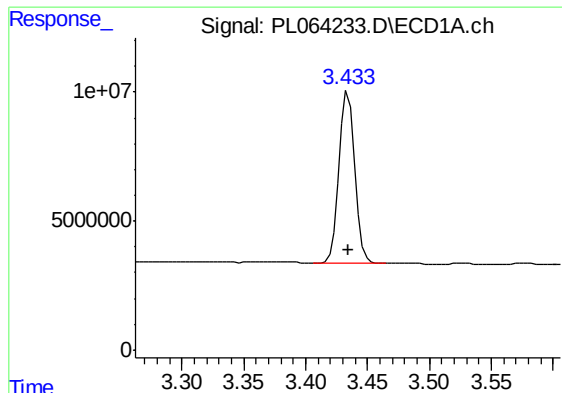

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 59057524
Conc: 19.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

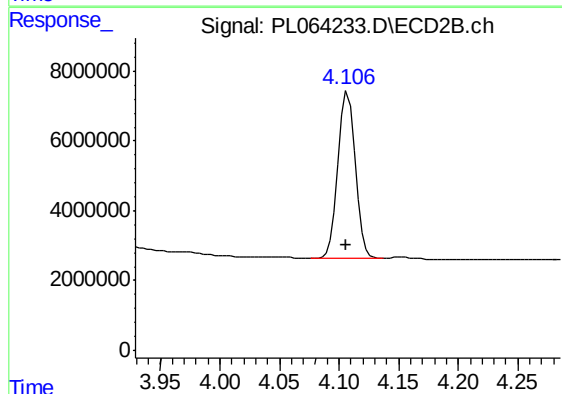


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.001 min
Response: 47857204
Conc: 18.72 ng/ml

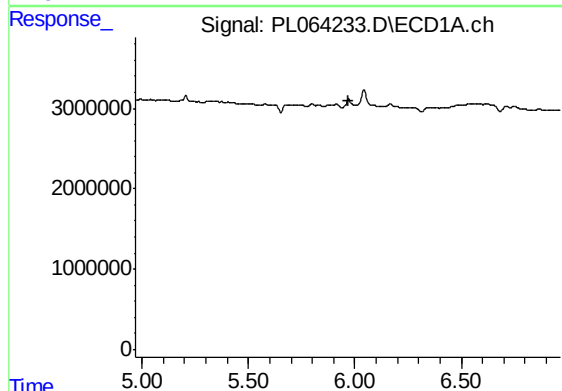


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.969 min
Response: 0
Conc: N.D.

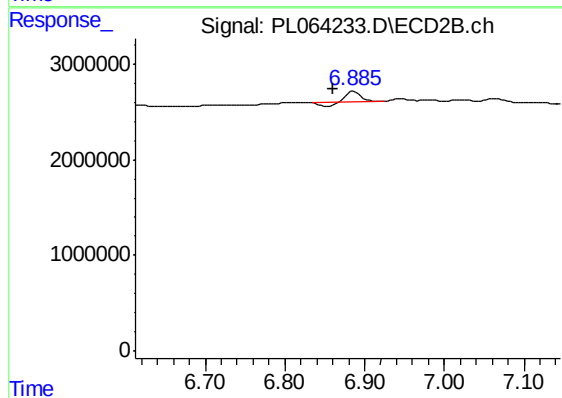

#14 Endrin


R.T.: 6.886 min
Delta R.T.: 0.026 min
Response: 1181658
Conc: 0.52 ng/ml

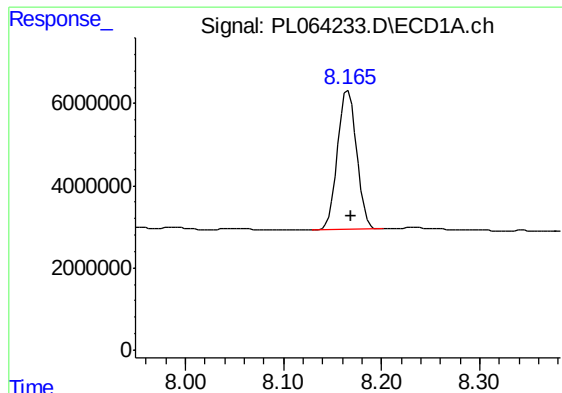

#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: -0.003 min
Response: 45816797
Conc: 15.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

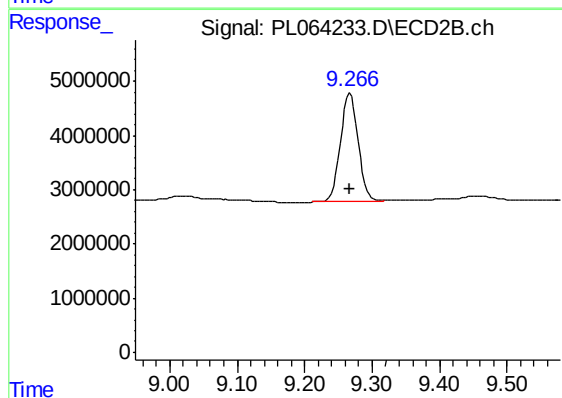

#28 Decachlorobiphenyl

R.T.: 9.267 min
Delta R.T.: 0.001 min
Response: 36958856
Conc: 15.57 ng/ml