

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011924\
 Data File : PL087873.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jan 2024 15:55
 Operator : AR\AJ
 Sample : P1163-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-INFLUENT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/22/2024
 Supervised By :Ankita Jodhani 01/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 19:08:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 03:17:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.674	56294754	28836499	18.804	23.805 #
28)	SA Decachlor...	8.983	7.859	71481749	17650856	25.099m	13.933m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011924\
Data File : PL087873.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jan 2024 15:55
Operator : AR\AJ
Sample : P1163-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/22/2024
Supervised By : Ankita Jodhani 01/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 19:08:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:17:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

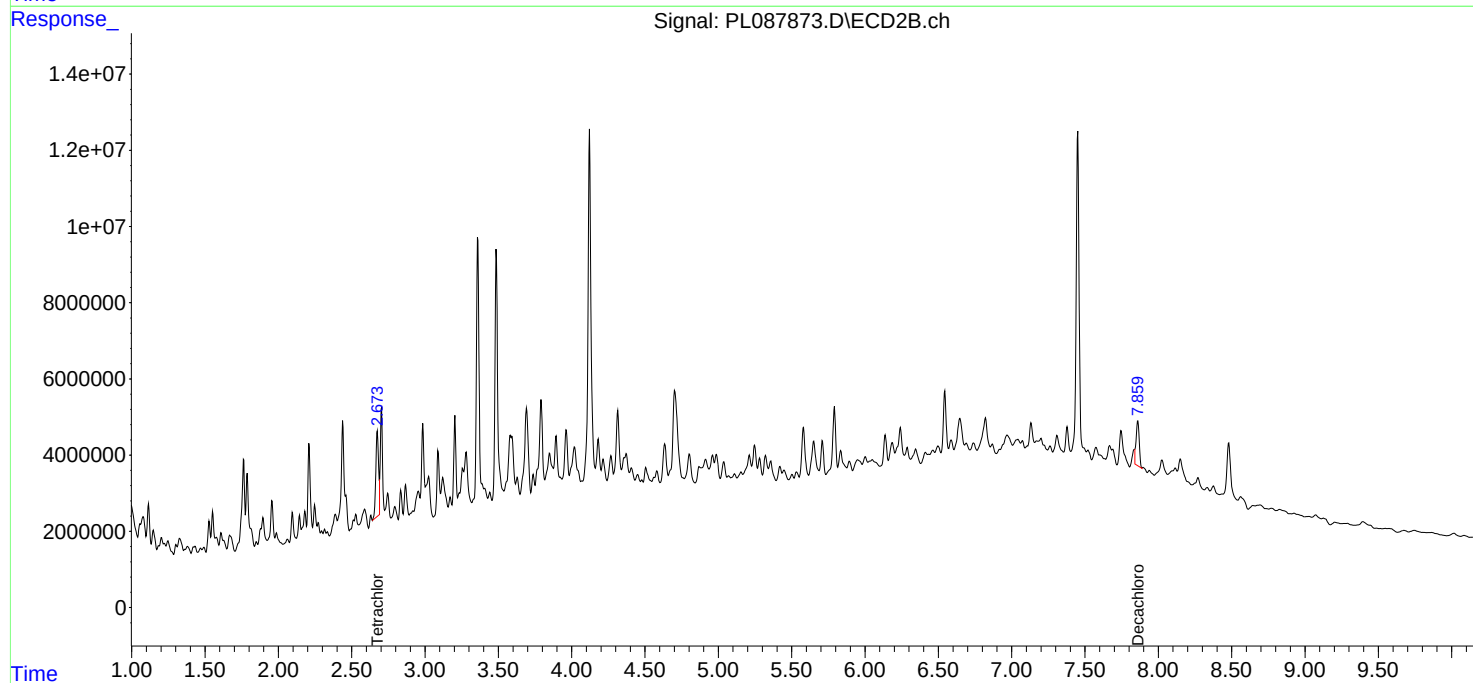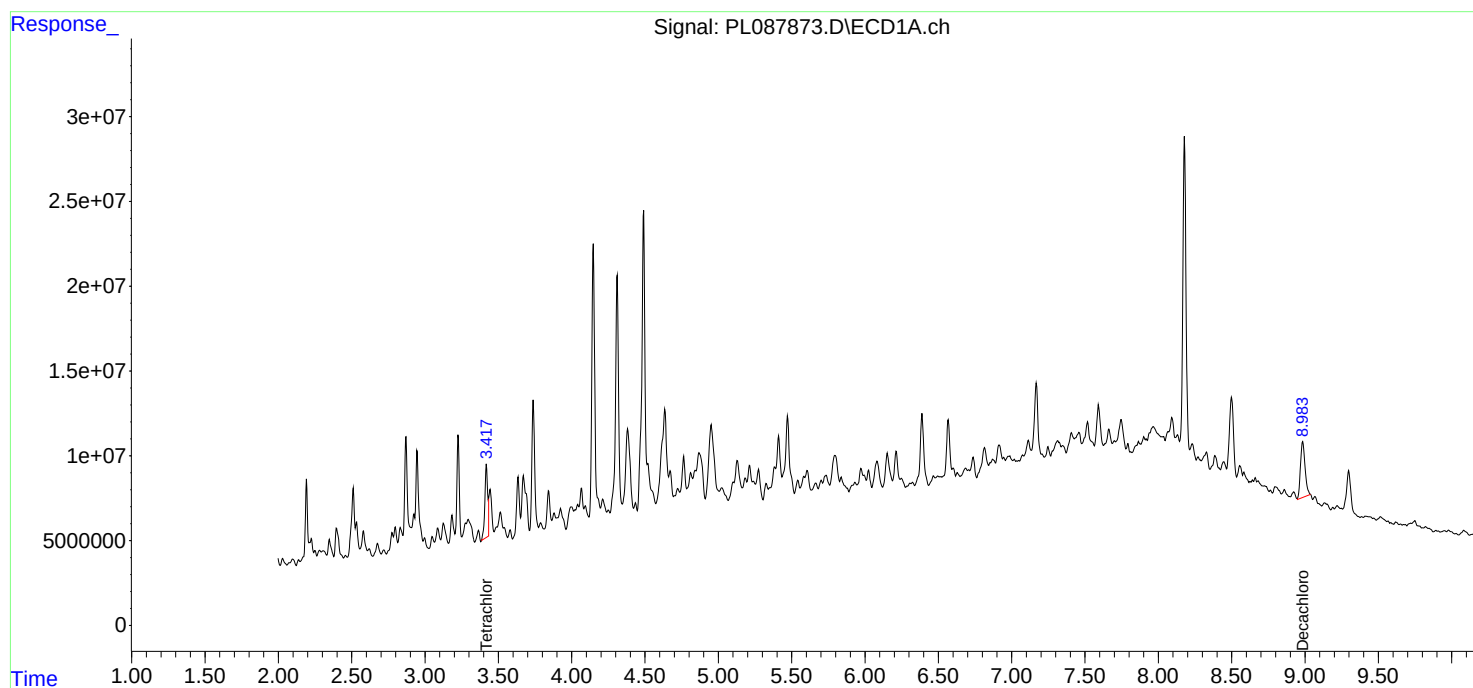

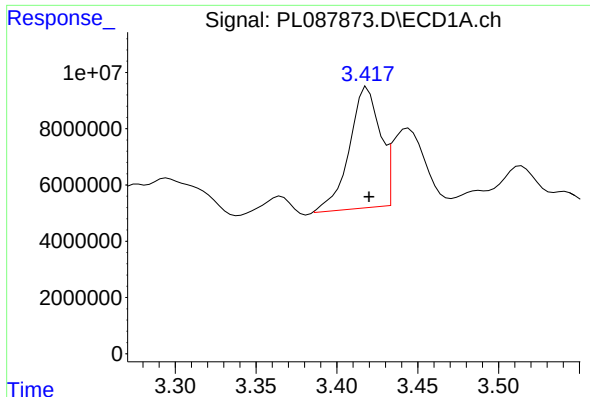


#1 Tetrachloro-m-xylene

R.T.: 3.419 min
Delta R.T.: -0.001 min
Response: 56294754
Conc: 18.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/22/2024
Supervised By :Ankita Jodhani 01/22/2024

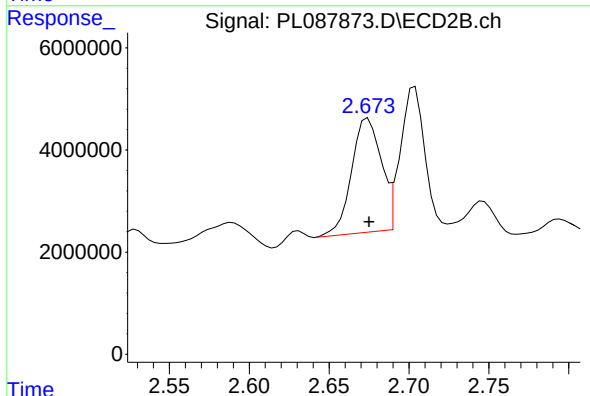


#1 Tetrachloro-m-xylene

R.T.: 2.674 min
Delta R.T.: 0.000 min
Response: 28836499
Conc: 23.81 ng/ml

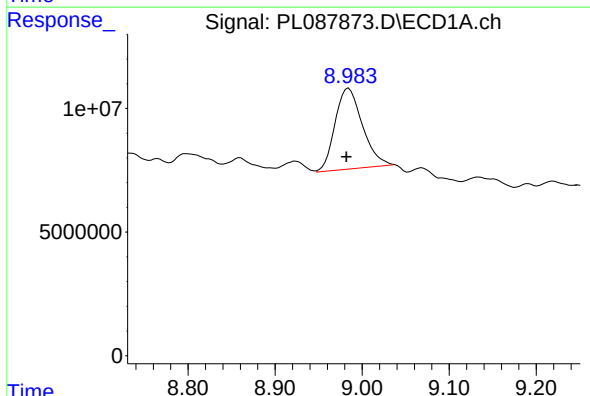

#28 Decachlorobiphenyl

R.T.: 8.983 min
Delta R.T.: 0.001 min
Response: 71481749
Conc: 25.10 ng/ml m

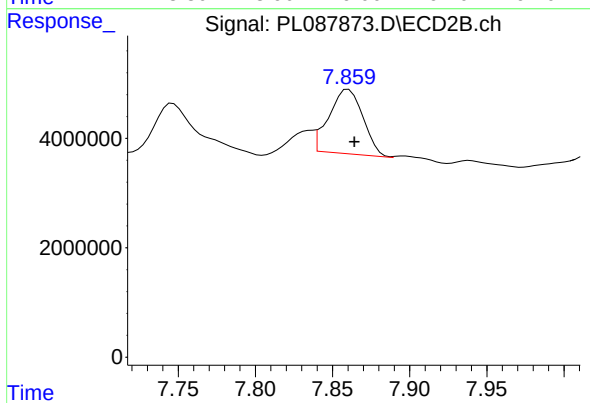

#28 Decachlorobiphenyl

R.T.: 7.859 min
Delta R.T.: -0.005 min
Response: 17650856
Conc: 13.93 ng/ml m