

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
 Data File : PL055867.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2020 19:58
 Operator : AJ\MA
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 01:28:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 01:25:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.489	3.967	1134.8E6	289.5E6	103.274	102.636
28)	SA Decachlor...	8.234	8.952	1054.9E6	218.0E6	99.342	96.778
Target Compounds							
23)	Chlordane-1	4.359	4.943	380.9E6	104.7E6	1035.487	1008.463
24)	Chlordane-2	4.860	5.404	425.9E6	103.4E6	990.542	974.382
25)	Chlordane-3	5.428	6.041	1289.2E6	396.1E6	1001.319	1027.518
26)	Chlordane-4	5.486	6.114	1075.5E6	461.7E6	1005.368	1021.516
27)	Chlordane-5	6.321	6.909	412.6E6	81282636	1141.511	1004.964



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
Data File : PL055867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2020 19:58
Operator : AJ\MA
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 01:28:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 01:25:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

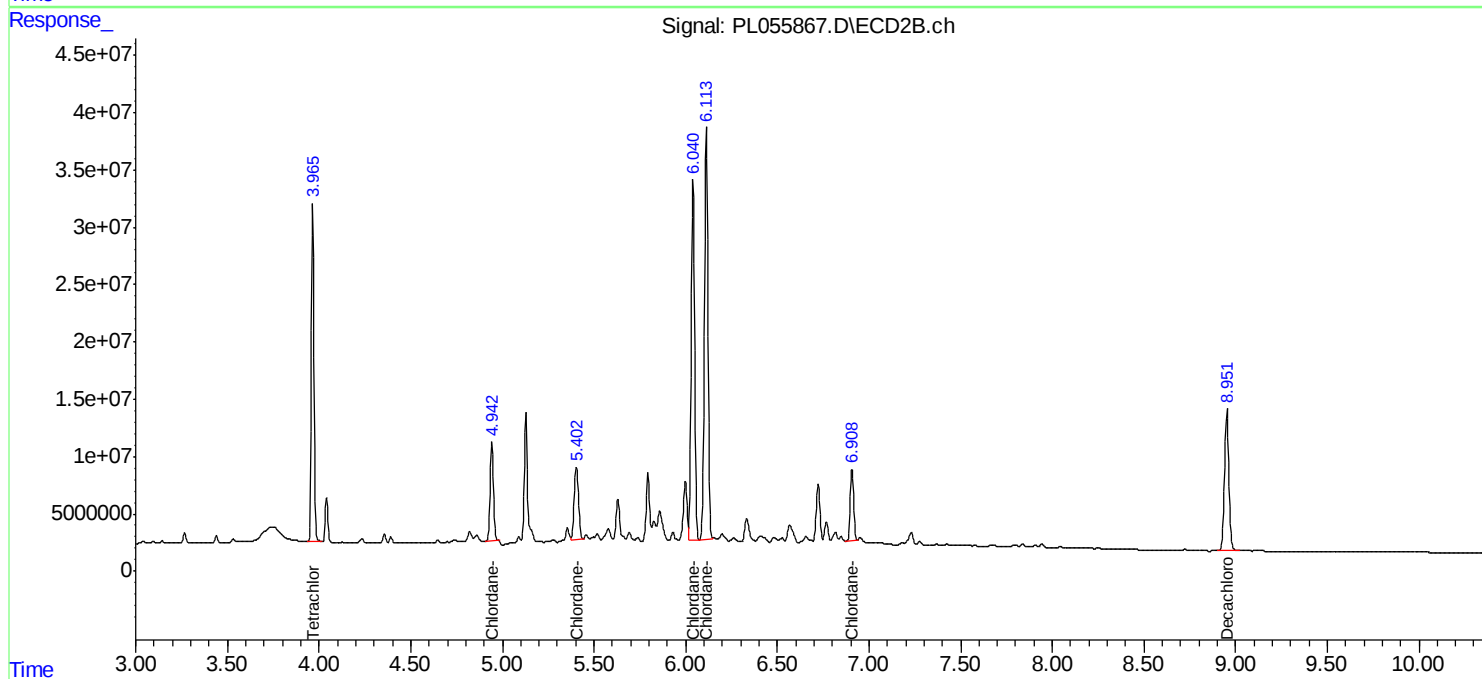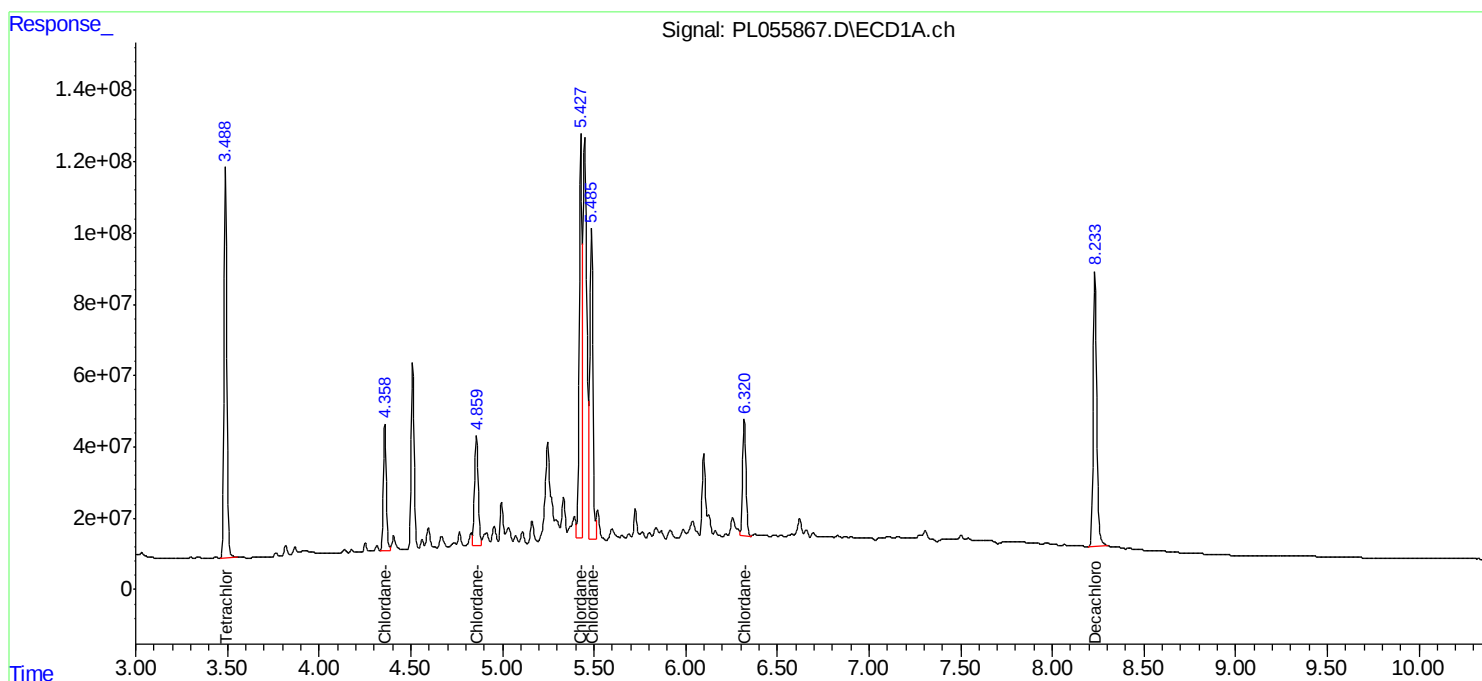


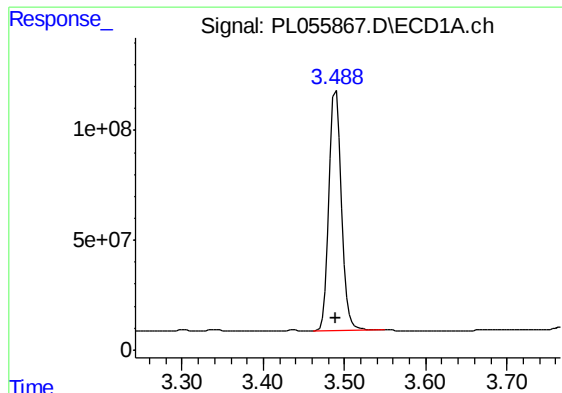

#1 Tetrachloro-m-xylene


R.T.: 3.489 min
Delta R.T.: 0.000 min
Response: 1134840837
Conc: 103.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

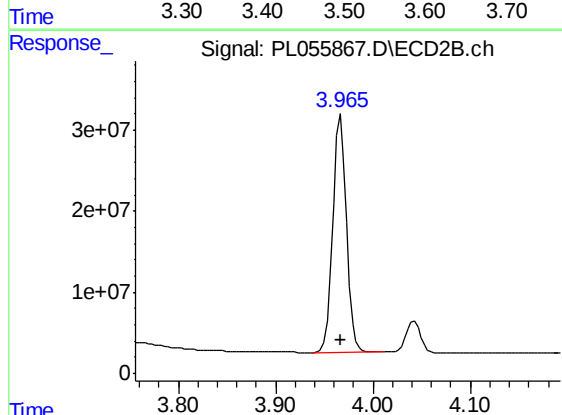


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 289466243
Conc: 102.64 ng/ml

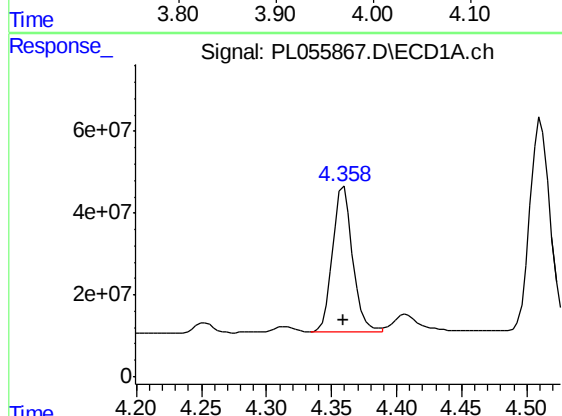


#23 Chlordane-1

R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 380940603
Conc: 1035.49 ng/ml

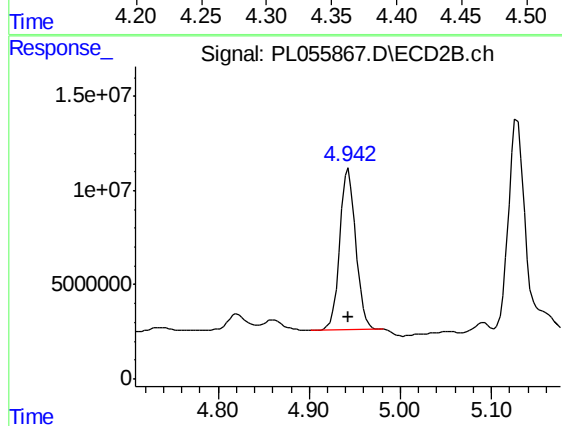

#23 Chlordane-1


R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 104734190
Conc: 1008.46 ng/ml

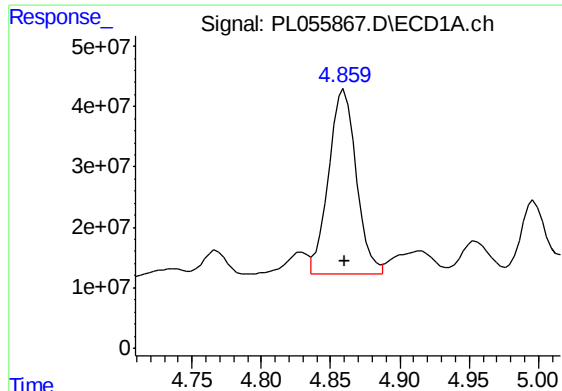

#24 Chlordane-2


R.T.: 4.860 min
Delta R.T.: 0.000 min
Response: 425872520
Conc: 990.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

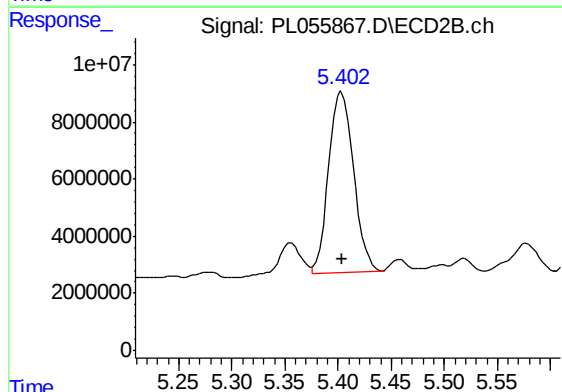


#24 Chlordane-2

R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 103407961
Conc: 974.38 ng/ml

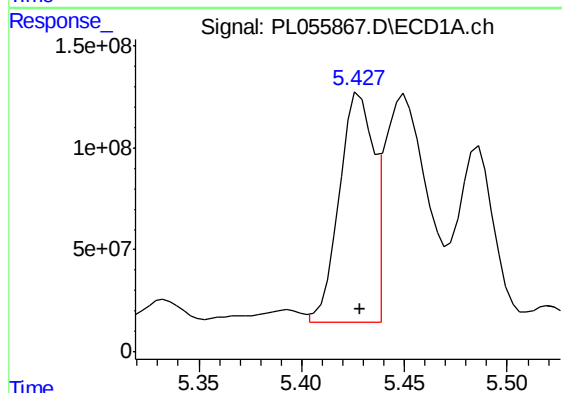


#25 Chlordane-3

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 1289163338
Conc: 1001.32 ng/ml

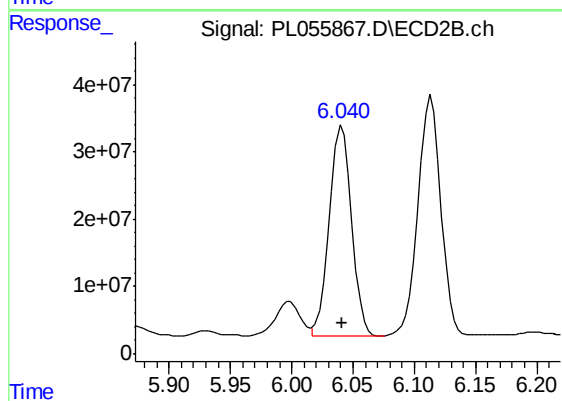

#25 Chlordane-3


R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 396111640
Conc: 1027.52 ng/ml

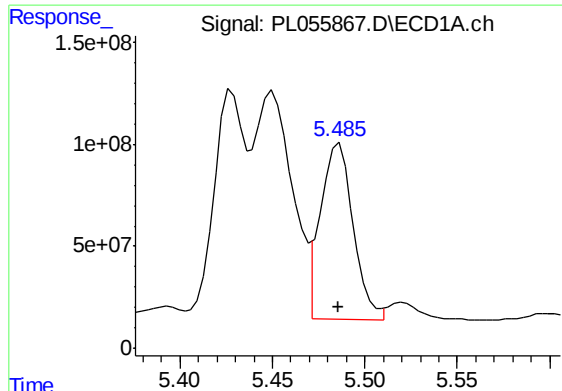

#26 Chlordane-4


R.T.: 5.486 min
Delta R.T.: 0.000 min
Response: 1075504597
Conc: 1005.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

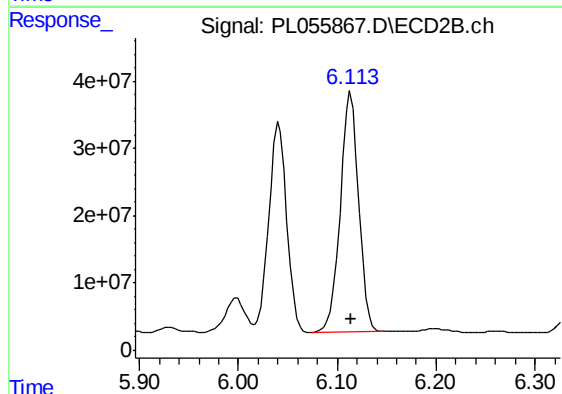


#26 Chlordane-4

R.T.: 6.114 min
Delta R.T.: 0.000 min
Response: 461713379
Conc: 1021.52 ng/ml

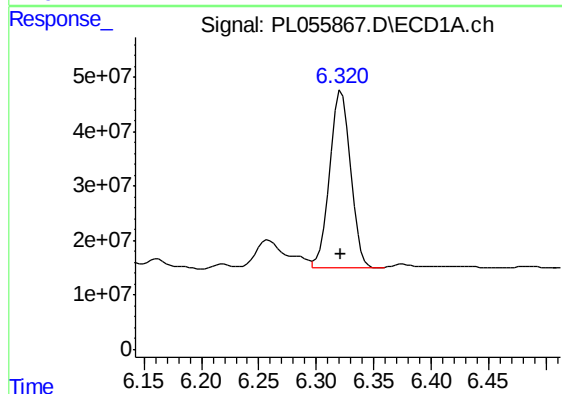


#27 Chlordane-5

R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 412584426
Conc: 1141.51 ng/ml

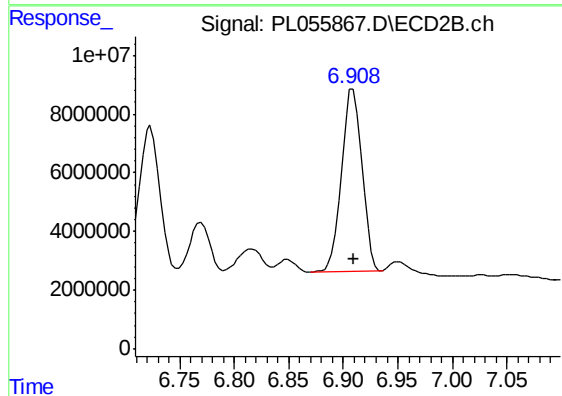

#27 Chlordane-5


R.T.: 6.909 min
Delta R.T.: -0.001 min
Response: 81282636
Conc: 1004.96 ng/ml

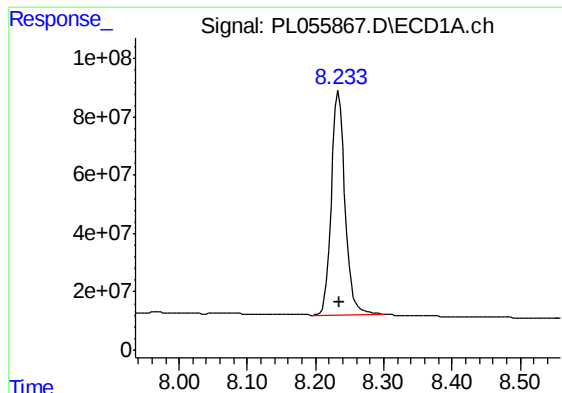

#28 Decachlorobiphenyl

R.T.: 8.234 min
Delta R.T.: 0.000 min
Response: 1054889598
Conc: 99.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

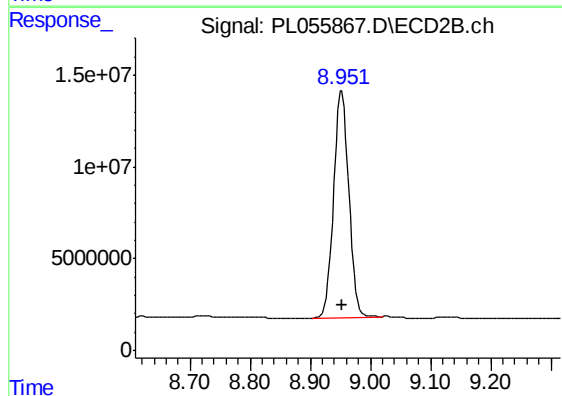

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.001 min
Response: 218011258
Conc: 96.78 ng/ml