

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
 Data File : PL055868.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2020 20:12
 Operator : AJ\MA
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 01:28:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 01:25:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	3.967	846.0E6	213.5E6	76.992	75.690
28)	SA Decachlor...	8.235	8.955	792.2E6	165.7E6	74.603	73.575
Target Compounds							
23)	Chlordane-1	4.360	4.944	285.3E6	78928268	775.400	759.984
24)	Chlordane-2	4.860	5.404	339.2E6	78475392	788.920	739.450
25)	Chlordane-3	5.429	6.042	960.9E6	294.9E6	746.321	764.914
26)	Chlordane-4	5.486	6.114	813.4E6	343.8E6	760.390	760.531
27)	Chlordane-5	6.322	6.910	317.2E6	61018805	877.517	754.426



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
Data File : PL055868.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2020 20:12
Operator : AJ\MA
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 01:28:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 01:25:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

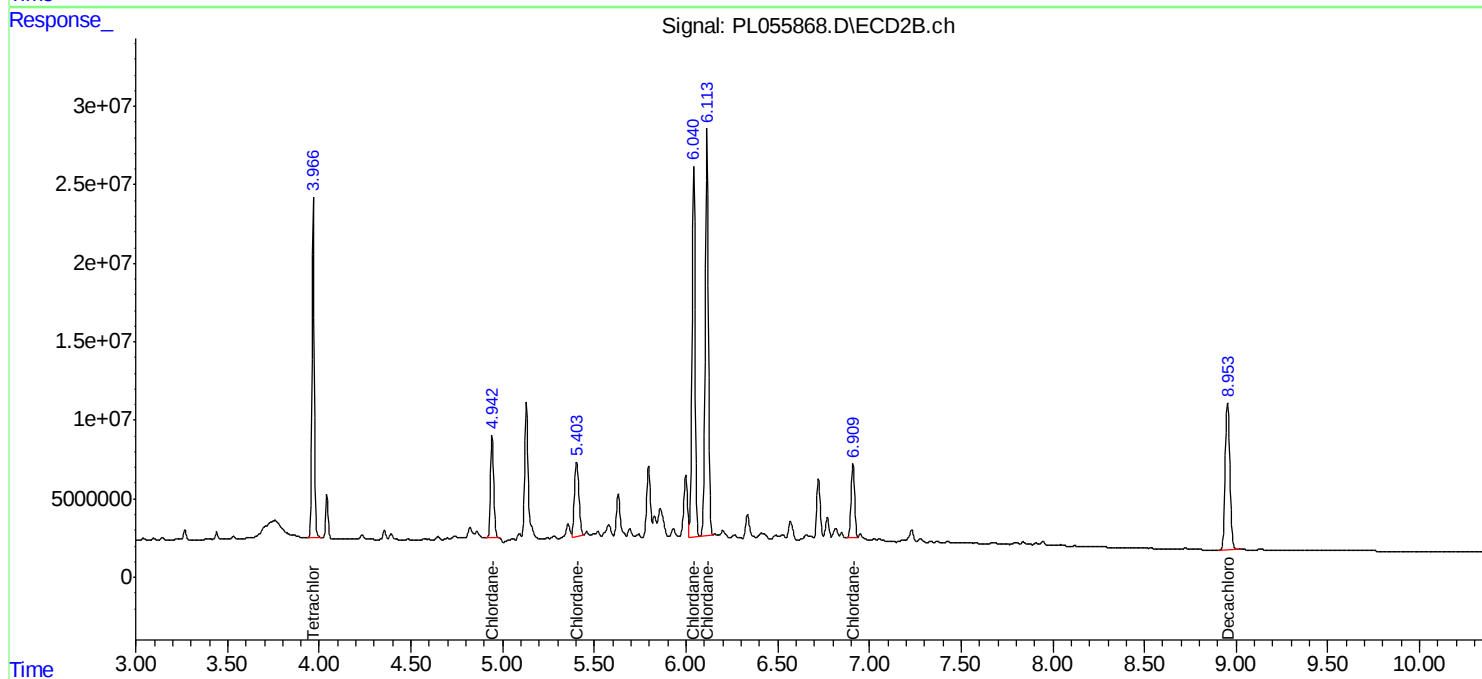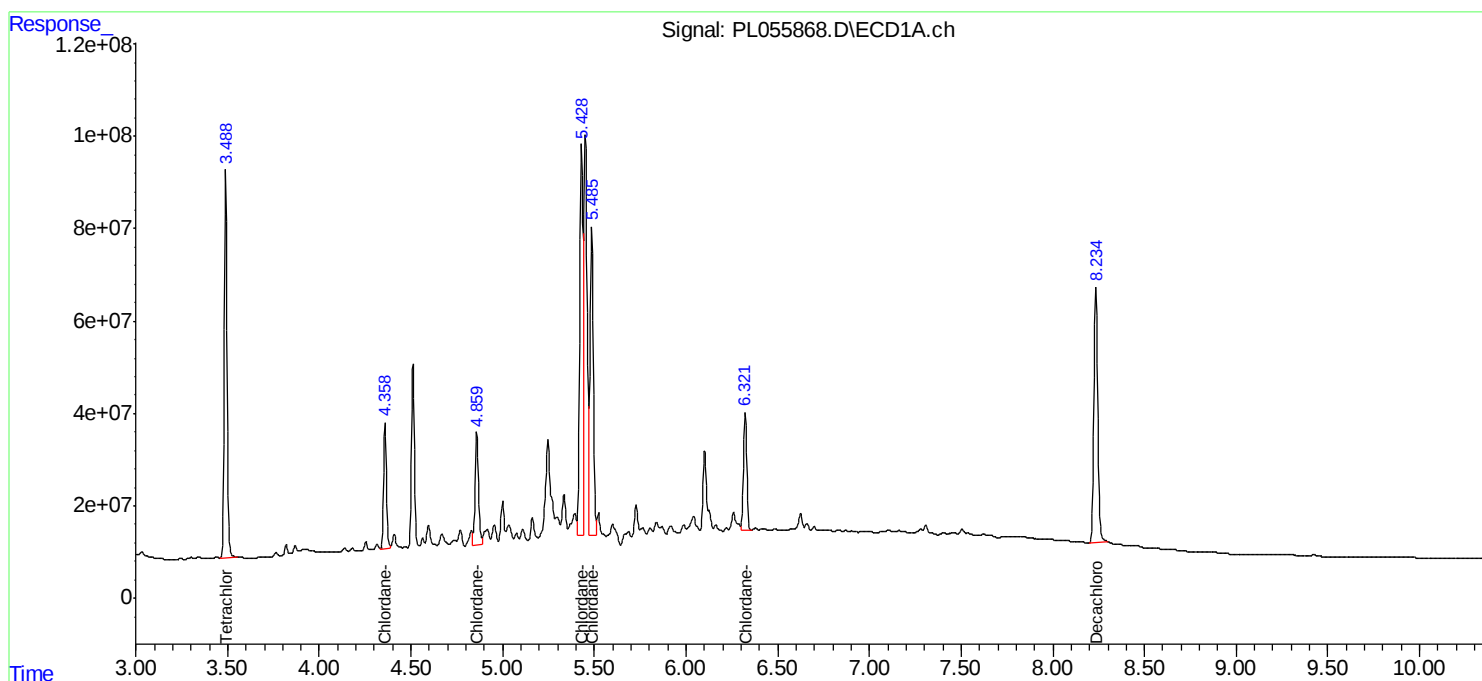


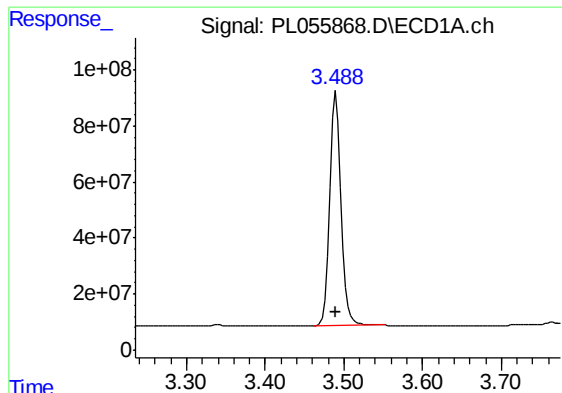

#1 Tetrachloro-m-xylene


R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 846040188
Conc: 76.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

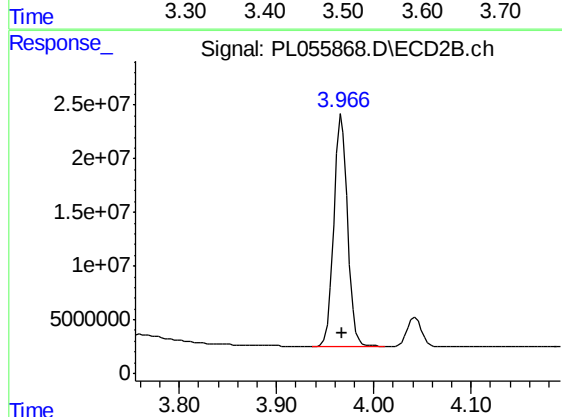


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 213468963
Conc: 75.69 ng/ml

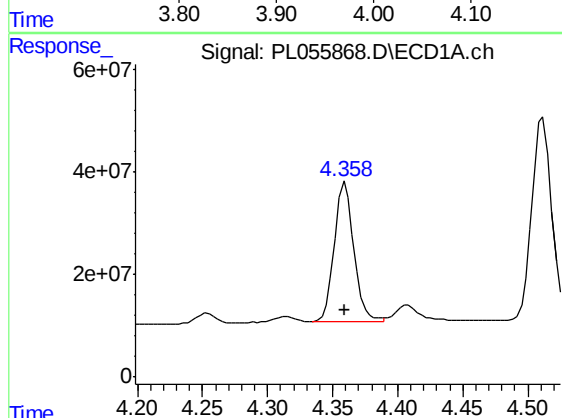


#23 Chlordane-1

R.T.: 4.360 min
Delta R.T.: 0.000 min
Response: 285258579
Conc: 775.40 ng/ml

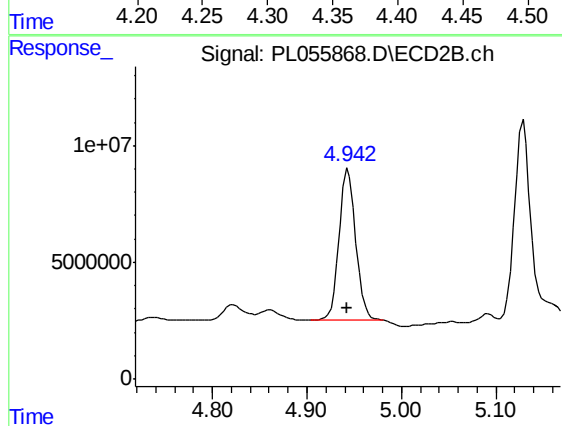

#23 Chlordane-1


R.T.: 4.944 min
Delta R.T.: 0.000 min
Response: 78928268
Conc: 759.98 ng/ml

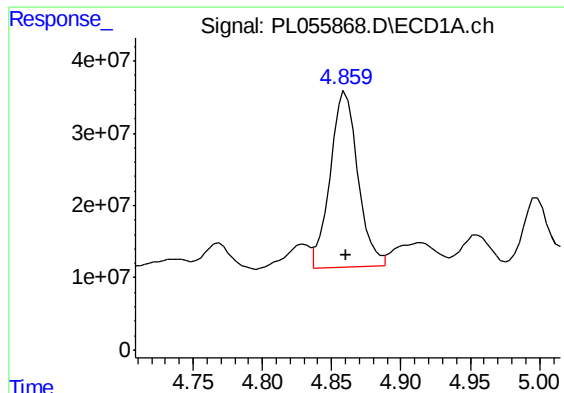

#24 Chlordane-2


R.T.: 4.860 min
Delta R.T.: 0.000 min
Response: 339187481
Conc: 788.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

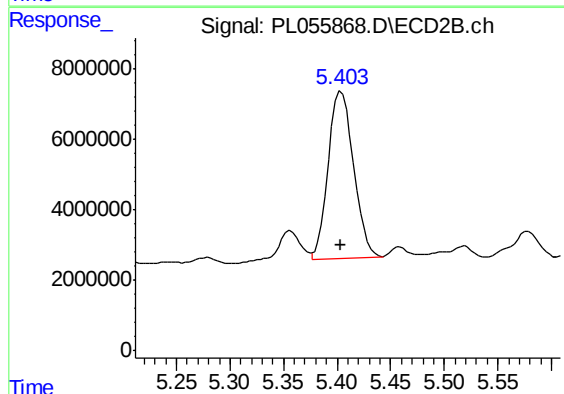


#24 Chlordane-2

R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 78475392
Conc: 739.45 ng/ml

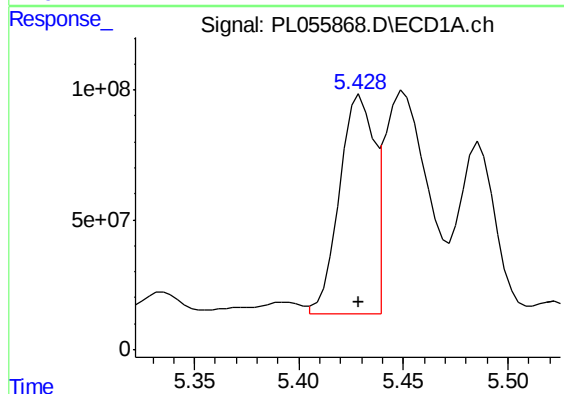


#25 Chlordane-3

R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 960863021
Conc: 746.32 ng/ml

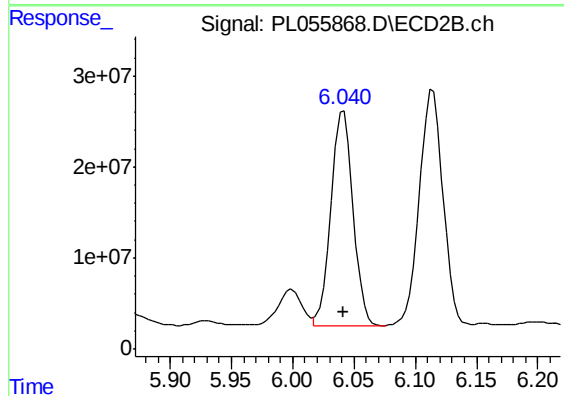

#25 Chlordane-3


R.T.: 6.042 min
Delta R.T.: 0.000 min
Response: 294876883
Conc: 764.91 ng/ml

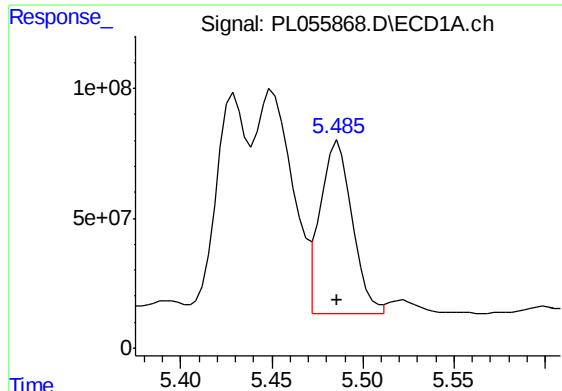

#26 Chlordane-4


R.T.: 5.486 min
Delta R.T.: 0.000 min
Response: 813436325
Conc: 760.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

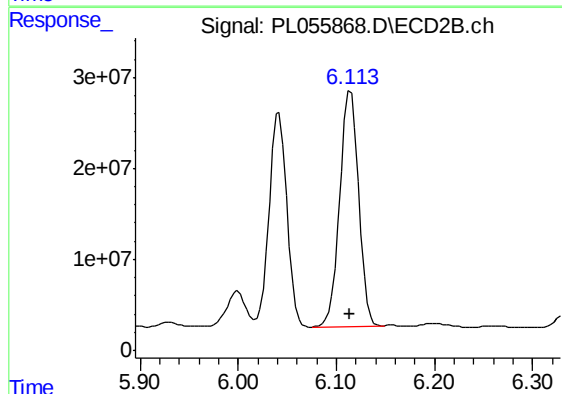


#26 Chlordane-4

R.T.: 6.114 min
Delta R.T.: 0.000 min
Response: 343751251
Conc: 760.53 ng/ml

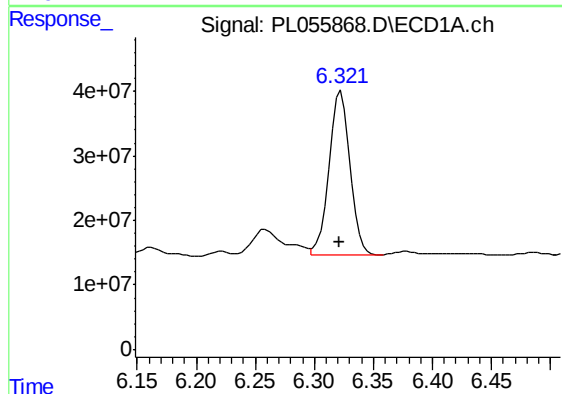


#27 Chlordane-5

R.T.: 6.322 min
Delta R.T.: 0.000 min
Response: 317167454
Conc: 877.52 ng/ml

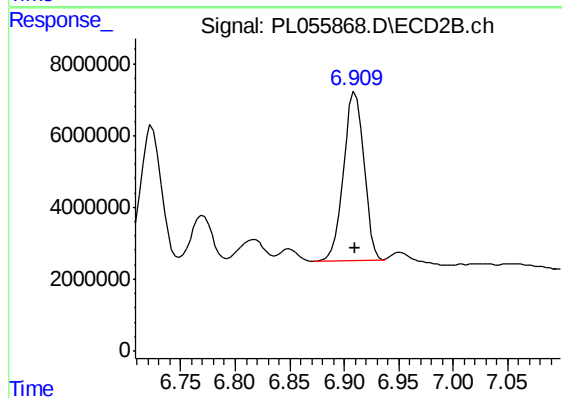

#27 Chlordane-5


R.T.: 6.910 min
Delta R.T.: 0.000 min
Response: 61018805
Conc: 754.43 ng/ml

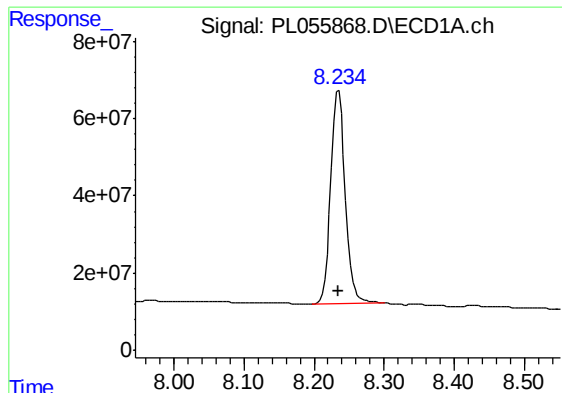

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: 0.000 min
Response: 792189563
Conc: 74.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

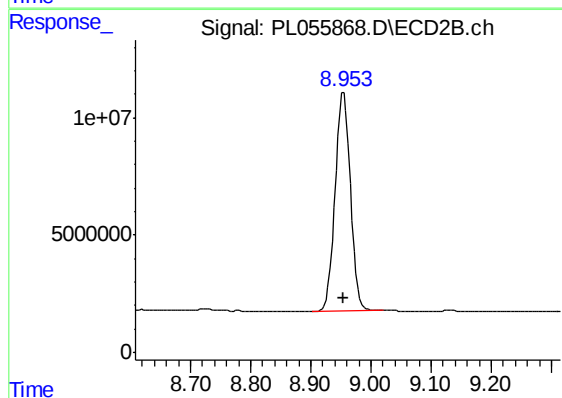

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: 0.001 min
Response: 165743068
Conc: 73.58 ng/ml