

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
 Data File : PL055869.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2020 20:27
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 01:29:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 01:25:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	3.967	549.4E6	141.0E6	50.000	50.000
28)	SA Decachlor...	8.235	8.954	530.9E6	112.6E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.359	4.943	183.9E6	51927619	500.000	500.000
24)	Chlordane-2	4.860	5.403	215.0E6	53063349	500.000	500.000
25)	Chlordane-3	5.428	6.041	643.7E6	192.8E6	500.000	500.000
26)	Chlordane-4	5.486	6.114	534.9E6	226.0E6	500.000	500.000
27)	Chlordane-5	6.322	6.910	180.7E6	40440569	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
Data File : PL055869.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2020 20:27
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 01:29:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 01:25:20 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

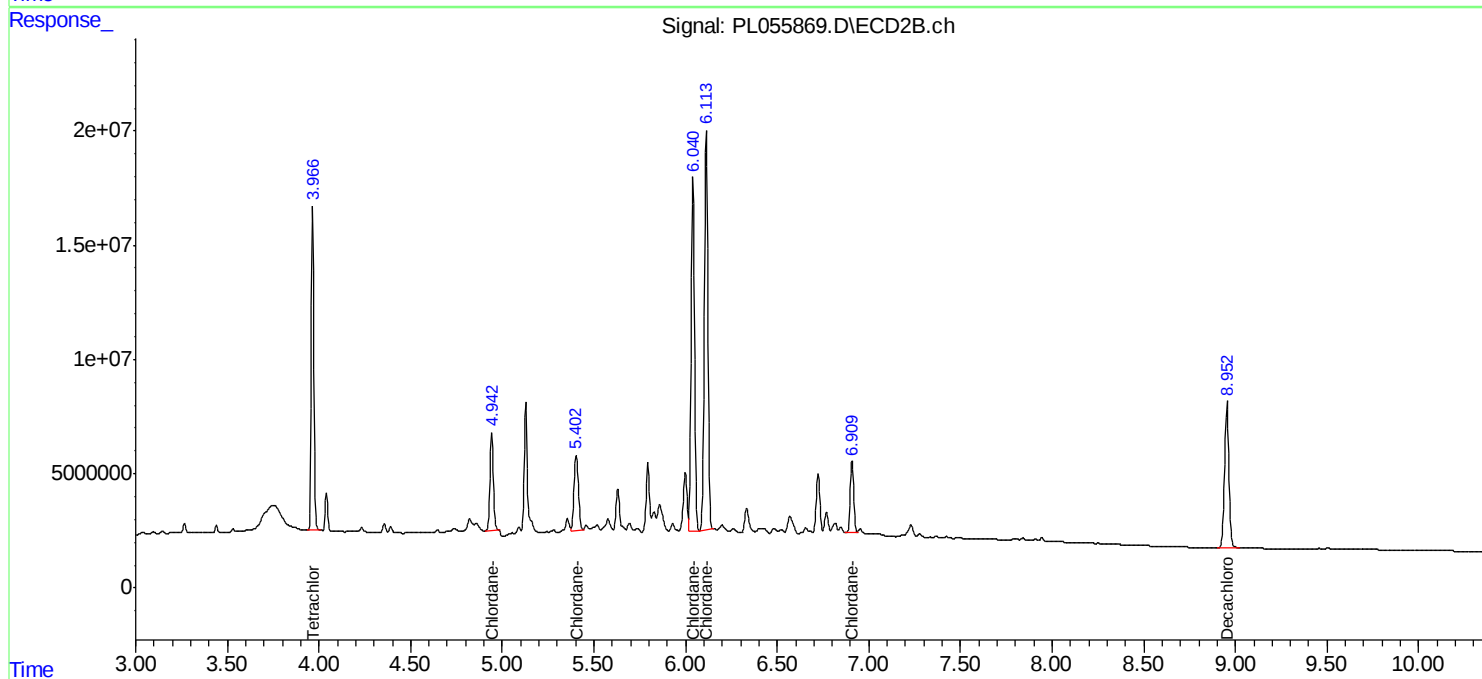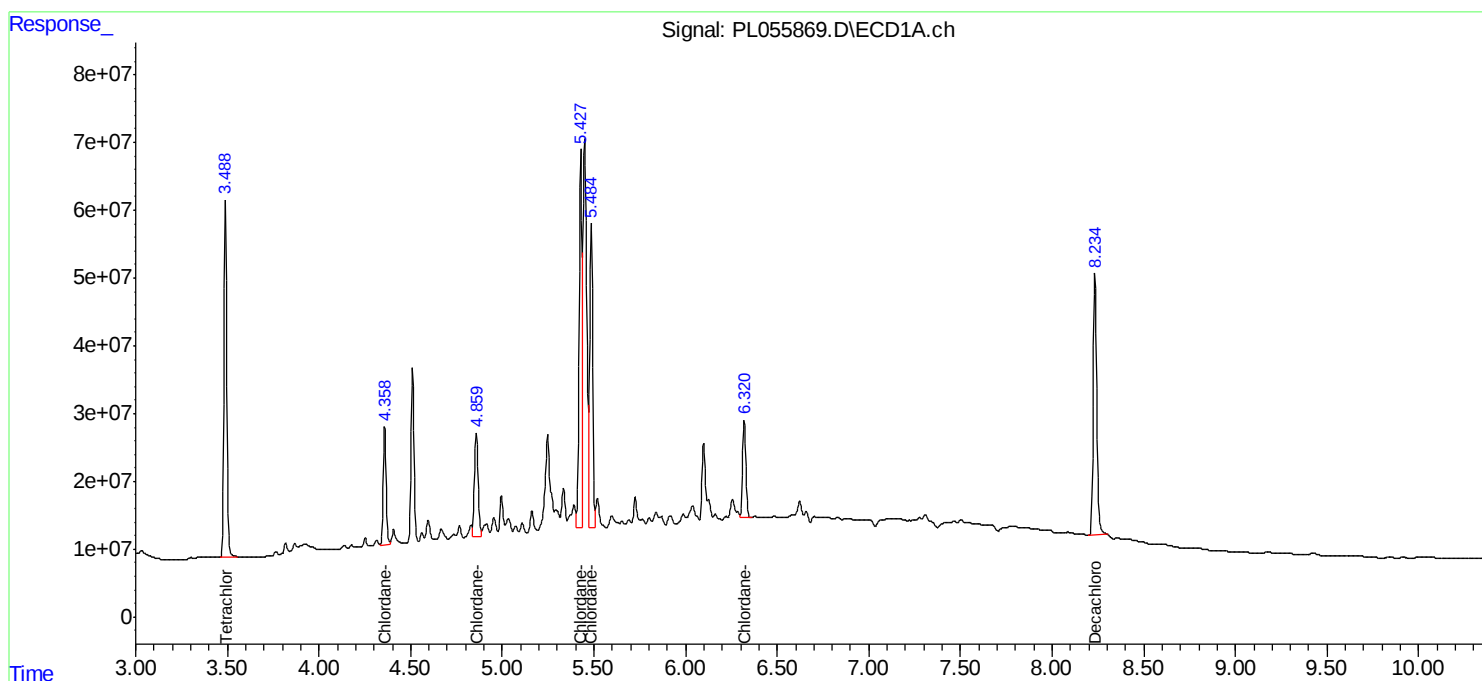


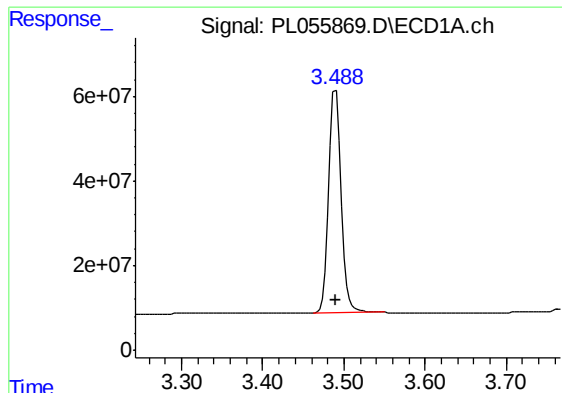

#1 Tetrachloro-m-xylene


R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 549432462
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

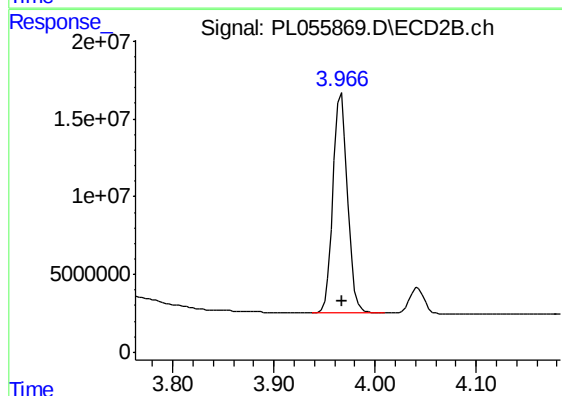


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 141015964
Conc: 50.00 ng/ml

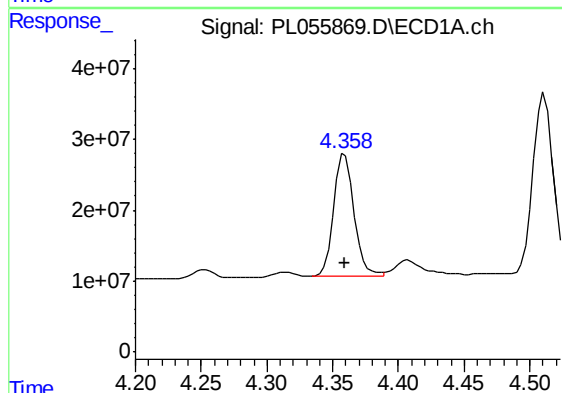


#23 Chlordane-1

R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 183942756
Conc: 500.00 ng/ml

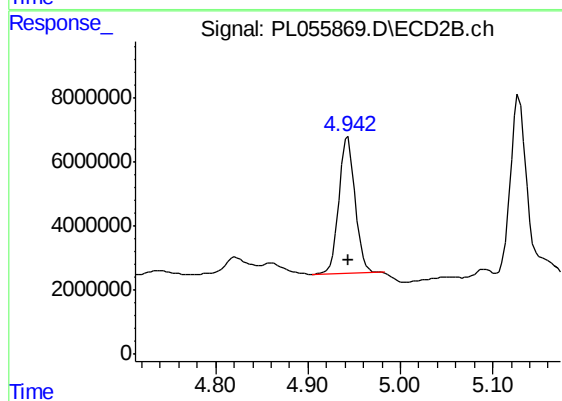

#23 Chlordane-1


R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 51927619
Conc: 500.00 ng/ml

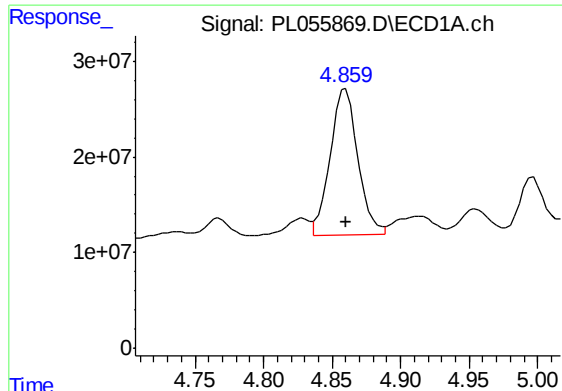

#24 Chlordane-2


R.T.: 4.860 min
Delta R.T.: 0.000 min
Response: 214969471
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

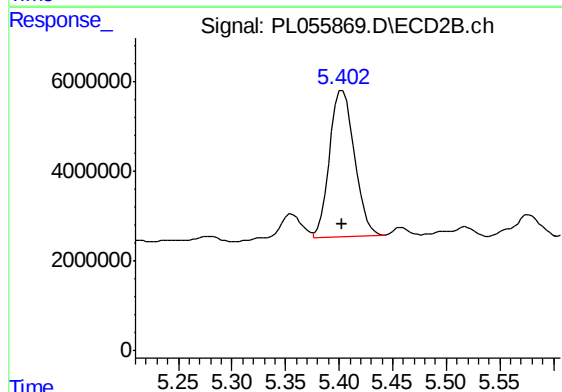


#24 Chlordane-2

R.T.: 5.403 min
Delta R.T.: 0.000 min
Response: 53063349
Conc: 500.00 ng/ml

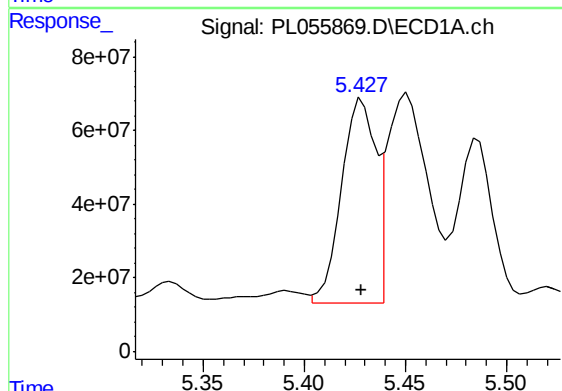


#25 Chlordane-3

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 643732679
Conc: 500.00 ng/ml

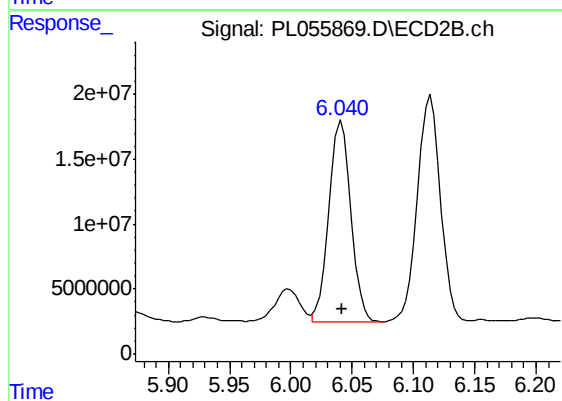

#25 Chlordane-3


R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 192751685
Conc: 500.00 ng/ml

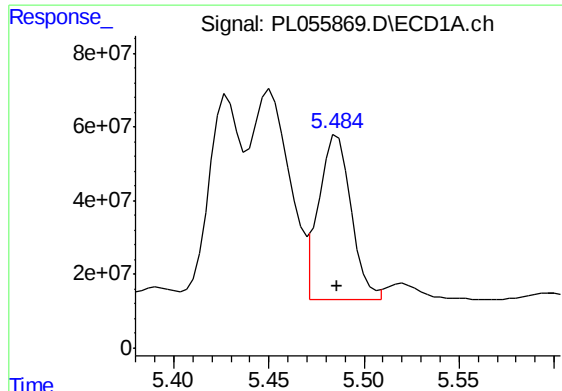

#26 Chlordane-4


R.T.: 5.486 min
Delta R.T.: 0.000 min
Response: 534880913
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

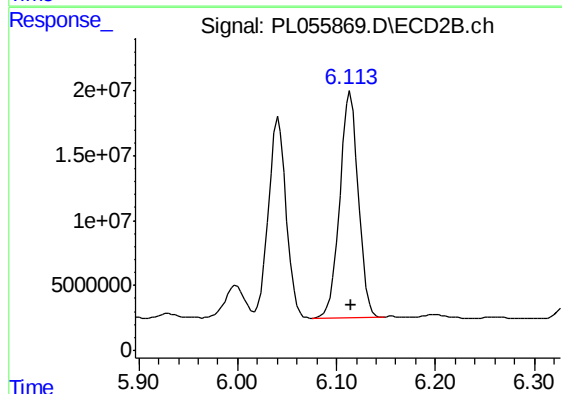


#26 Chlordane-4

R.T.: 6.114 min
Delta R.T.: 0.000 min
Response: 225994245
Conc: 500.00 ng/ml

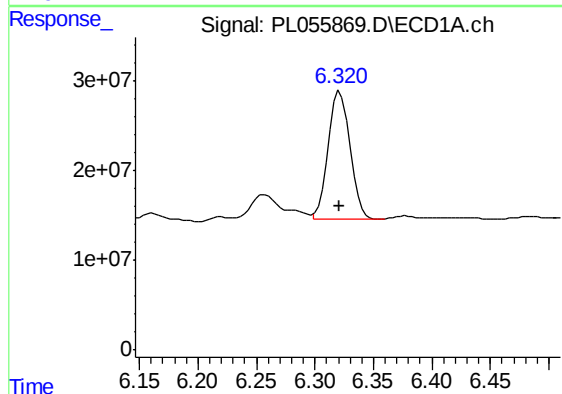


#27 Chlordane-5

R.T.: 6.322 min
Delta R.T.: 0.000 min
Response: 180718595
Conc: 500.00 ng/ml

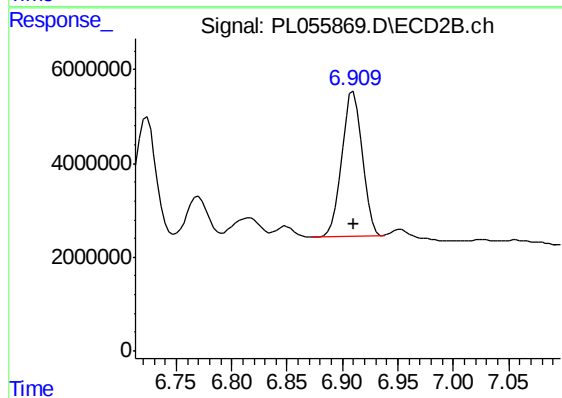

#27 Chlordane-5


R.T.: 6.910 min
Delta R.T.: 0.000 min
Response: 40440569
Conc: 500.00 ng/ml

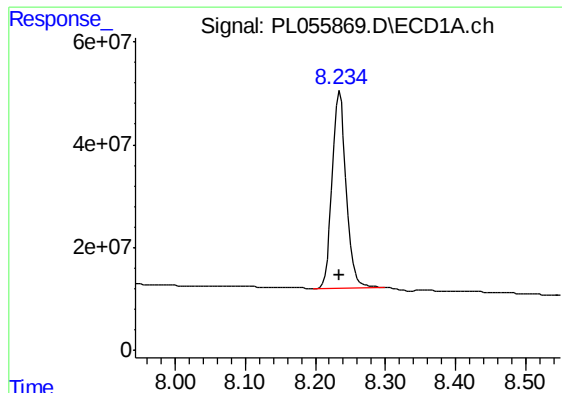

#28 Decachlorobiphenyl

R.T.: 8.235 min
Delta R.T.: 0.000 min
Response: 530937208
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

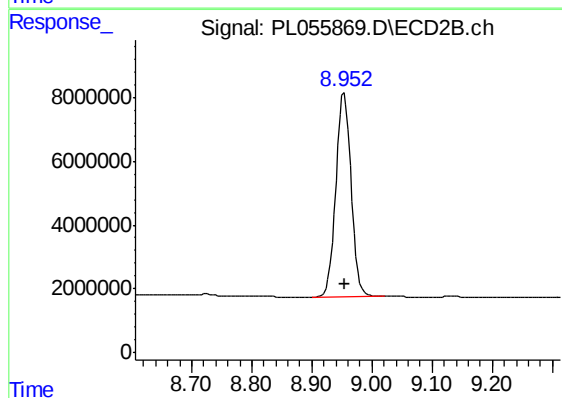

#28 Decachlorobiphenyl

R.T.: 8.954 min
Delta R.T.: 0.000 min
Response: 112635160
Conc: 50.00 ng/ml