

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
 Data File : PL055904.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 04:41
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 06:42:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	3.967	195.6E6	59554671	20.409	21.072
28)	SA Decachlor...	8.234	8.952	221.3E6	49707966	21.164	21.697
Target Compounds							
2)	A alpha-BHC	3.927	0.000	12521337	0	0.755	N.D. #
6)	B beta-BHC	4.480f	0.000	852574	0	0.133	N.D. #
9)	A Endosulfan I	5.544	0.000	5251372	0	0.405	N.D. #
11)	B alpha-Chl...	5.479	0.000	35661074	0	2.580	N.D. #
14)	MA Endrin	6.048	6.634	4025017	1972298	0.319	0.778 #
18)	B Endrin al...	6.485	0.000	6053637	0	0.582	N.D. #
24)	Chlordane-2	4.883f	0.000	44093528	0	101.892	N.D. #
26)	Chlordane-4	5.479	0.000	35661074	0	34.584	N.D. #
27)	Chlordane-5	6.348f	0.000	2503631	0	6.401	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
Data File : PL055904.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 04:41
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 06:42:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

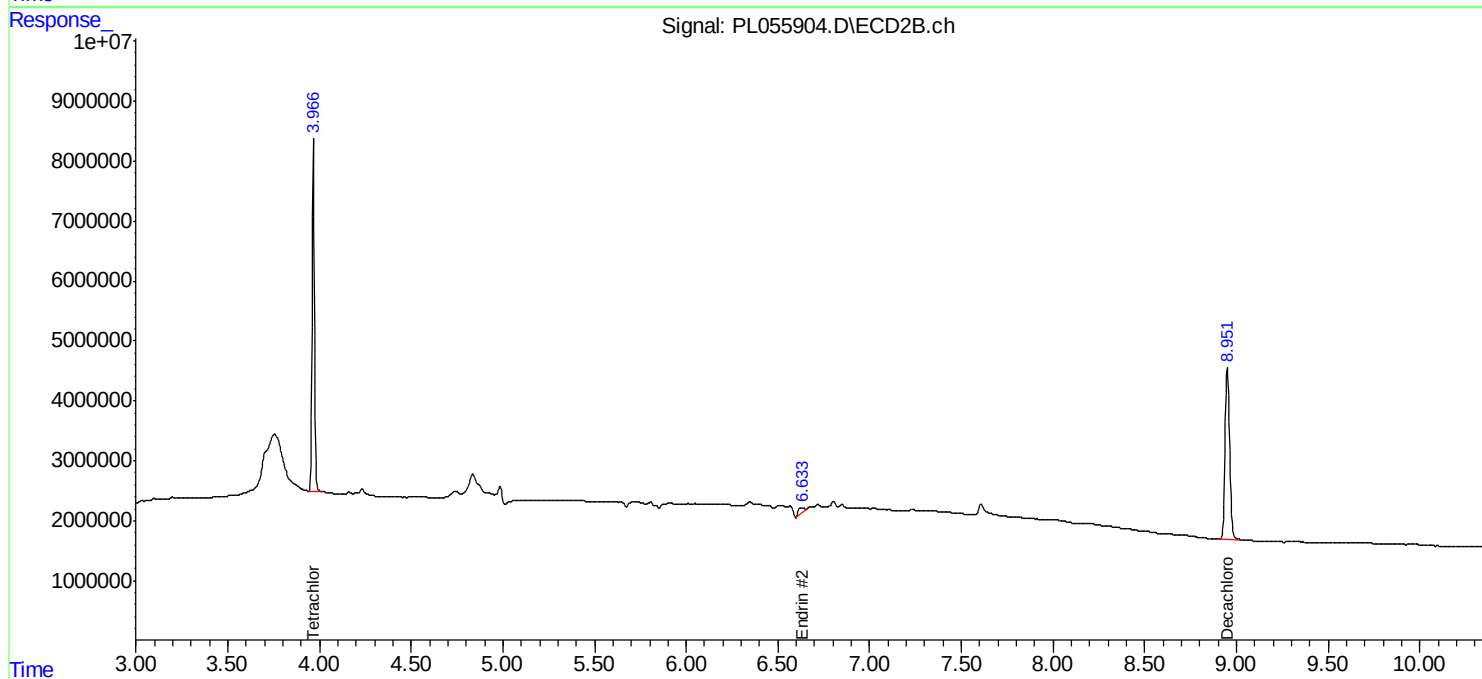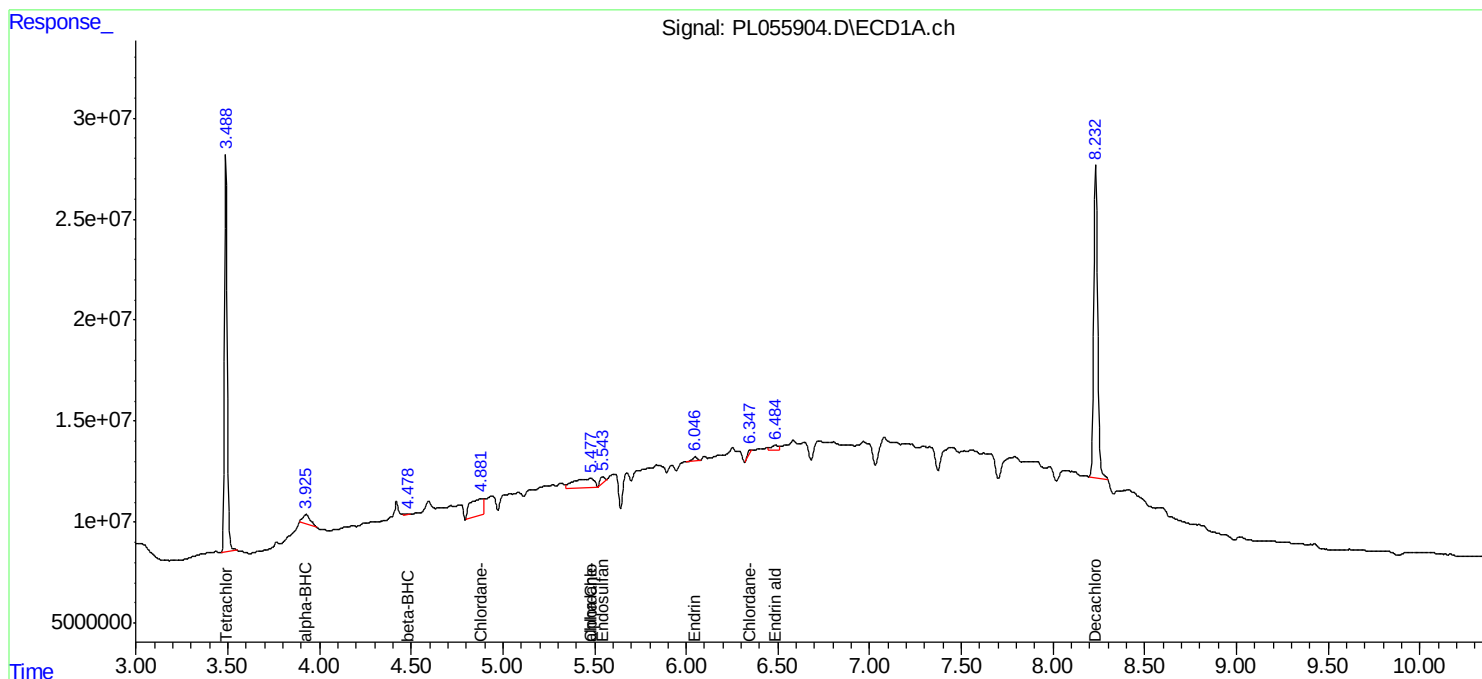


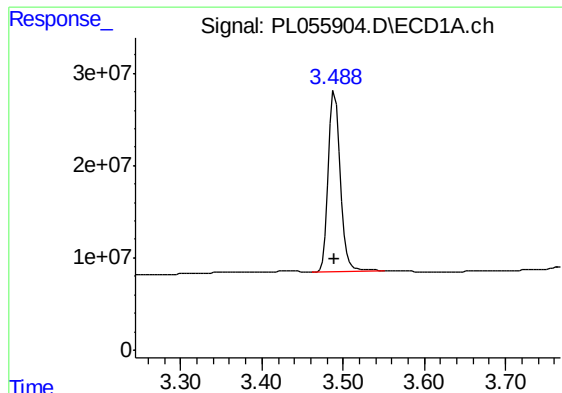

#1 Tetrachloro-m-xylene


R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 195607790
Conc: 20.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

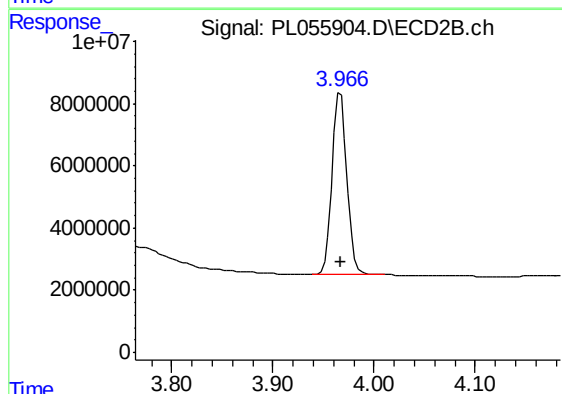


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 59554671
Conc: 21.07 ng/ml

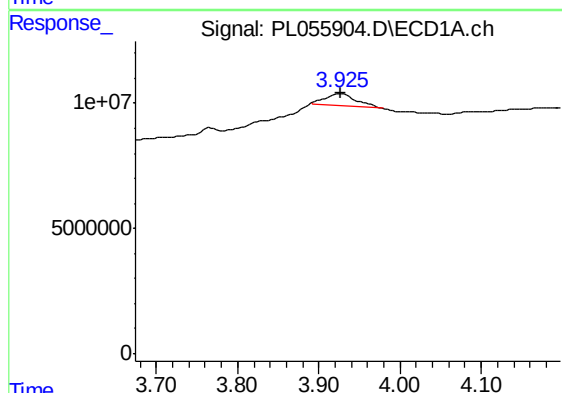


#2 alpha-BHC

R.T.: 3.927 min
Delta R.T.: 0.000 min
Response: 12521337
Conc: 0.75 ng/ml

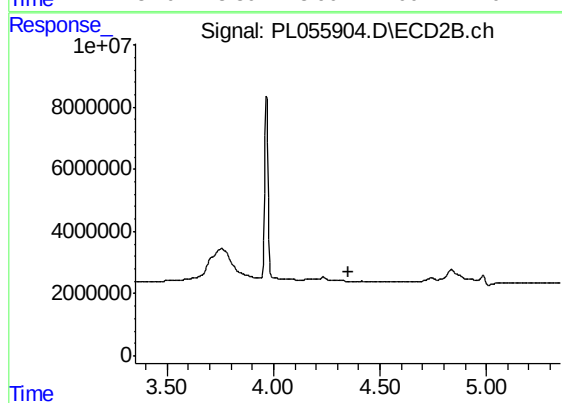

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.350 min
Response: 0
Conc: N.D.

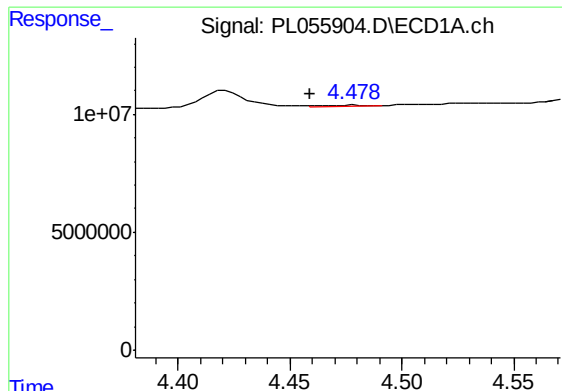

#6 beta-BHC


R.T.: 4.480 min
Delta R.T.: 0.021 min
Response: 852574
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

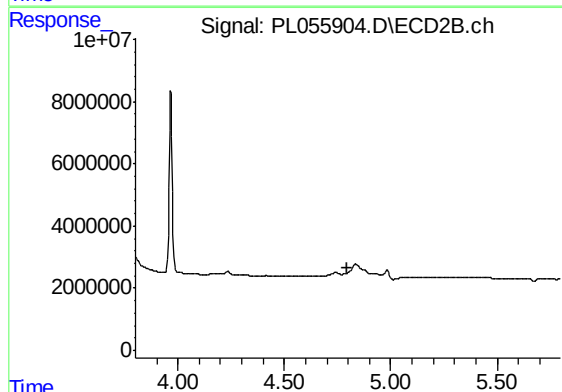


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.798 min
Response: 0
Conc: N.D.

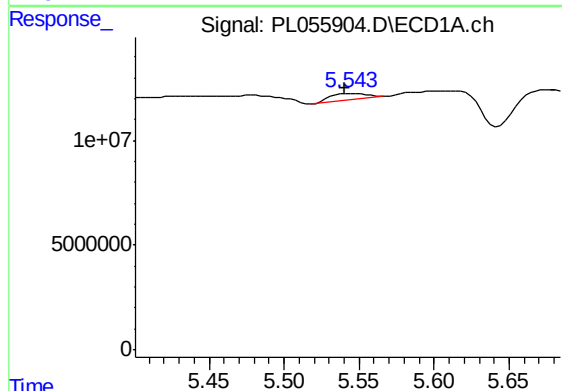


#9 Endosulfan I

R.T.: 5.544 min
Delta R.T.: 0.004 min
Response: 5251372
Conc: 0.40 ng/ml

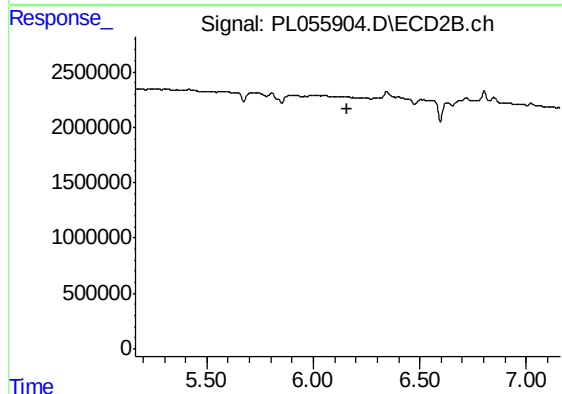

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

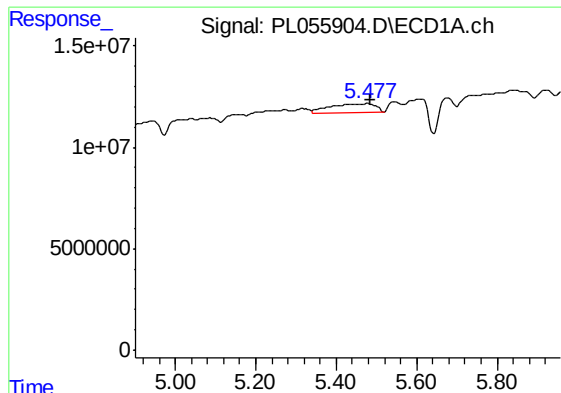

#11 alpha-Chlordane


R.T.: 5.479 min
Delta R.T.: -0.008 min
Response: 35661074
Conc: 2.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

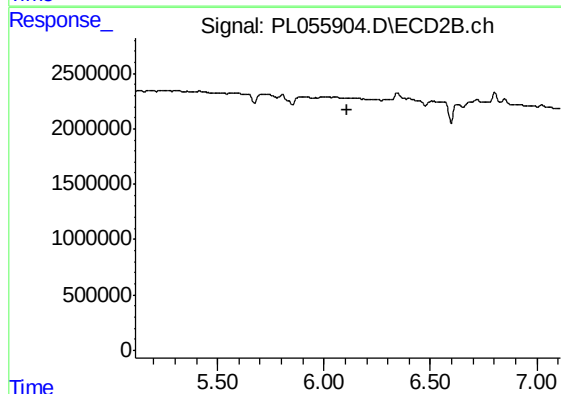


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

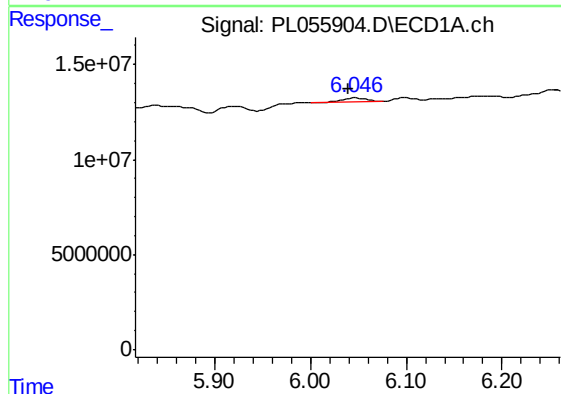


#14 Endrin

R.T.: 6.048 min
Delta R.T.: 0.007 min
Response: 4025017
Conc: 0.32 ng/ml

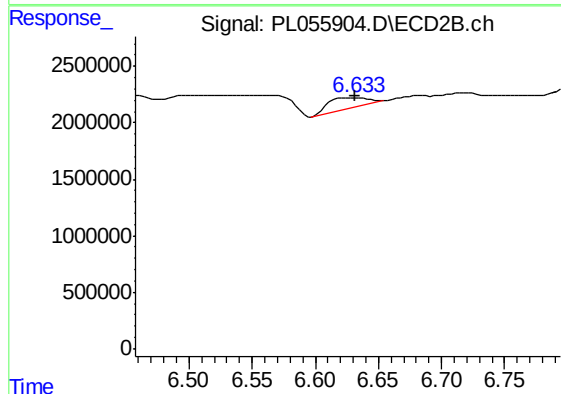

#14 Endrin


R.T.: 6.634 min
Delta R.T.: 0.002 min
Response: 1972298
Conc: 0.78 ng/ml

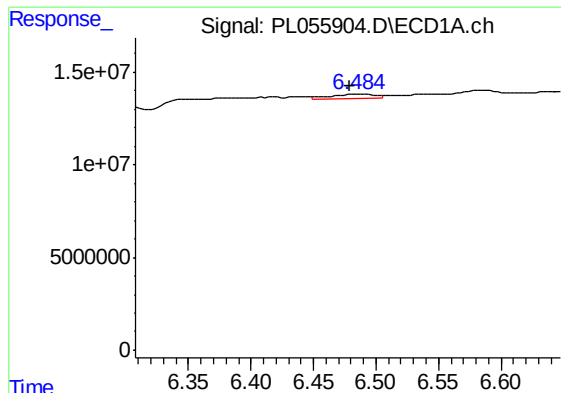

#18 Endrin aldehyde


R.T.: 6.485 min
Delta R.T.: 0.006 min
Response: 6053637
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

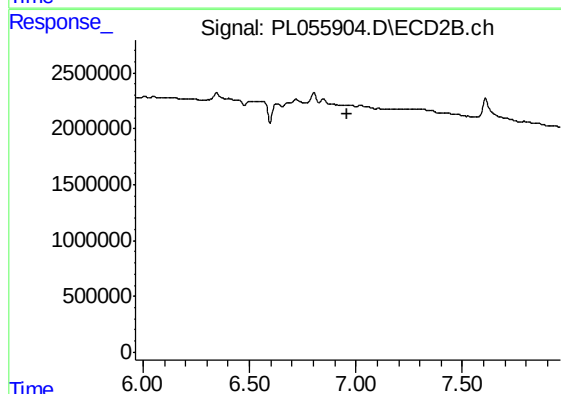


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.962 min
Response: 0
Conc: N.D.

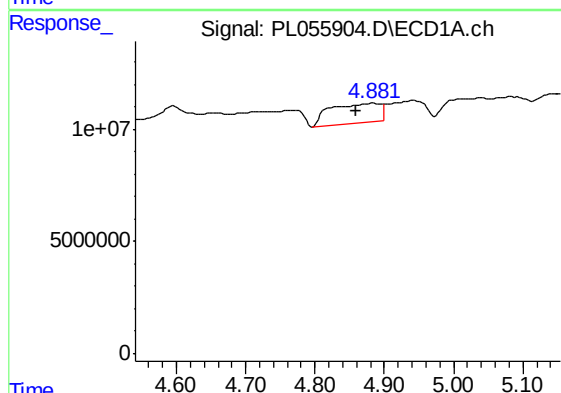


#24 Chlordane-2

R.T.: 4.883 min
Delta R.T.: 0.023 min
Response: 44093528
Conc: 101.89 ng/ml

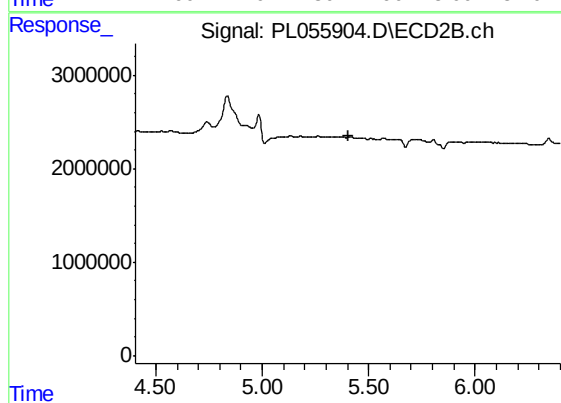

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.403 min
Response: 0
Conc: N.D.

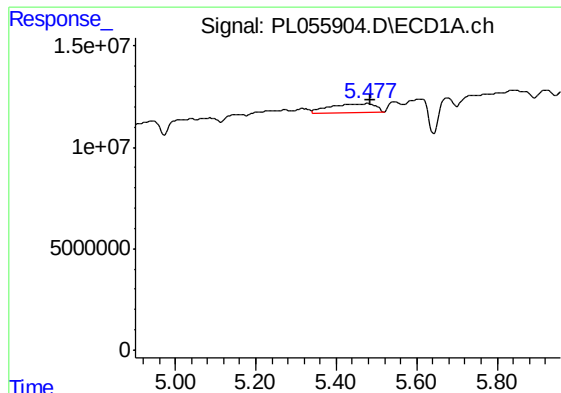

#26 Chlordane-4


R.T.: 5.479 min
Delta R.T.: -0.007 min
Response: 35661074
Conc: 34.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

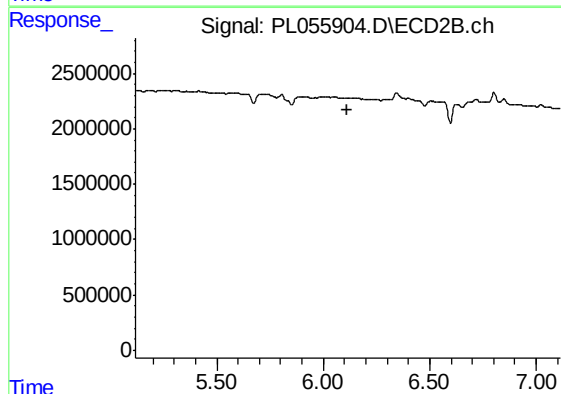


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

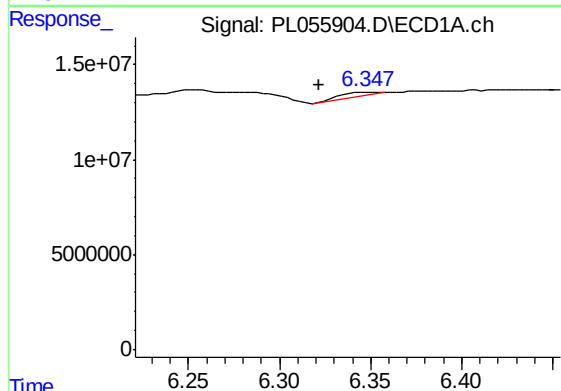


#27 Chlordane-5

R.T.: 6.348 min
Delta R.T.: 0.027 min
Response: 2503631
Conc: 6.40 ng/ml

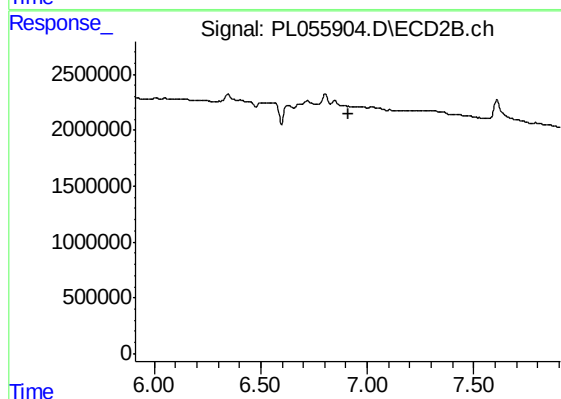

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.910 min
Response: 0
Conc: N.D.

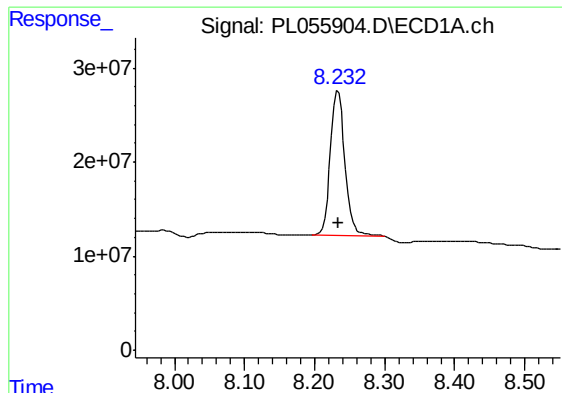

#28 Decachlorobiphenyl

R.T.: 8.234 min
Delta R.T.: 0.000 min
Response: 221282029
Conc: 21.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

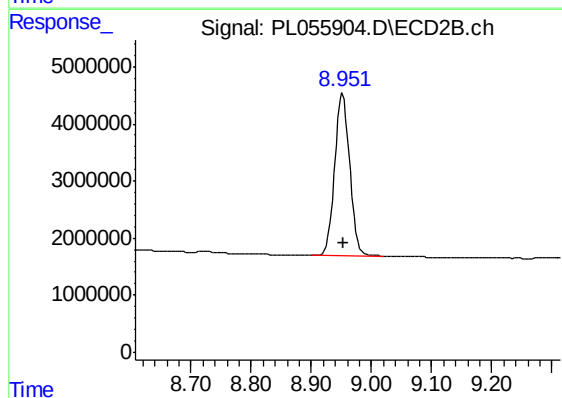

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: 0.000 min
Response: 49707966
Conc: 21.70 ng/ml