

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
 Data File : PL055907.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 05:23
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 06:43:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	3.966	202.7E6	61583406	21.150	21.790
28)	SA Decachlor...	8.234	8.951	230.4E6	50876054	22.033	22.207
Target Compounds							
2)	A alpha-BHC	3.925	0.000	13090147	0	0.789	N.D. #
4)	MA Heptachlor	4.540f	0.000	2324286	0	0.156	N.D. #
9)	A Endosulfan I	5.548	0.000	6375135	0	0.491	N.D. #
11)	B alpha-Chl...	5.475	0.000	54606720	0	3.950	N.D. #
14)	MA Endrin	6.046	6.625	4919744	2744881	0.389	1.083 #
18)	B Endrin al...	6.481	0.000	1079413	0	0.104	N.D. #
26)	Chlordane-4	5.475	0.000	54606720	0	52.957	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
Data File : PL055907.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 05:23
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 06:43:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

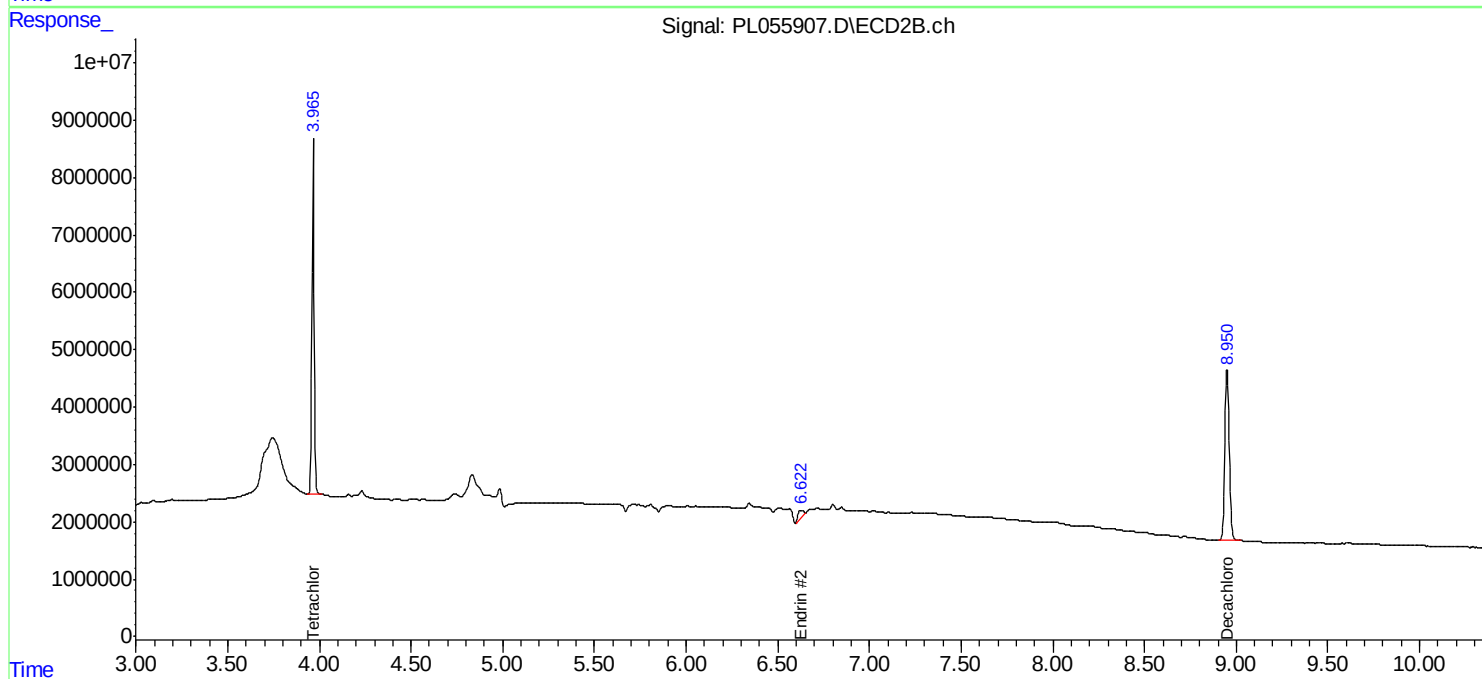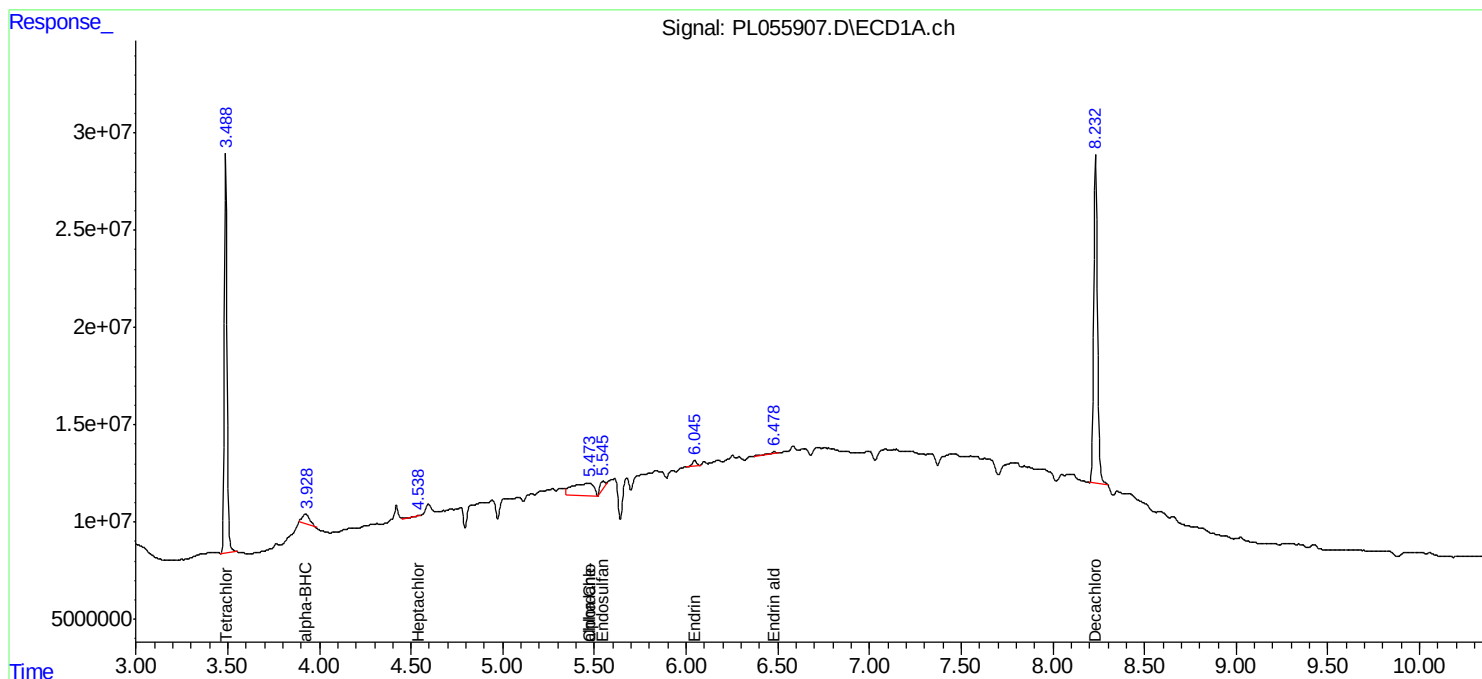


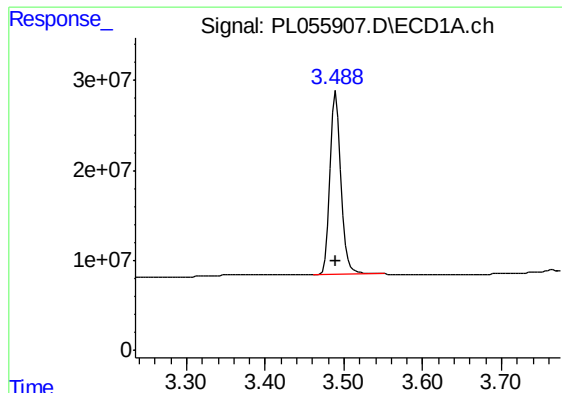

#1 Tetrachloro-m-xylene


R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 202707314
Conc: 21.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

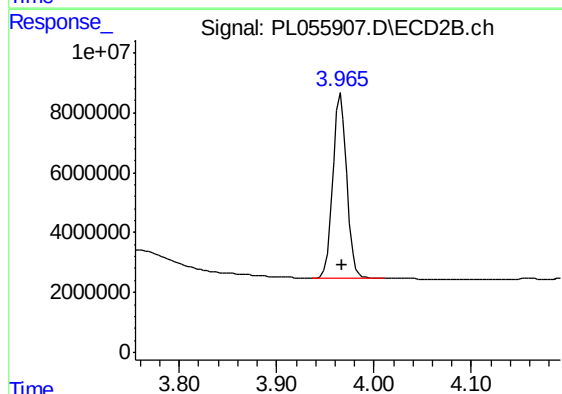


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 61583406
Conc: 21.79 ng/ml

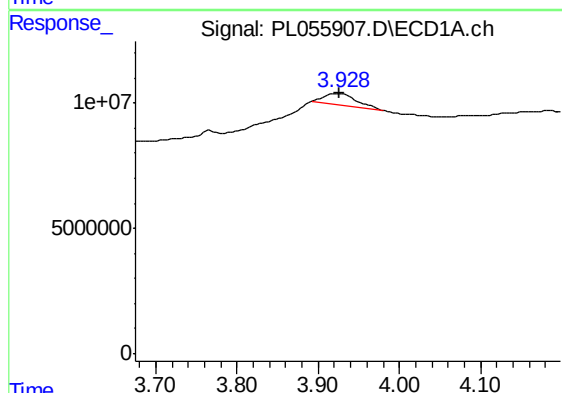


#2 alpha-BHC

R.T.: 3.925 min
Delta R.T.: -0.002 min
Response: 13090147
Conc: 0.79 ng/ml

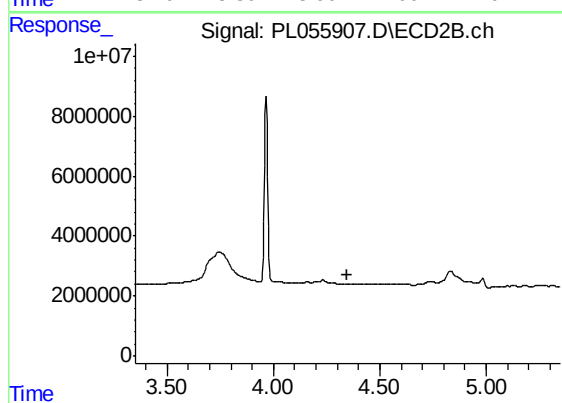

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.350 min
Response: 0
Conc: N.D.

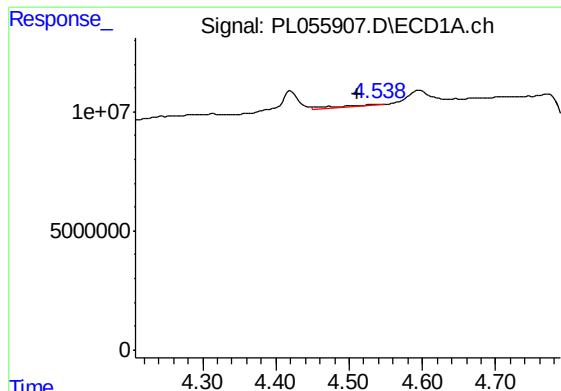

#4 Heptachlor


R.T.: 4.540 min
Delta R.T.: 0.029 min
Response: 2324286
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

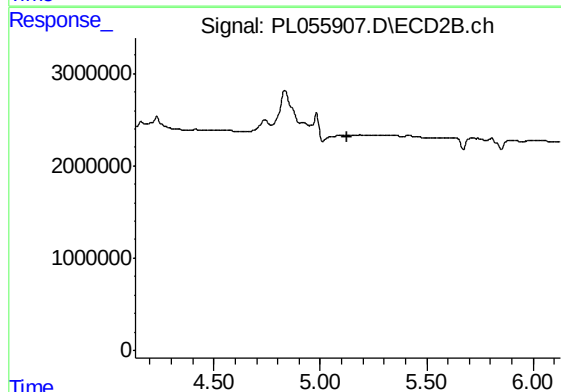


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.129 min
Response: 0
Conc: N.D.

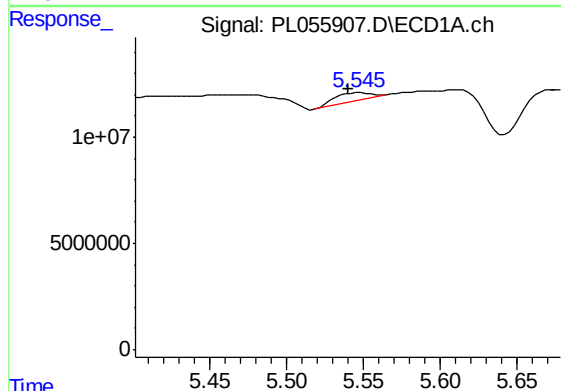


#9 Endosulfan I

R.T.: 5.548 min
Delta R.T.: 0.007 min
Response: 6375135
Conc: 0.49 ng/ml

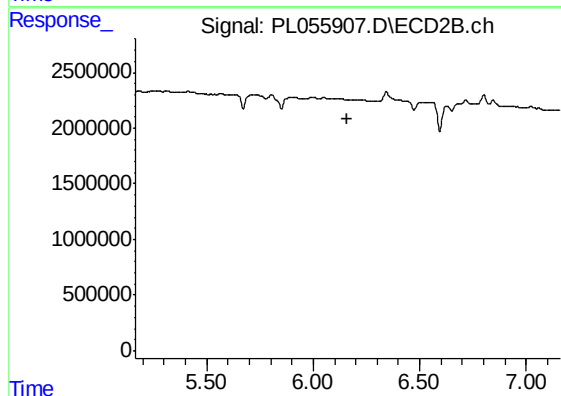

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

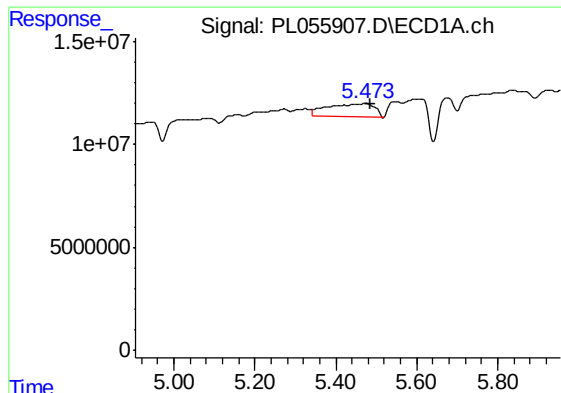

#11 alpha-Chlordane


R.T.: 5.475 min
Delta R.T.: -0.012 min
Response: 54606720
Conc: 3.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

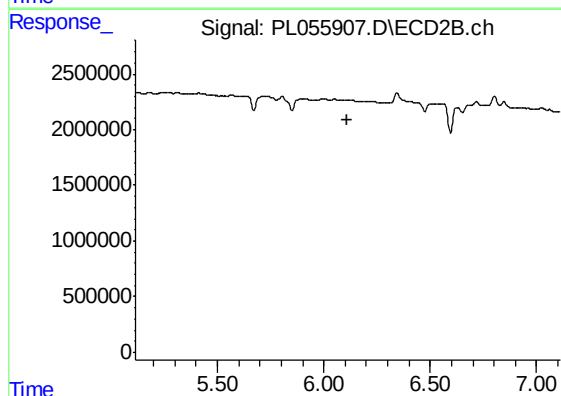


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

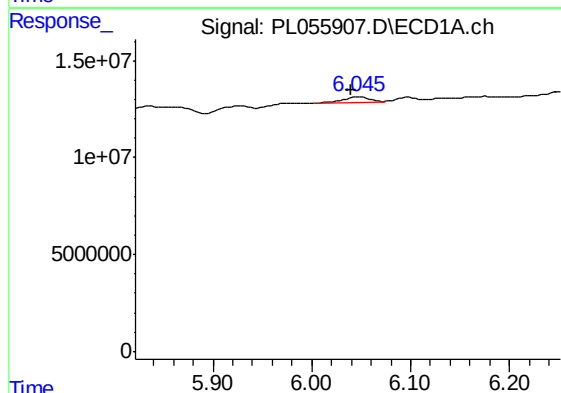


#14 Endrin

R.T.: 6.046 min
Delta R.T.: 0.006 min
Response: 4919744
Conc: 0.39 ng/ml

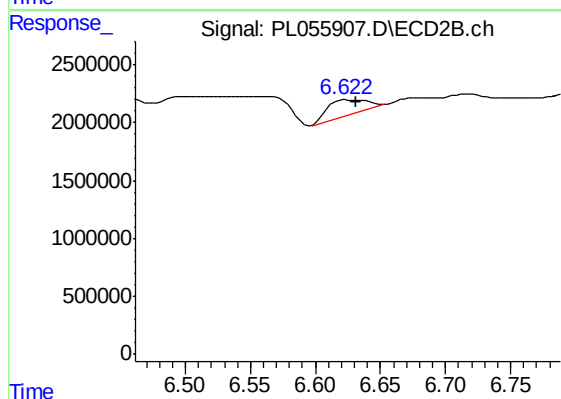

#14 Endrin


R.T.: 6.625 min
Delta R.T.: -0.006 min
Response: 2744881
Conc: 1.08 ng/ml

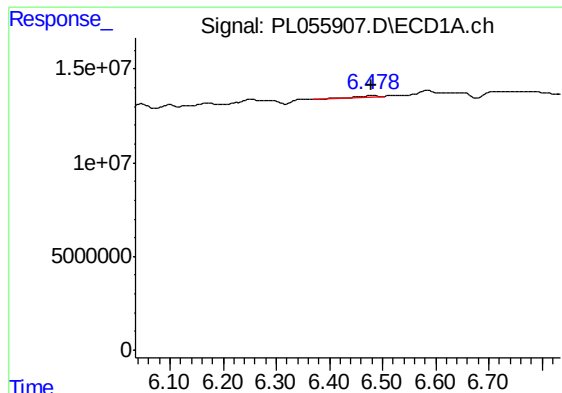

#18 Endrin aldehyde


R.T.: 6.481 min
Delta R.T.: 0.001 min
Response: 1079413
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

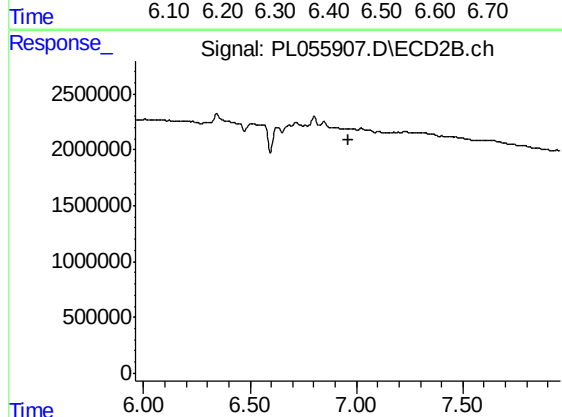


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.962 min
Response: 0
Conc: N.D.

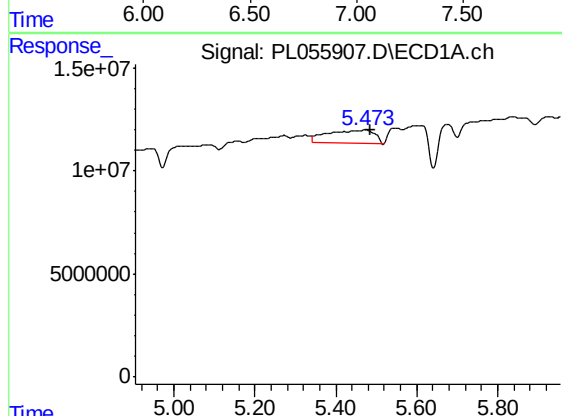


#26 Chlordane-4

R.T.: 5.475 min
Delta R.T.: -0.011 min
Response: 54606720
Conc: 52.96 ng/ml

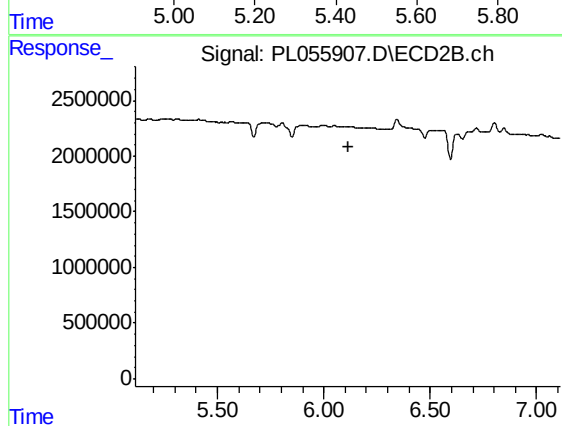

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

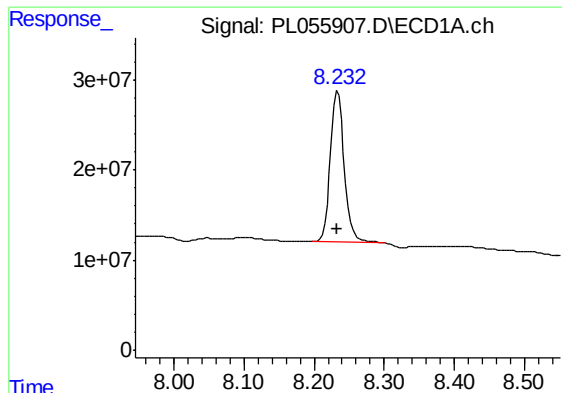

#28 Decachlorobiphenyl

R.T.: 8.234 min
Delta R.T.: 0.000 min
Response: 230373970
Conc: 22.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

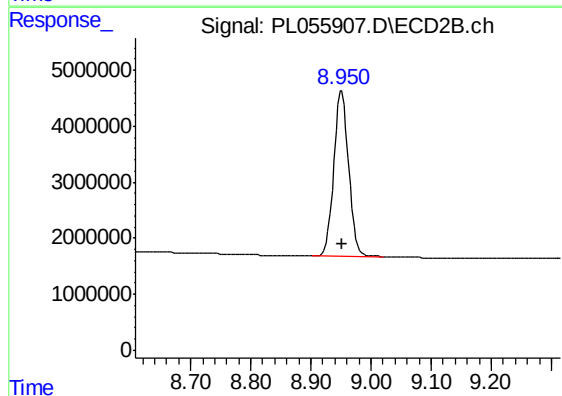

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: -0.001 min
Response: 50876054
Conc: 22.21 ng/ml