

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
 Data File : PL055927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 10:48
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 11:01:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	3.965	203.4E6	61349363	21.220	21.707
28)	SA Decachlor...	8.234	8.952	208.9E6	48051244	19.979	20.974
Target Compounds							
6)	B beta-BHC	0.000	4.828f	0	8728580	N.D.	5.500 #
9)	A Endosulfan I	5.548	0.000	7155177	0	0.551	N.D. #
10)	B gamma-Chl...	5.446f	0.000	41066795	0	2.927	N.D. #
11)	B alpha-Chl...	5.471f	0.000	21532908	0	1.558	N.D. #
14)	MA Endrin	6.045	6.627	5488510	2908516	0.434	1.148 #
18)	B Endrin al...	6.490	0.000	5247746	0	0.505	N.D. #
24)	Chlordane-2	4.883f	0.000	66944801	0	154.698	N.D. #
25)	Chlordane-3	5.446f	0.000	41066795	0	32.978	N.D. #
26)	Chlordane-4	5.471	0.000	21532908	0	20.882	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
Data File : PL055927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 10:48
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 11:01:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

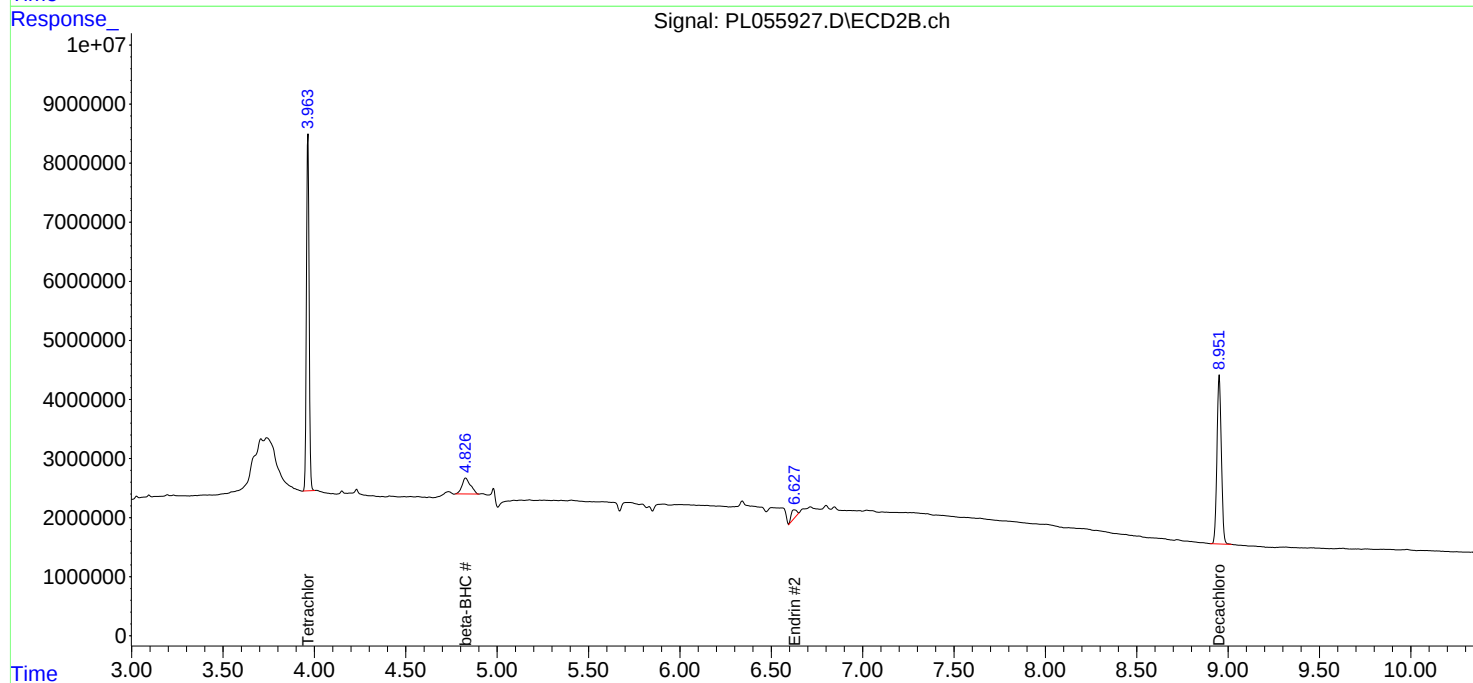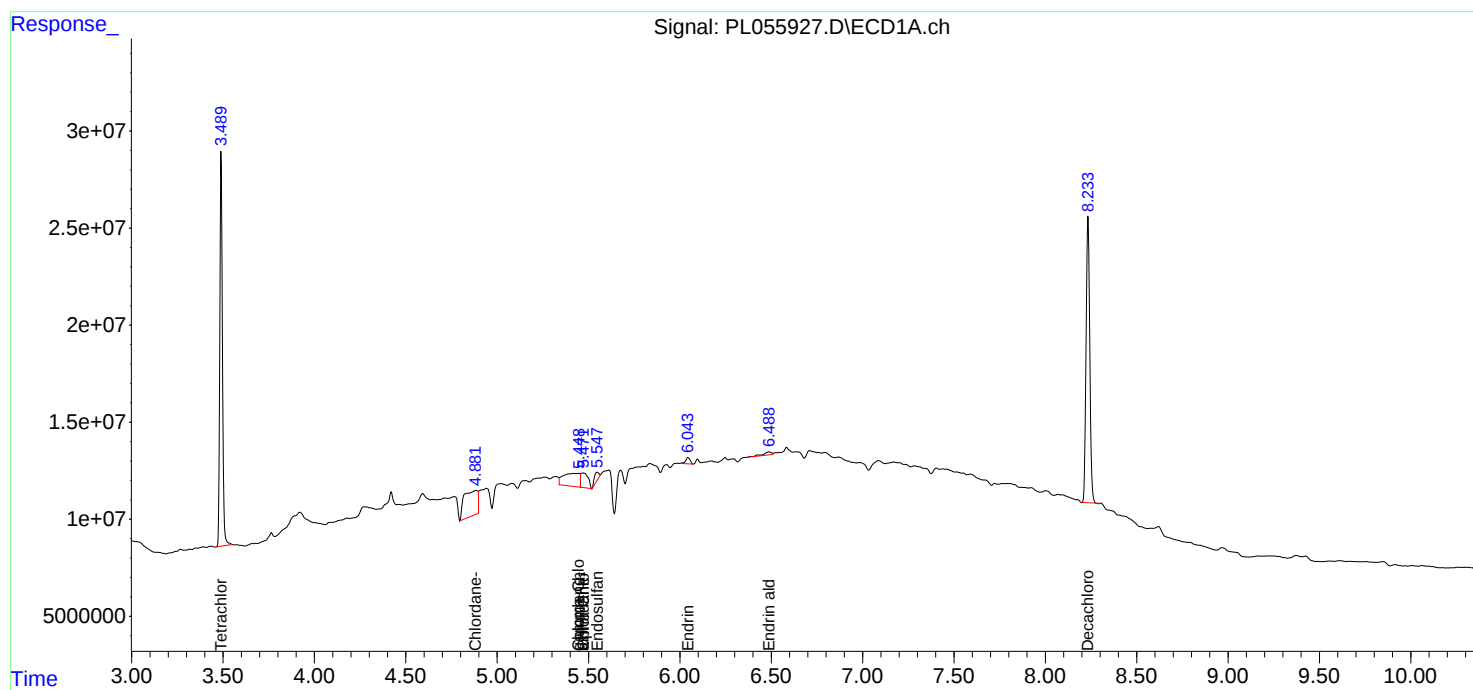


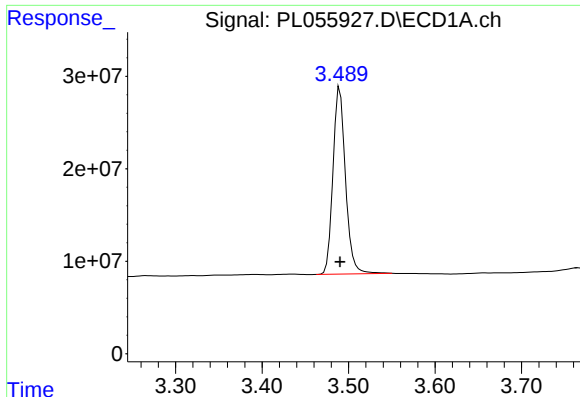

#1 Tetrachloro-m-xylene


R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 203381808
Conc: 21.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

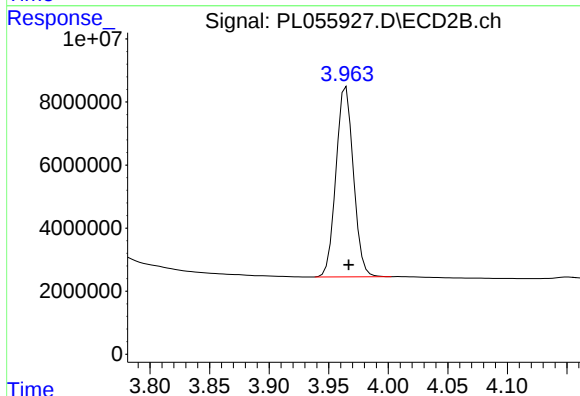


#1 Tetrachloro-m-xylene

R.T.: 3.965 min
Delta R.T.: -0.002 min
Response: 61349363
Conc: 21.71 ng/ml

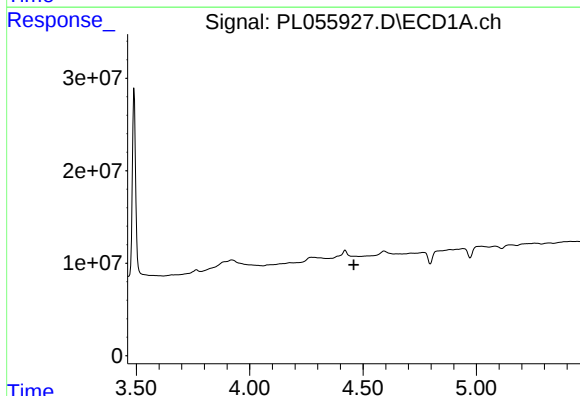


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.459 min
Response: 0
Conc: N.D.

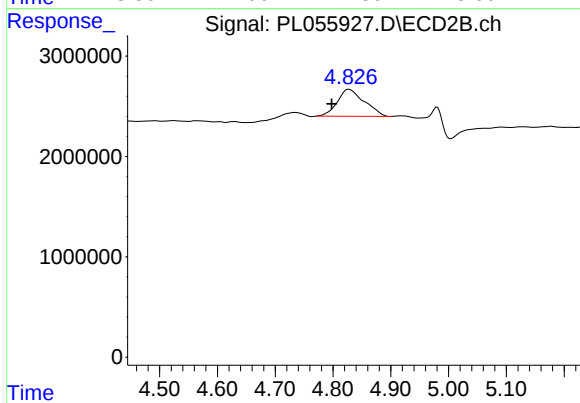

#6 beta-BHC


R.T.: 4.828 min
Delta R.T.: 0.030 min
Response: 8728580
Conc: 5.50 ng/ml

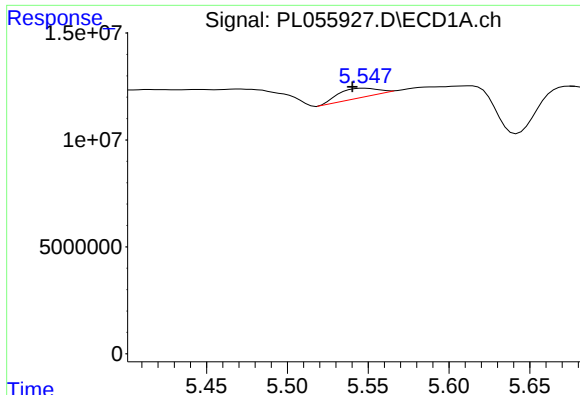

#9 Endosulfan I


R.T.: 5.548 min
Delta R.T.: 0.008 min
Response: 7155177
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

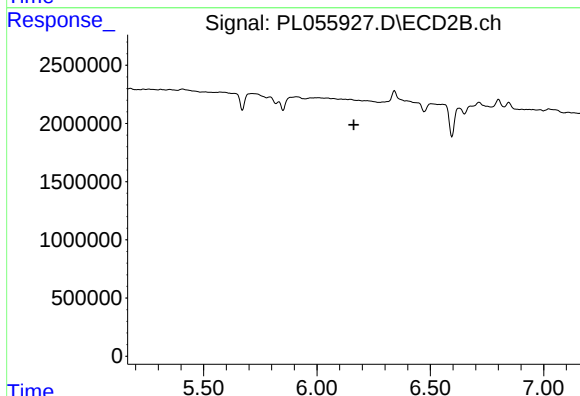


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

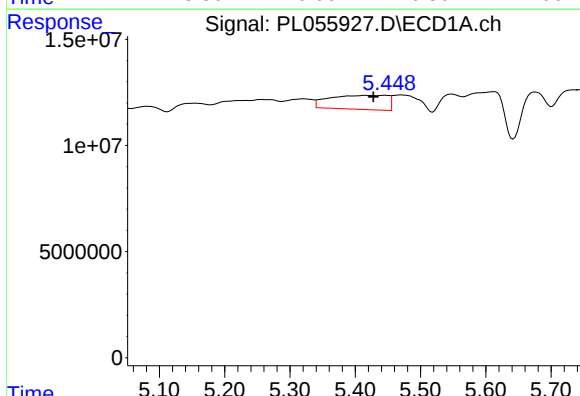


#10 gamma-Chlordane

R.T.: 5.446 min
Delta R.T.: 0.018 min
Response: 41066795
Conc: 2.93 ng/ml

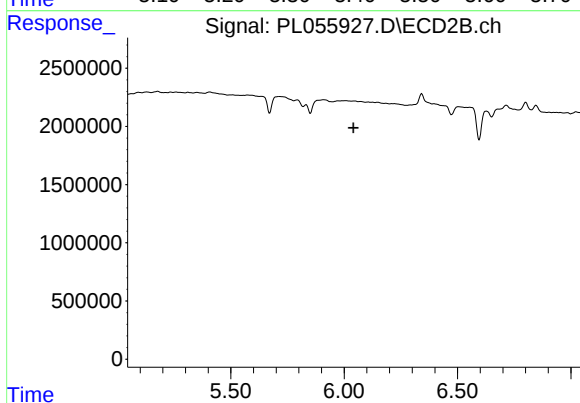

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.041 min
Response: 0
Conc: N.D.

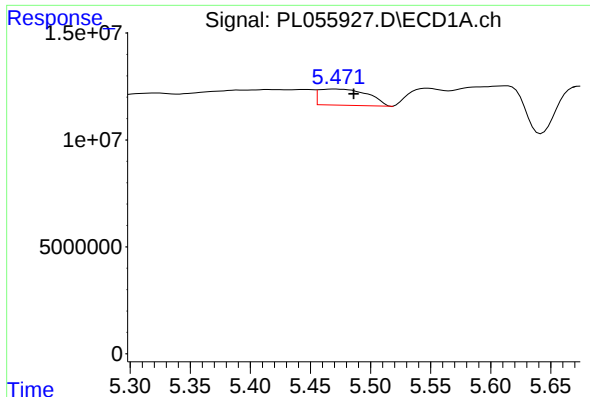

#11 alpha-Chlordane


R.T.: 5.471 min
Delta R.T.: -0.015 min
Response: 21532908
Conc: 1.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

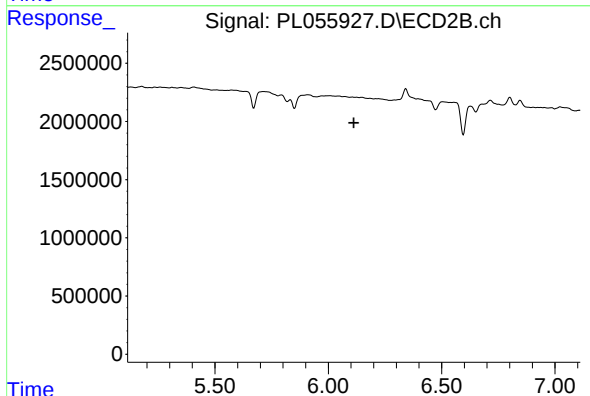


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

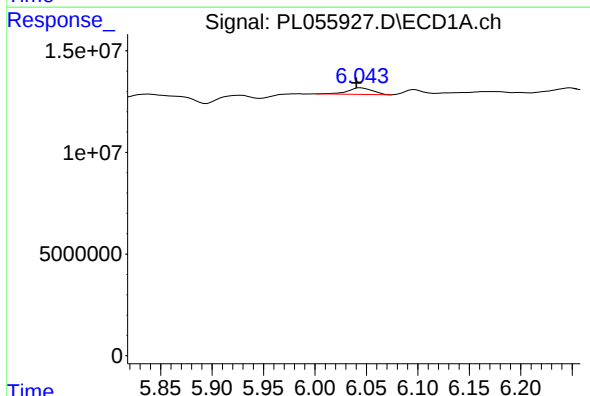


#14 Endrin

R.T.: 6.045 min
Delta R.T.: 0.004 min
Response: 5488510
Conc: 0.43 ng/ml

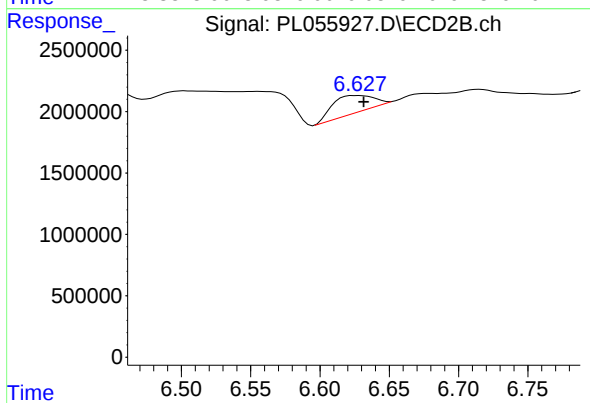

#14 Endrin


R.T.: 6.627 min
Delta R.T.: -0.004 min
Response: 2908516
Conc: 1.15 ng/ml

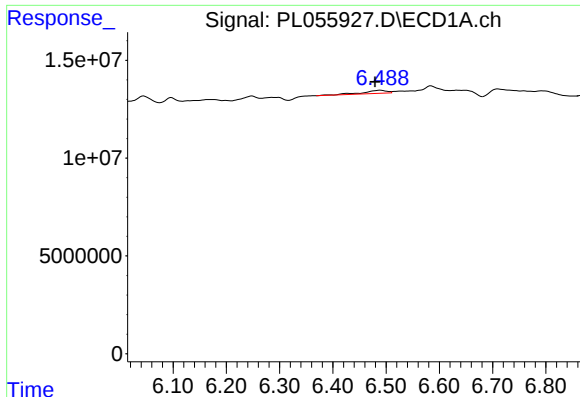

#18 Endrin aldehyde


R.T.: 6.490 min
Delta R.T.: 0.010 min
Response: 5247746
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

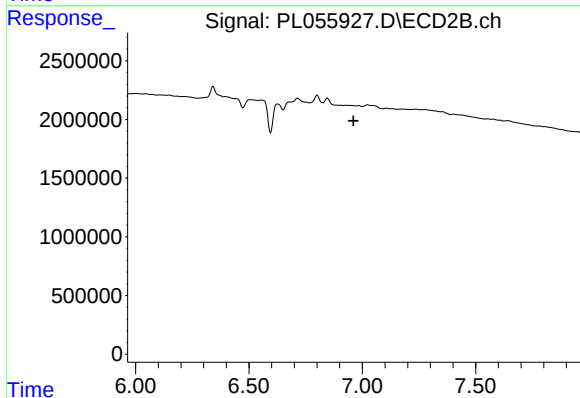


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.962 min
Response: 0
Conc: N.D.

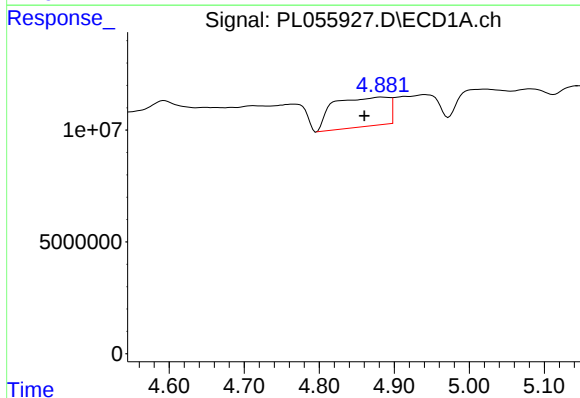


#24 Chlordane-2

R.T.: 4.883 min
Delta R.T.: 0.023 min
Response: 66944801
Conc: 154.70 ng/ml

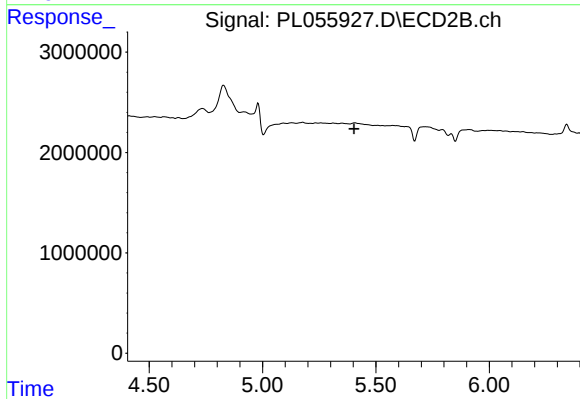

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.403 min
Response: 0
Conc: N.D.

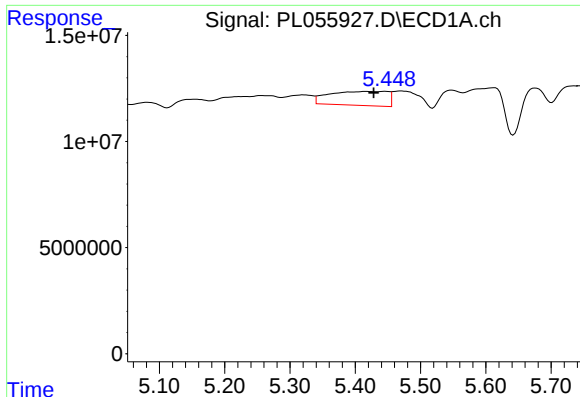

#25 Chlordane-3


R.T.: 5.446 min
Delta R.T.: 0.017 min
Response: 41066795
Conc: 32.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

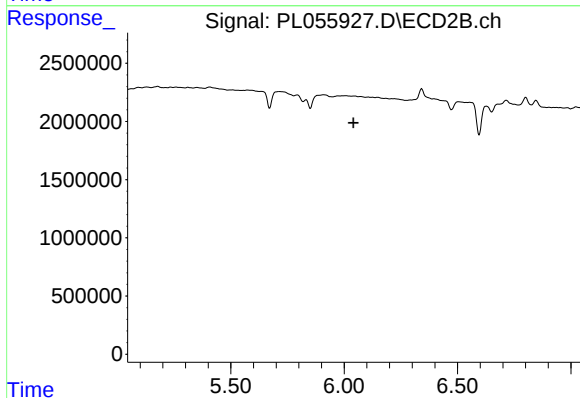


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.041 min
Response: 0
Conc: N.D.

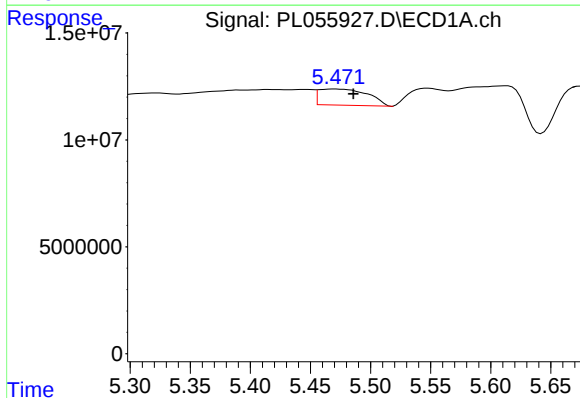


#26 Chlordane-4

R.T.: 5.471 min
Delta R.T.: -0.015 min
Response: 21532908
Conc: 20.88 ng/ml

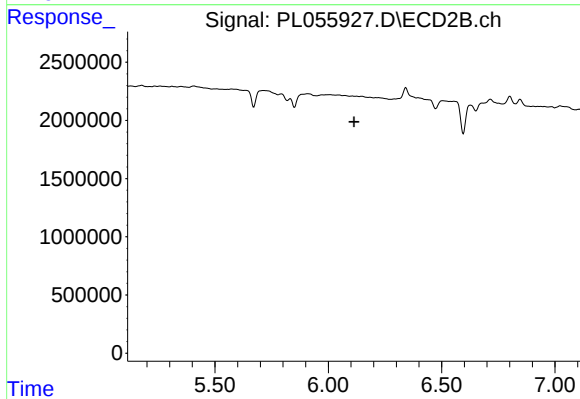

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

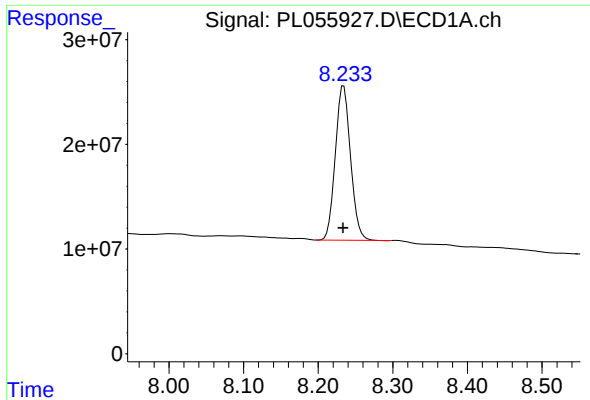

#28 Decachlorobiphenyl

R.T.: 8.234 min
Delta R.T.: 0.000 min
Response: 208898624
Conc: 19.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

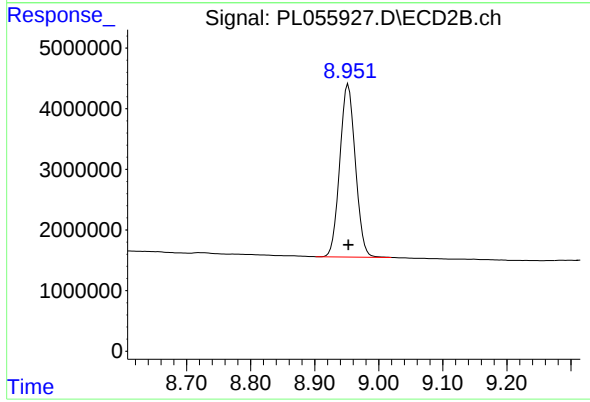

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: 0.000 min
Response: 48051244
Conc: 20.97 ng/ml