

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
 Data File : PL055878.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2020 22:33
 Operator : AJ\MA
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL012020CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 03:05:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.489	3.967	546.3E6	143.6E6	57.002	50.821
28)	SA Decachlor...	8.234	8.951	529.2E6	112.5E6	50.615	49.100
Target Compounds							
23)	Chlordane-1	4.359	4.943	183.3E6	52843613	499.925	501.849
24)	Chlordane-2	4.859	5.403	216.5E6	54025071	500.283	490.039
25)	Chlordane-3	5.428	6.041	632.5E6	193.9E6	507.935	488.410
26)	Chlordane-4	5.485	6.114	531.5E6	228.0E6	515.427	485.621
27)	Chlordane-5	6.321	6.910	201.2E6	40618566	514.321	495.795



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
Data File : PL055878.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2020 22:33
Operator : AJ\MA
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL012020CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 03:05:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

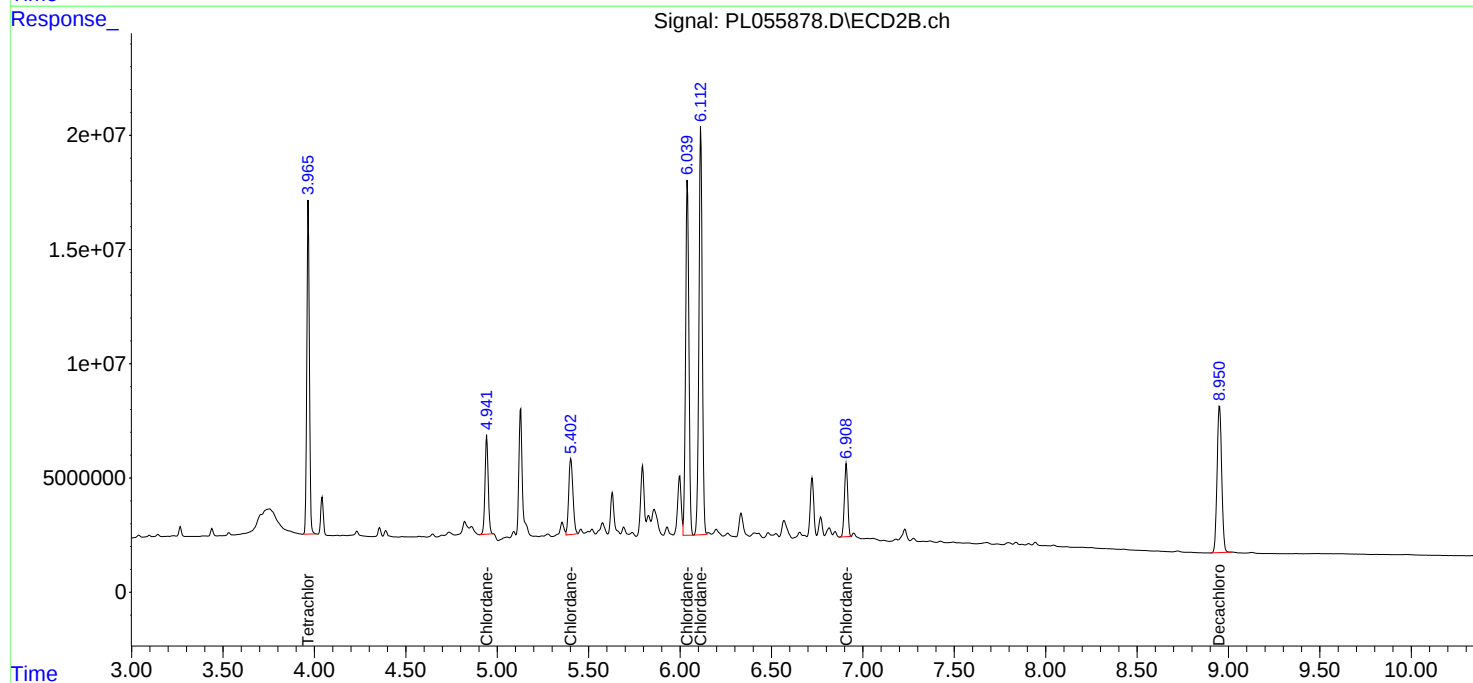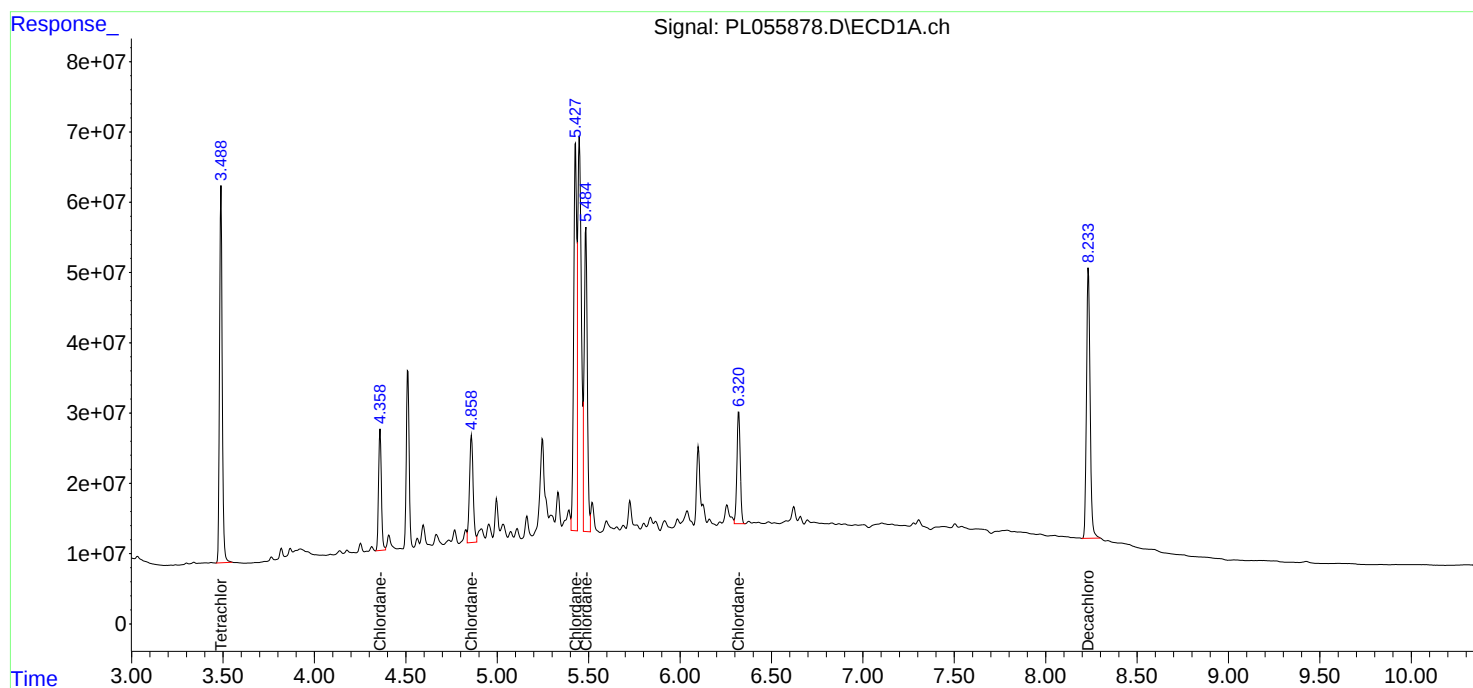


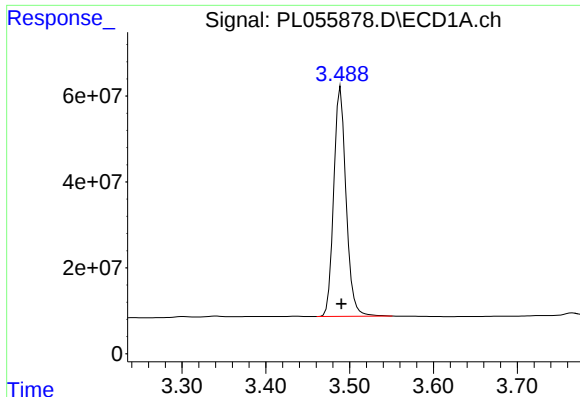

#1 Tetrachloro-m-xylene


R.T.: 3.489 min
Delta R.T.: 0.000 min
Response: 546339502
Conc: 57.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL012020CHLOR

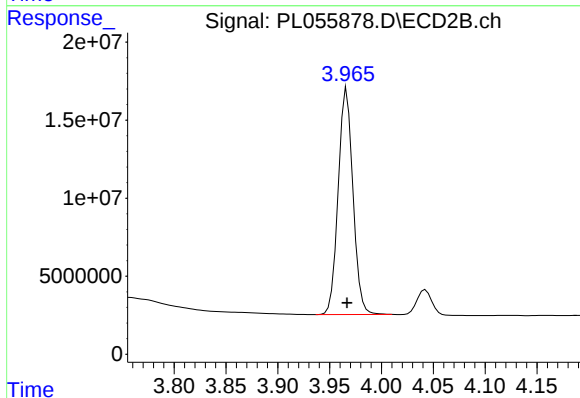


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 143631804
Conc: 50.82 ng/ml

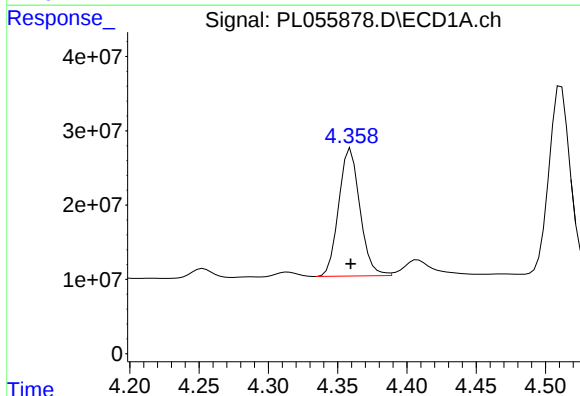


#23 Chlordane-1

R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 183293137
Conc: 499.93 ng/ml

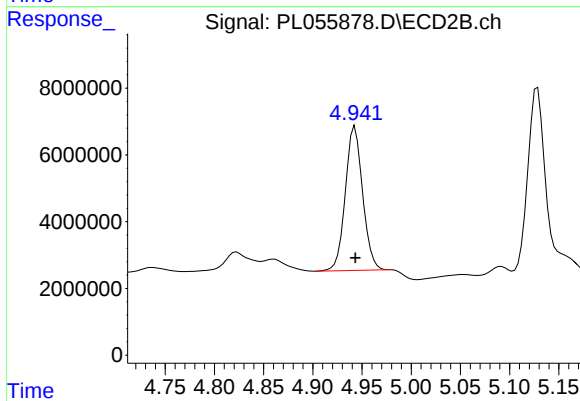

#23 Chlordane-1


R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 52843613
Conc: 501.85 ng/ml

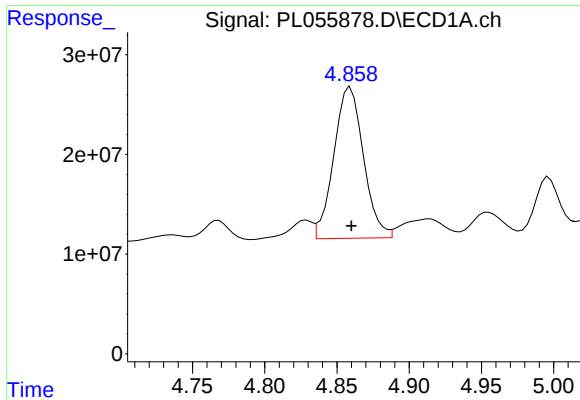

#24 Chlordane-2


R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 216495394
Conc: 500.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL012020CHLOR

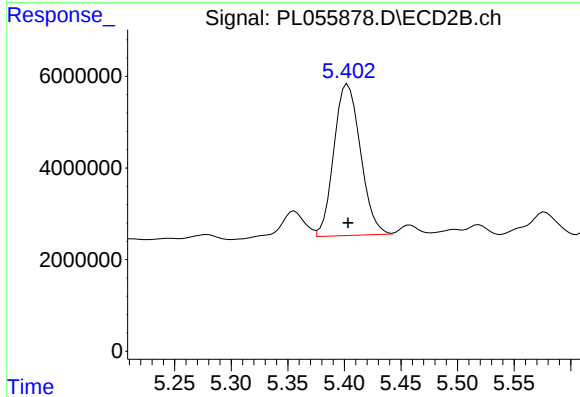


#24 Chlordane-2

R.T.: 5.403 min
Delta R.T.: 0.000 min
Response: 54025071
Conc: 490.04 ng/ml

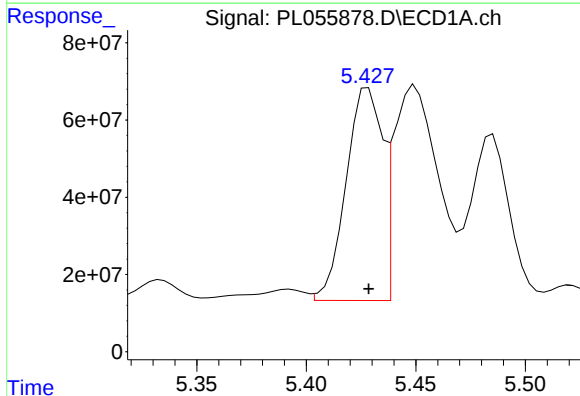


#25 Chlordane-3

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 632526270
Conc: 507.93 ng/ml

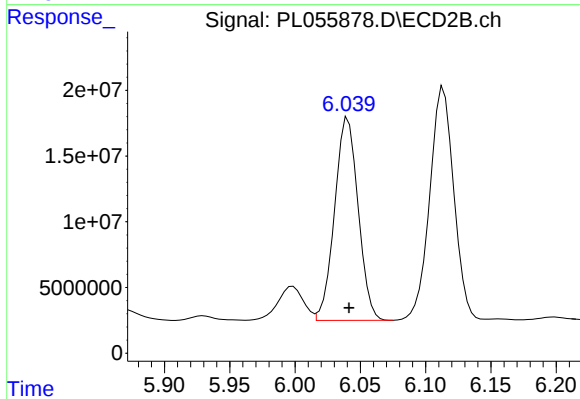

#25 Chlordane-3


R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 193858214
Conc: 488.41 ng/ml

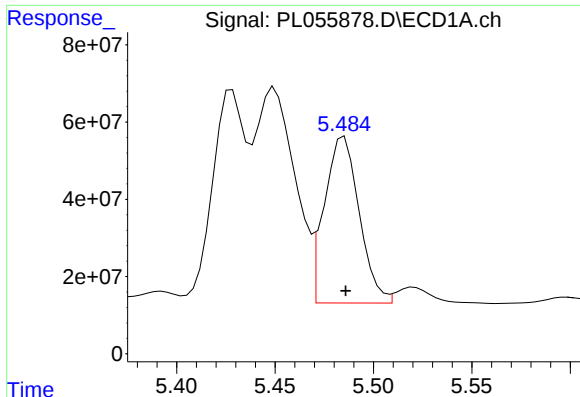

#26 Chlordane-4


R.T.: 5.485 min
Delta R.T.: 0.000 min
Response: 531481278
Conc: 515.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL012020CHLOR

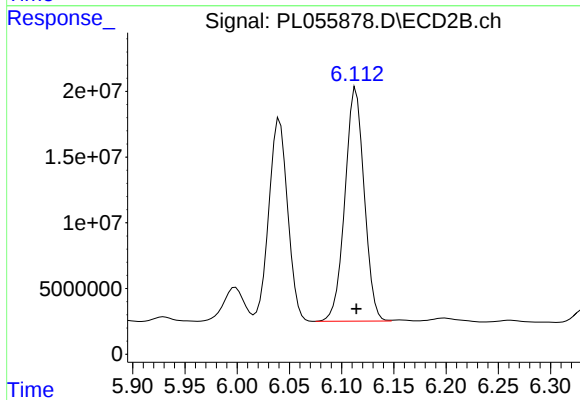


#26 Chlordane-4

R.T.: 6.114 min
Delta R.T.: 0.000 min
Response: 227962736
Conc: 485.62 ng/ml

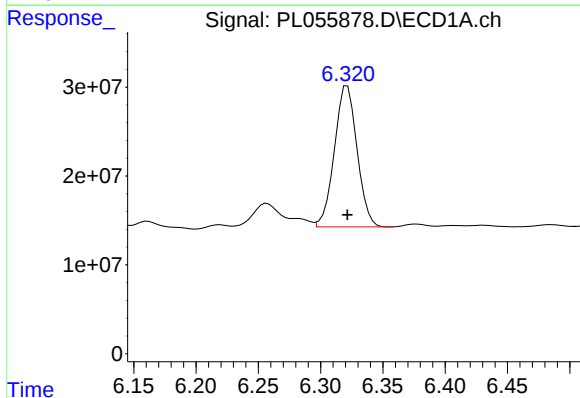


#27 Chlordane-5

R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 201158715
Conc: 514.32 ng/ml

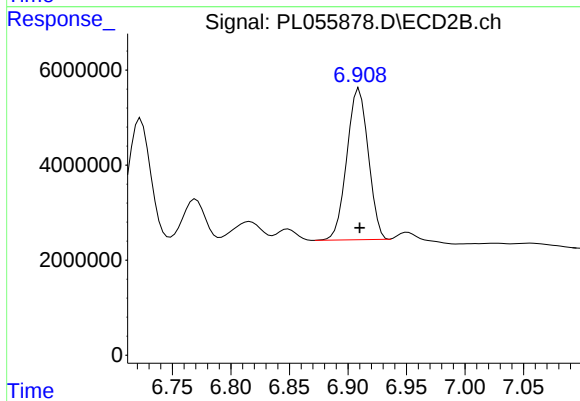

#27 Chlordane-5


R.T.: 6.910 min
Delta R.T.: 0.000 min
Response: 40618566
Conc: 495.80 ng/ml

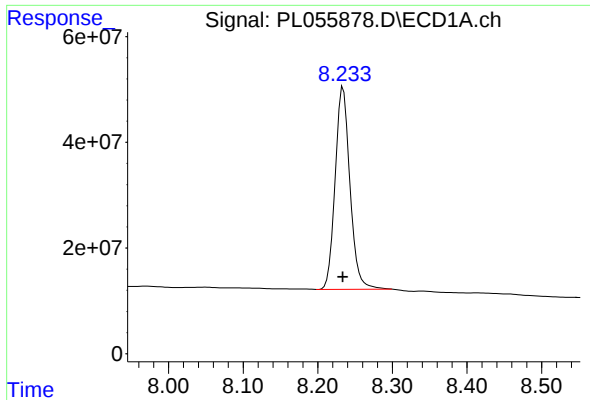

#28 Decachlorobiphenyl

R.T.: 8.234 min
Delta R.T.: 0.000 min
Response: 529216060
Conc: 50.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL012020CHLOR

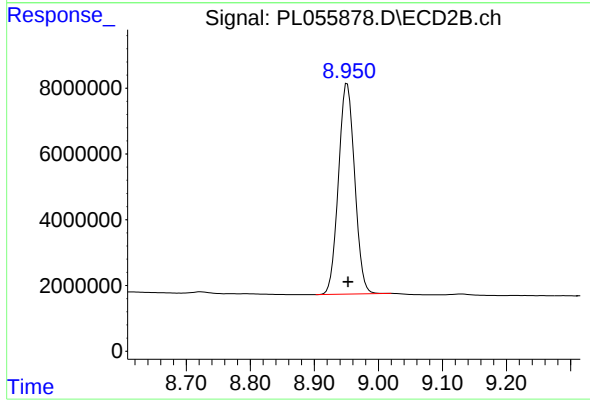

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: -0.001 min
Response: 112486564
Conc: 49.10 ng/ml