

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
 Data File : PL055894.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 02:19
 Operator : AJ\MA
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:13:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.489	3.966	554.1E6	146.4E6	57.808	51.812
28)	SA Decachlor...	8.233	8.951	555.9E6	116.9E6	53.170	51.039
Target Compounds							
23)	Chlordane-1	4.359	4.943	187.8E6	53942332	512.086	512.283
24)	Chlordane-2	4.860	5.403	229.2E6	55460218	529.583	503.057
25)	Chlordane-3	5.429	6.041	666.0E6	202.5E6	534.807	510.151
26)	Chlordane-4	5.486	6.113	550.6E6	236.6E6	534.016	504.064
27)	Chlordane-5	6.322	6.909	164.5E6	42234807	420.645	515.523



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
Data File : PL055894.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 02:19
Operator : AJ\MA
Sample : PCHLORCCC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:13:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

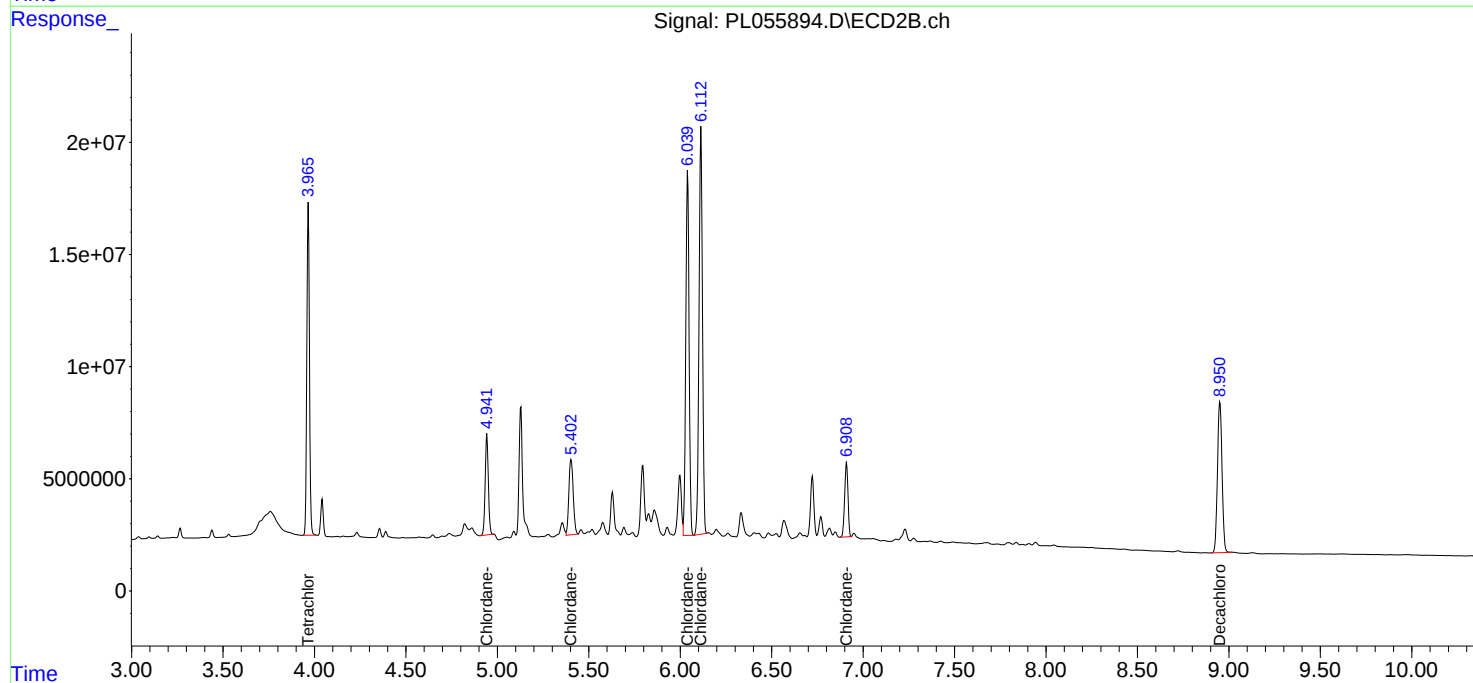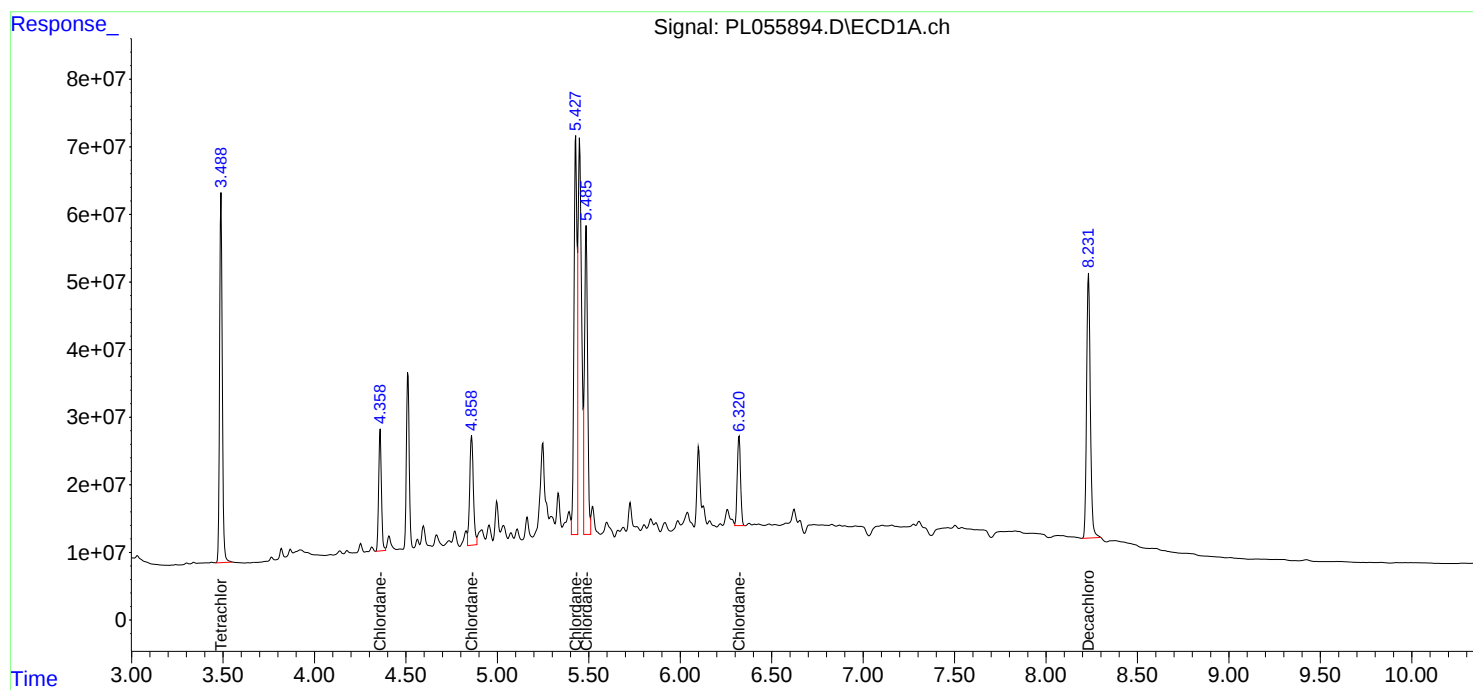


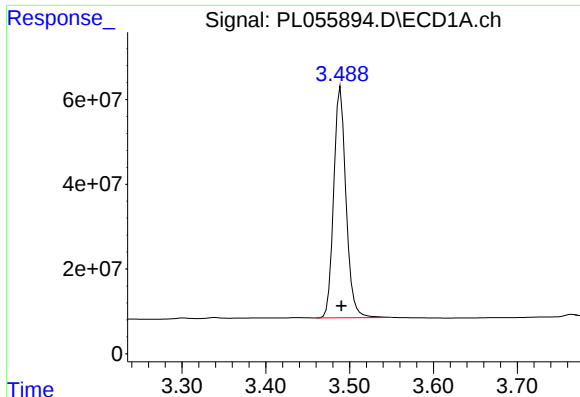

#1 Tetrachloro-m-xylene


R.T.: 3.489 min
Delta R.T.: 0.000 min
Response: 554055785
Conc: 57.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

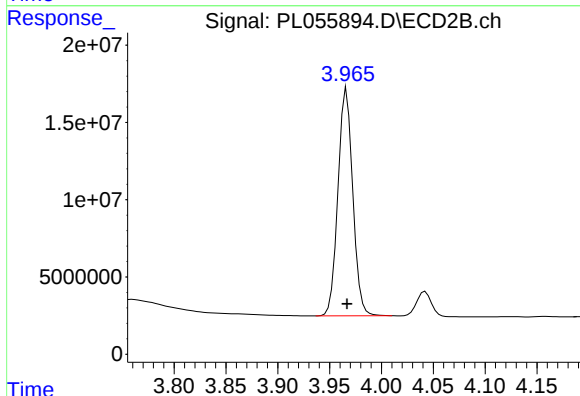


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 146433348
Conc: 51.81 ng/ml

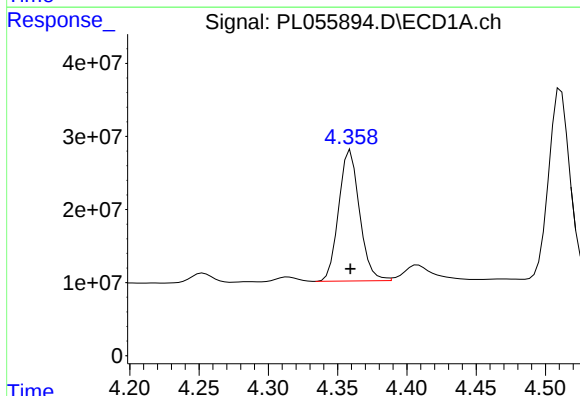


#23 Chlordane-1

R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 187751741
Conc: 512.09 ng/ml

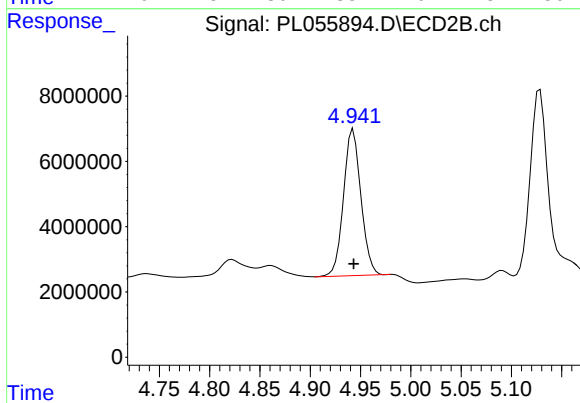

#23 Chlordane-1


R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 53942332
Conc: 512.28 ng/ml

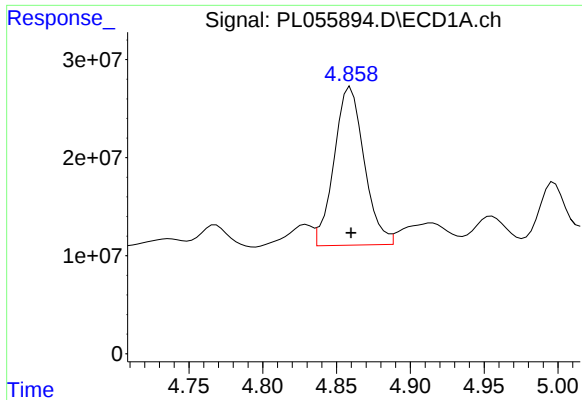

#24 Chlordane-2


R.T.: 4.860 min
Delta R.T.: 0.000 min
Response: 229174915
Conc: 529.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

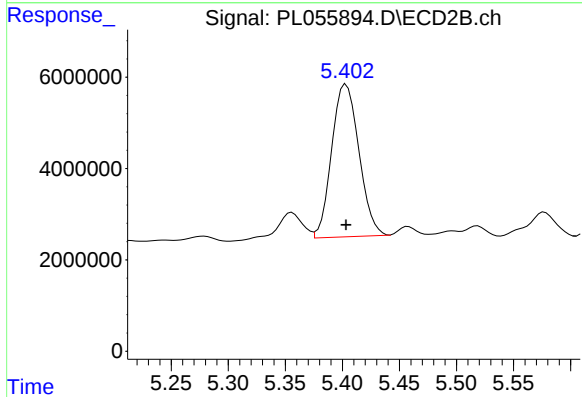


#24 Chlordane-2

R.T.: 5.403 min
Delta R.T.: 0.000 min
Response: 55460218
Conc: 503.06 ng/ml

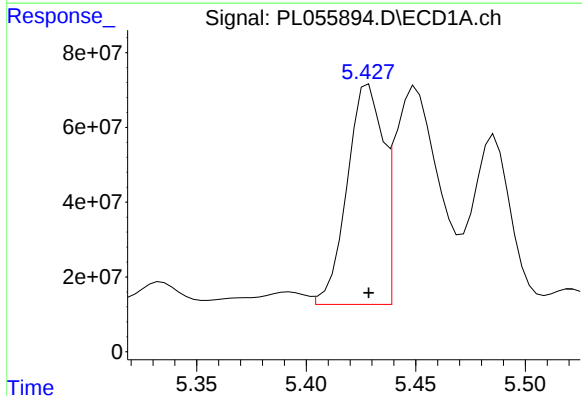


#25 Chlordane-3

R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 665990259
Conc: 534.81 ng/ml

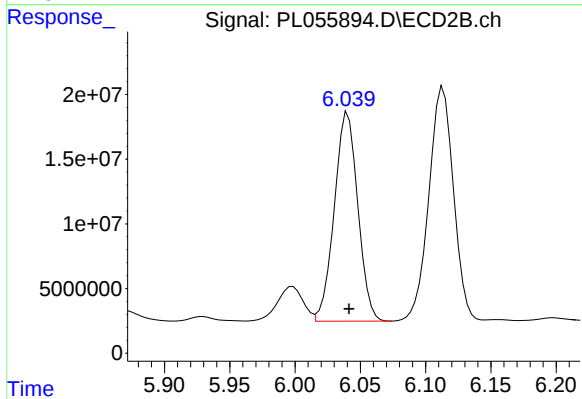

#25 Chlordane-3


R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 202487812
Conc: 510.15 ng/ml

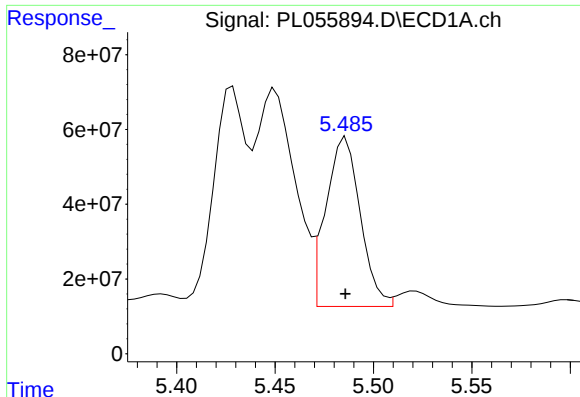

#26 Chlordane-4


R.T.: 5.486 min
Delta R.T.: 0.000 min
Response: 550649606
Conc: 534.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

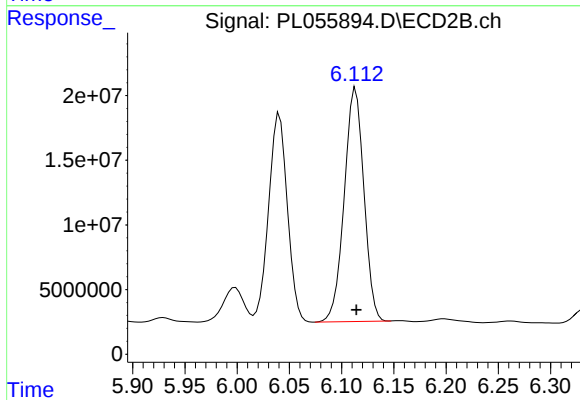


#26 Chlordane-4

R.T.: 6.113 min
Delta R.T.: 0.000 min
Response: 236620327
Conc: 504.06 ng/ml

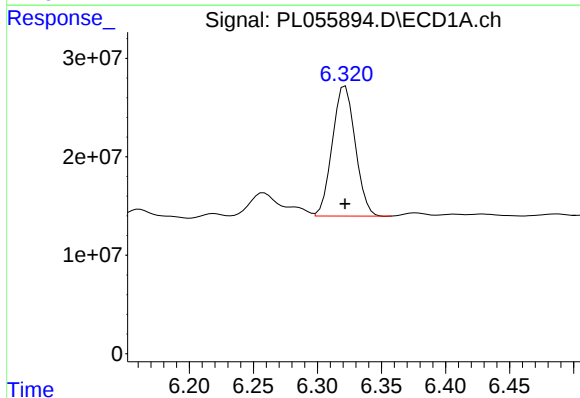


#27 Chlordane-5

R.T.: 6.322 min
Delta R.T.: 0.000 min
Response: 164520547
Conc: 420.64 ng/ml

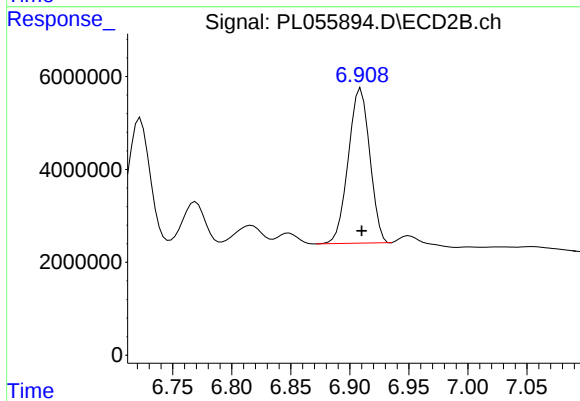

#27 Chlordane-5


R.T.: 6.909 min
Delta R.T.: 0.000 min
Response: 42234807
Conc: 515.52 ng/ml

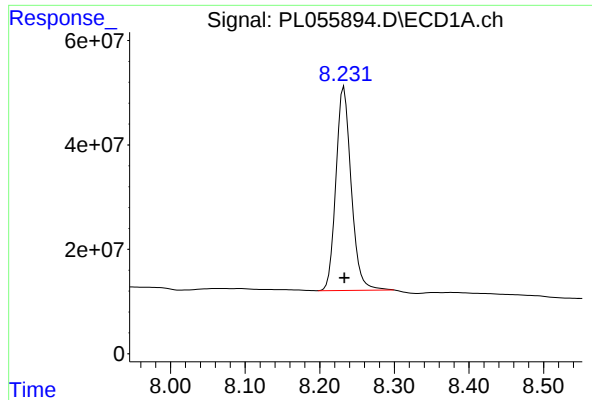

#28 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: 0.000 min
Response: 555928365
Conc: 53.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

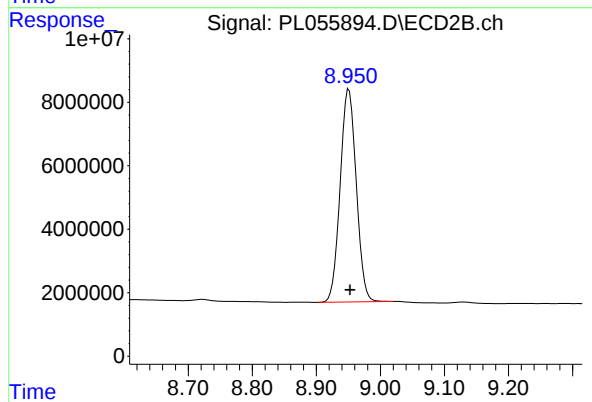

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: -0.002 min
Response: 116928241
Conc: 51.04 ng/ml