

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
 Data File : PL055905.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 04:55
 Operator : AJ\MA
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 06:43:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.489	3.967	554.8E6	149.3E6	57.883	52.840
28)	SA Decachlor...	8.233	8.953	548.3E6	117.5E6	52.436	51.279
Target Compounds							
23)	Chlordane-1	4.359	4.943	189.0E6	54558451	515.626	518.134
24)	Chlordane-2	4.859	5.403	244.1E6	56478945	564.180	512.297
25)	Chlordane-3	5.428	6.041	659.7E6	204.7E6	529.716	515.750
26)	Chlordane-4	5.485	6.114	542.4E6	240.5E6	526.003	512.284
27)	Chlordane-5	6.321	6.910	208.0E6	43954836	531.772	536.518


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
Data File : PL055905.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 04:55
Operator : AJ\MA
Sample : PCHLORCCC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 06:43:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

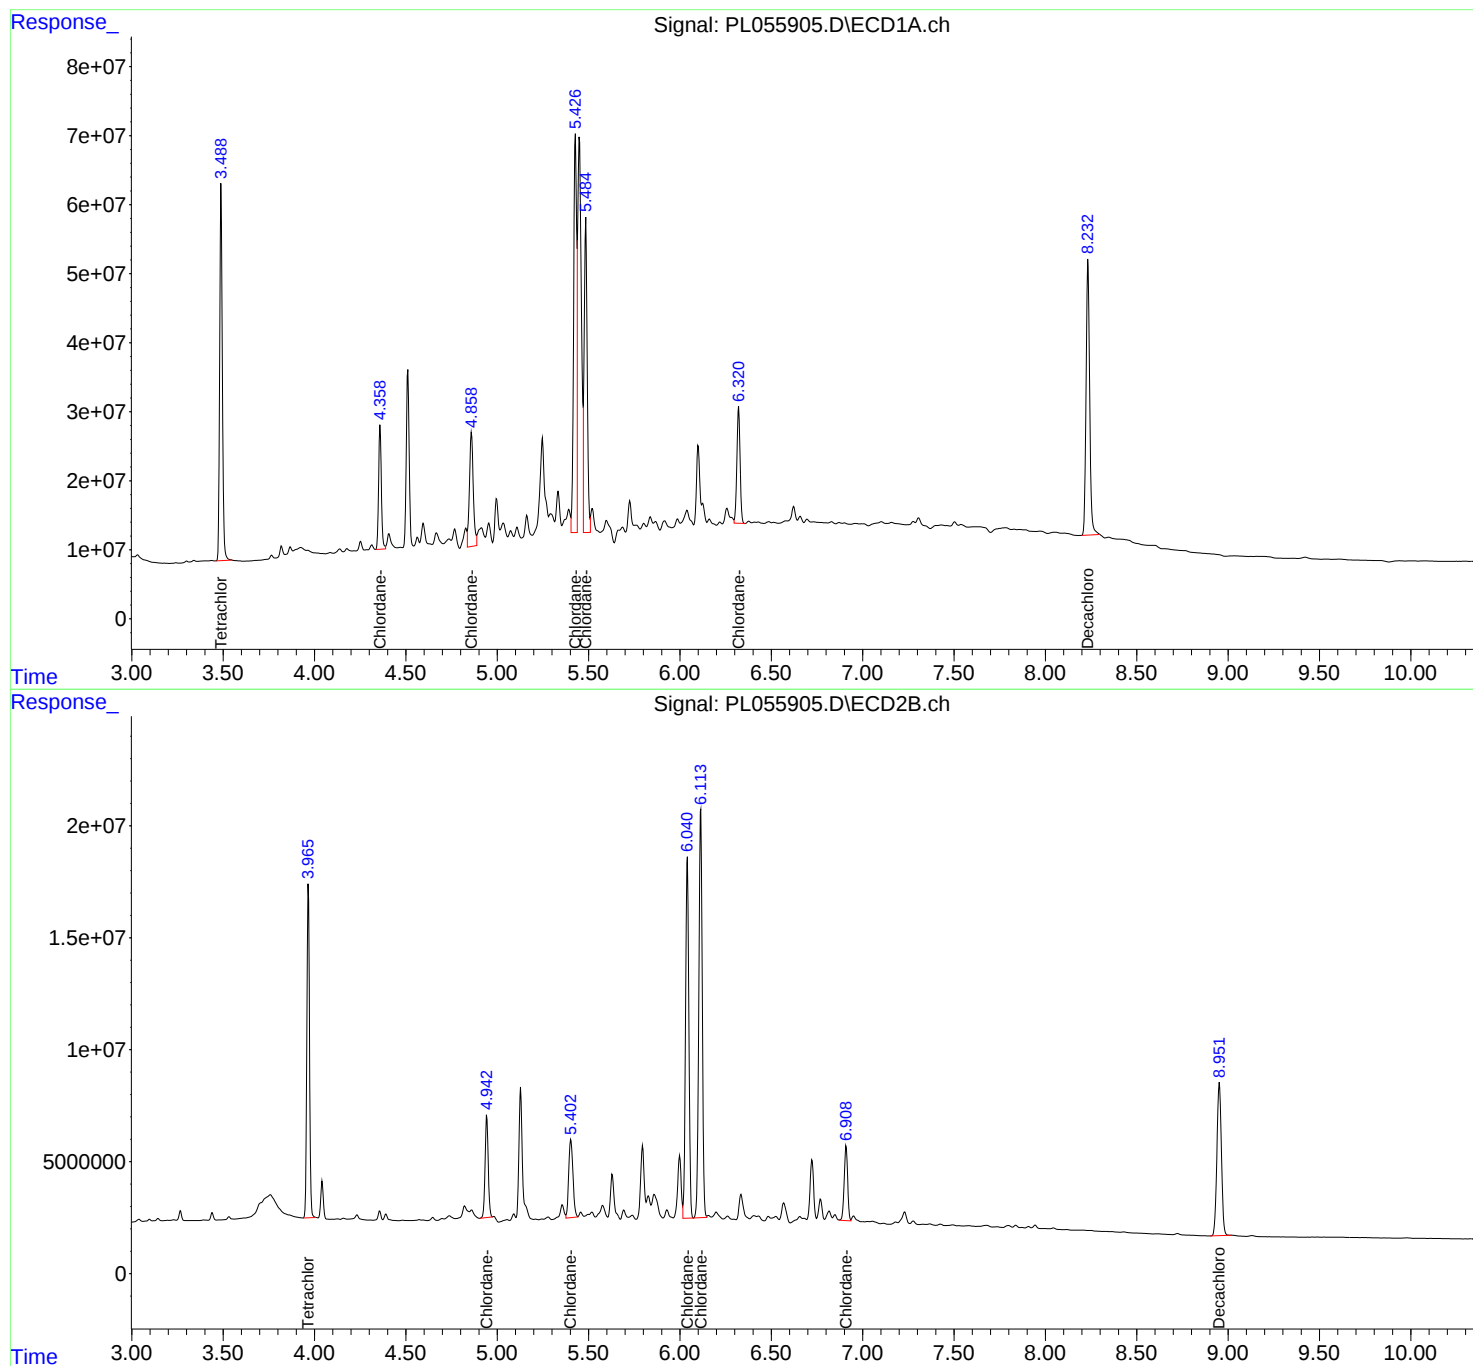


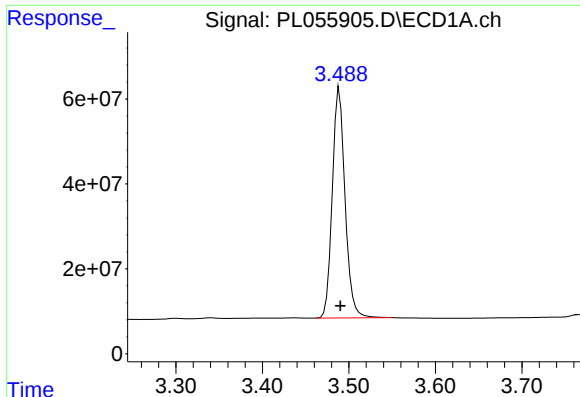

#1 Tetrachloro-m-xylene


R.T.: 3.489 min
Delta R.T.: 0.000 min
Response: 554778081
Conc: 57.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

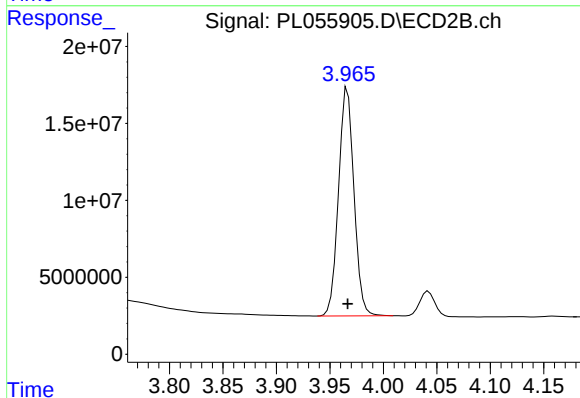


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 149338875
Conc: 52.84 ng/ml

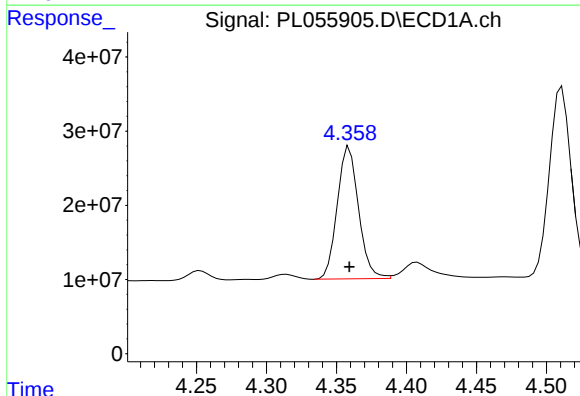


#23 Chlordane-1

R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 189049889
Conc: 515.63 ng/ml

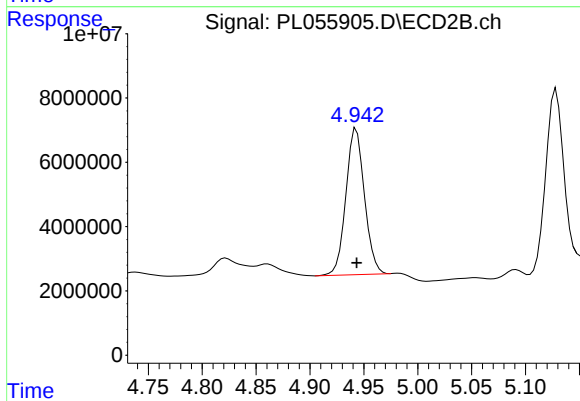

#23 Chlordane-1


R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 54558451
Conc: 518.13 ng/ml

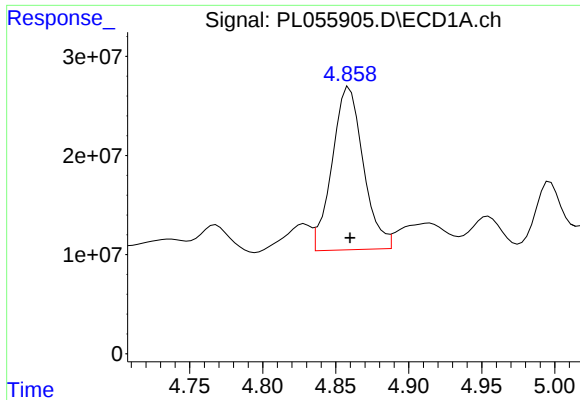

#24 Chlordane-2


R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 244146455
Conc: 564.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

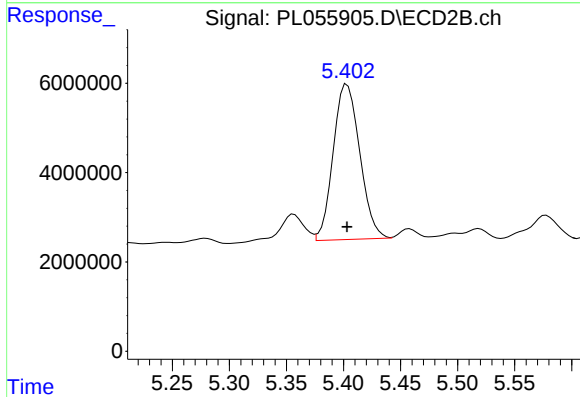


#24 Chlordane-2

R.T.: 5.403 min
Delta R.T.: 0.000 min
Response: 56478945
Conc: 512.30 ng/ml

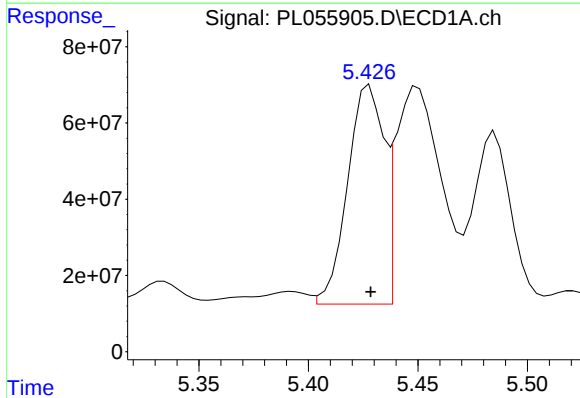


#25 Chlordane-3

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 659650011
Conc: 529.72 ng/ml

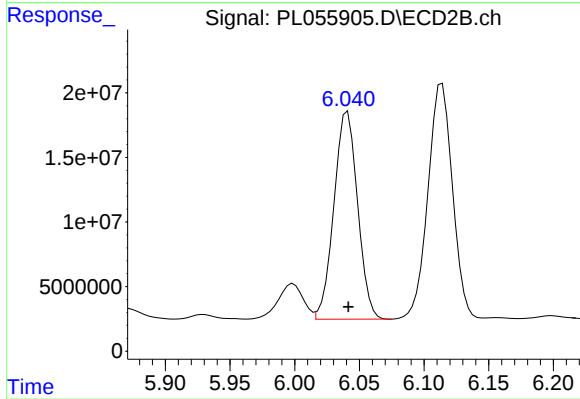

#25 Chlordane-3


R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 204710080
Conc: 515.75 ng/ml

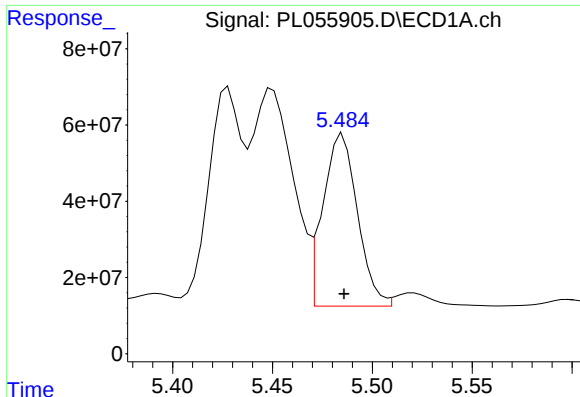

#26 Chlordane-4


R.T.: 5.485 min
Delta R.T.: 0.000 min
Response: 542386545
Conc: 526.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

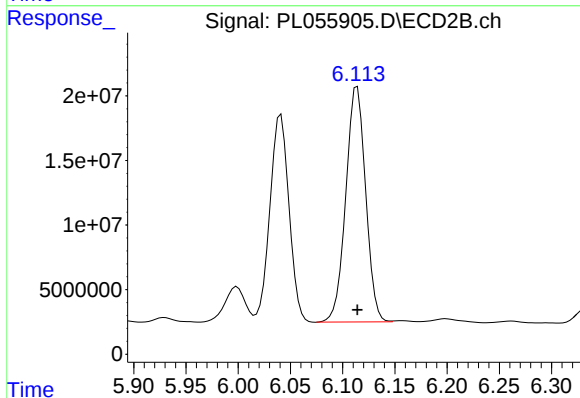


#26 Chlordane-4

R.T.: 6.114 min
Delta R.T.: 0.000 min
Response: 240478966
Conc: 512.28 ng/ml

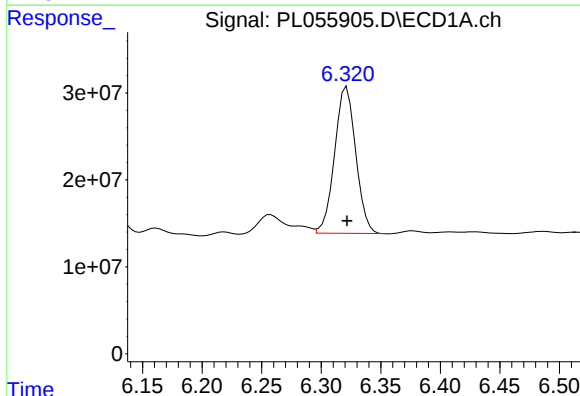


#27 Chlordane-5

R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 207984034
Conc: 531.77 ng/ml

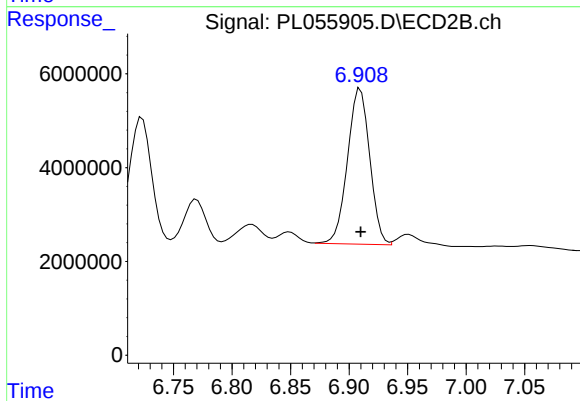

#27 Chlordane-5


R.T.: 6.910 min
Delta R.T.: 0.000 min
Response: 43954836
Conc: 536.52 ng/ml

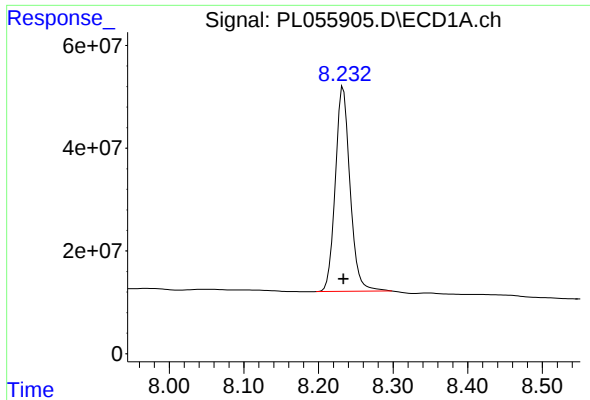

#28 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: 0.000 min
Response: 548255531
Conc: 52.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

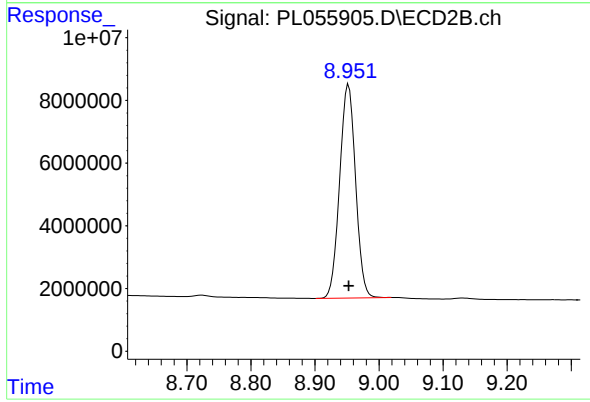

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: 0.000 min
Response: 117478477
Conc: 51.28 ng/ml