

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
 Data File : PL055923.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 09:51
 Operator : AJ\MA
 Sample : L1190-02
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TSP-02

Manual Integrations
 APPROVED

Ankita
 1/22/2020 9:39:35 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 10:13:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.489	3.966	81762829	26960053	8.531	9.539
28)	SA Decachlor...	8.233	8.951	70425881	17099855	6.736	7.464
Target Compounds							
10)	B gamma-Chl...	5.429	6.039	5800284	6650308	0.413m	2.157m#
11)	B alpha-Chl...	5.484	6.113	23122944	14958840	1.673m	4.845 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012020\
Data File : PL055923.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 09:51
Operator : AJ\MA
Sample : L1190-02
Misc :
ALS Vial : 52 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TSP-02


Manual Integrations
APPROVED

Ankita
1/22/2020 9:39:35 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 10:13:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

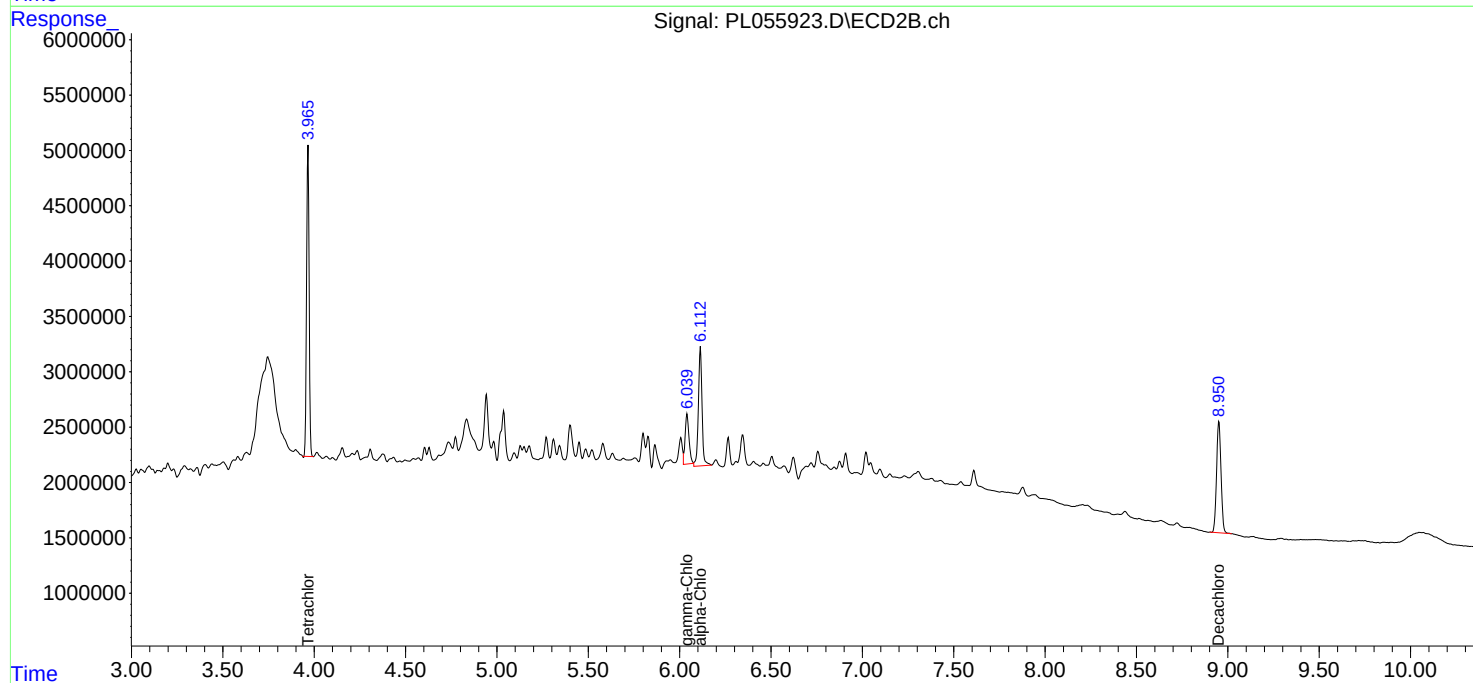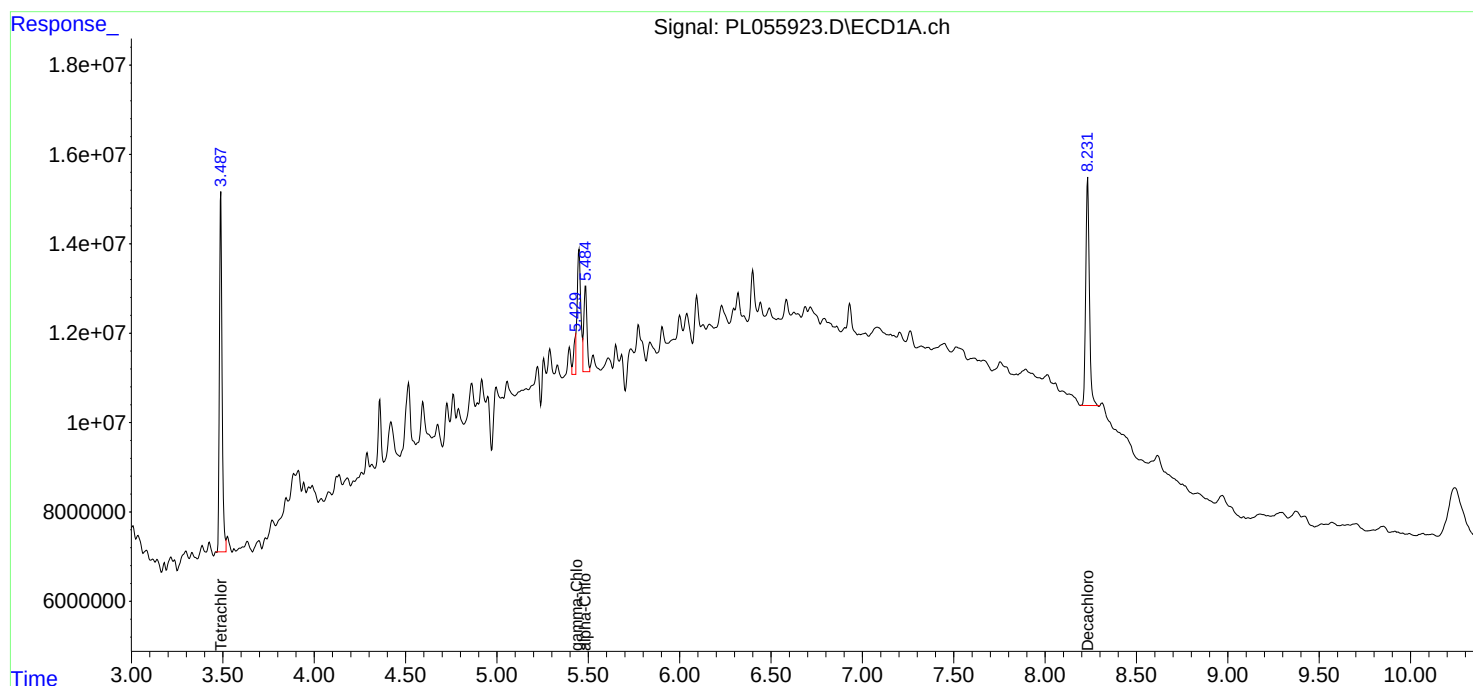

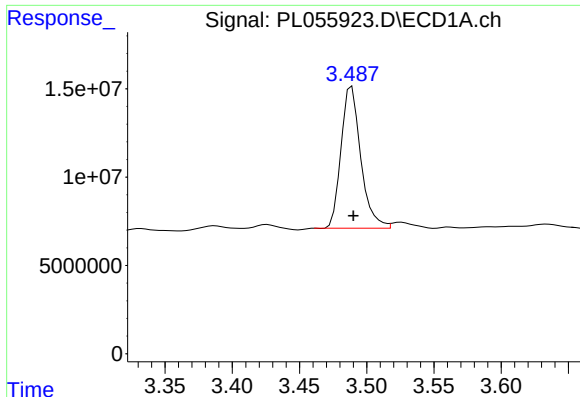


#1 Tetrachloro-m-xylene

R.T.: 3.489 min
Delta R.T.: -0.001 min
Response: 81762829
Conc: 8.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
TSP-02


Manual Integrations
APPROVED

Ankita
1/22/2020 9:39:35 AM

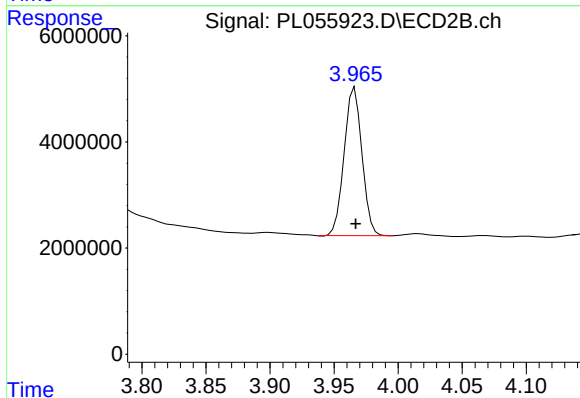


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 26960053
Conc: 9.54 ng/ml

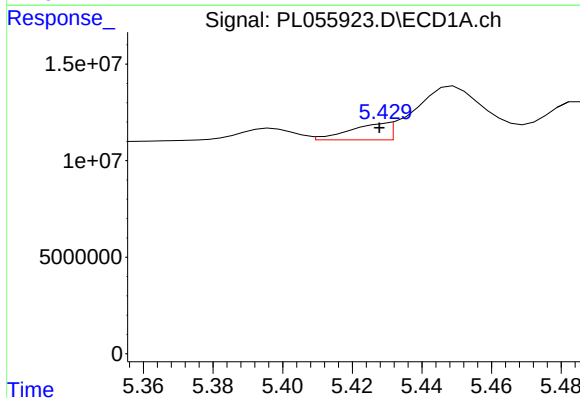


#10 gamma-Chlordane

R.T.: 5.429 min
Delta R.T.: 0.001 min
Response: 5800284
Conc: 0.41 ng/ml m

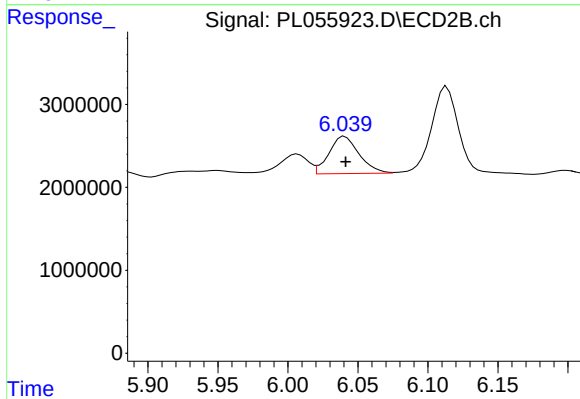

#10 gamma-Chlordane

R.T.: 6.039 min
Delta R.T.: -0.002 min
Response: 6650308
Conc: 2.16 ng/ml m

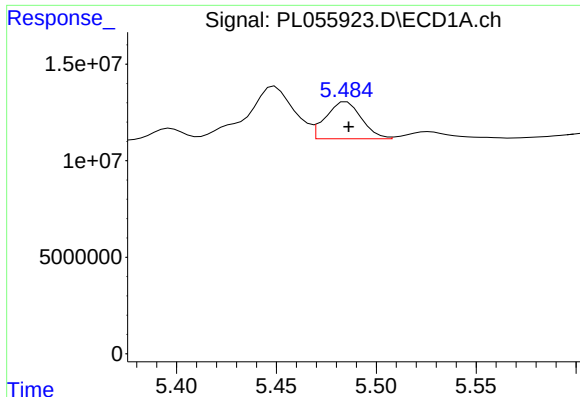


#11 alpha-Chlordane

R.T.: 5.484 min
Delta R.T.: -0.002 min
Response: 23122944
Conc: 1.67 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TSP-02


Manual Integrations
APPROVED

Ankita
1/22/2020 9:39:35 AM

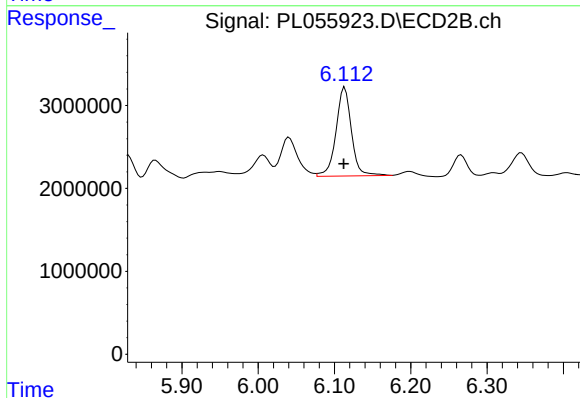


#11 alpha-Chlordane

R.T.: 6.113 min
Delta R.T.: 0.001 min
Response: 14958840
Conc: 4.84 ng/ml

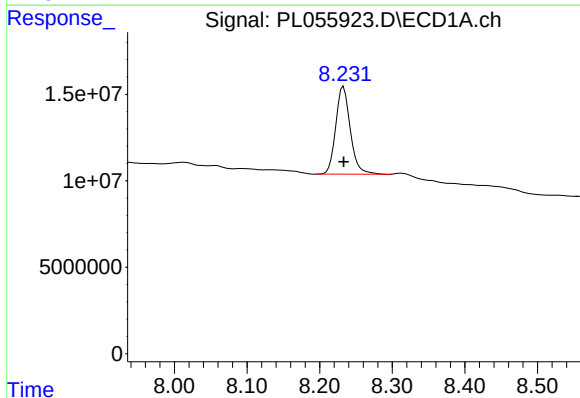

#28 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: 0.000 min
Response: 70425881
Conc: 6.74 ng/ml

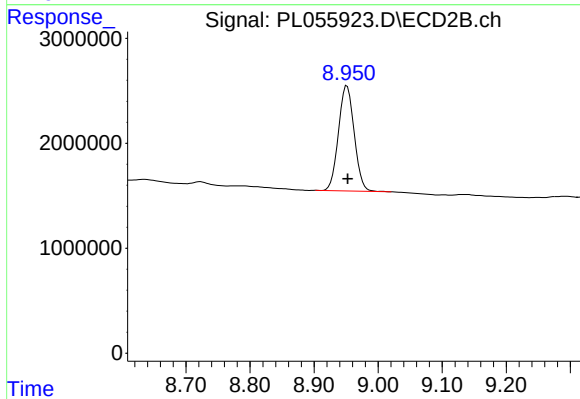

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: -0.001 min
Response: 17099855
Conc: 7.46 ng/ml