

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012021\
 Data File : PL064245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2021 11:46
 Operator : AR\AJ
 Sample : PB134234BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB134234BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 14:44:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.443	4.108	67182296	56227064	22.405	21.994
28) SA Decachlor...	8.180	9.275	60343885	44313153	19.771	18.671
Target Compounds						
15) B Endosulfa...	0.000	7.065	0	1854567	N.D.	0.734 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012021\
Data File : PL064245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2021 11:46
Operator : AR\AJ
Sample : PB134234BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PB134234BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 14:44:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

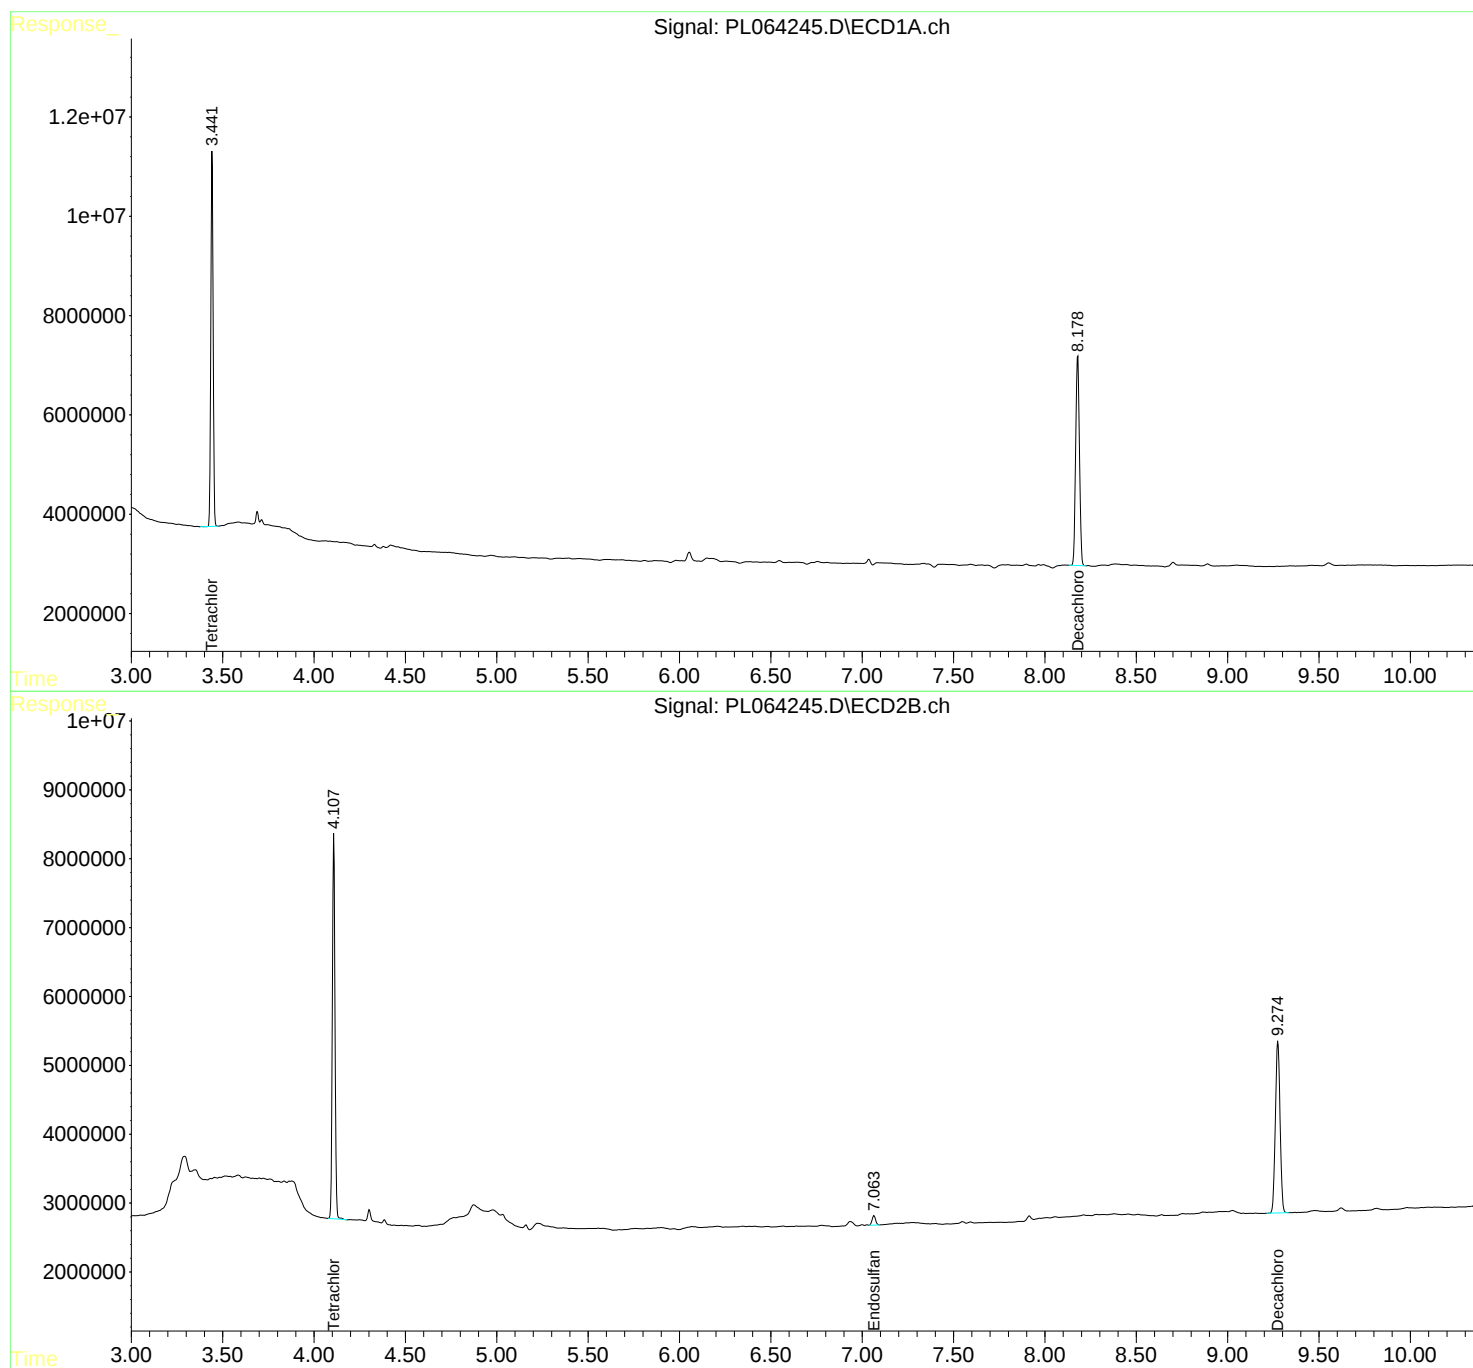


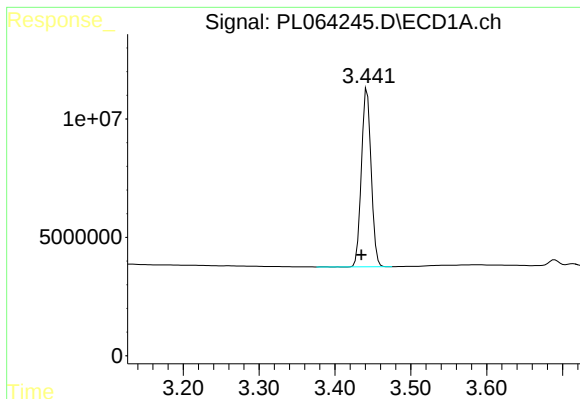

#1 Tetrachloro-m-xylene


R.T.: 3.443 min
Delta R.T.: 0.008 min
Response: 67182296
Conc: 22.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB134234BL

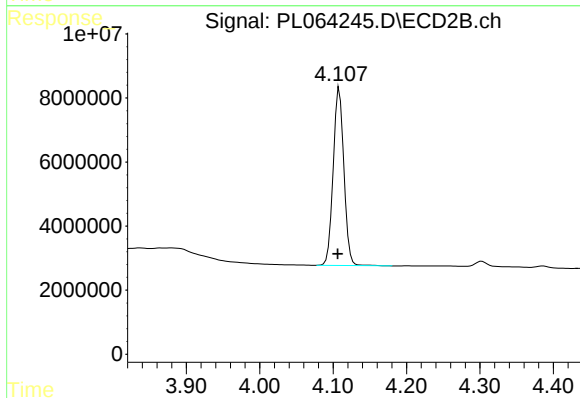


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.002 min
Response: 56227064
Conc: 21.99 ng/ml

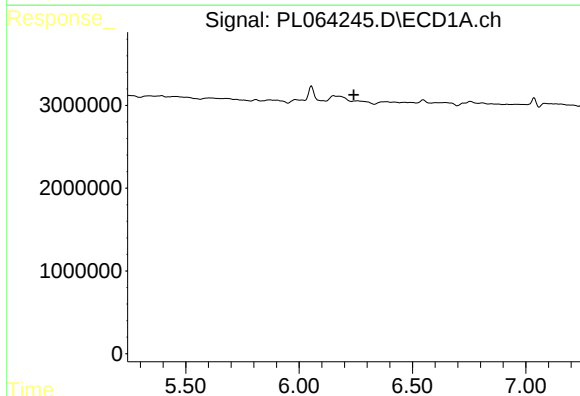


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

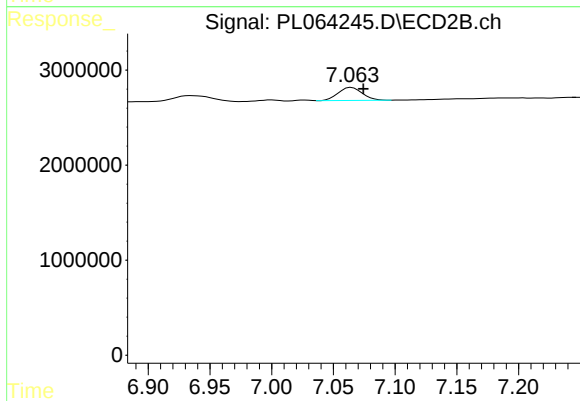

#15 Endosulfan II


R.T.: 7.065 min
Delta R.T.: -0.010 min
Response: 1854567
Conc: 0.73 ng/ml

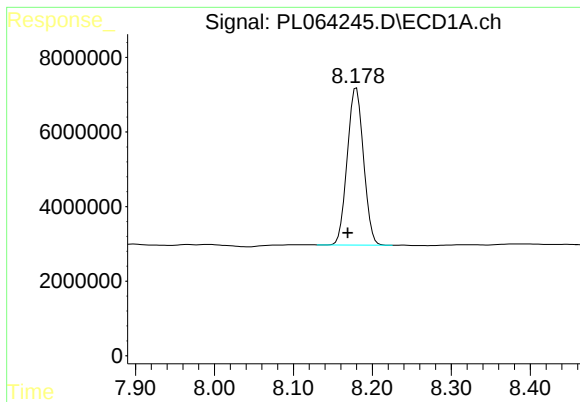

#28 Decachlorobiphenyl

R.T.: 8.180 min
Delta R.T.: 0.011 min
Response: 60343885
Conc: 19.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB134234BL

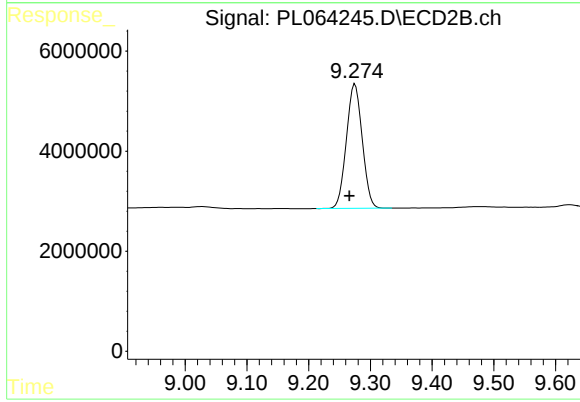

#28 Decachlorobiphenyl

R.T.: 9.275 min
Delta R.T.: 0.009 min
Response: 44313153
Conc: 18.67 ng/ml