

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012021\
 Data File : PL064257.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2021 15:15
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 15:52:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.107	58783011	47847979	19.604	18.717
28)	SA Decachlor...	8.167	9.268	49508280	37102588	16.221	15.633
Target Compounds							
6)	B beta-BHC	0.000	4.984	0	8416129	N.D.	1.552 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012021\
Data File : PL064257.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2021 15:15
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 15:52:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

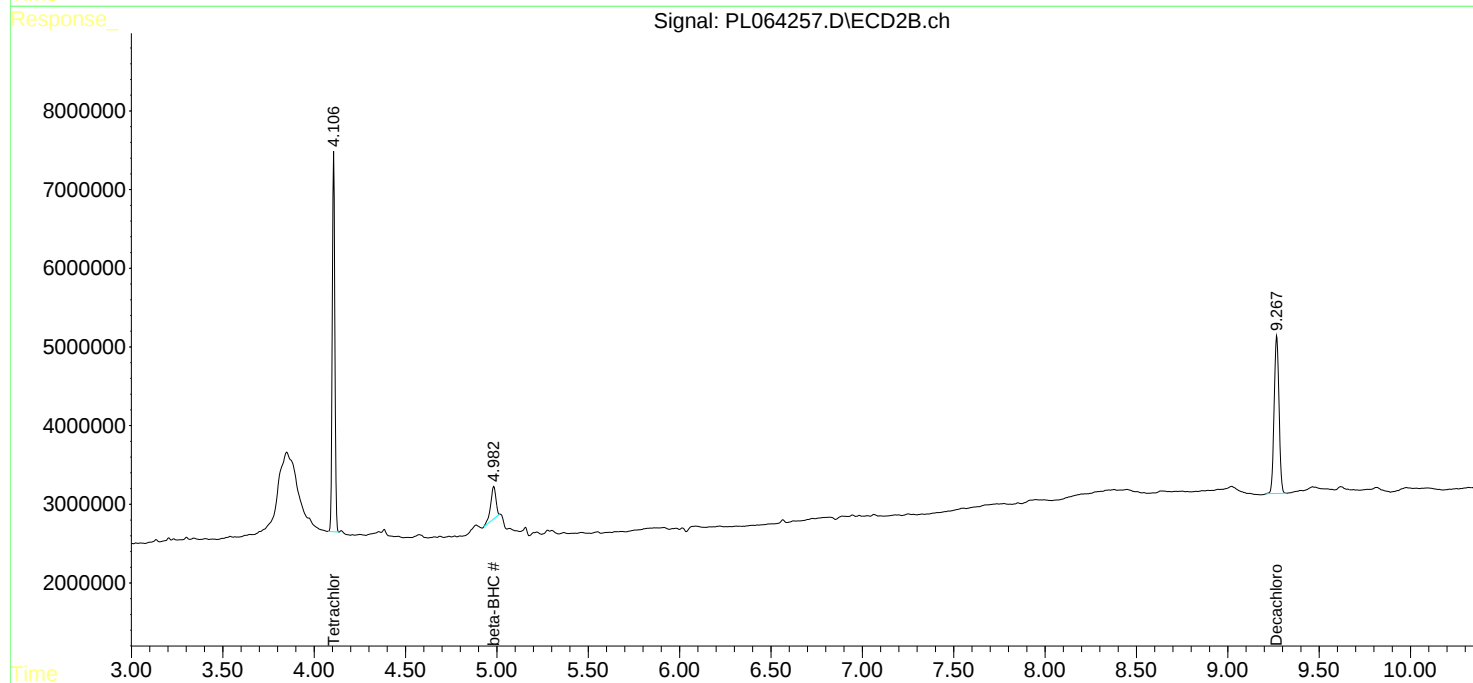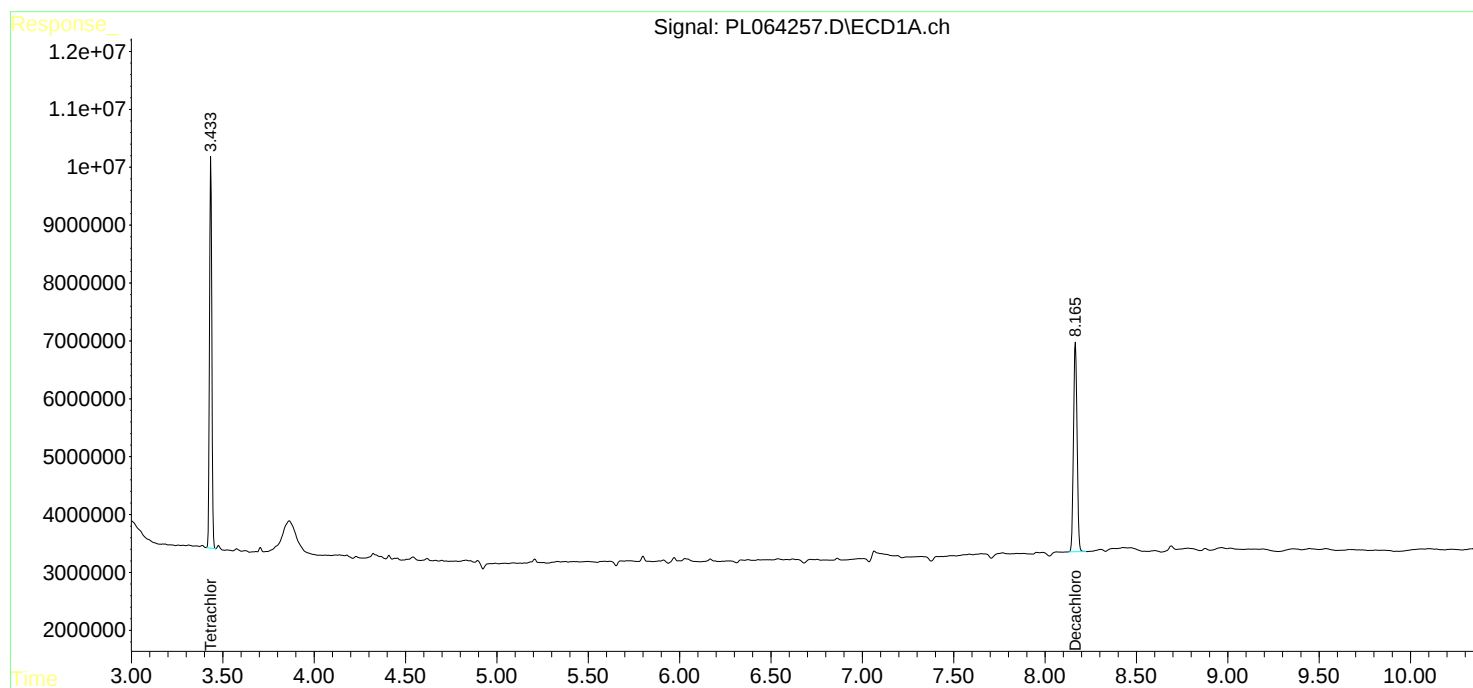


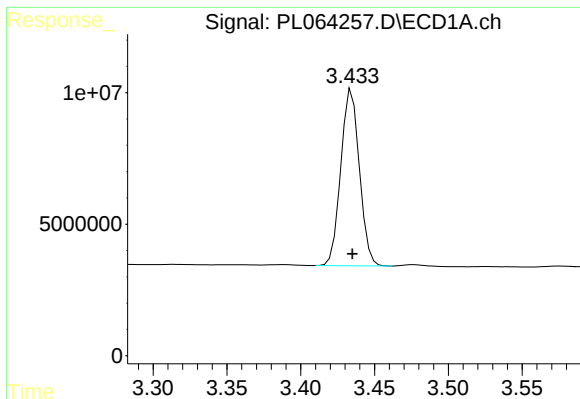

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 58783011
Conc: 19.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

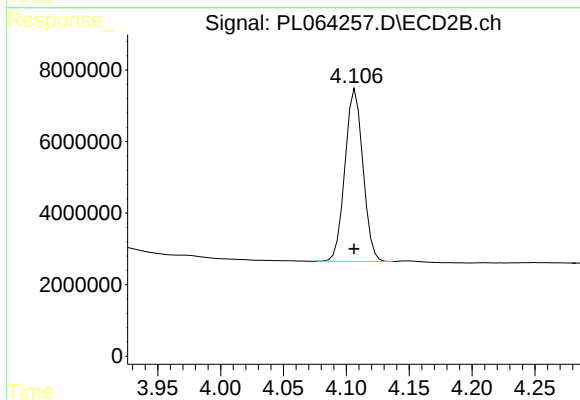


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 47847979
Conc: 18.72 ng/ml

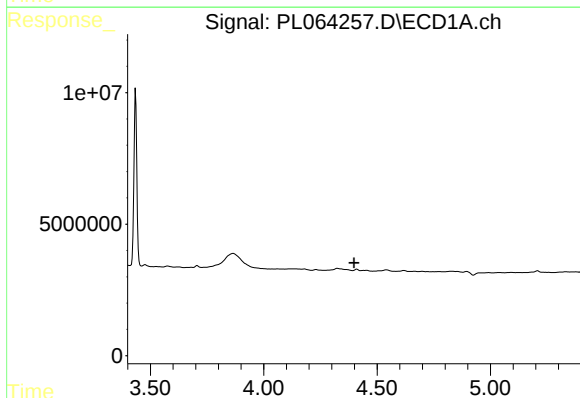


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.398 min
Response: 0
Conc: N.D.

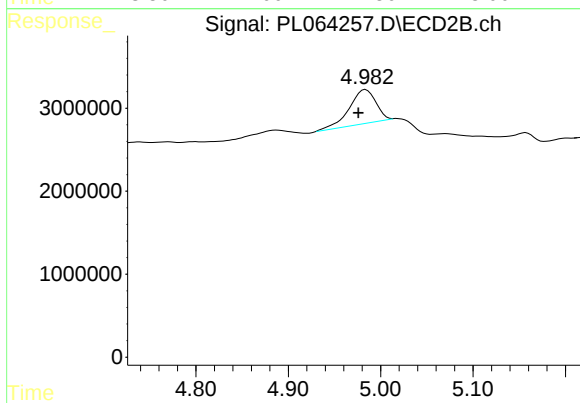

#6 beta-BHC


R.T.: 4.984 min
Delta R.T.: 0.008 min
Response: 8416129
Conc: 1.55 ng/ml

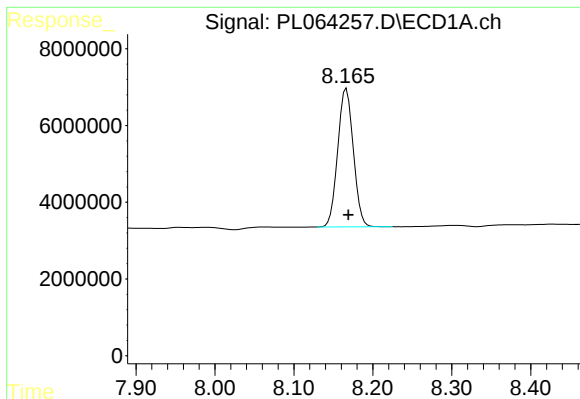

#28 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: -0.002 min
Response: 49508280
Conc: 16.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

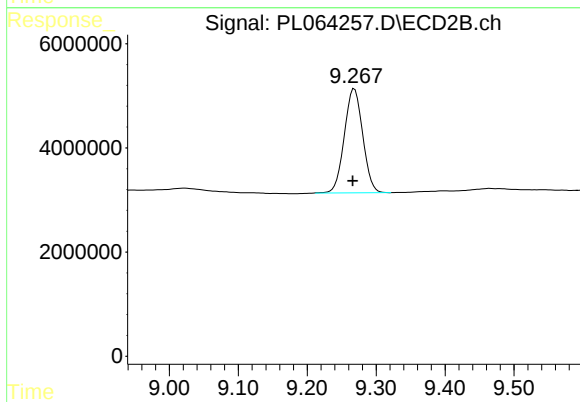

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.002 min
Response: 37102588
Conc: 15.63 ng/ml