

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012021\
 Data File : PL064253.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2021 14:18
 Operator : AR\AJ
 Sample : M1177-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PILE-2-(1.5-2.0)

Manual Integrations
 APPROVED

Ankita
 1/21/2021 3:18:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 15:51:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.108	68436637	53618249	22.824	20.974
28)	SA Decachlor...	8.166	9.268	44136035	32319745	14.461	13.617
Target Compounds							
12)	B 4,4'-DDE	5.584	6.482	2260274	1468025	0.642	0.551
17)	MA 4,4'-DDT	6.337	7.276	1845111	3190297	0.618	1.409m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012021\
Data File : PL064253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2021 14:18
Operator : AR\AJ
Sample : M1177-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
PILE-2-(1.5-2.0)


Manual Integrations
APPROVED

Ankita
1/21/2021 3:18:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 15:51:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

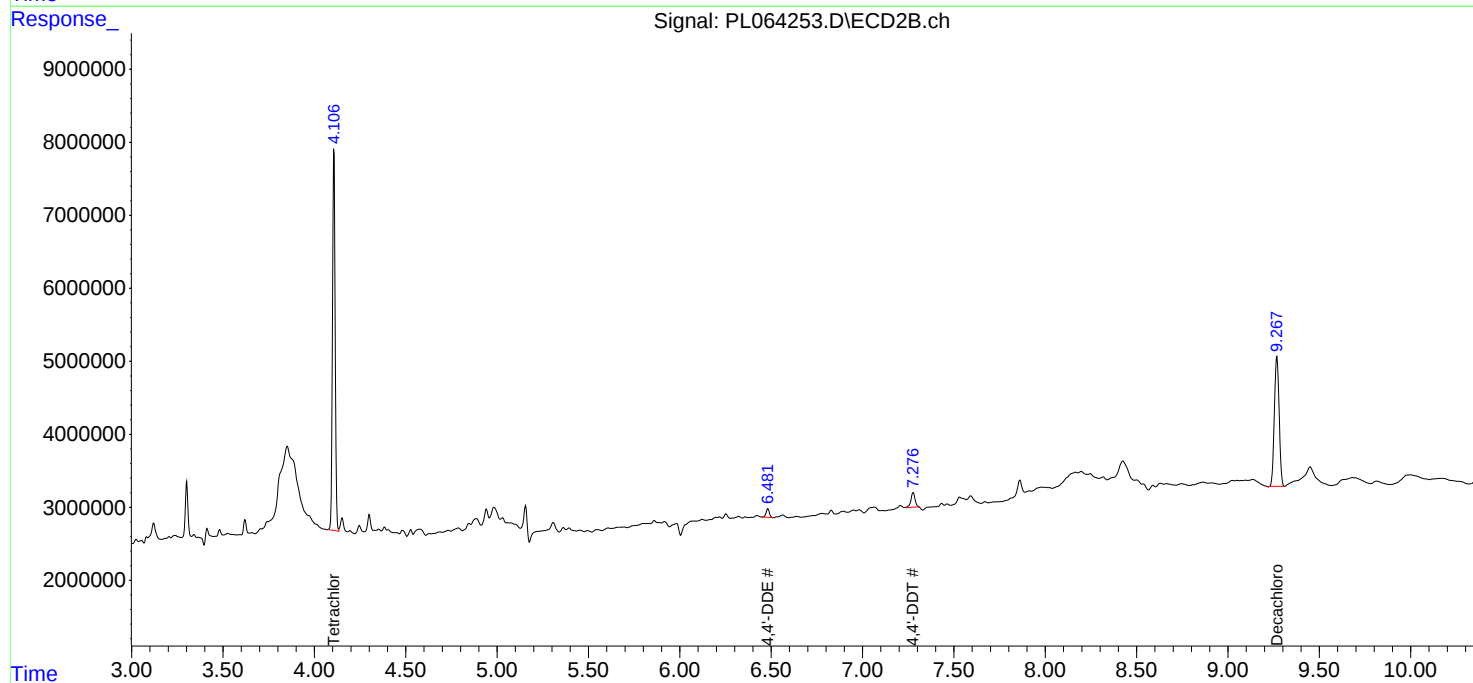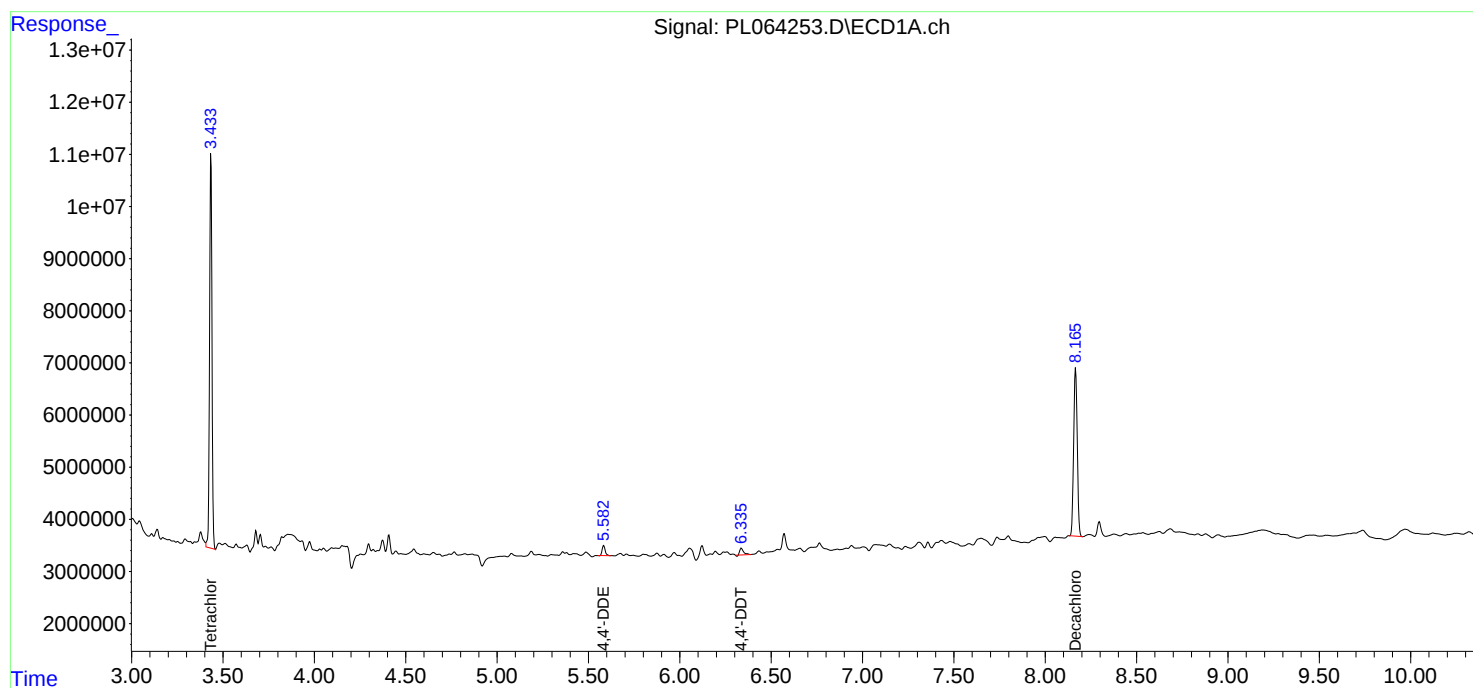

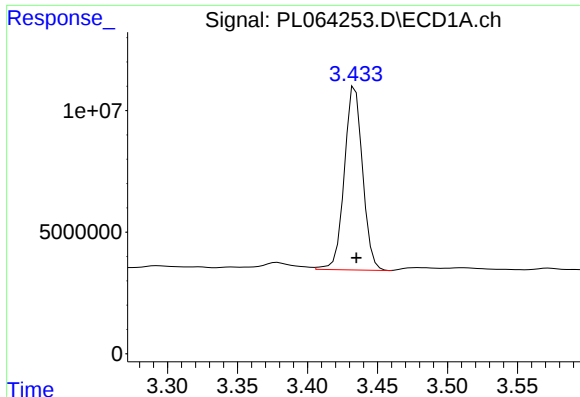


#1 Tetrachloro-m-xylene

R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 68436637
Conc: 22.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PILE-2-(1.5-2.0)


Manual Integrations
APPROVED

Ankita
1/21/2021 3:18:23 PM

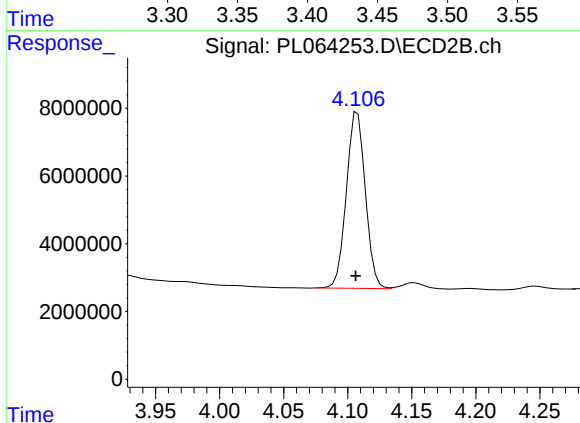


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.001 min
Response: 53618249
Conc: 20.97 ng/ml

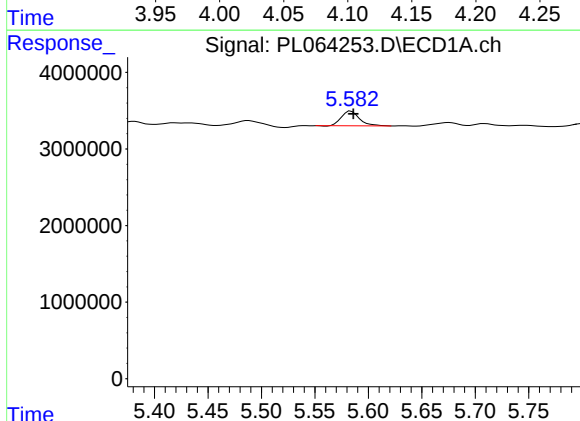


#12 4,4'-DDE

R.T.: 5.584 min
Delta R.T.: -0.002 min
Response: 2260274
Conc: 0.64 ng/ml

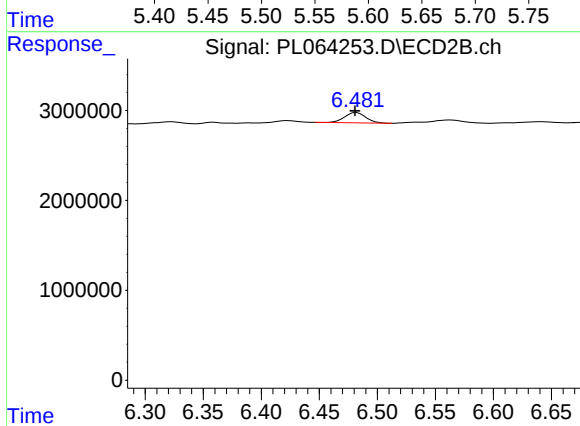

#12 4,4'-DDE

R.T.: 6.482 min
Delta R.T.: 0.002 min
Response: 1468025
Conc: 0.55 ng/ml

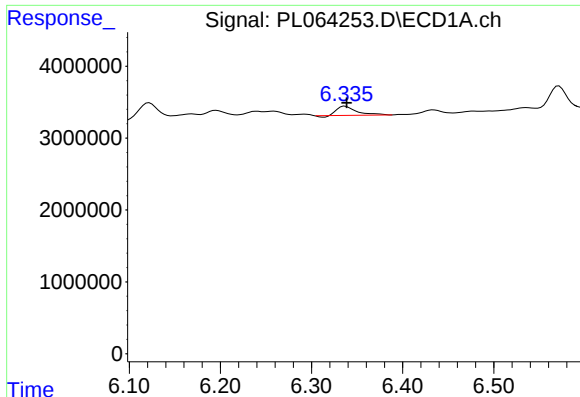


#17 4,4'-DDT

R.T.: 6.337 min
Delta R.T.: -0.002 min
Response: 1845111
Conc: 0.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PILE-2-(1.5-2.0)


Manual Integrations
APPROVED

Ankita
1/21/2021 3:18:23 PM

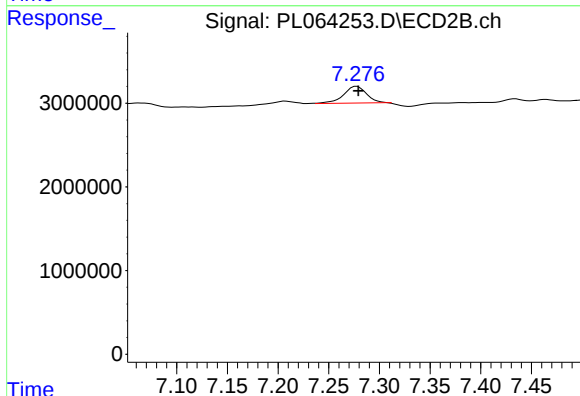


#17 4,4'-DDT

R.T.: 7.276 min
Delta R.T.: -0.003 min
Response: 3190297
Conc: 1.41 ng/ml m

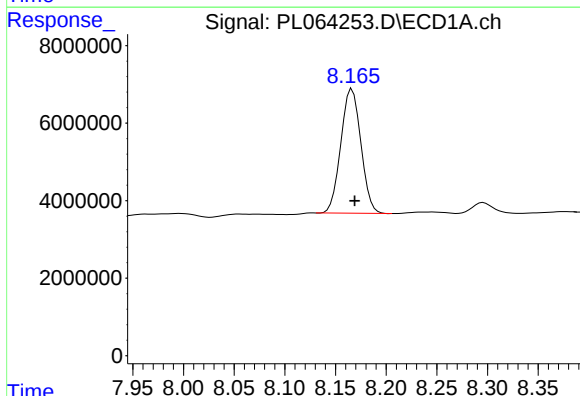

#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: -0.002 min
Response: 44136035
Conc: 14.46 ng/ml

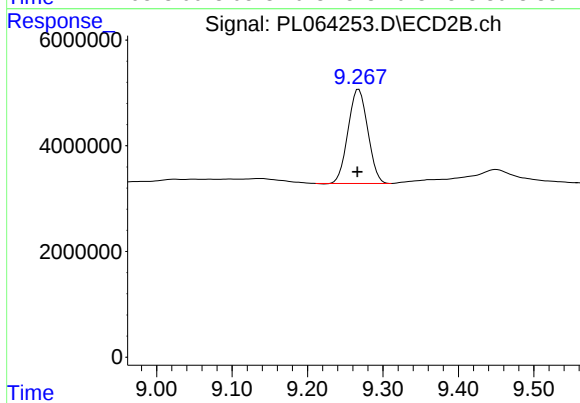

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.002 min
Response: 32319745
Conc: 13.62 ng/ml