

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012022\
 Data File : PL072110.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2022 08:33
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:18:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.493	10373303	31794770	18.684	19.577
28)	SA Decachlor...	10.320	11.387	16481547	29401721	18.551	18.222
Target Compounds							
7)	B delta-BHC	0.000	7.018f	0	207023	N.D.	0.084 #
8)	B Heptachlo...	0.000	7.963	0	1822728	N.D.	0.910 #
9)	A Endosulfan I	0.000	8.372	0	133613	N.D.	0.074 #
10)	B gamma-Chl...	0.000	8.230	0	682786	N.D.	0.338 #
11)	B alpha-Chl...	0.000	8.302	0	1257343	N.D.	0.634 #
14)	MA Endrin	8.002f	0.000	164992	0	0.235	N.D. #
15)	B Endosulfa...	0.000	9.146f	0	352109	N.D.	0.205 #
16)	A 4,4'-DDD	0.000	9.068f	0	205671	N.D.	0.144 #
18)	B Endrin al...	0.000	9.288f	0	143526	N.D.	0.116 #
19)	B Endosulfa...	0.000	9.497	0	55367	N.D.	0.035 #
25)	Chlordane-3	0.000	8.230	0	682786	N.D.	2.458 #
26)	Chlordane-4	0.000	8.302	0	1257343	N.D.	3.786 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012022\
Data File : PL072110.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2022 08:33
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:18:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

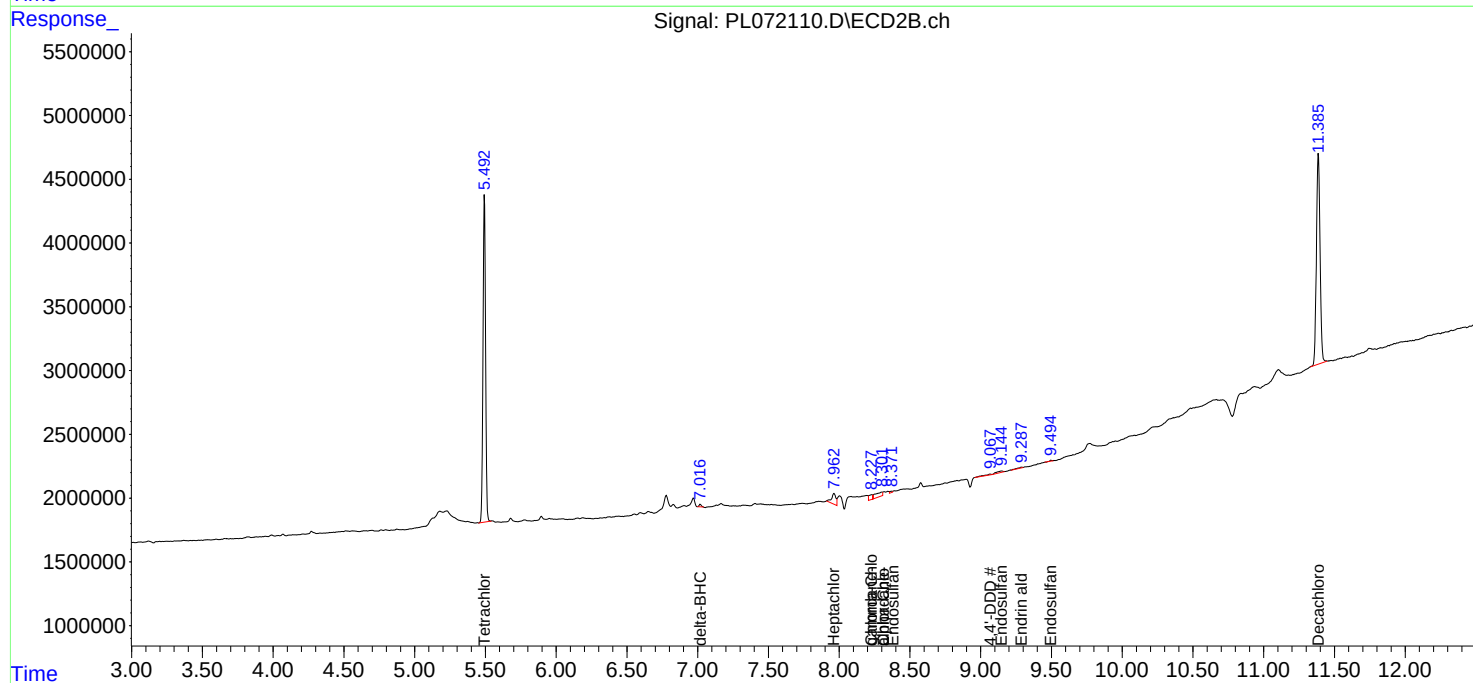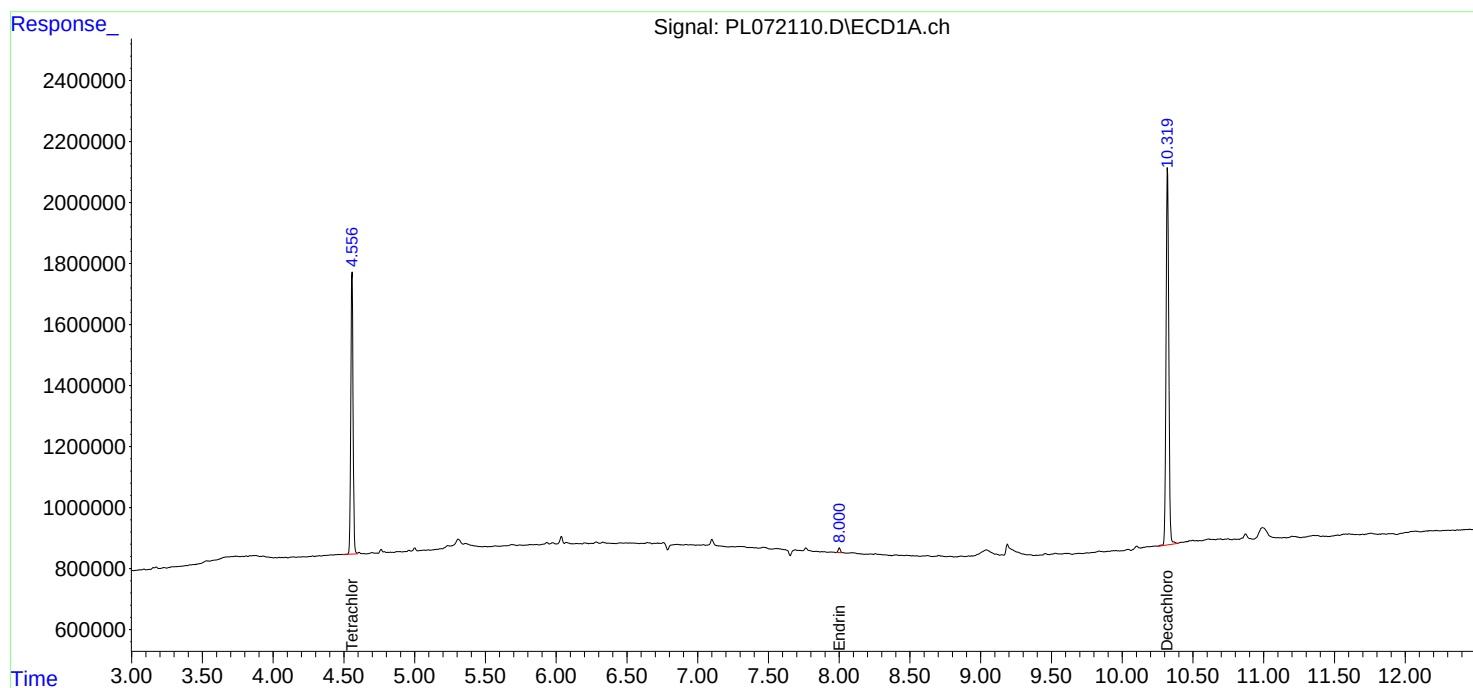


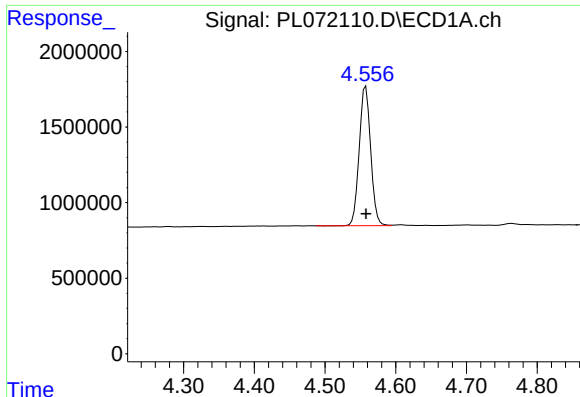

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.000 min
Response: 10373303
Conc: 18.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

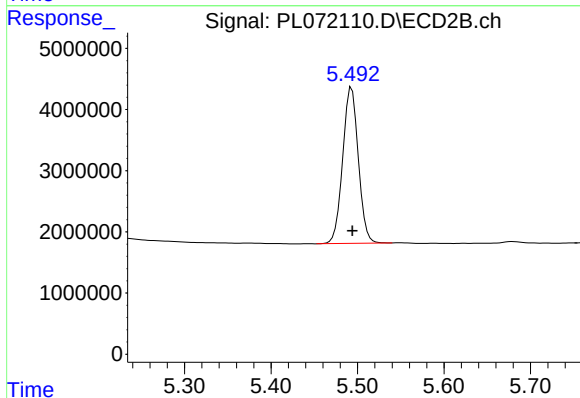


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 31794770
Conc: 19.58 ng/ml

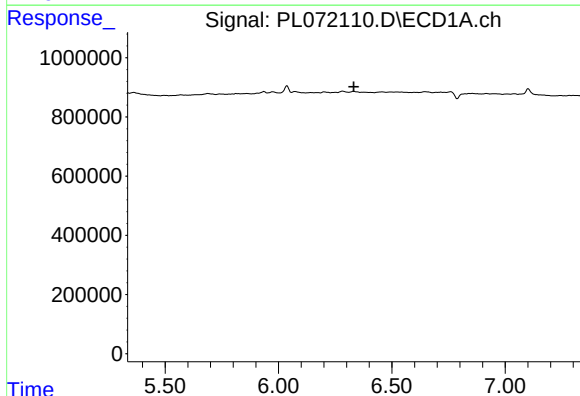


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

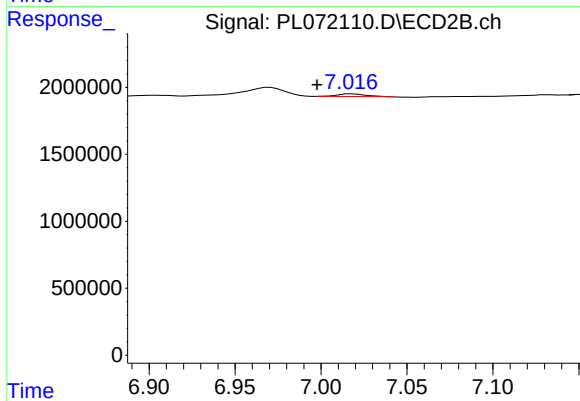

#7 delta-BHC


R.T.: 7.018 min
Delta R.T.: 0.020 min
Response: 207023
Conc: 0.08 ng/ml

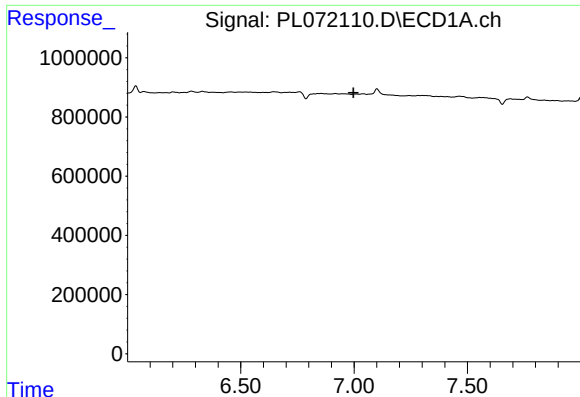

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.998 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

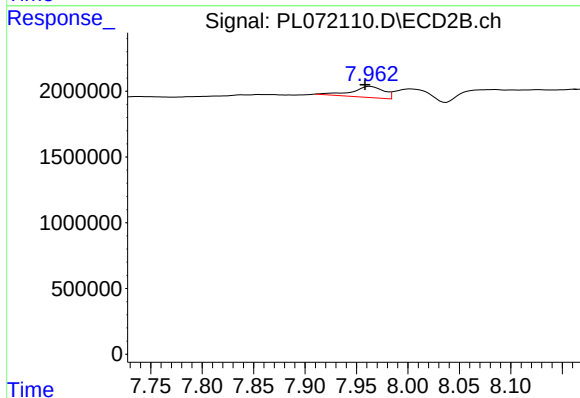


#8 Heptachlor epoxide

R.T.: 7.963 min
Delta R.T.: 0.005 min
Response: 1822728
Conc: 0.91 ng/ml

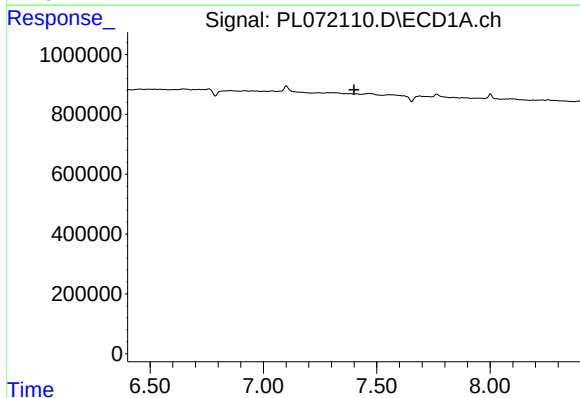


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

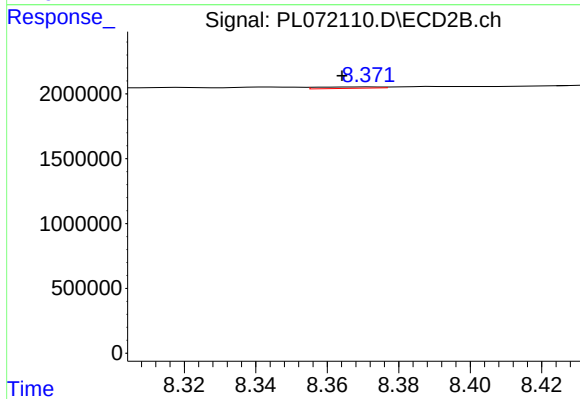

#9 Endosulfan I


R.T.: 8.372 min
Delta R.T.: 0.008 min
Response: 133613
Conc: 0.07 ng/ml

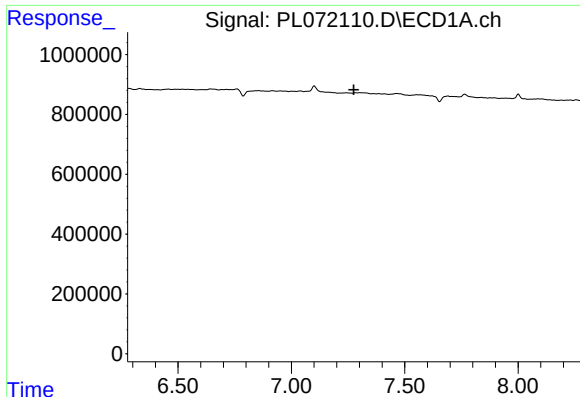

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

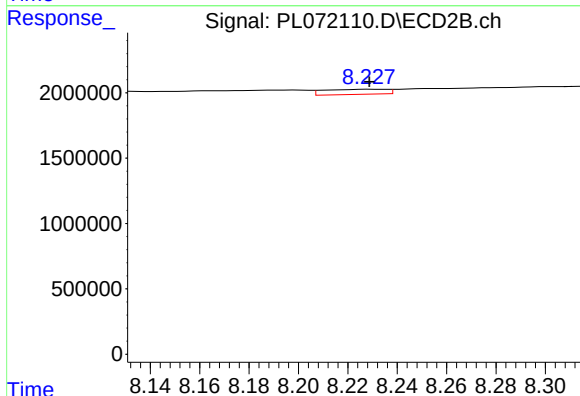


#10 gamma-Chlordane

R.T.: 8.230 min
Delta R.T.: 0.002 min
Response: 682786
Conc: 0.34 ng/ml

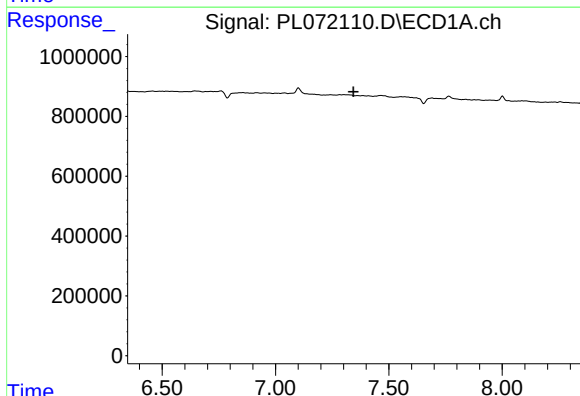


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

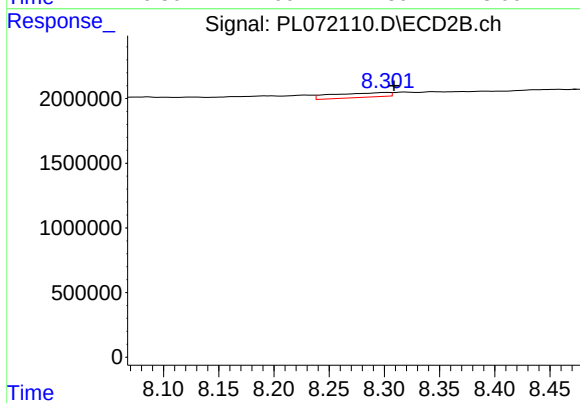

#11 alpha-Chlordane


R.T.: 8.302 min
Delta R.T.: -0.006 min
Response: 1257343
Conc: 0.63 ng/ml

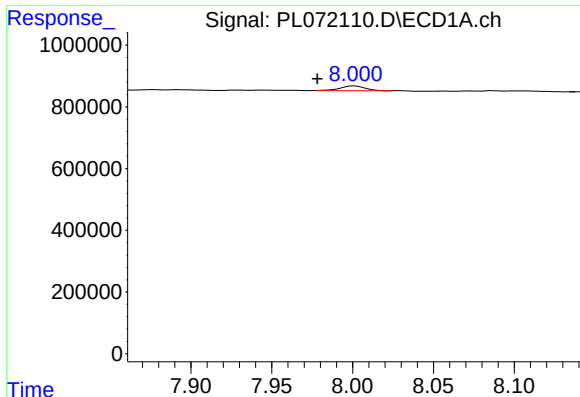

#14 Endrin


R.T.: 8.002 min
Delta R.T.: 0.023 min
Response: 164992
Conc: 0.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

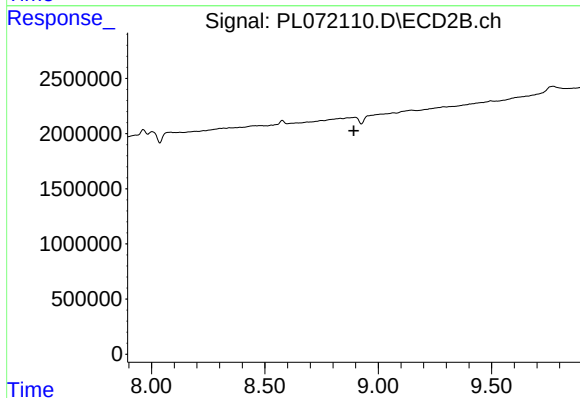


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.893 min
Response: 0
Conc: N.D.

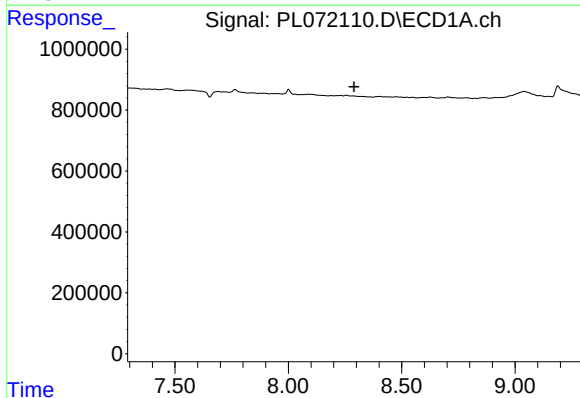


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.291 min
Response: 0
Conc: N.D.

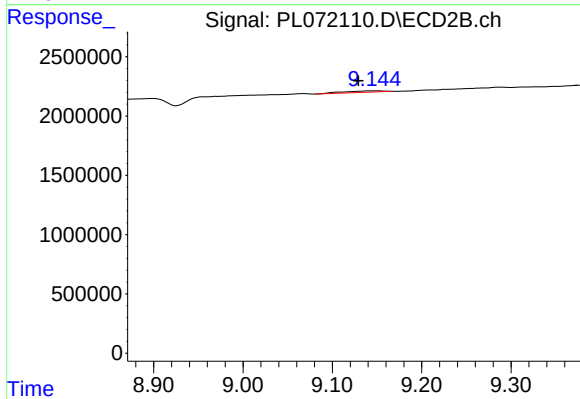

#15 Endosulfan II


R.T.: 9.146 min
Delta R.T.: 0.017 min
Response: 352109
Conc: 0.21 ng/ml

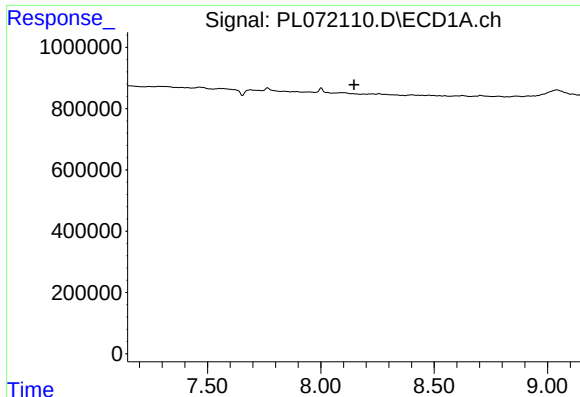

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

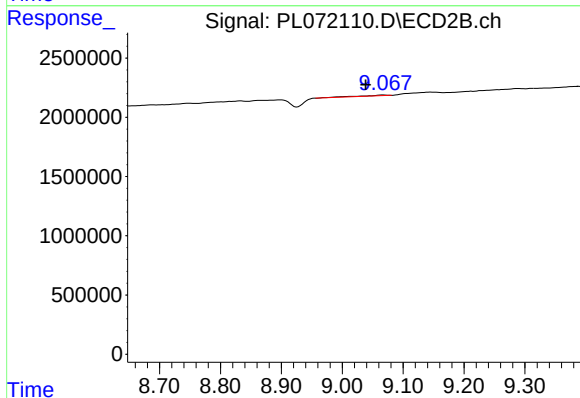


#16 4,4'-DDD

R.T.: 9.068 min
Delta R.T.: 0.029 min
Response: 205671
Conc: 0.14 ng/ml

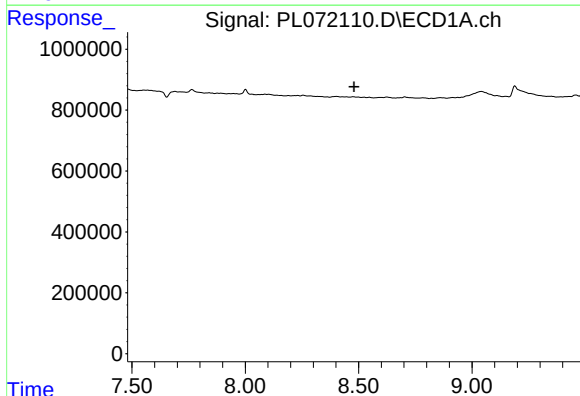


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

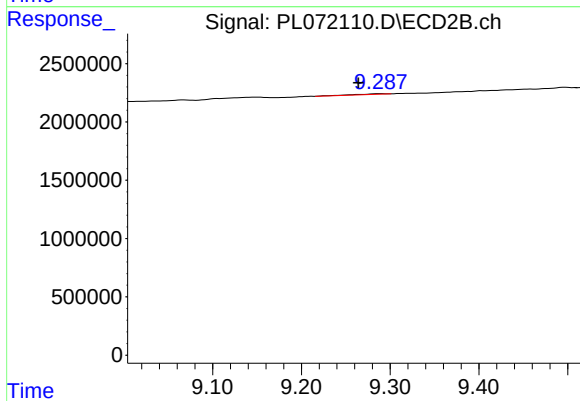

#18 Endrin aldehyde


R.T.: 9.288 min
Delta R.T.: 0.024 min
Response: 143526
Conc: 0.12 ng/ml

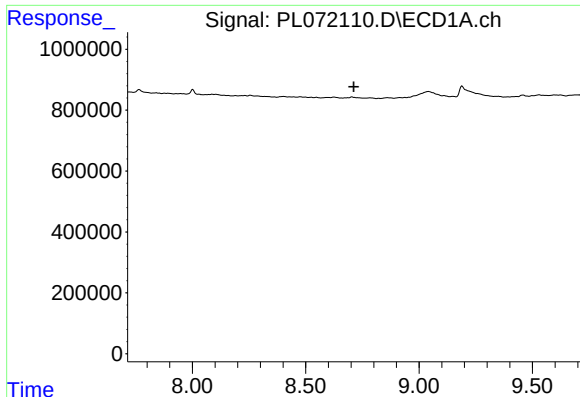

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

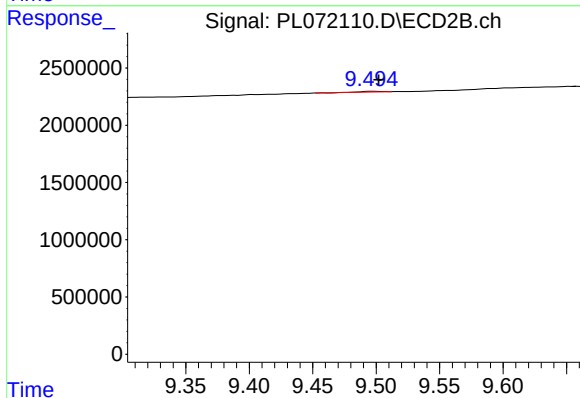


#19 Endosulfan Sulfate

R.T.: 9.497 min
Delta R.T.: -0.005 min
Response: 55367
Conc: 0.04 ng/ml

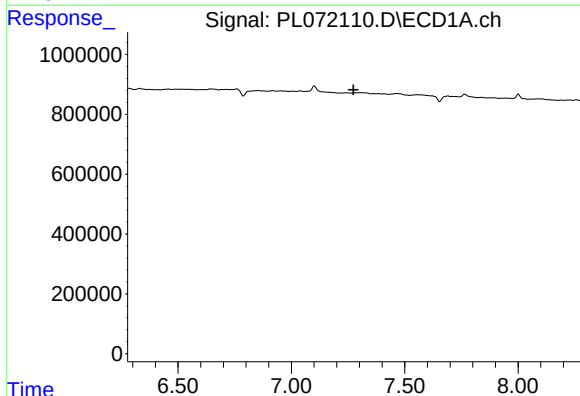


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

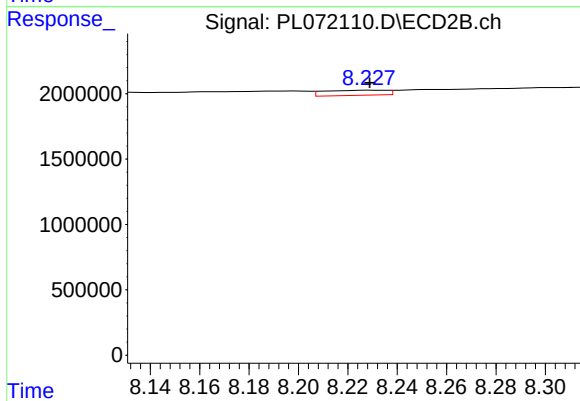

#25 Chlordane-3


R.T.: 8.230 min
Delta R.T.: 0.001 min
Response: 682786
Conc: 2.46 ng/ml

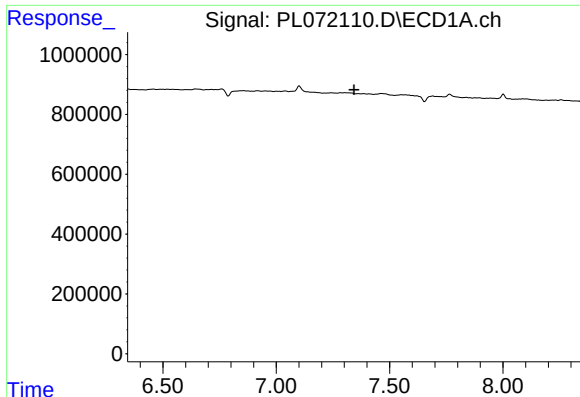

#26 Chlorine-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

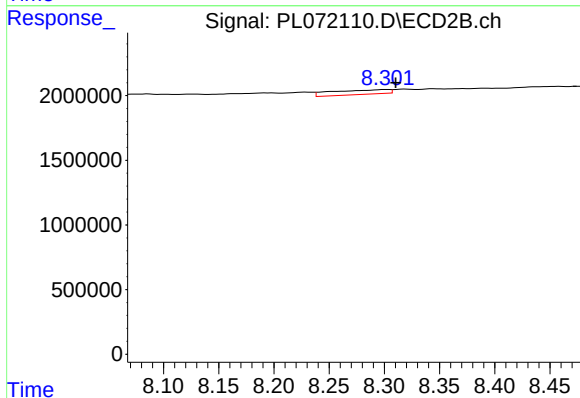


#26 Chlorine-4

R.T.: 8.302 min
Delta R.T.: -0.008 min
Response: 1257343
Conc: 3.79 ng/ml

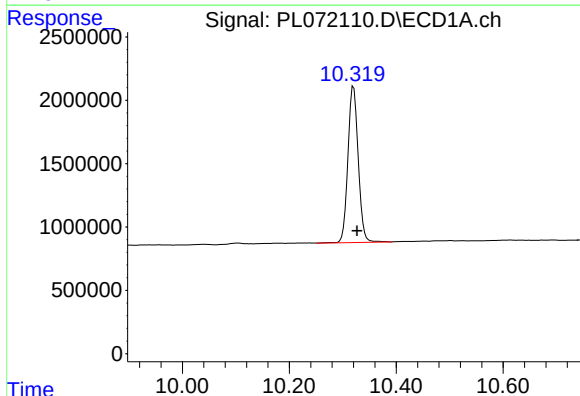

#28 Decachlorobiphenyl

R.T.: 10.320 min
Delta R.T.: -0.006 min
Response: 16481547
Conc: 18.55 ng/ml

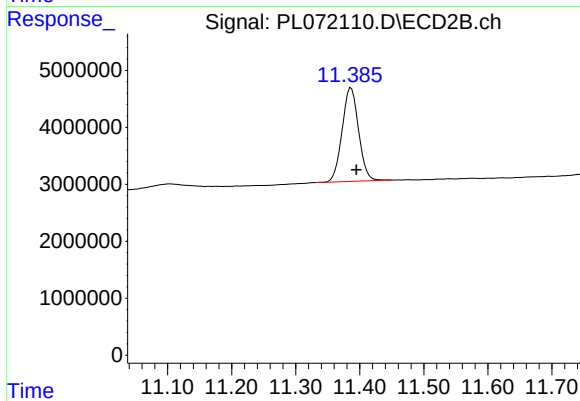

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: -0.008 min
Response: 29401721
Conc: 18.22 ng/ml