

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012022\
 Data File : PL072128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2022 15:07
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:21:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	10528372	31033066	18.964	19.108
28)	SA Decachlor...	10.317	11.384	15957425	29211139	17.961	18.104
Target Compounds							
7)	B delta-BHC	0.000	7.017f	0	778727	N.D.	0.317 #
8)	B Heptachlo...	0.000	7.962	0	846726	N.D.	0.423 #
9)	A Endosulfan I	0.000	8.364	0	73137	N.D.	0.040 #
10)	B gamma-Chl...	0.000	8.226	0	2167818	N.D.	1.073 #
11)	B alpha-Chl...	0.000	8.324	0	985181	N.D.	0.497 #
13)	MA Dieldrin	7.680	0.000	45557	0	0.060	N.D. #
14)	MA Endrin	7.998f	0.000	474066	0	0.677	N.D. #
15)	B Endosulfa...	0.000	9.147f	0	400854	N.D.	0.234 #
25)	Chlordane-3	0.000	8.226	0	2167818	N.D.	7.803 #
26)	Chlordane-4	0.000	8.324	0	985181	N.D.	2.967 #
27)	Chlordane-5	0.000	9.199	0	94863	N.D.	1.555 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012022\
Data File : PL072128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2022 15:07
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:21:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

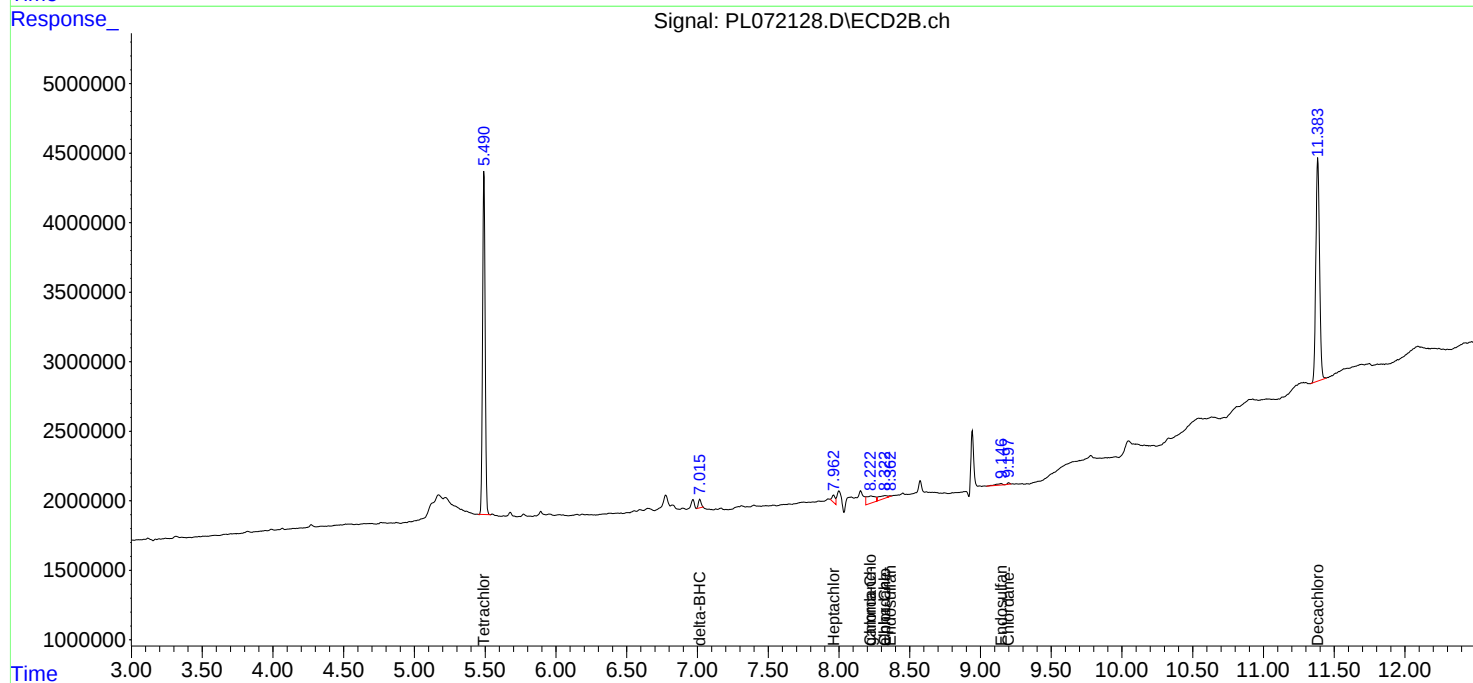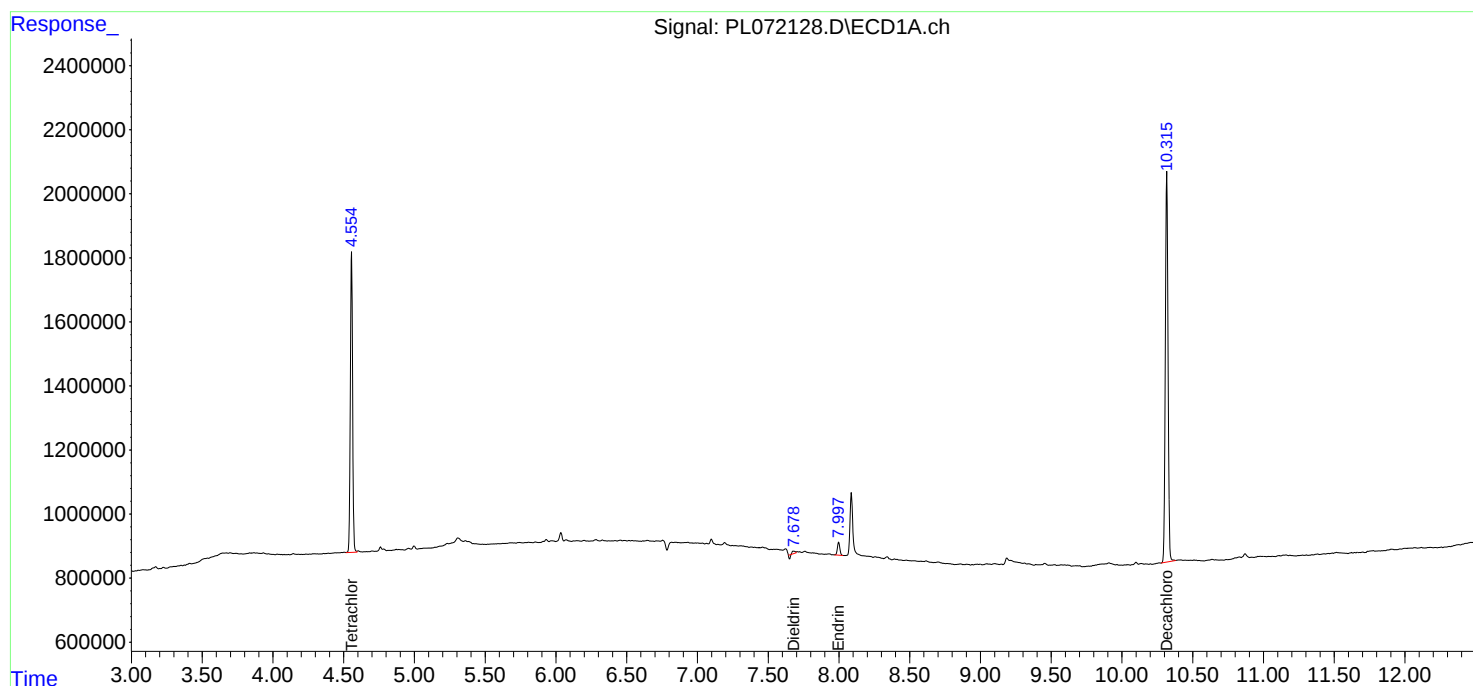


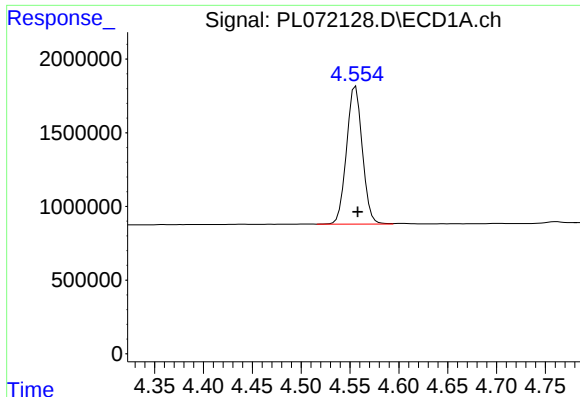

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 10528372
Conc: 18.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

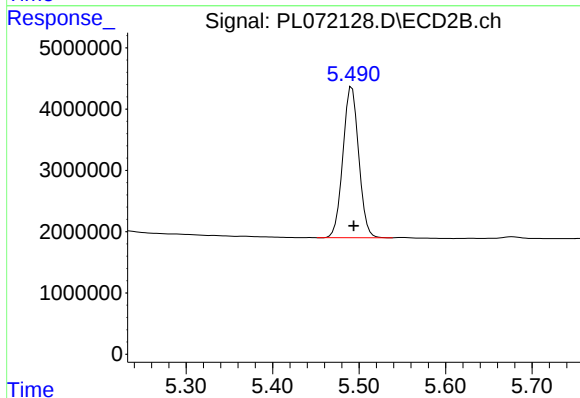


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 31033066
Conc: 19.11 ng/ml

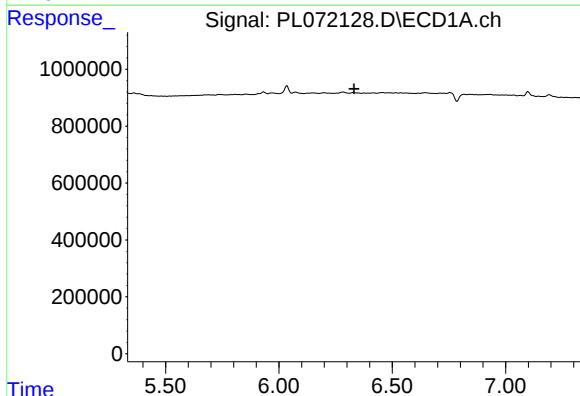


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

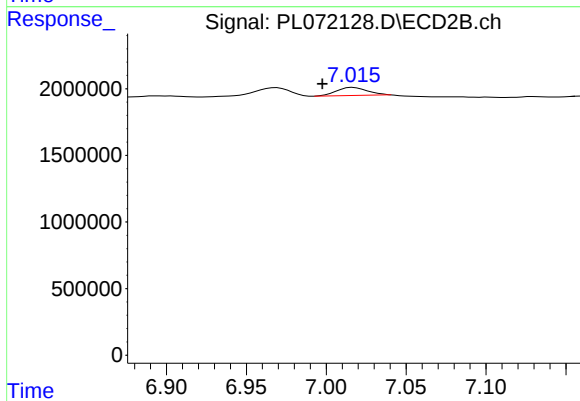

#7 delta-BHC


R.T.: 7.017 min
Delta R.T.: 0.019 min
Response: 778727
Conc: 0.32 ng/ml

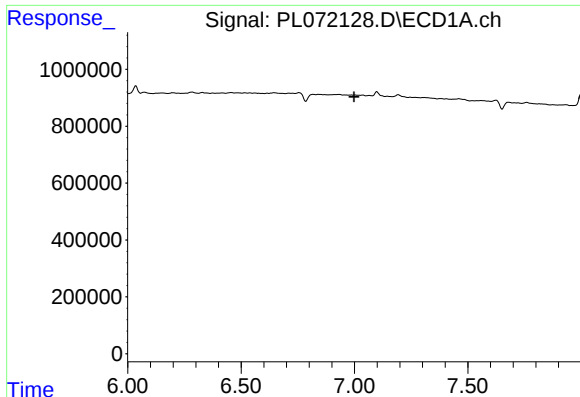

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.998 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

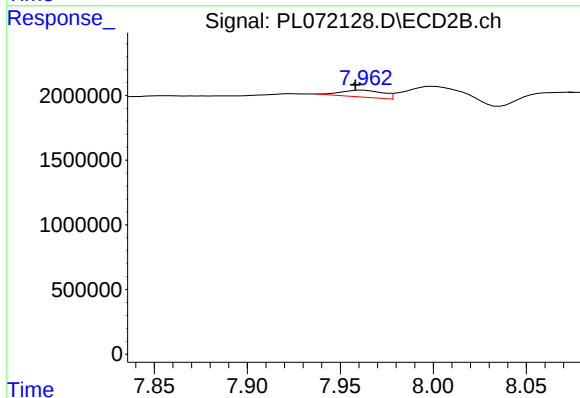


#8 Heptachlor epoxide

R.T.: 7.962 min
Delta R.T.: 0.004 min
Response: 846726
Conc: 0.42 ng/ml

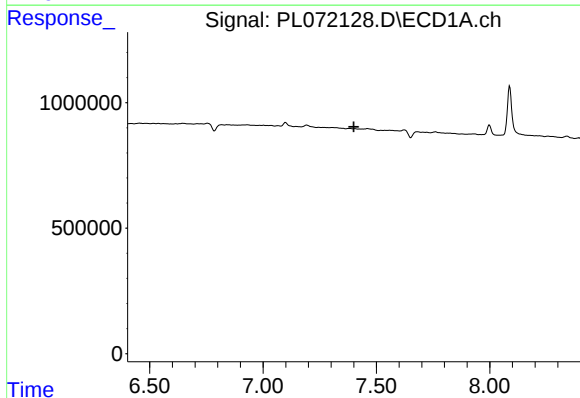


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

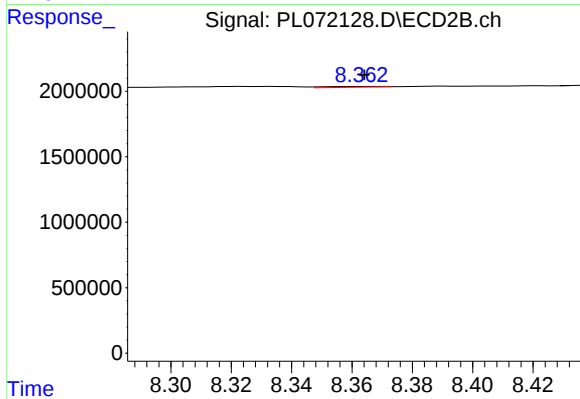

#9 Endosulfan I


R.T.: 8.364 min
Delta R.T.: 0.000 min
Response: 73137
Conc: 0.04 ng/ml

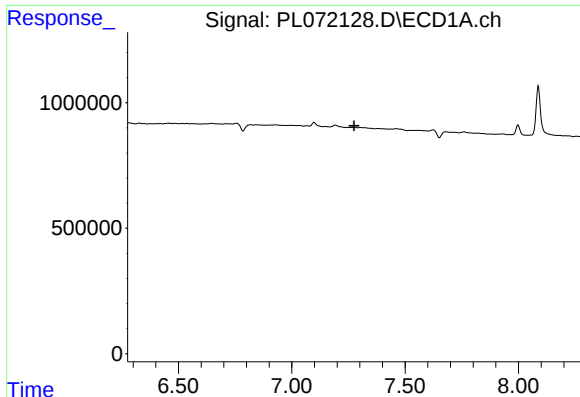

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

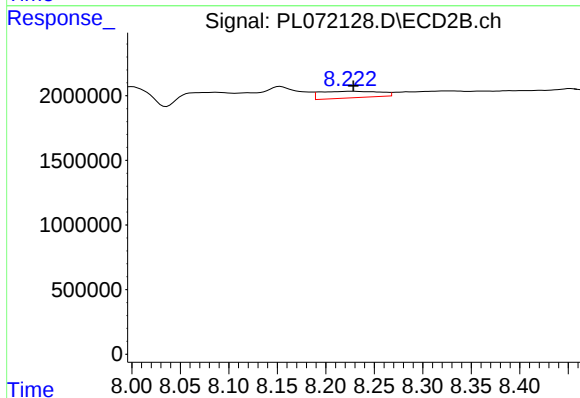


#10 gamma-Chlordane

R.T.: 8.226 min
Delta R.T.: -0.003 min
Response: 2167818
Conc: 1.07 ng/ml

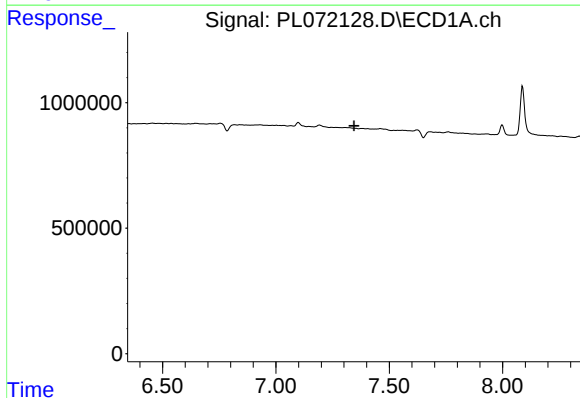


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

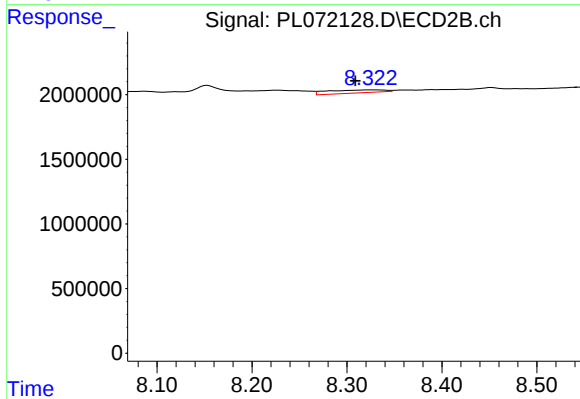

#11 alpha-Chlordane


R.T.: 8.324 min
Delta R.T.: 0.015 min
Response: 985181
Conc: 0.50 ng/ml

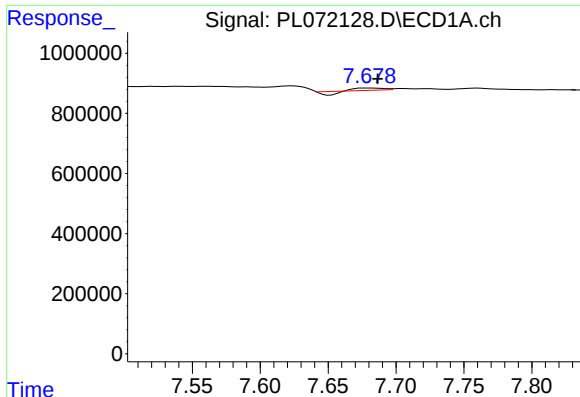

#13 Dieldrin


R.T.: 7.680 min
Delta R.T.: -0.007 min
Response: 45557
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

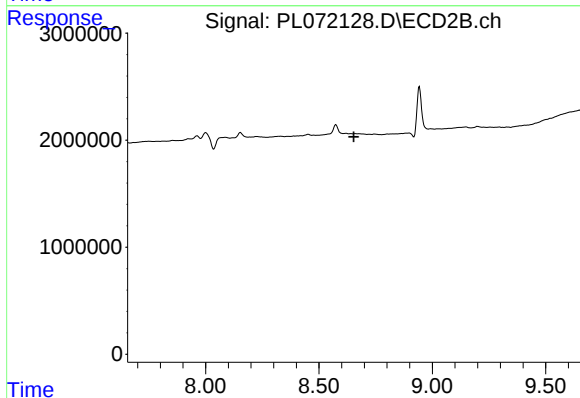


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.653 min
Response: 0
Conc: N.D.

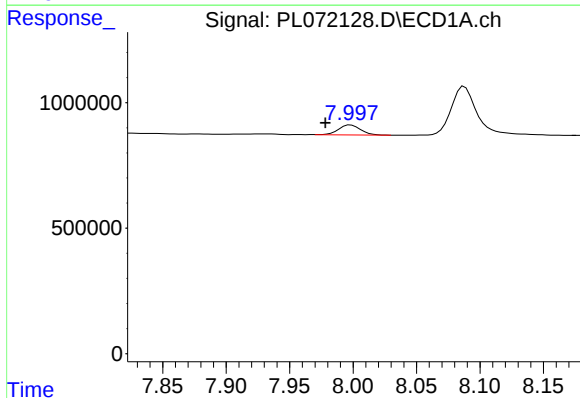


#14 Endrin

R.T.: 7.998 min
Delta R.T.: 0.020 min
Response: 474066
Conc: 0.68 ng/ml

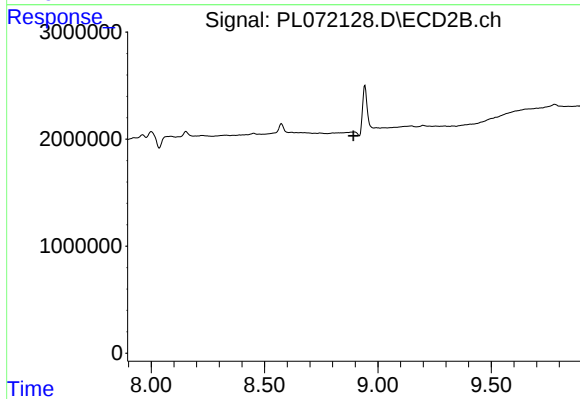

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.893 min
Response: 0
Conc: N.D.

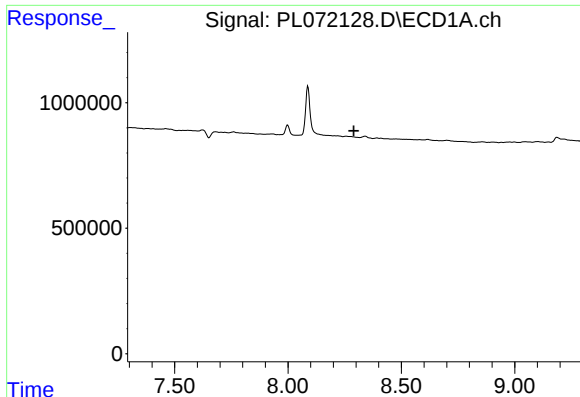

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

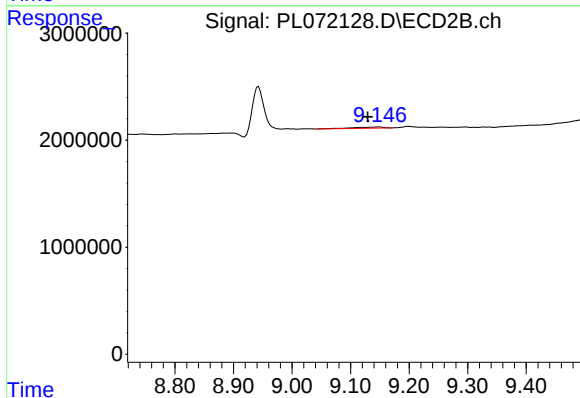


#15 Endosulfan II

R.T.: 9.147 min
Delta R.T.: 0.018 min
Response: 400854
Conc: 0.23 ng/ml

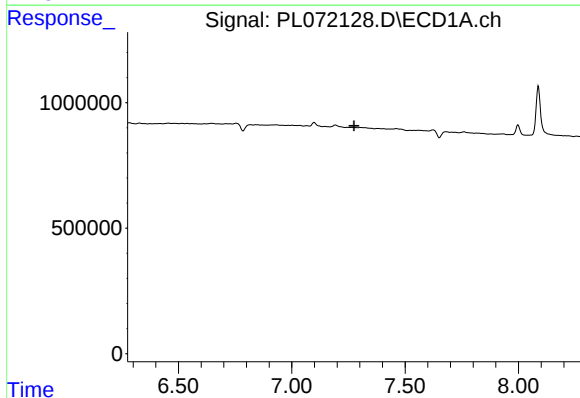


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

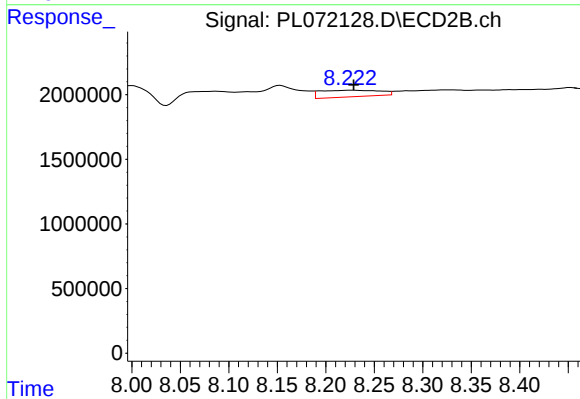

#25 Chlordane-3


R.T.: 8.226 min
Delta R.T.: -0.003 min
Response: 2167818
Conc: 7.80 ng/ml

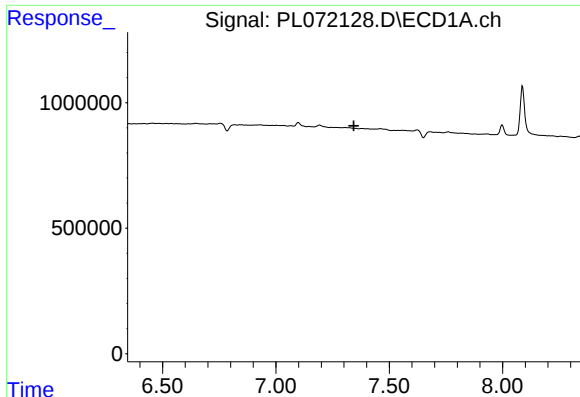

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

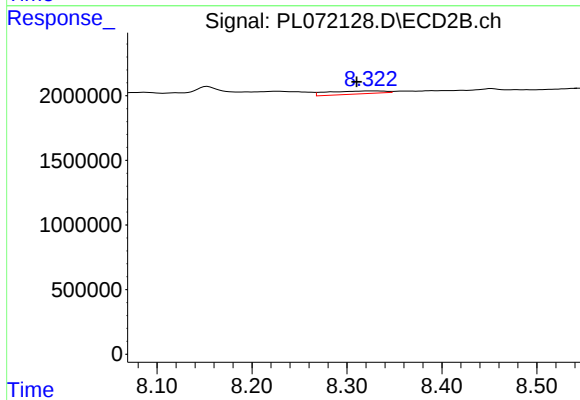


#26 Chlordane-4

R.T.: 8.324 min
Delta R.T.: 0.013 min
Response: 985181
Conc: 2.97 ng/ml

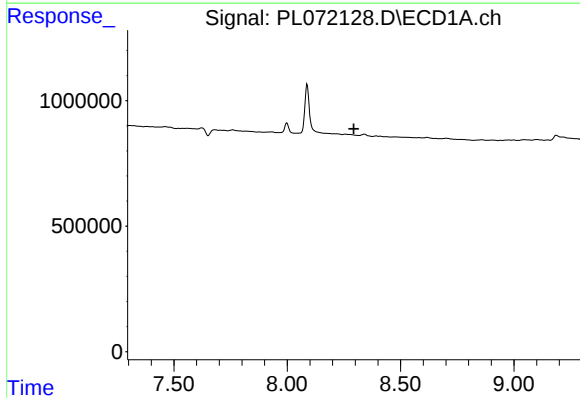


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

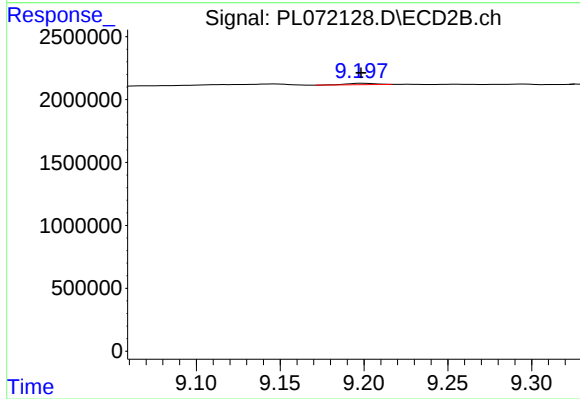

#27 Chlordane-5


R.T.: 9.199 min
Delta R.T.: 0.000 min
Response: 94863
Conc: 1.55 ng/ml

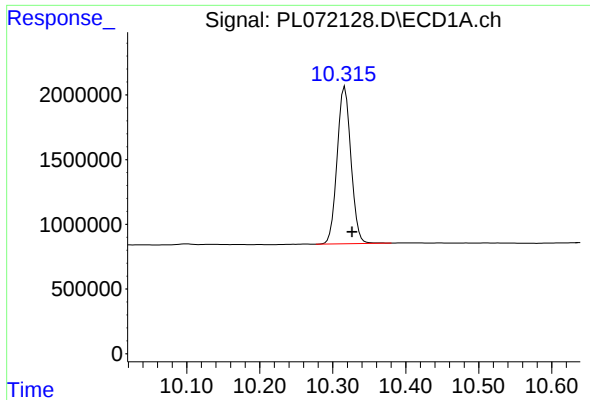

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: -0.010 min
Response: 15957425
Conc: 17.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

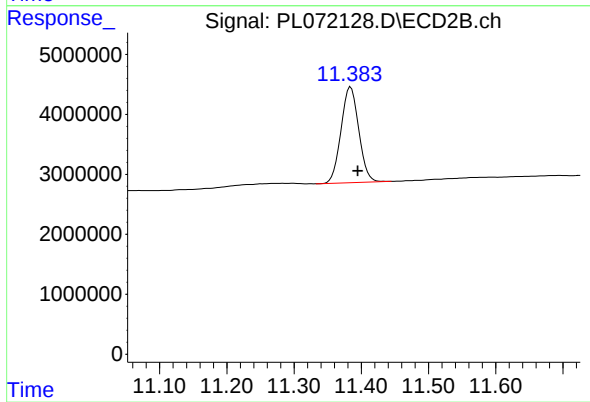

#28 Decachlorobiphenyl

R.T.: 11.384 min
Delta R.T.: -0.011 min
Response: 29211139
Conc: 18.10 ng/ml