

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012022\
 Data File : PL072130.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2022 15:40
 Operator : AR\AJ
 Sample : N1189-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:21:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	10760281	32213527	19.381	19.835
28)	SA Decachlor...	10.317	11.384	14569403	26616458	16.399	16.496
Target Compounds							
2)	A alpha-BHC	0.000	6.104f	0	135395	N.D.	0.056 #
7)	B delta-BHC	0.000	7.018f	0	458795	N.D.	0.186 #
9)	A Endosulfan I	0.000	8.388f	0	43119	N.D.	0.024 #
13)	MA Dieldrin	0.000	8.682f	0	182730	N.D.	0.093 #
15)	B Endosulfa...	0.000	9.146f	0	260237	N.D.	0.152 #
17)	MA 4,4'-DDT	0.000	9.331f	0	118100	N.D.	0.075 #
19)	B Endosulfa...	0.000	9.508	0	241860	N.D.	0.155 #
22)	Mirex	0.000	10.476	0	46835	N.D.	0.038 #
27)	Chlordane-5	0.000	9.183f	0	23339	N.D.	0.382 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012022\
Data File : PL072130.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2022 15:40
Operator : AR\AJ
Sample : N1189-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:21:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

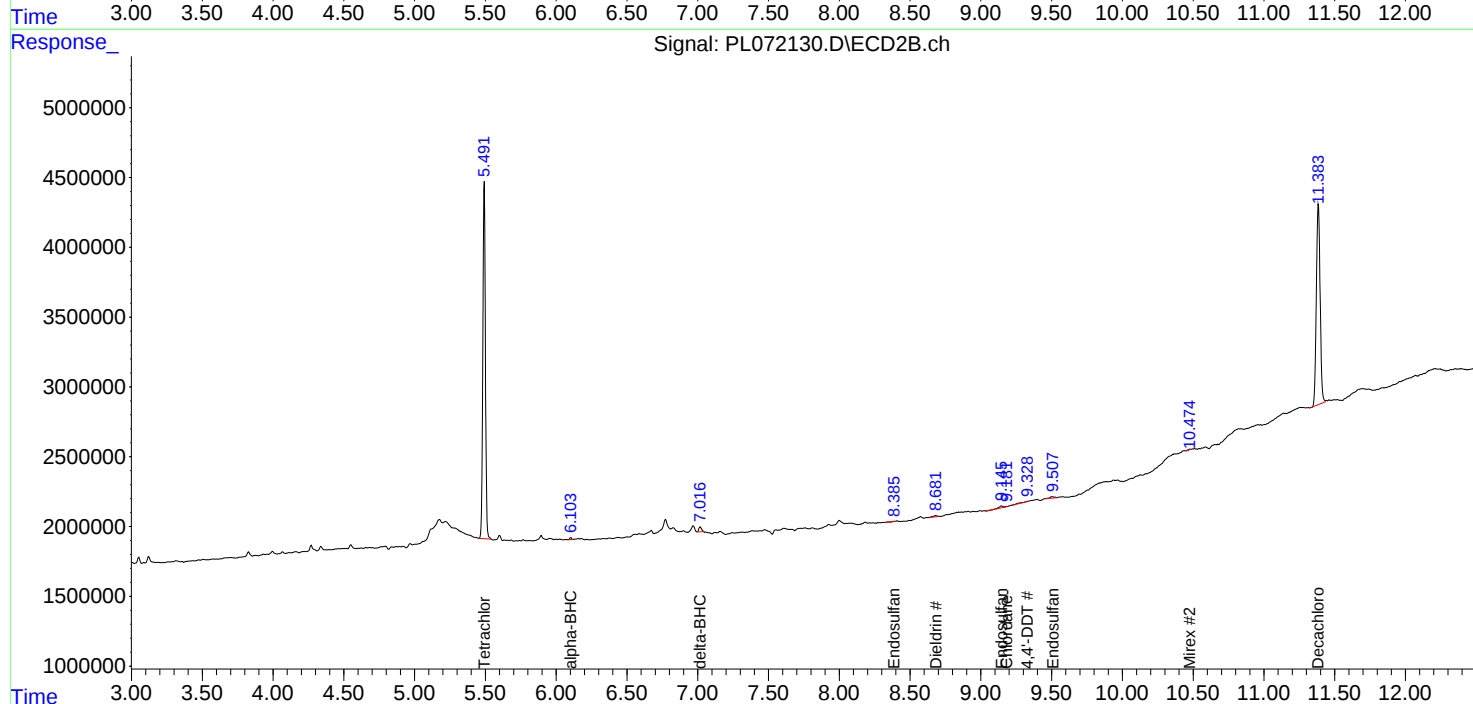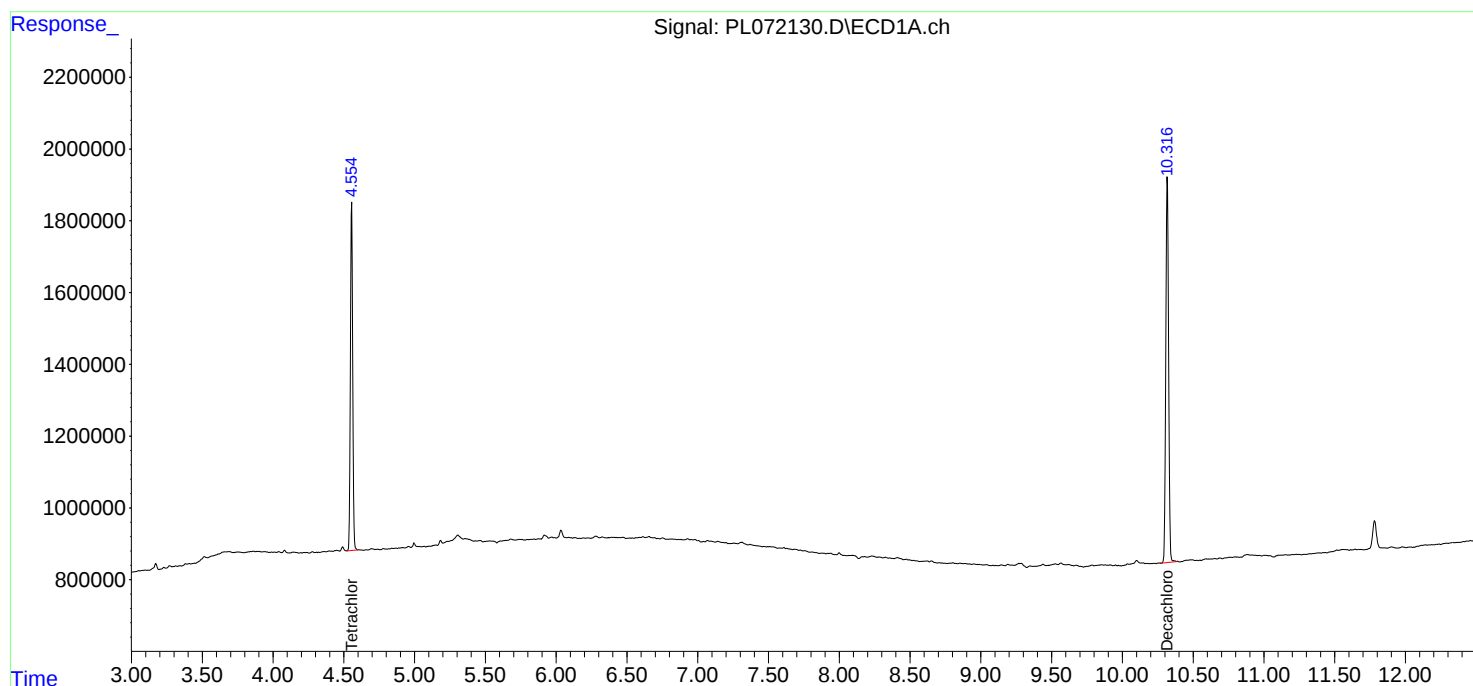


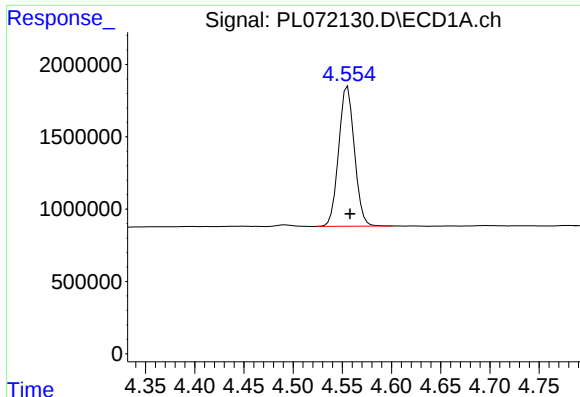

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 10760281
Conc: 19.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

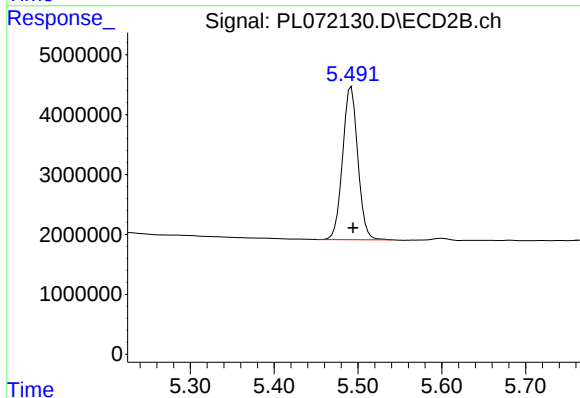


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 32213527
Conc: 19.83 ng/ml

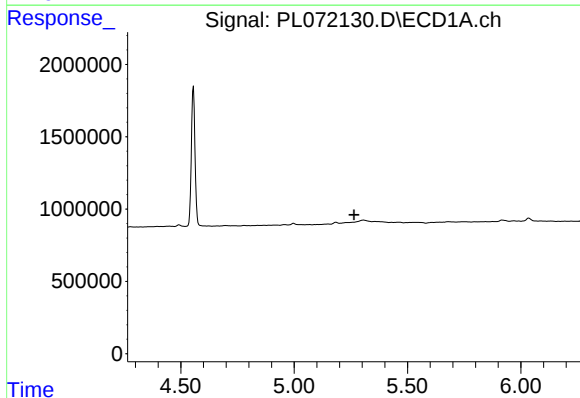


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.265 min
Response: 0
Conc: N.D.

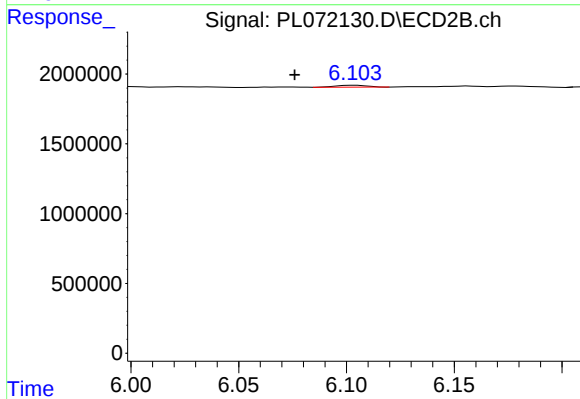

#2 alpha-BHC


R.T.: 6.104 min
Delta R.T.: 0.028 min
Response: 135395
Conc: 0.06 ng/ml

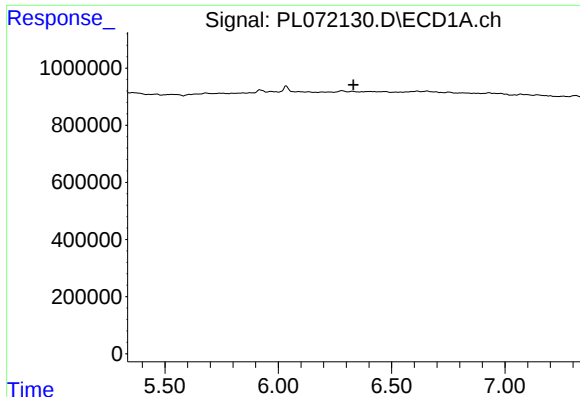

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

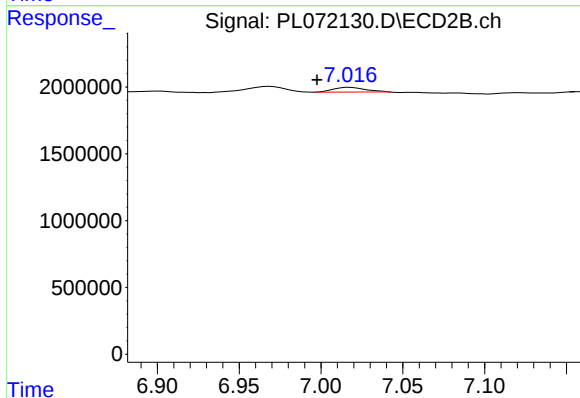


#7 delta-BHC

R.T.: 7.018 min
Delta R.T.: 0.020 min
Response: 458795
Conc: 0.19 ng/ml

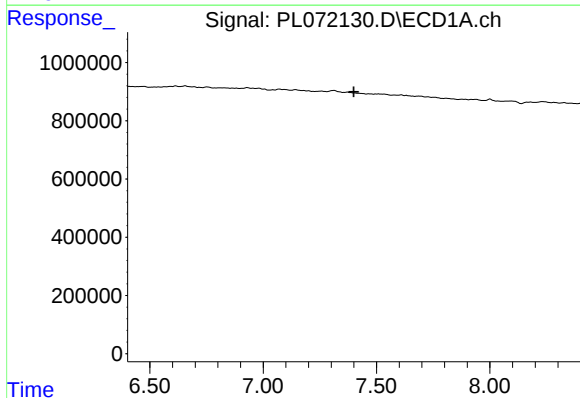


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.400 min
Response: 0
Conc: N.D.

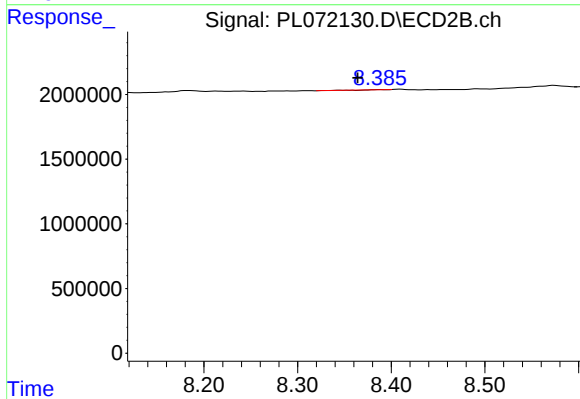

#9 Endosulfan I


R.T.: 8.388 min
Delta R.T.: 0.024 min
Response: 43119
Conc: 0.02 ng/ml

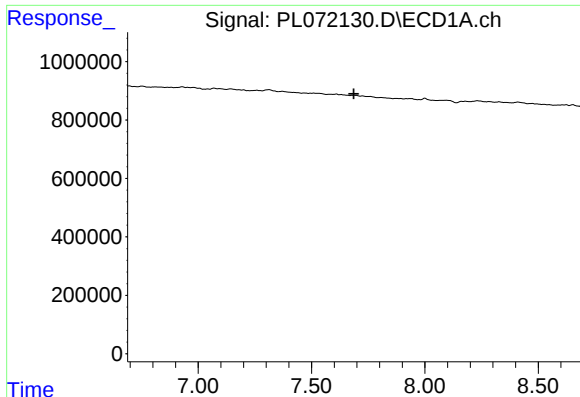

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.686 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

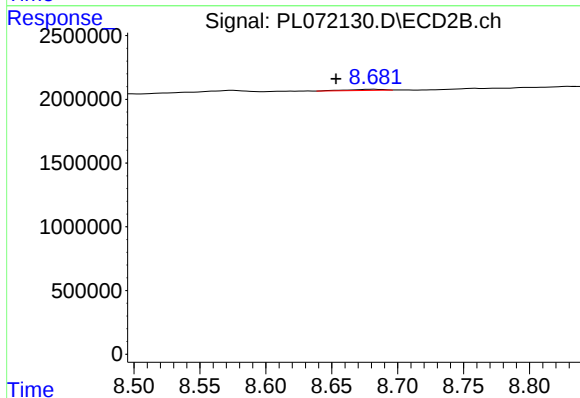


#13 Dieldrin

R.T.: 8.682 min
Delta R.T.: 0.029 min
Response: 182730
Conc: 0.09 ng/ml

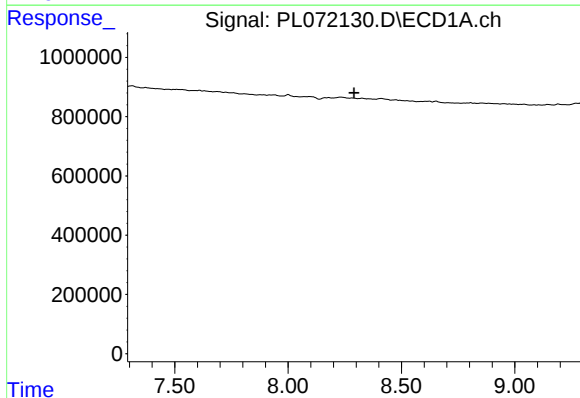


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

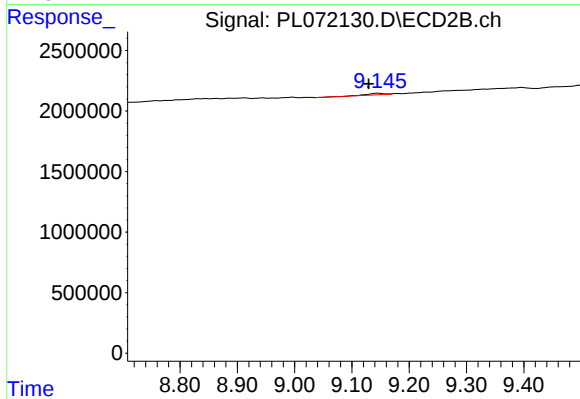

#15 Endosulfan II


R.T.: 9.146 min
Delta R.T.: 0.017 min
Response: 260237
Conc: 0.15 ng/ml

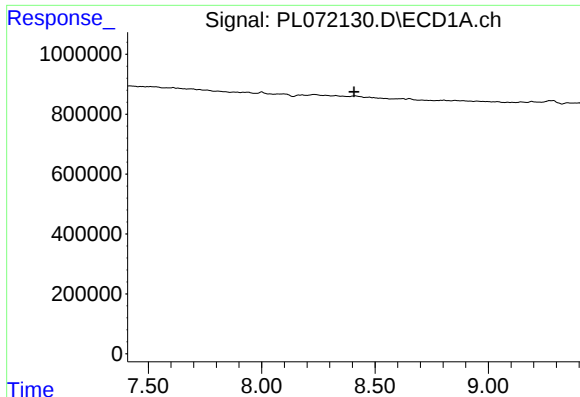

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

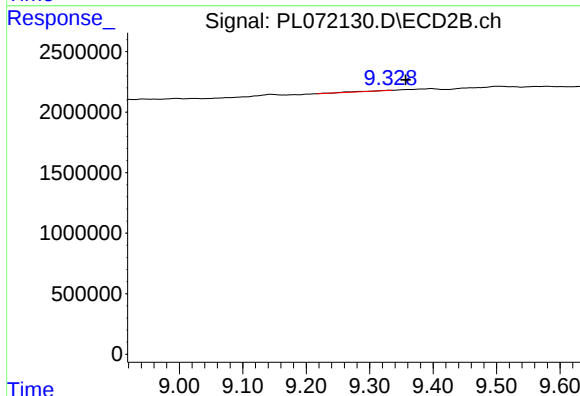


#17 4,4'-DDT

R.T.: 9.331 min
Delta R.T.: -0.026 min
Response: 118100
Conc: 0.07 ng/ml

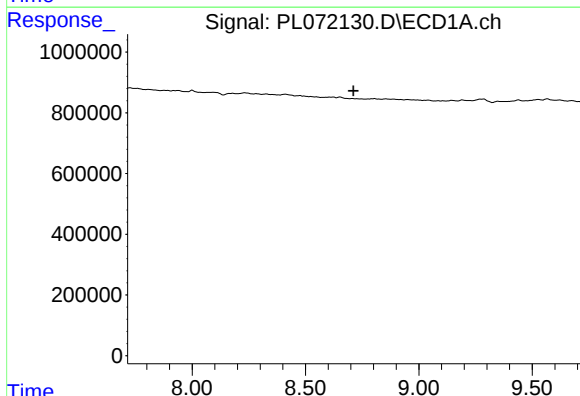


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

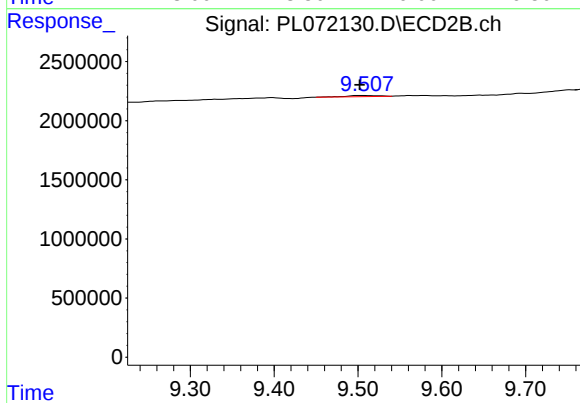

#19 Endosulfan Sulfate


R.T.: 9.508 min
Delta R.T.: 0.006 min
Response: 241860
Conc: 0.15 ng/ml

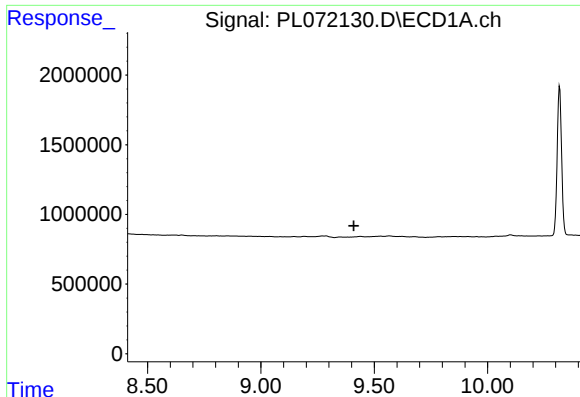

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.410 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

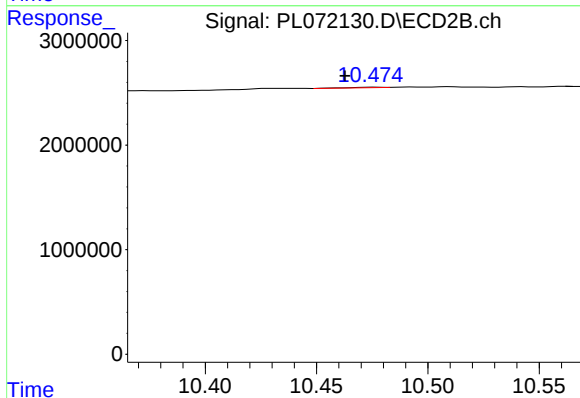


#22 Mirex

R.T.: 10.476 min
Delta R.T.: 0.013 min
Response: 46835
Conc: 0.04 ng/ml

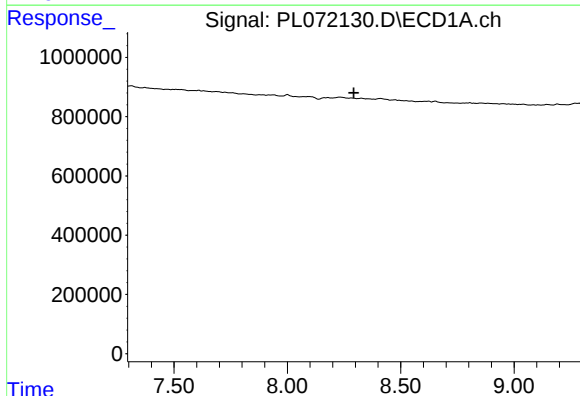


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

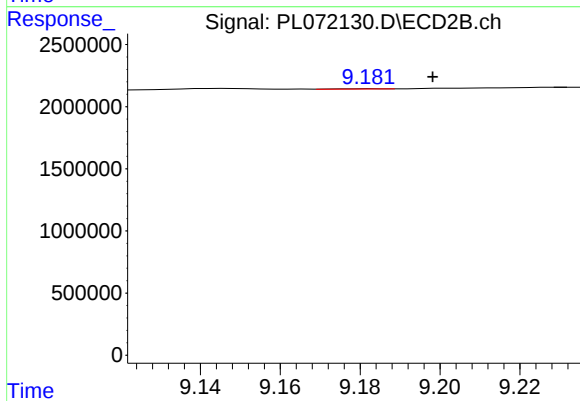

#27 Chlordane-5


R.T.: 9.183 min
Delta R.T.: -0.016 min
Response: 23339
Conc: 0.38 ng/ml

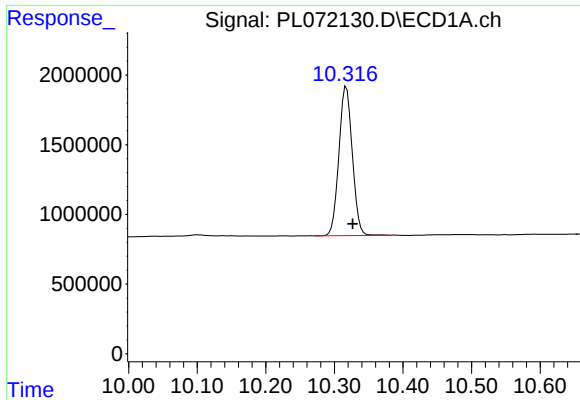

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: -0.009 min
Response: 14569403
Conc: 16.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

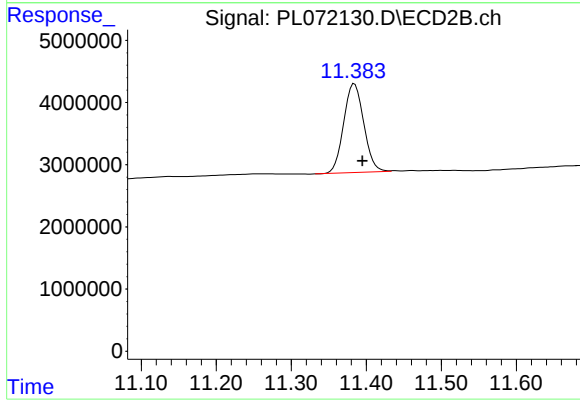

#28 Decachlorobiphenyl

R.T.: 11.384 min
Delta R.T.: -0.010 min
Response: 26616458
Conc: 16.50 ng/ml