

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012022\
 Data File : PL072133.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2022 16:29
 Operator : AR\AJ
 Sample : N1189-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:21:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	9826376	29313743	17.699	18.049
28)	SA Decachlor...	10.316	11.385	14201825	25852373	15.985	16.023
Target Compounds							
2)	A alpha-BHC	0.000	6.105f	0	141789	N.D.	0.059 #
7)	B delta-BHC	0.000	7.018f	0	548526	N.D.	0.223 #
9)	A Endosulfan I	0.000	8.379f	0	186480	N.D.	0.103 #
15)	B Endosulfa...	0.000	9.137	0	267484	N.D.	0.156 #
19)	B Endosulfa...	0.000	9.502	0	211227	N.D.	0.135 #
22)	Mirex	0.000	10.471	0	111158	N.D.	0.089 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012022\
Data File : PL072133.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2022 16:29
Operator : AR\AJ
Sample : N1189-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:21:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

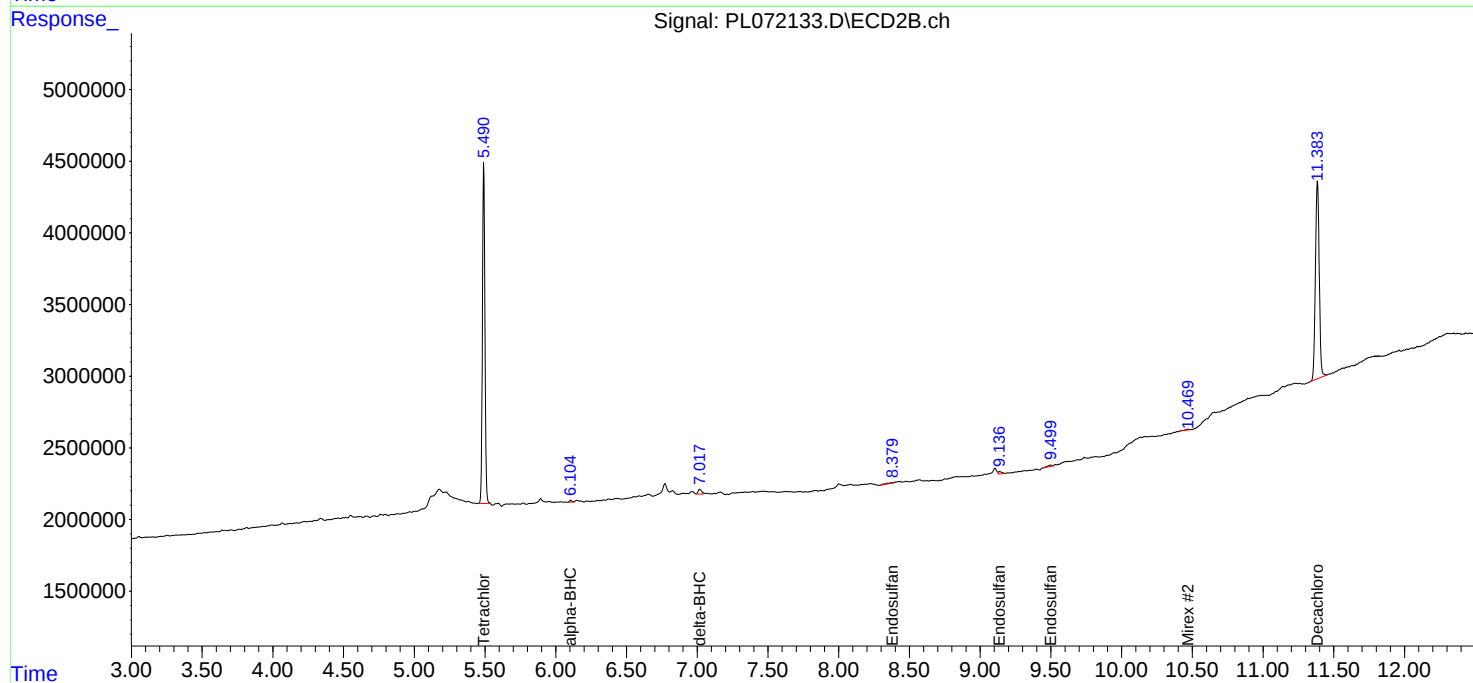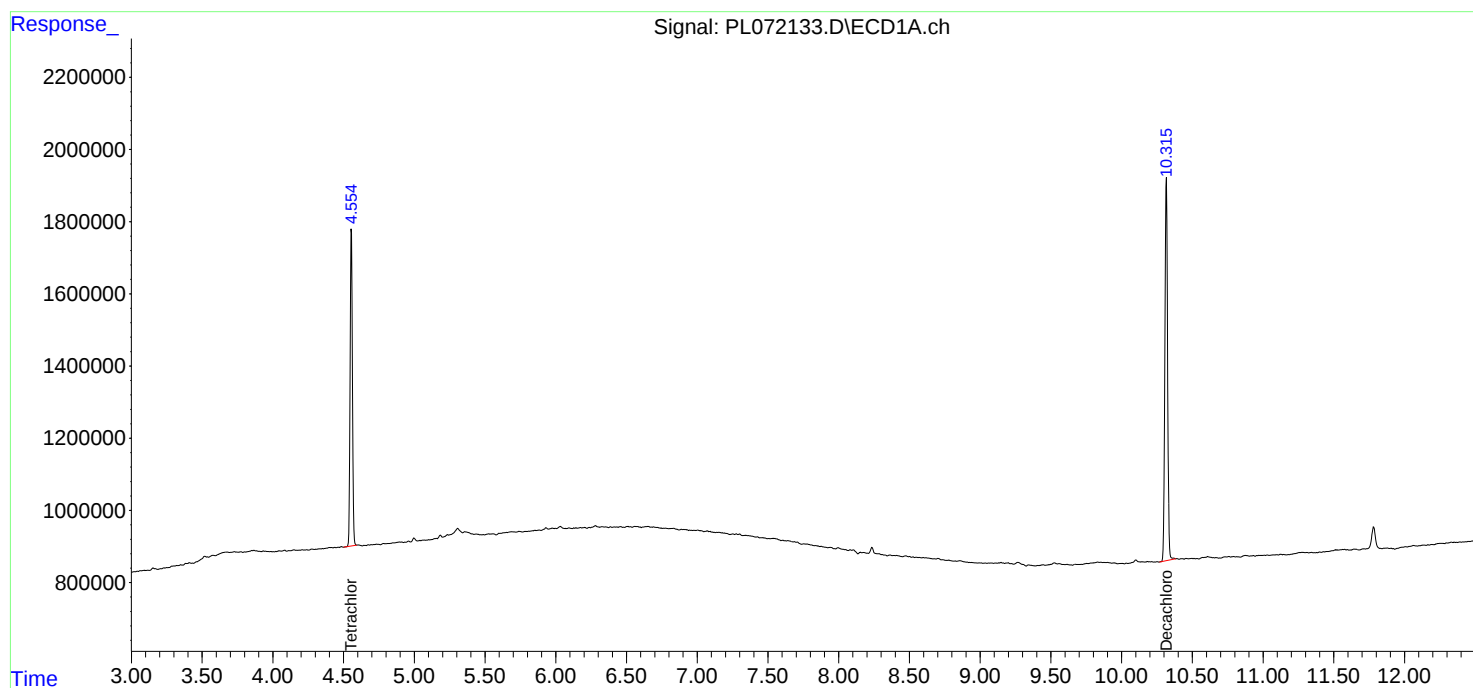


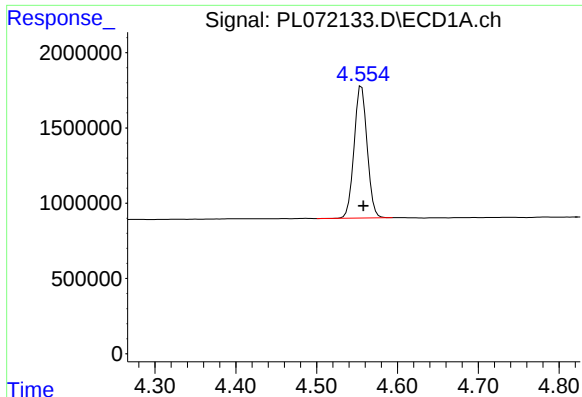

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 9826376
Conc: 17.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

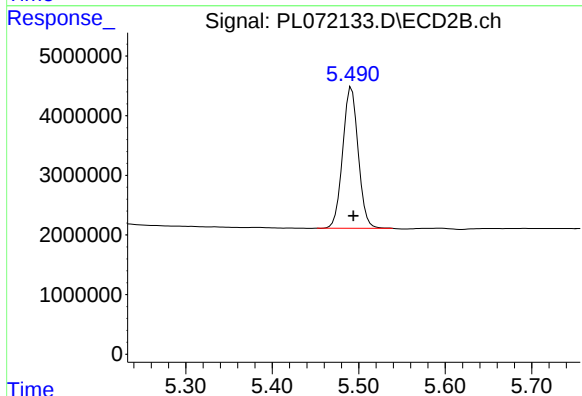


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 29313743
Conc: 18.05 ng/ml

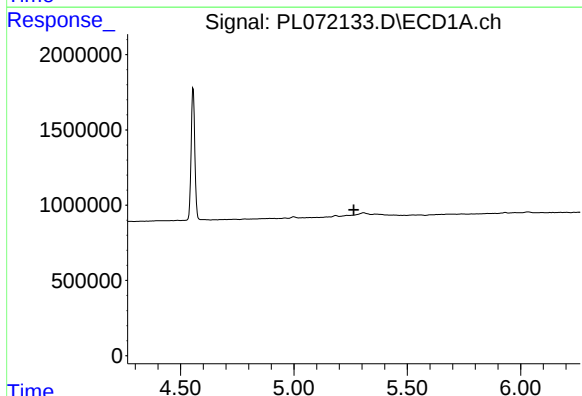


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.265 min
Response: 0
Conc: N.D.

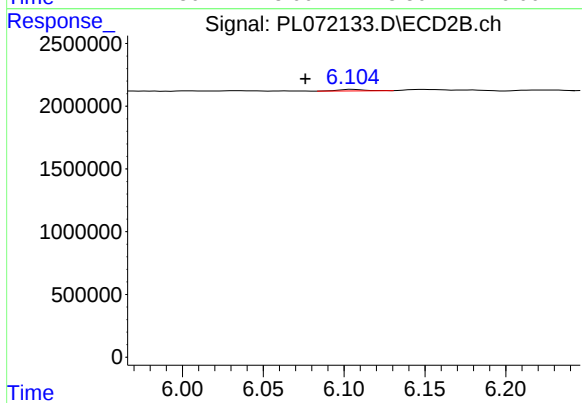

#2 alpha-BHC


R.T.: 6.105 min
Delta R.T.: 0.029 min
Response: 141789
Conc: 0.06 ng/ml

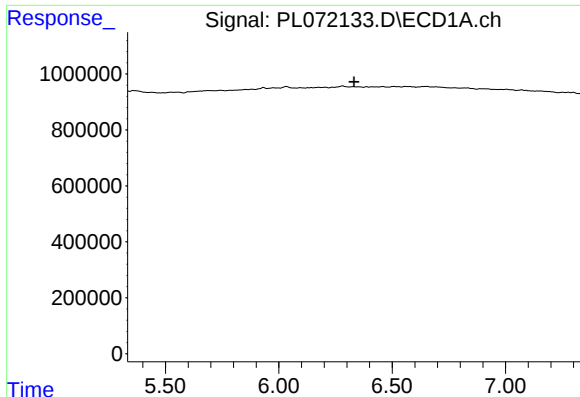

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

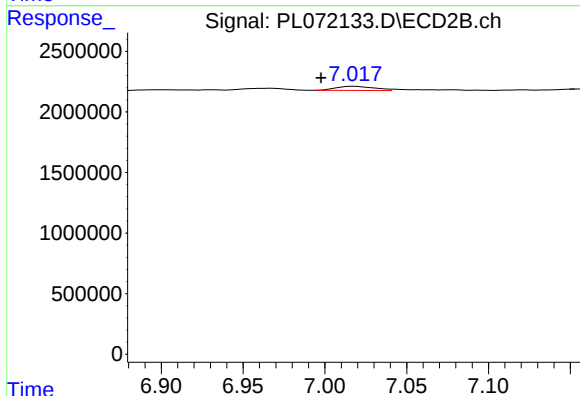


#7 delta-BHC

R.T.: 7.018 min
Delta R.T.: 0.021 min
Response: 548526
Conc: 0.22 ng/ml

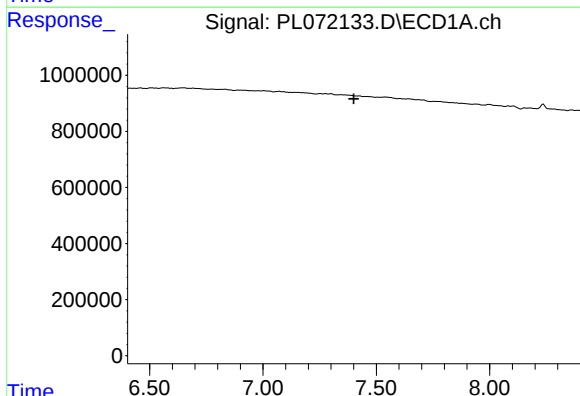


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

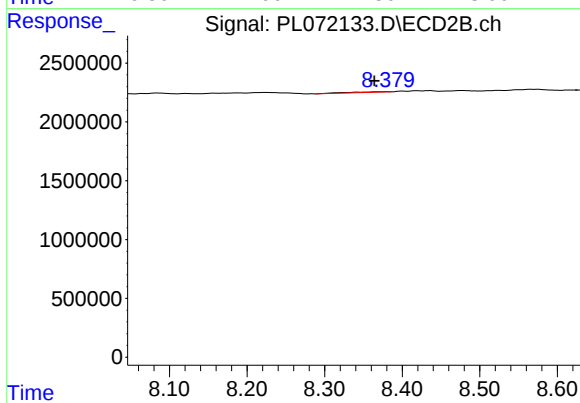

#9 Endosulfan I


R.T.: 8.379 min
Delta R.T.: 0.015 min
Response: 186480
Conc: 0.10 ng/ml

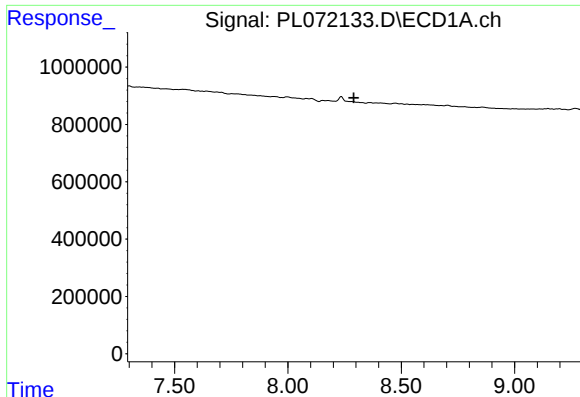

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

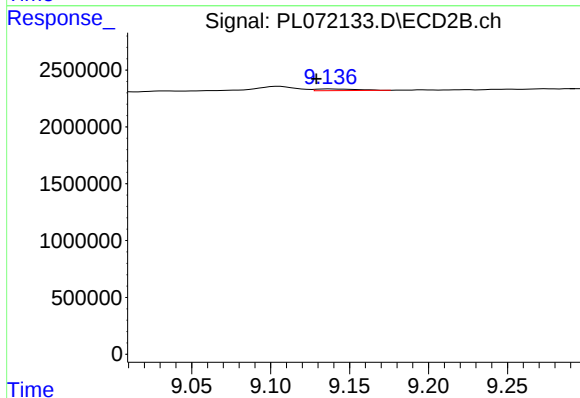


#15 Endosulfan II

R.T.: 9.137 min
Delta R.T.: 0.008 min
Response: 267484
Conc: 0.16 ng/ml

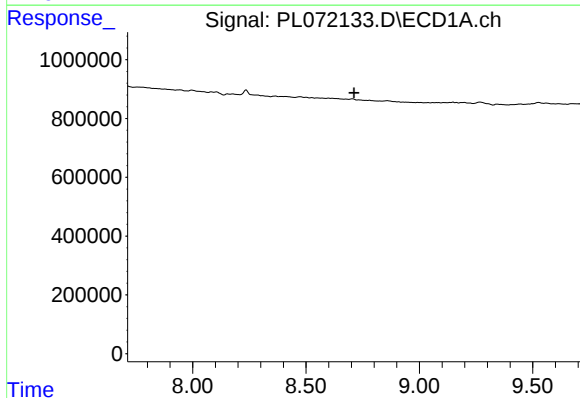


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

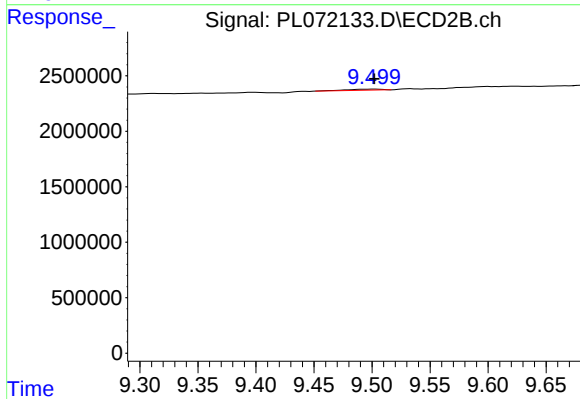

#19 Endosulfan Sulfate


R.T.: 9.502 min
Delta R.T.: 0.000 min
Response: 211227
Conc: 0.14 ng/ml

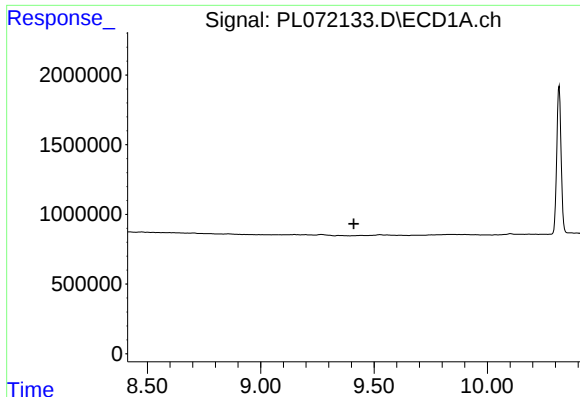

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.410 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

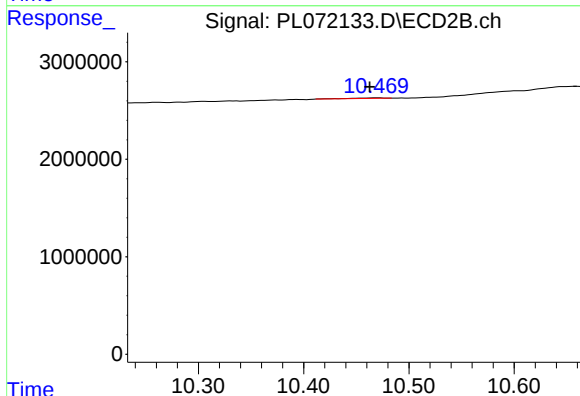


#22 Mirex

R.T.: 10.471 min
Delta R.T.: 0.008 min
Response: 111158
Conc: 0.09 ng/ml

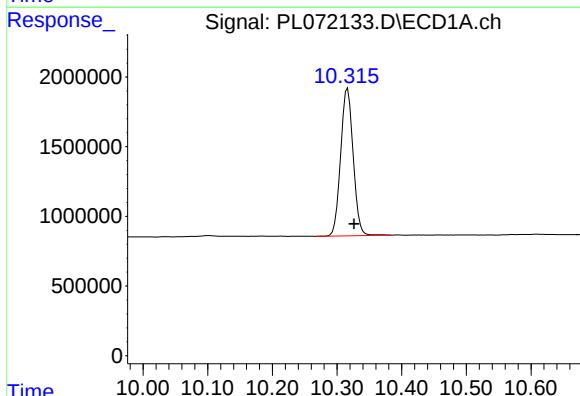

#28 Decachlorobiphenyl

R.T.: 10.316 min
Delta R.T.: -0.010 min
Response: 14201825
Conc: 15.99 ng/ml

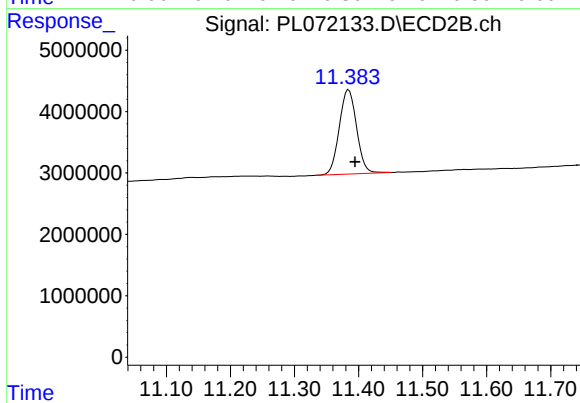

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: -0.010 min
Response: 25852373
Conc: 16.02 ng/ml