

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012022\
 Data File : PL072136.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2022 17:18
 Operator : AR\AJ
 Sample : N1189-21
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:22:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	10248489	29904261	18.460	18.413
28)	SA Decachlor...	10.317	11.383	12696014	22228268	14.290	13.776
Target Compounds							
2)	A alpha-BHC	0.000	6.105f	0	130750	N.D.	0.054 #
5)	MB Aldrin	0.000	7.481	0	4757398	N.D.	2.151 #
7)	B delta-BHC	0.000	7.019f	0	501479	N.D.	0.204 #
10)	B gamma-Chl...	0.000	8.238	0	135223	N.D.	0.067 #
15)	B Endosulfa...	0.000	9.135	0	357395	N.D.	0.208 #
17)	MA 4,4'-DDT	0.000	9.353	0	183376	N.D.	0.116 #
22)	Mirex	0.000	10.436f	0	125200	N.D.	0.100 #
24)	Chlordane-2	0.000	7.481	0	4757398	N.D.	68.066 #
25)	Chlordane-3	0.000	8.238	0	135223	N.D.	0.487 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012022\
Data File : PL072136.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2022 17:18
Operator : AR\AJ
Sample : N1189-21
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:22:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

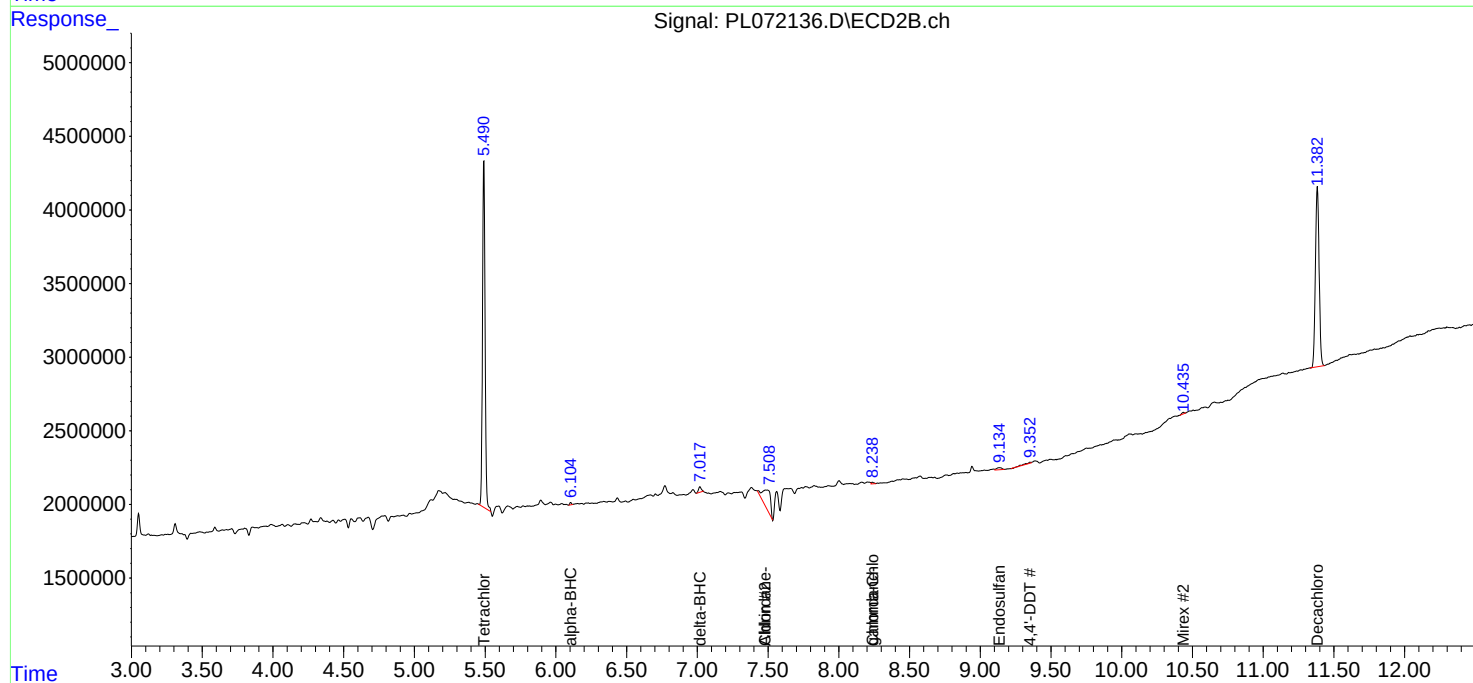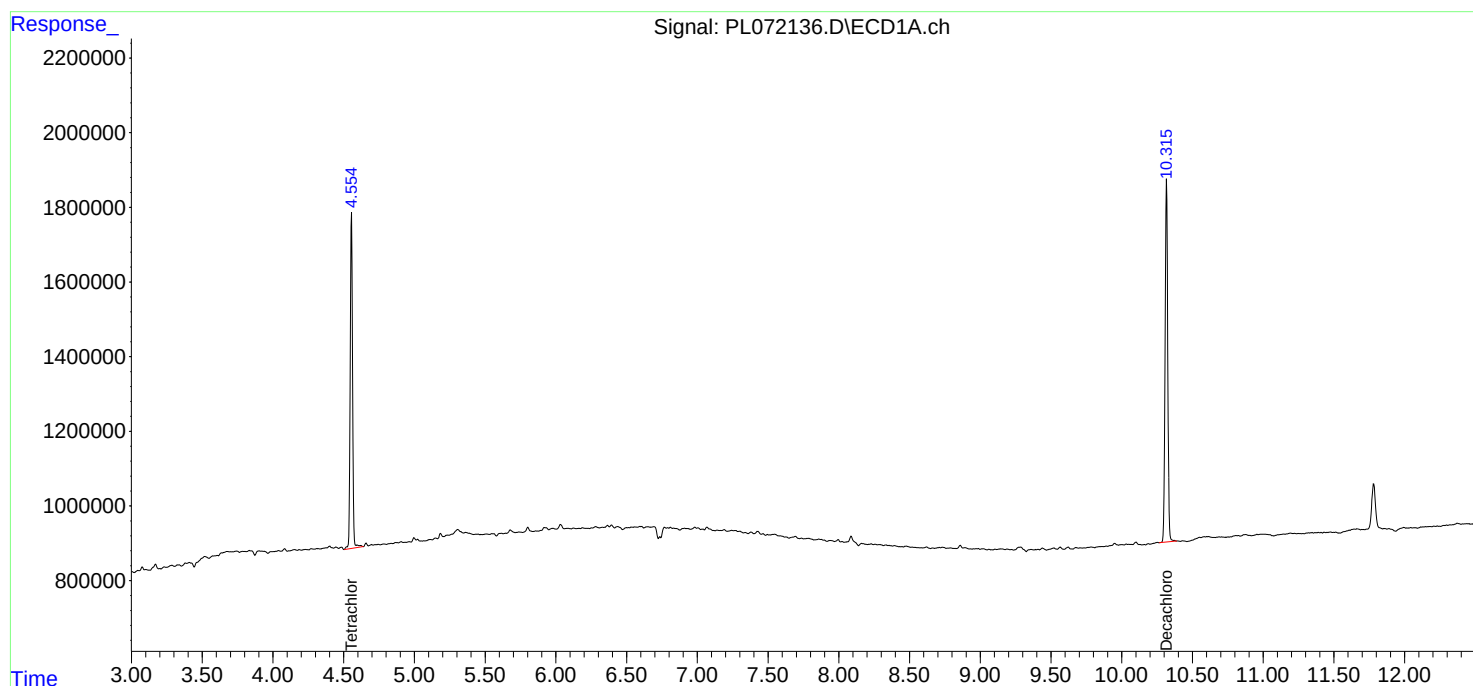


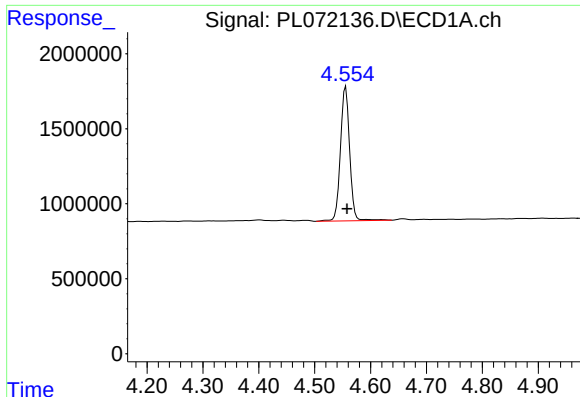

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 10248489
Conc: 18.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

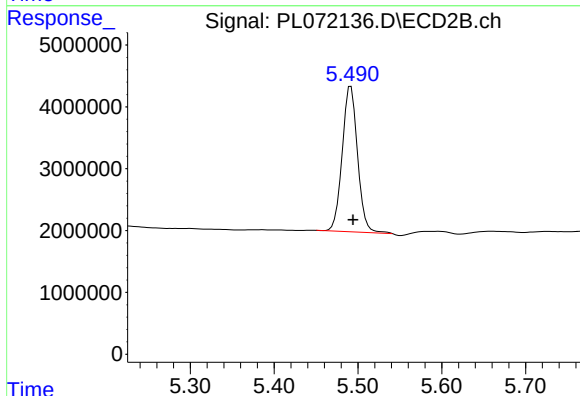


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 29904261
Conc: 18.41 ng/ml

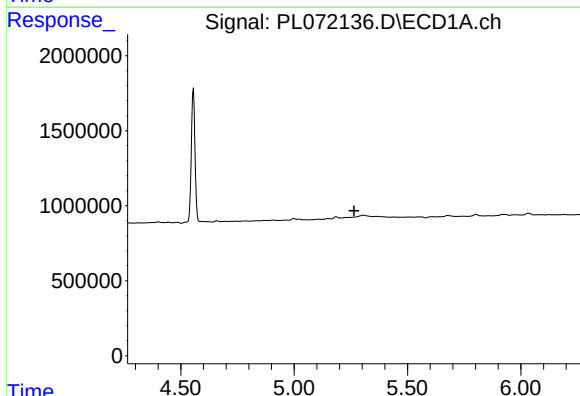


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.265 min
Response: 0
Conc: N.D.

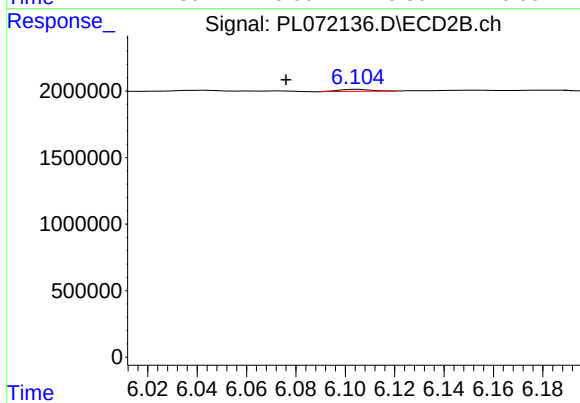

#2 alpha-BHC


R.T.: 6.105 min
Delta R.T.: 0.029 min
Response: 130750
Conc: 0.05 ng/ml

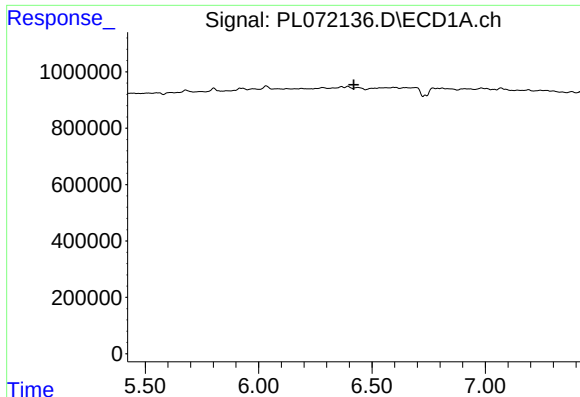

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

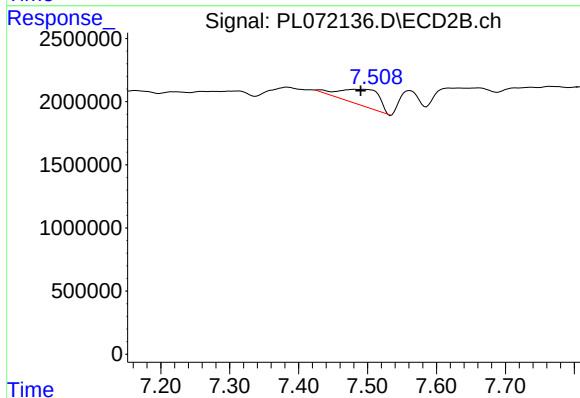


#5 Aldrin

R.T.: 7.481 min
Delta R.T.: -0.009 min
Response: 4757398
Conc: 2.15 ng/ml

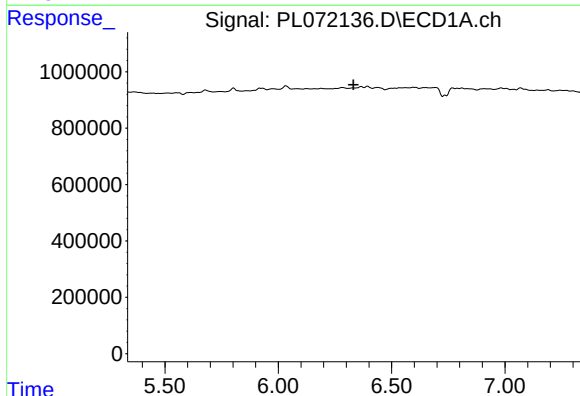


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

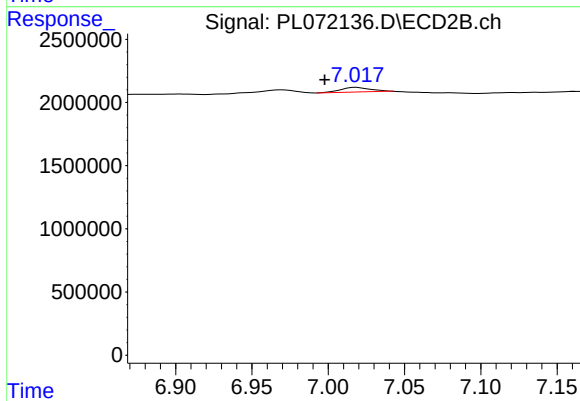

#7 delta-BHC


R.T.: 7.019 min
Delta R.T.: 0.021 min
Response: 501479
Conc: 0.20 ng/ml

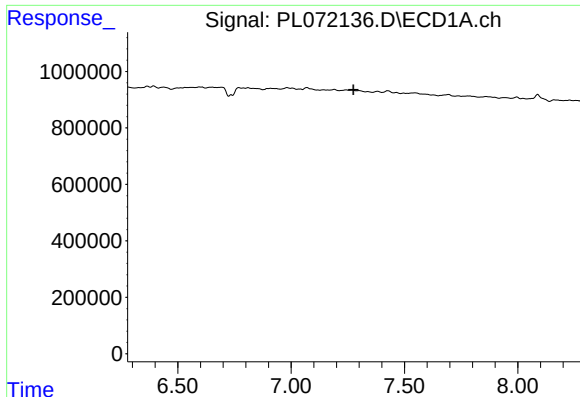

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

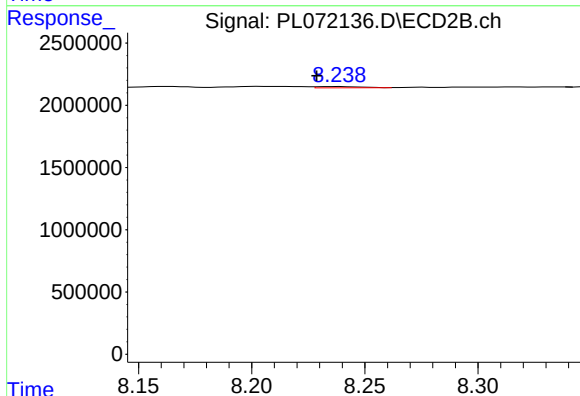


#10 gamma-Chlordane

R.T.: 8.238 min
Delta R.T.: 0.009 min
Response: 135223
Conc: 0.07 ng/ml

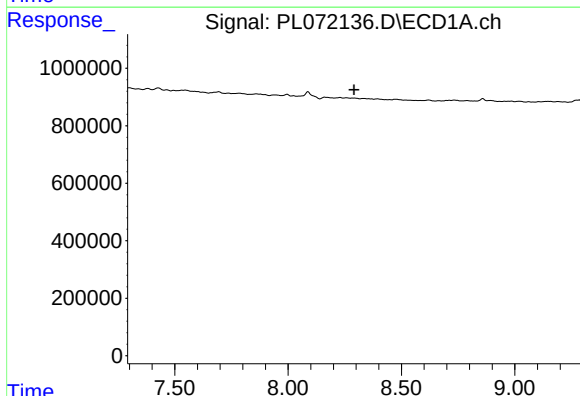


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

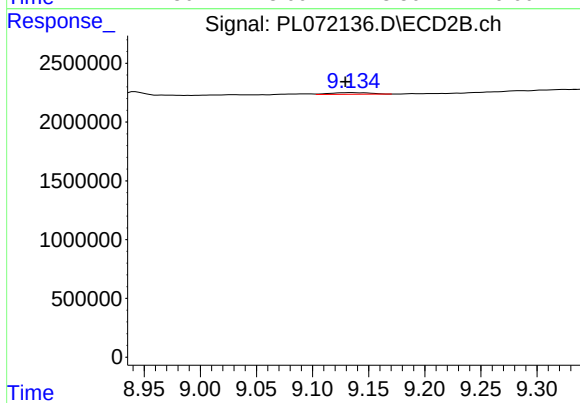

#15 Endosulfan II


R.T.: 9.135 min
Delta R.T.: 0.006 min
Response: 357395
Conc: 0.21 ng/ml

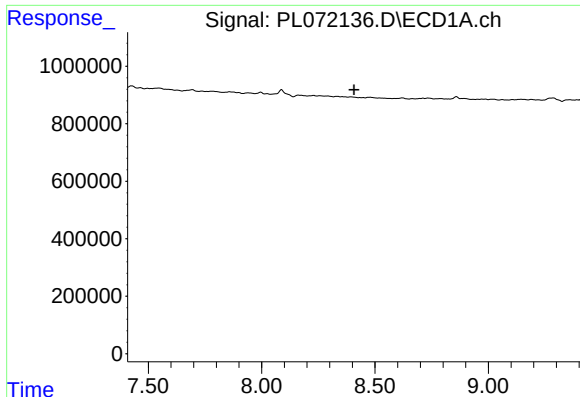

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

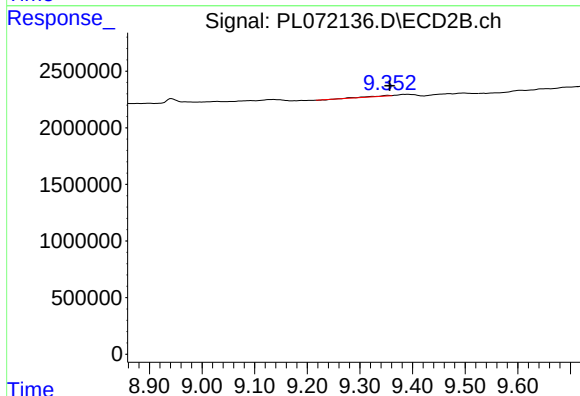


#17 4,4'-DDT

R.T.: 9.353 min
Delta R.T.: -0.004 min
Response: 183376
Conc: 0.12 ng/ml

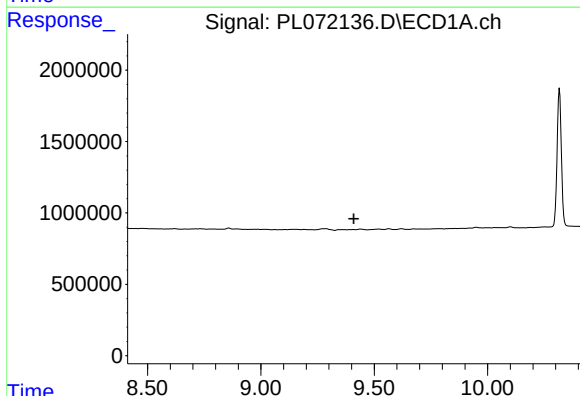


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 9.410 min
Response: 0
Conc: N.D.

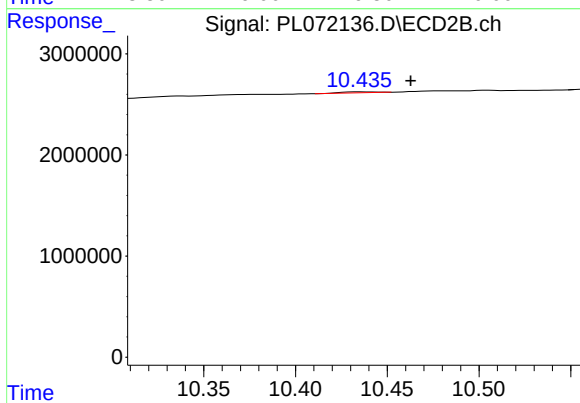

#22 Mirex


R.T.: 10.436 min
Delta R.T.: -0.027 min
Response: 125200
Conc: 0.10 ng/ml

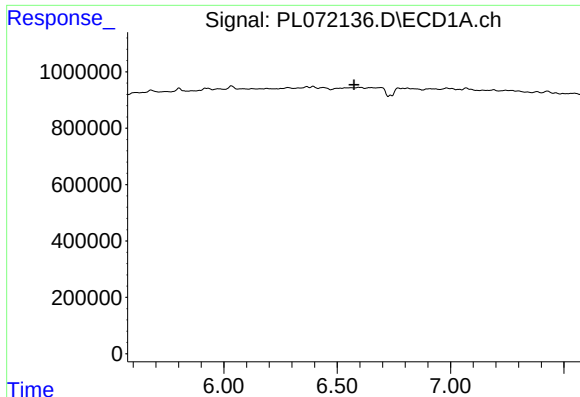

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

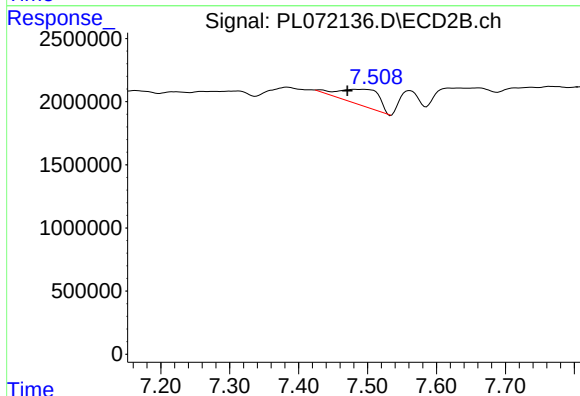


#24 Chlordane-2

R.T.: 7.481 min
Delta R.T.: 0.011 min
Response: 4757398
Conc: 68.07 ng/ml

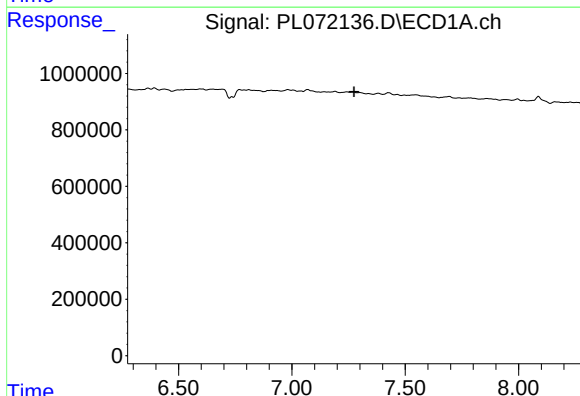


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

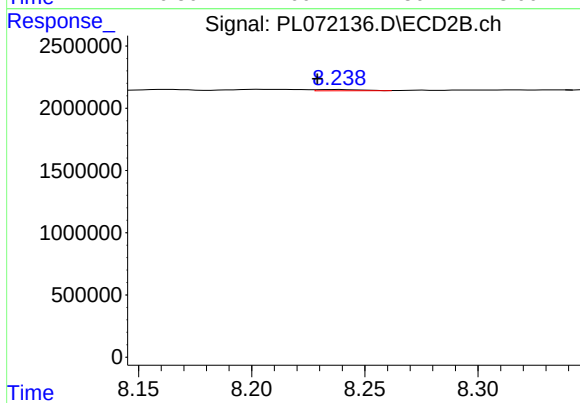

#25 Chlordane-3


R.T.: 8.238 min
Delta R.T.: 0.009 min
Response: 135223
Conc: 0.49 ng/ml

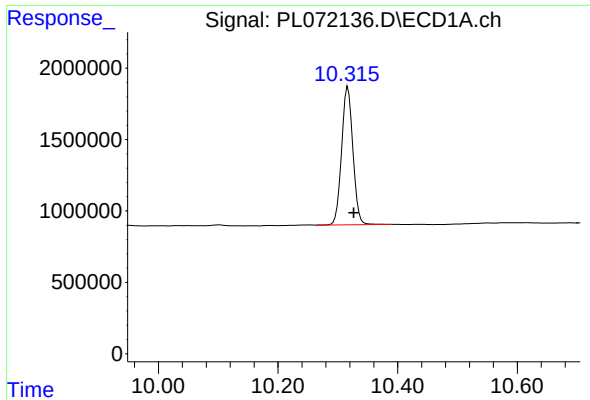

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: -0.010 min
Response: 12696014
Conc: 14.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

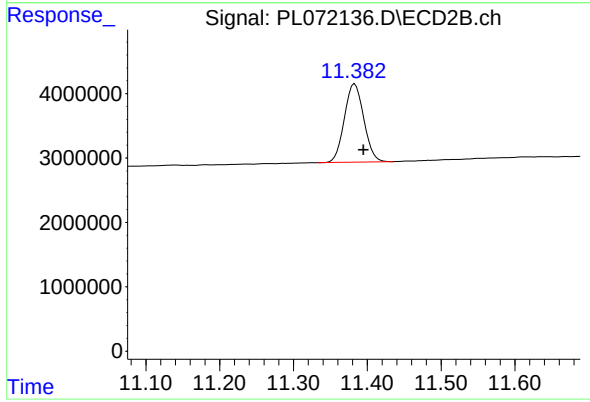

#28 Decachlorobiphenyl

R.T.: 11.383 min
Delta R.T.: -0.012 min
Response: 22228268
Conc: 13.78 ng/ml