

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012022\
 Data File : PL072138.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2022 17:50
 Operator : AR\AJ
 Sample : N1189-25
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:22:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	8771999	25913366	15.800	15.955
28)	SA Decachlor...	10.317	11.384	11625830	21140596	13.086	13.102
Target Compounds							
7)	B delta-BHC	0.000	7.017f	0	1081044	N.D.	0.439 #
10)	B gamma-Chl...	0.000	8.210f	0	662020	N.D.	0.328 #
15)	B Endosulfa...	0.000	9.146f	0	243026	N.D.	0.142 #
19)	B Endosulfa...	0.000	9.532f	0	143279	N.D.	0.092 #
25)	Chlordane-3	0.000	8.210f	0	662020	N.D.	2.383 #
27)	Chlordane-5	0.000	9.204	0	44124	N.D.	0.723 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012022\
Data File : PL072138.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2022 17:50
Operator : AR\AJ
Sample : N1189-25
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:22:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

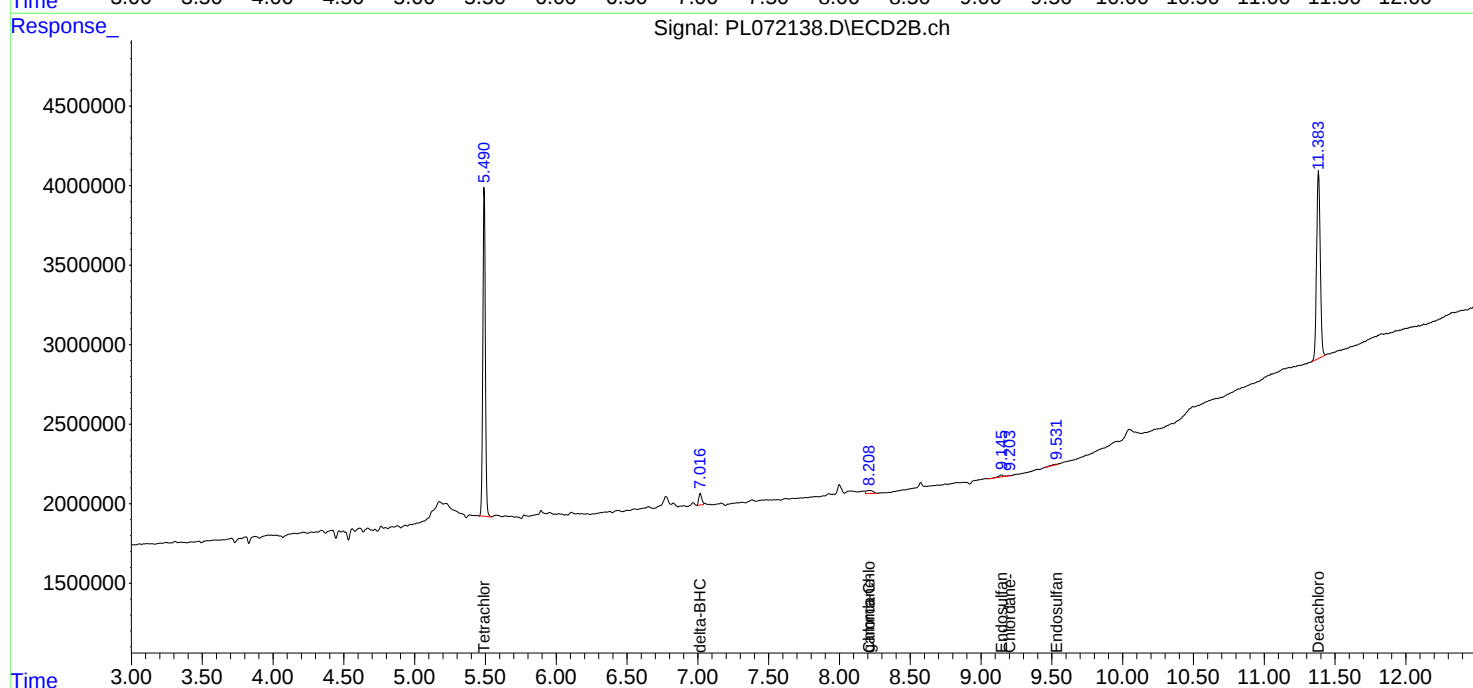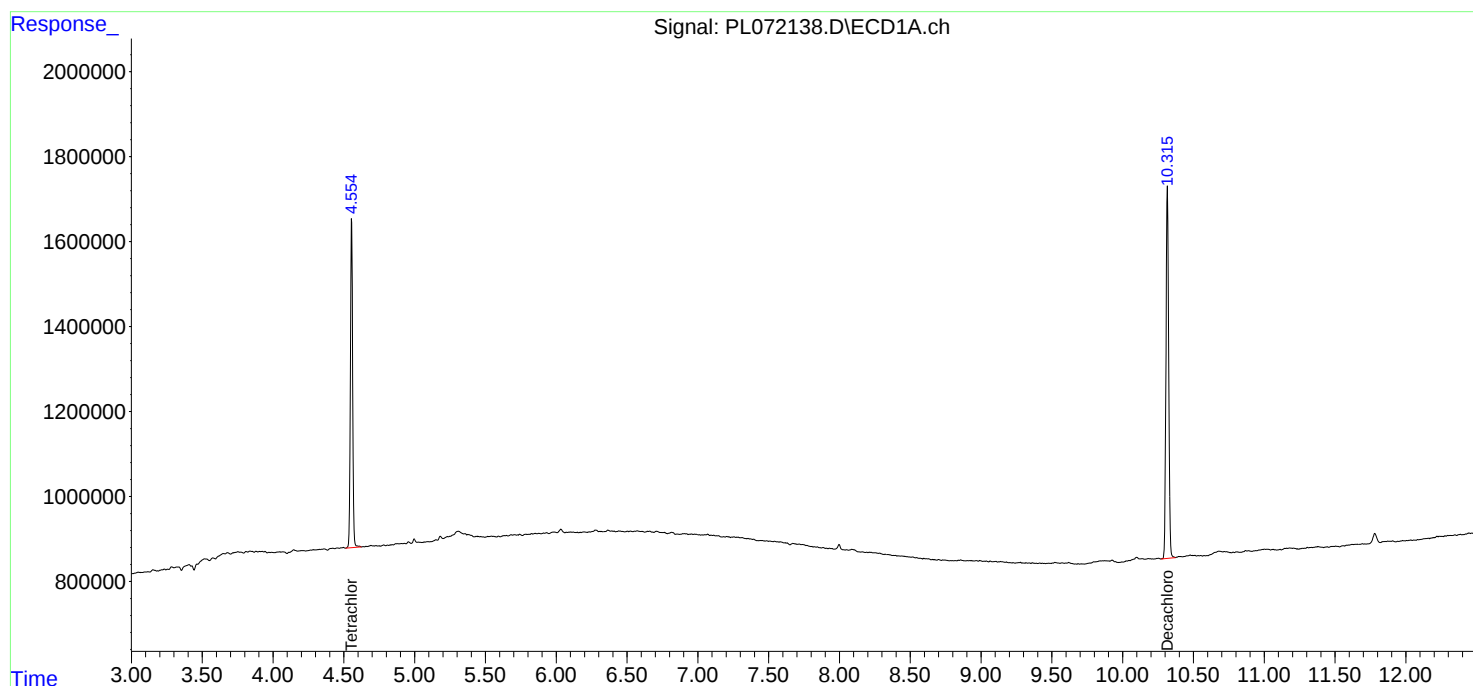


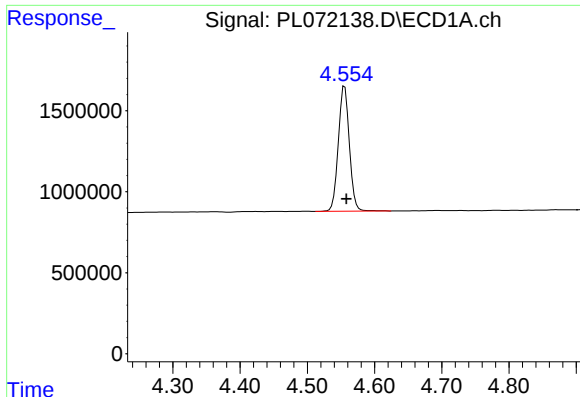

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 8771999
Conc: 15.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

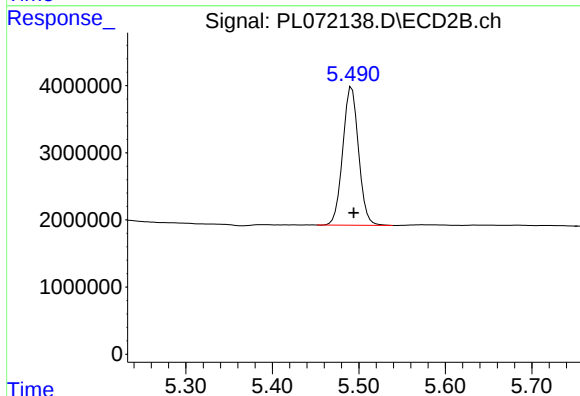


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 25913366
Conc: 15.96 ng/ml

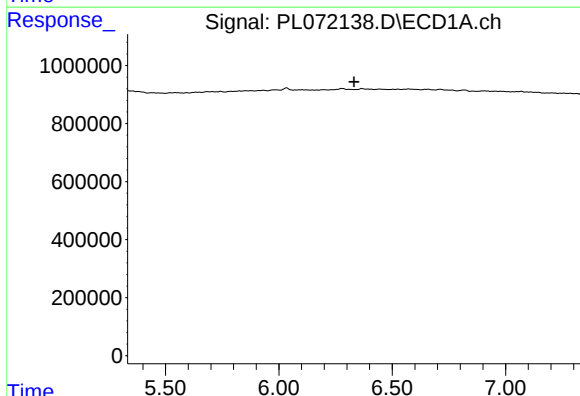


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

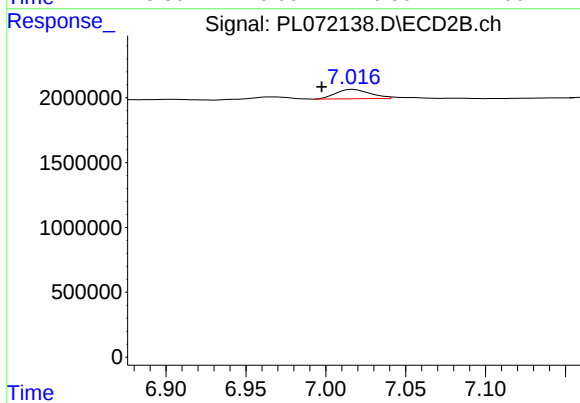

#7 delta-BHC


R.T.: 7.017 min
Delta R.T.: 0.020 min
Response: 1081044
Conc: 0.44 ng/ml

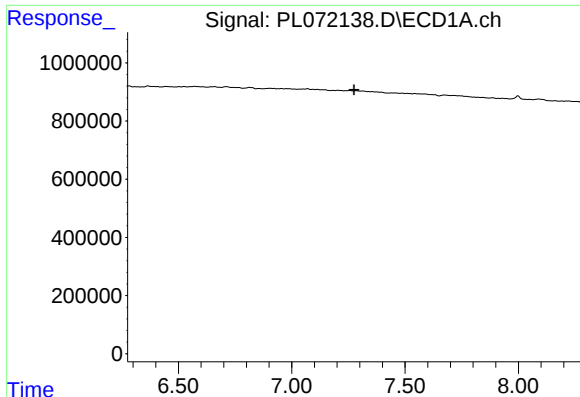

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

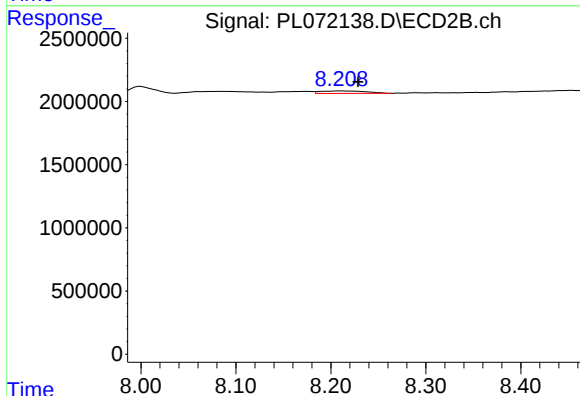


#10 gamma-Chlordane

R.T.: 8.210 min
Delta R.T.: -0.019 min
Response: 662020
Conc: 0.33 ng/ml

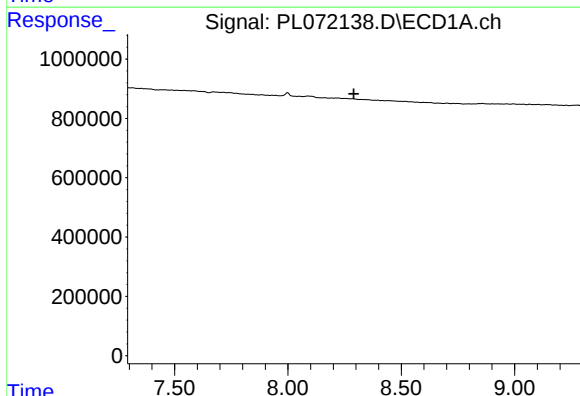


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

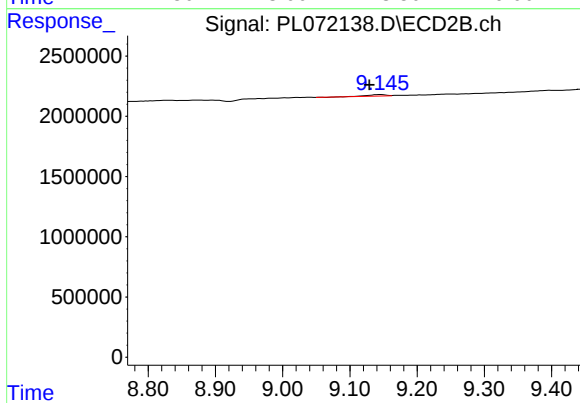

#15 Endosulfan II


R.T.: 9.146 min
Delta R.T.: 0.017 min
Response: 243026
Conc: 0.14 ng/ml

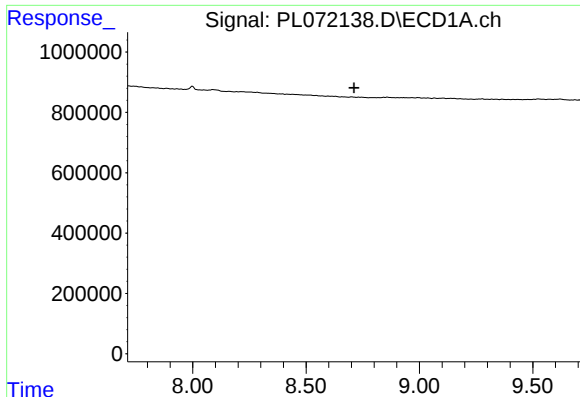

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

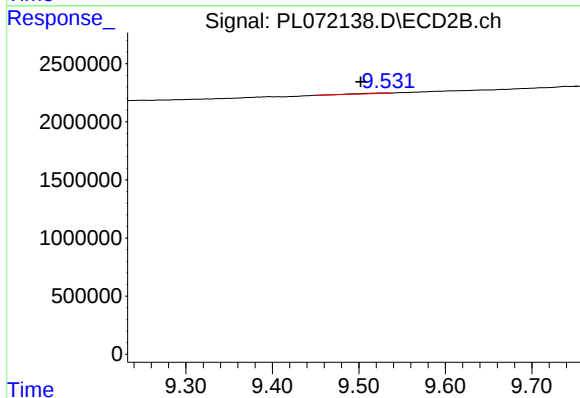


#19 Endosulfan Sulfate

R.T.: 9.532 min
Delta R.T.: 0.030 min
Response: 143279
Conc: 0.09 ng/ml

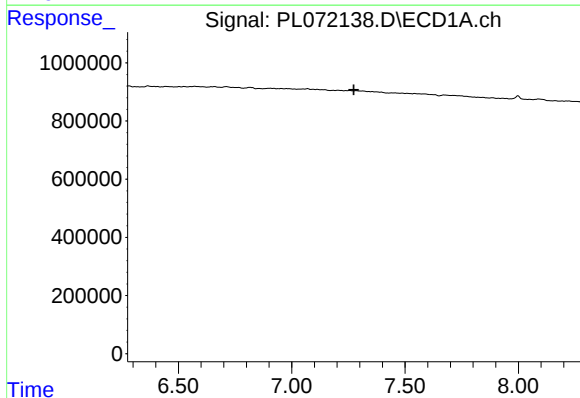


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

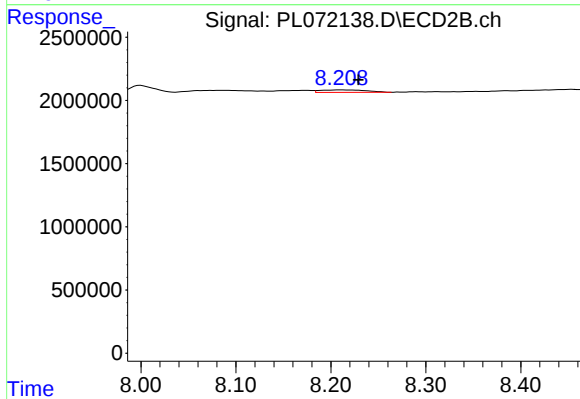

#25 Chlordane-3


R.T.: 8.210 min
Delta R.T.: -0.019 min
Response: 662020
Conc: 2.38 ng/ml

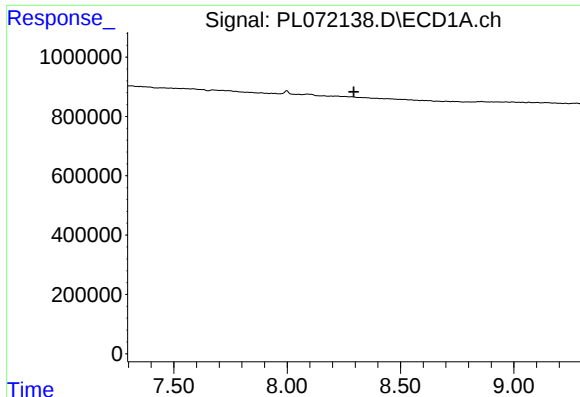

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

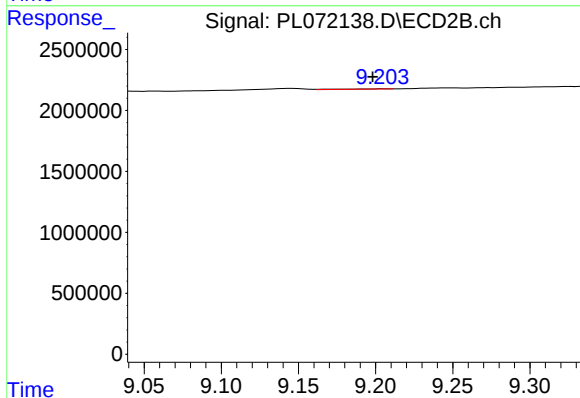


#27 Chlordane-5

R.T.: 9.204 min
Delta R.T.: 0.006 min
Response: 44124
Conc: 0.72 ng/ml

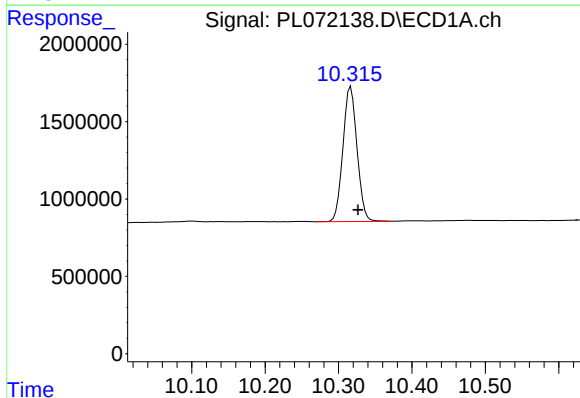

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: -0.010 min
Response: 11625830
Conc: 13.09 ng/ml

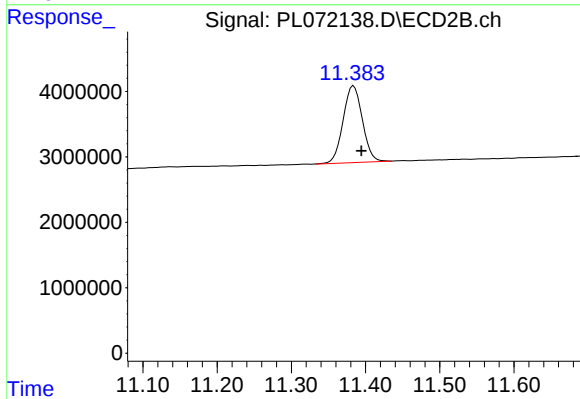

#28 Decachlorobiphenyl

R.T.: 11.384 min
Delta R.T.: -0.011 min
Response: 21140596
Conc: 13.10 ng/ml