

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012023\
 Data File : PL080413.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2023 15:50
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 16:52:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 20 16:52:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.689	215.8E6	279.7E6	101.199	99.095
28)	SA Decachlor...	8.791	7.840	167.5E6	231.9E6	83.836	92.566
Target Compounds							
23)	Chlordane-1	4.500	3.687	88625127	83982099	992.339	1010.163
24)	Chlordane-2	5.027	4.264	94398171	89219162	978.359	972.718
25)	Chlordane-3	5.732	4.895	358.4E6	283.2E6	1032.721	1053.915
26)	Chlordane-4	5.815	4.957	448.5E6	284.6E6	1012.557	1030.427
27)	Chlordane-5	6.656	5.625	74671122	74076245	998.464	1026.614


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012023\
Data File : PL080413.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2023 15:50
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 16:52:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Fri Jan 20 16:52:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

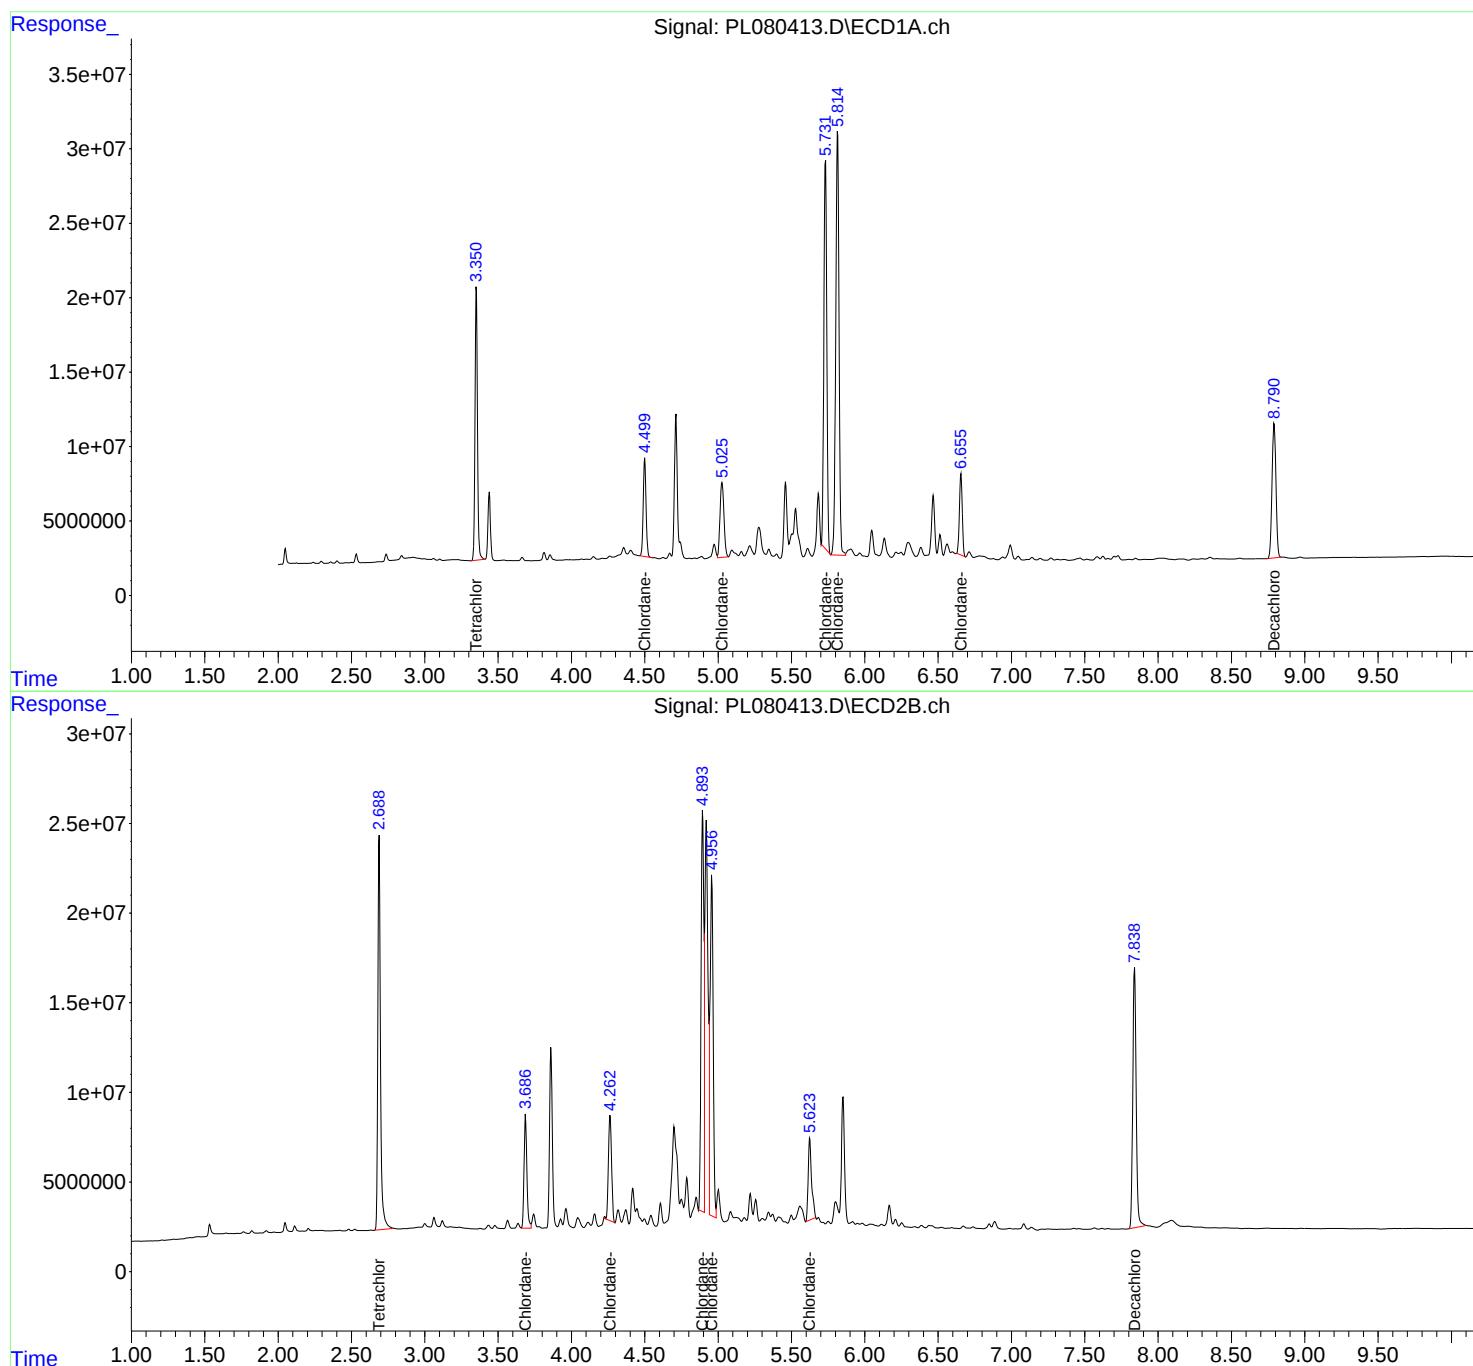


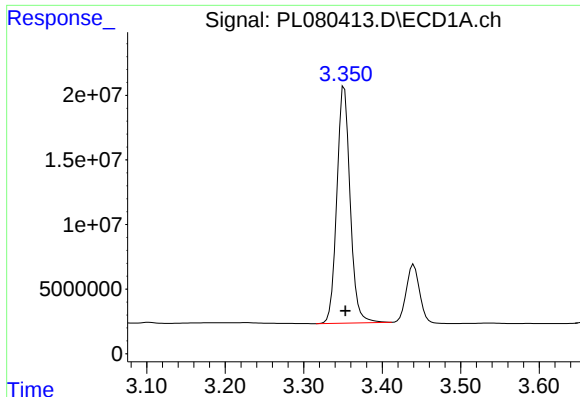

#1 Tetrachloro-m-xylene


R.T.: 3.352 min
Delta R.T.: -0.001 min
Response: 215767322
Conc: 101.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

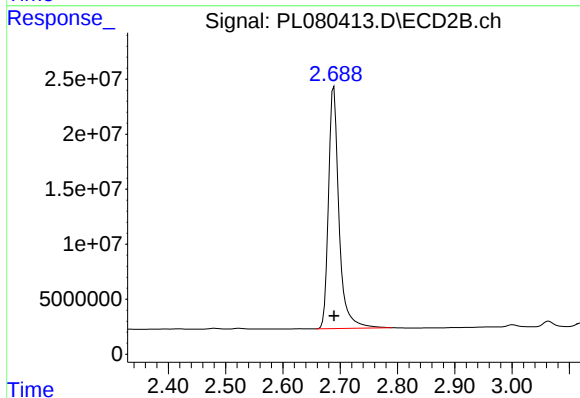


#1 Tetrachloro-m-xylene

R.T.: 2.689 min
Delta R.T.: 0.000 min
Response: 279689984
Conc: 99.09 ng/ml

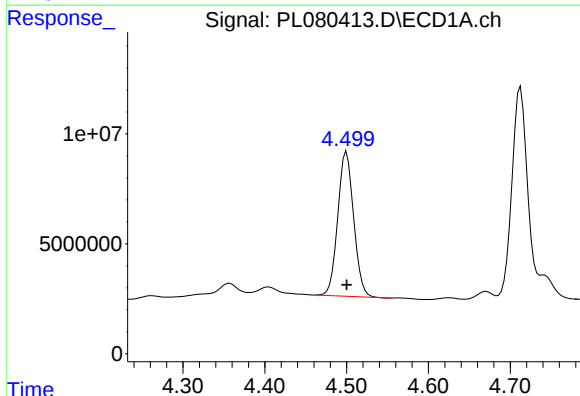


#23 Chlordane-1

R.T.: 4.500 min
Delta R.T.: 0.000 min
Response: 88625127
Conc: 992.34 ng/ml

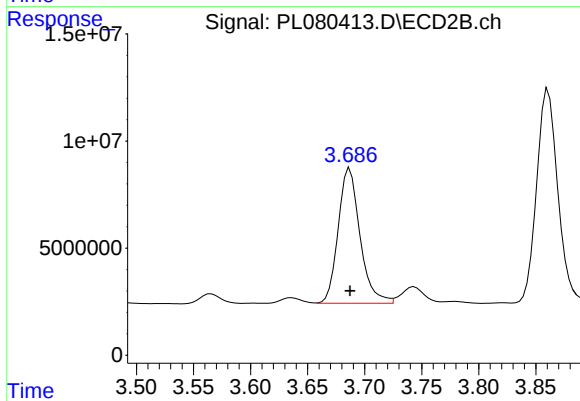

#23 Chlordane-1


R.T.: 3.687 min
Delta R.T.: 0.000 min
Response: 83982099
Conc: 1010.16 ng/ml

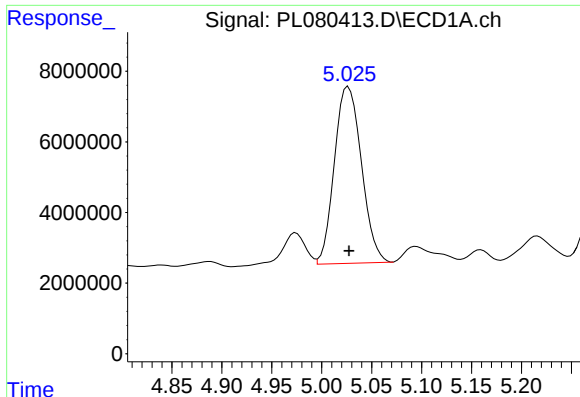

#24 Chlordane-2


R.T.: 5.027 min
Delta R.T.: 0.000 min
Response: 94398171
Conc: 978.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

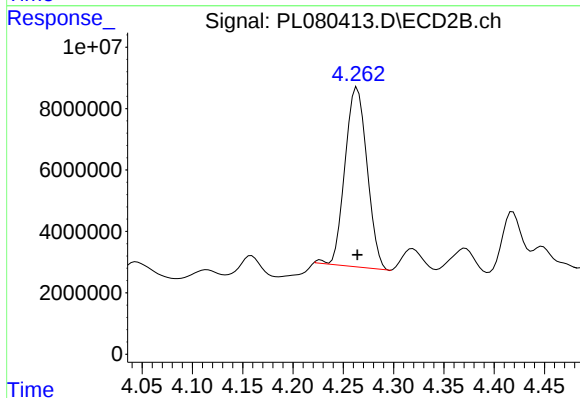


#24 Chlordane-2

R.T.: 4.264 min
Delta R.T.: 0.000 min
Response: 89219162
Conc: 972.72 ng/ml

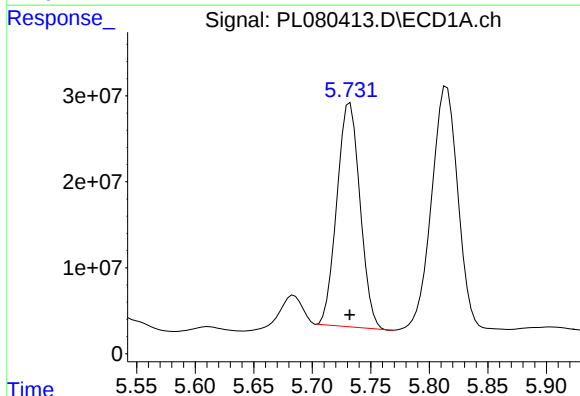


#25 Chlordane-3

R.T.: 5.732 min
Delta R.T.: 0.000 min
Response: 358409991
Conc: 1032.72 ng/ml

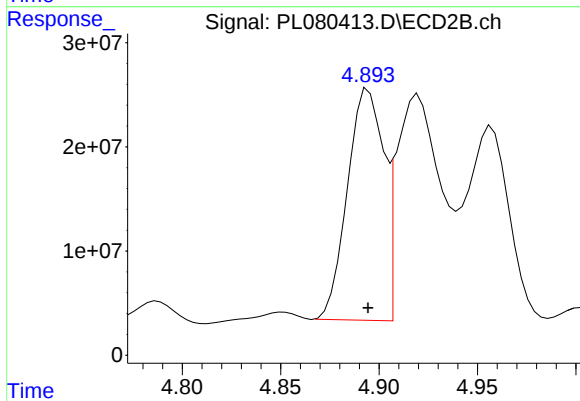

#25 Chlordane-3


R.T.: 4.895 min
Delta R.T.: 0.000 min
Response: 283168311
Conc: 1053.91 ng/ml

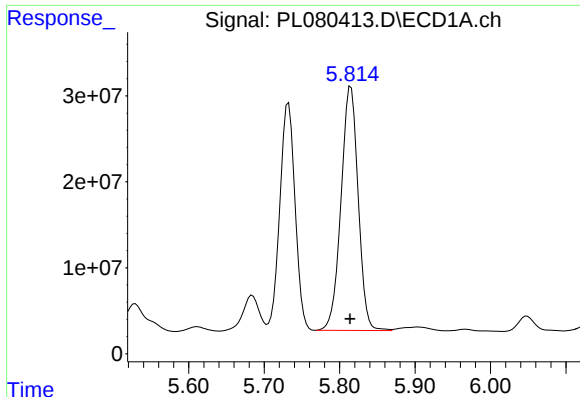

#26 Chlordane-4


R.T.: 5.815 min
Delta R.T.: 0.000 min
Response: 448478317
Conc: 1012.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

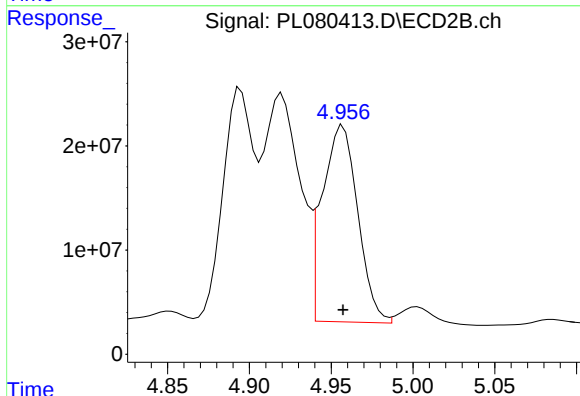


#26 Chlordane-4

R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 284635656
Conc: 1030.43 ng/ml

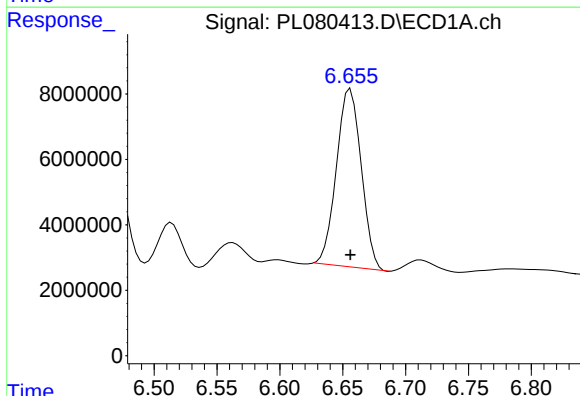


#27 Chlordane-5

R.T.: 6.656 min
Delta R.T.: 0.000 min
Response: 74671122
Conc: 998.46 ng/ml

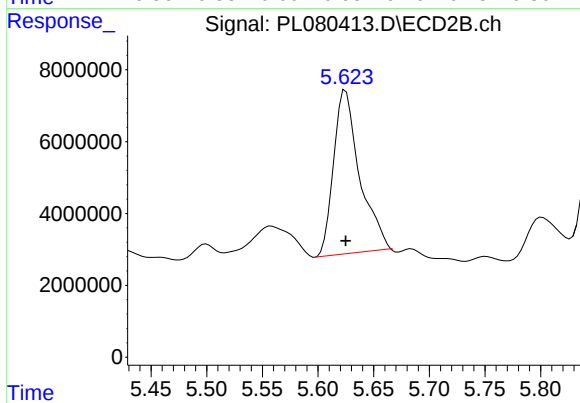

#27 Chlordane-5


R.T.: 5.625 min
Delta R.T.: 0.000 min
Response: 74076245
Conc: 1026.61 ng/ml

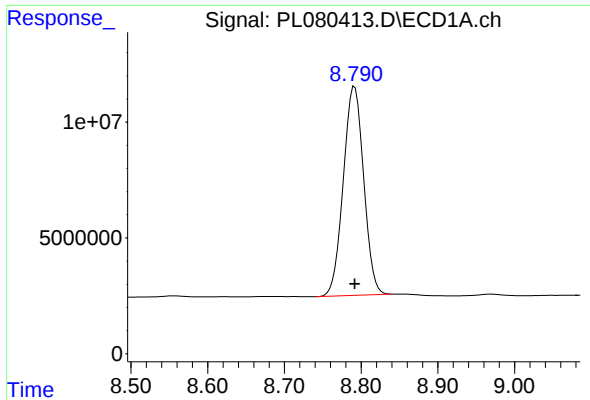

#28 Decachlorobiphenyl

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 167494780
Conc: 83.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

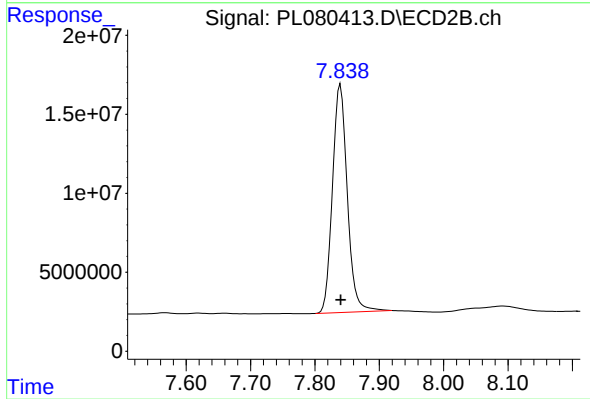

#28 Decachlorobiphenyl

R.T.: 7.840 min
Delta R.T.: 0.000 min
Response: 231943243
Conc: 92.57 ng/ml