

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012023\
 Data File : PL080415.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2023 16:18
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 16:53:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 20 16:52:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.353	2.690	106.6E6	141.1E6	50.000	50.000
28)	SA Decachlor...	8.792	7.840	99894251	125.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.500	3.687	44654651	41568591	500.000	500.000
24)	Chlordane-2	5.027	4.264	48243138	45860768	500.000	500.000
25)	Chlordane-3	5.732	4.894	173.5E6	134.3E6	500.000	500.000
26)	Chlordane-4	5.814	4.957	221.5E6	138.1E6	500.000	500.000
27)	Chlordane-5	6.656	5.625	37393004	36077954	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012023\
Data File : PL080415.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2023 16:18
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 16:53:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Fri Jan 20 16:52:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

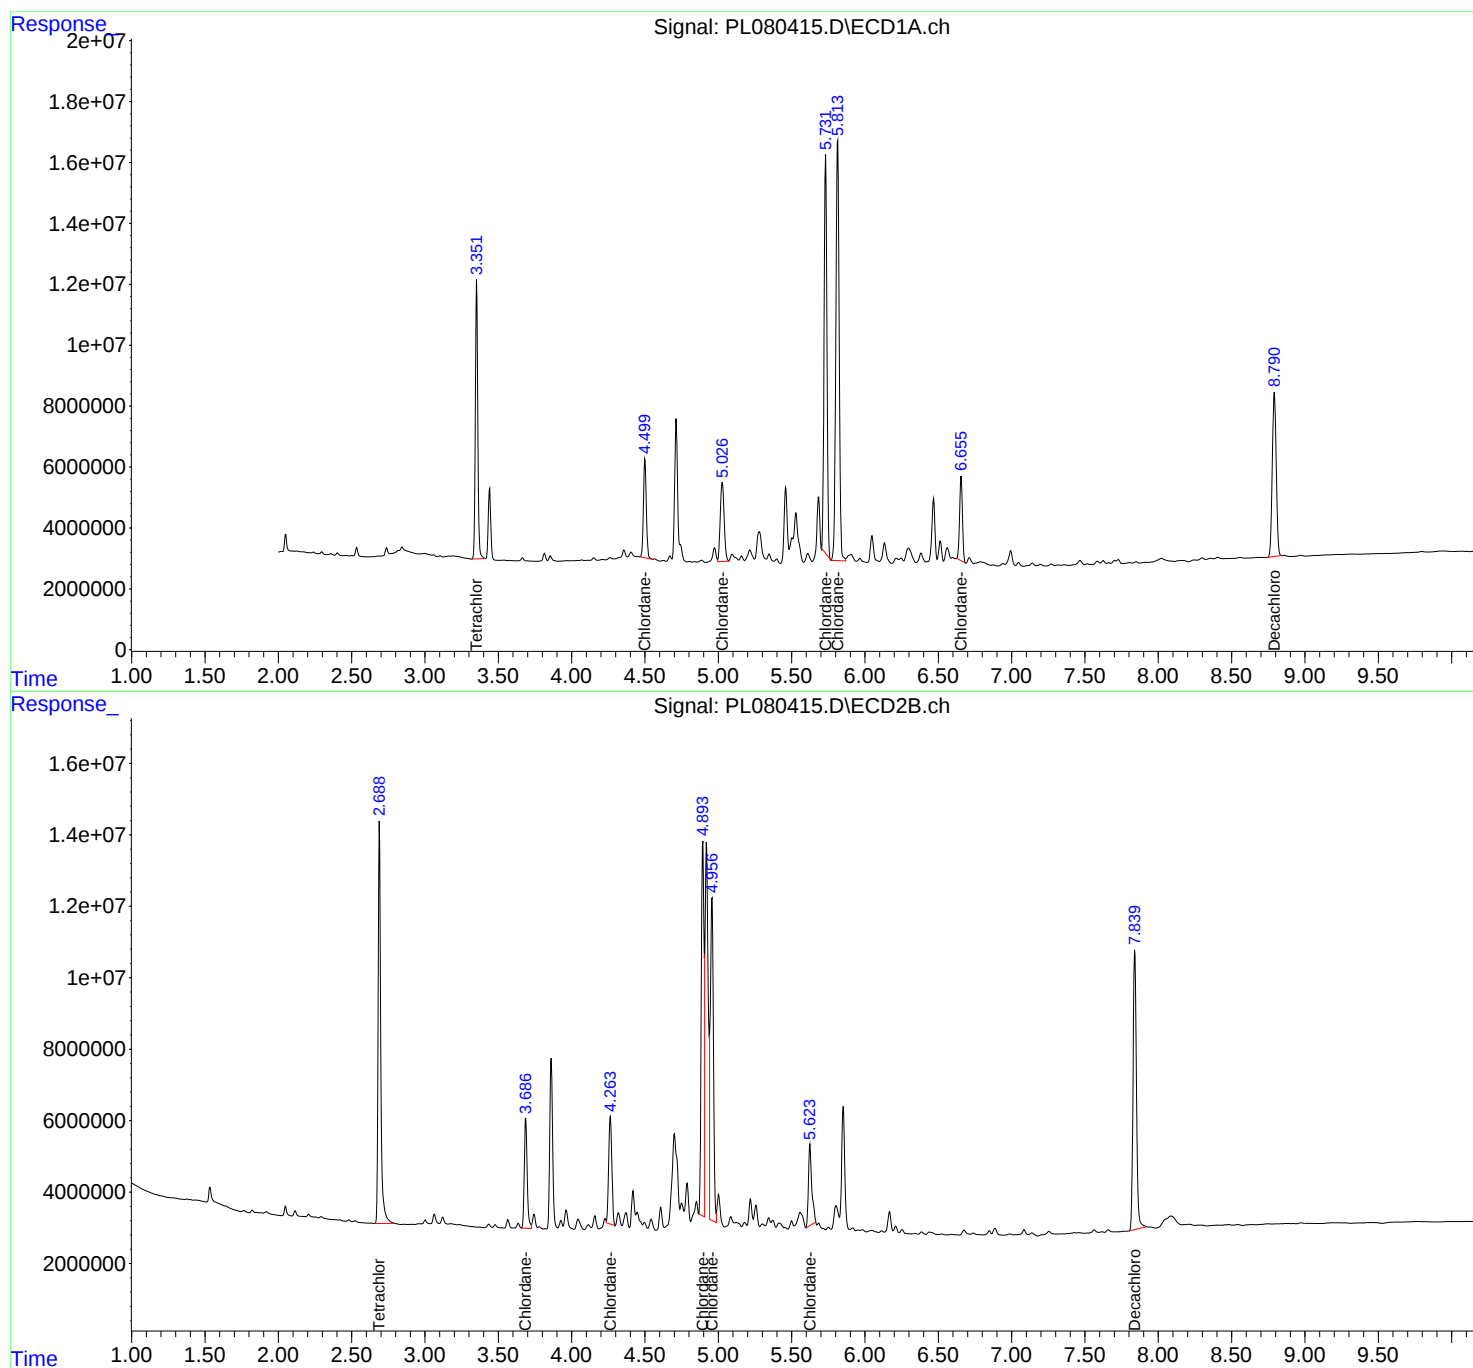


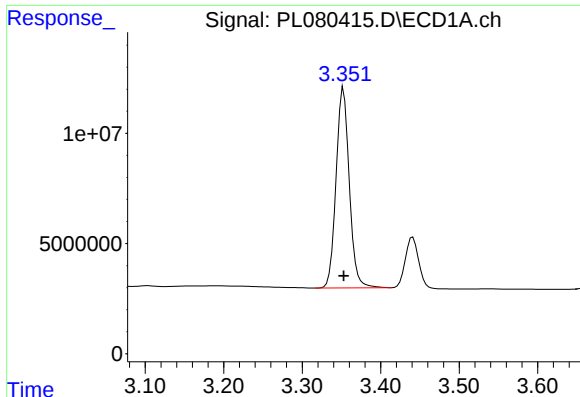

#1 Tetrachloro-m-xylene


R.T.: 3.353 min
Delta R.T.: 0.000 min
Response: 106605136
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

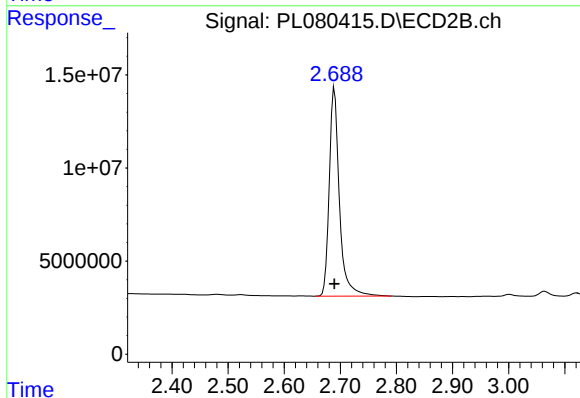


#1 Tetrachloro-m-xylene

R.T.: 2.690 min
Delta R.T.: 0.000 min
Response: 141122191
Conc: 50.00 ng/ml

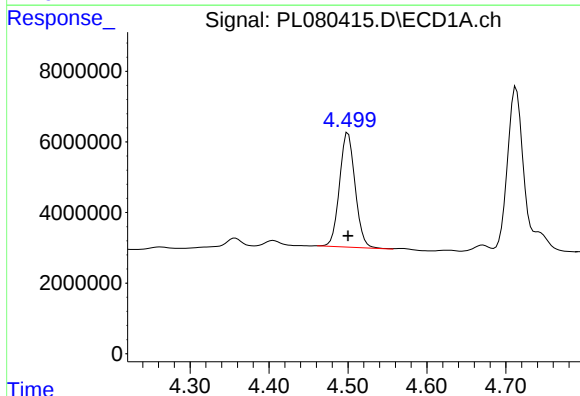


#23 Chlordane-1

R.T.: 4.500 min
Delta R.T.: 0.000 min
Response: 44654651
Conc: 500.00 ng/ml

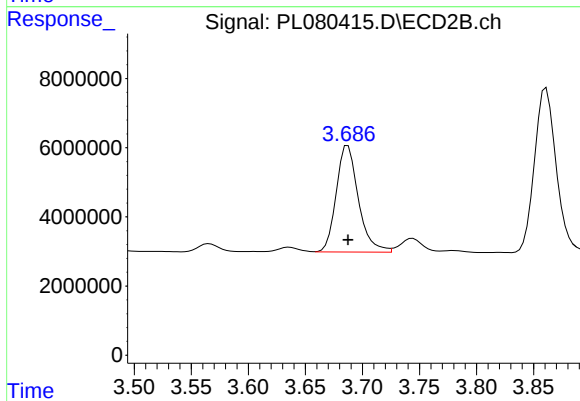

#23 Chlordane-1


R.T.: 3.687 min
Delta R.T.: 0.000 min
Response: 41568591
Conc: 500.00 ng/ml

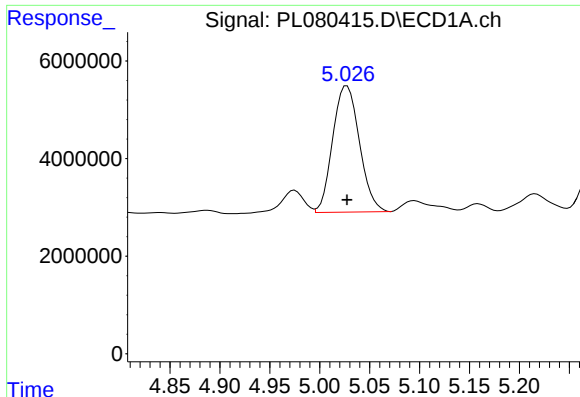

#24 Chlordane-2


R.T.: 5.027 min
Delta R.T.: 0.000 min
Response: 48243138
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

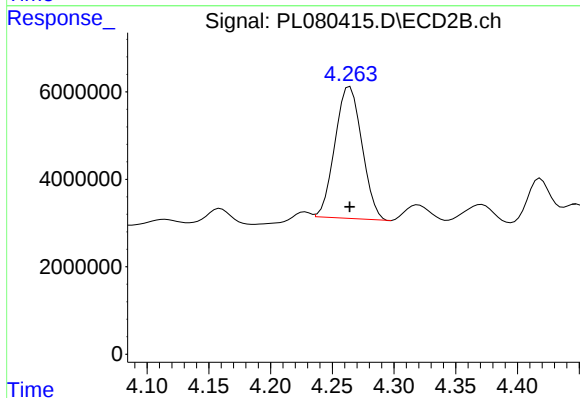


#24 Chlordane-2

R.T.: 4.264 min
Delta R.T.: 0.000 min
Response: 45860768
Conc: 500.00 ng/ml

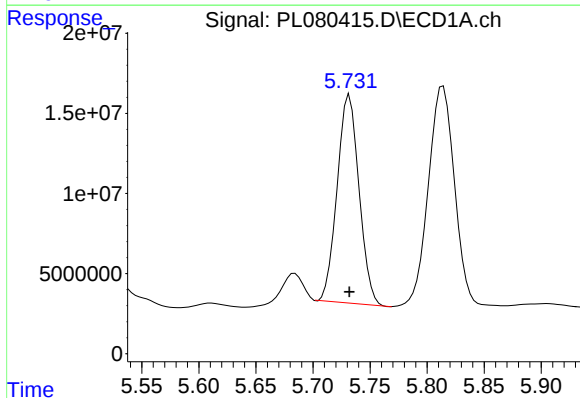


#25 Chlordane-3

R.T.: 5.732 min
Delta R.T.: 0.000 min
Response: 173526956
Conc: 500.00 ng/ml

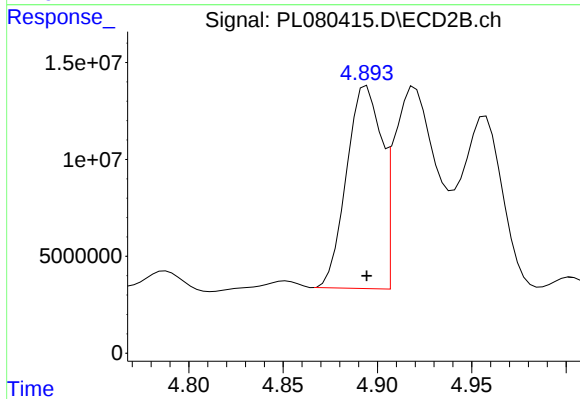

#25 Chlordane-3


R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 134341189
Conc: 500.00 ng/ml

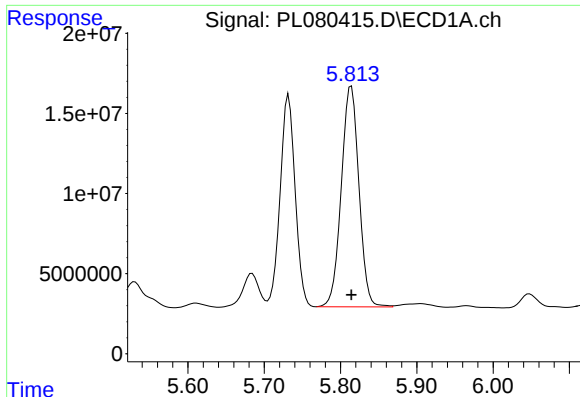

#26 Chlordane-4


R.T.: 5.814 min
Delta R.T.: 0.000 min
Response: 221458406
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

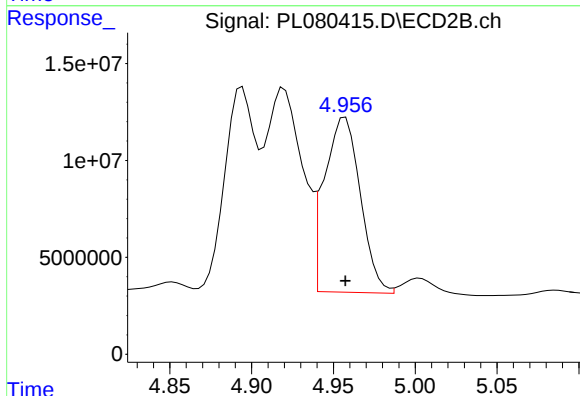


#26 Chlordane-4

R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 138115360
Conc: 500.00 ng/ml

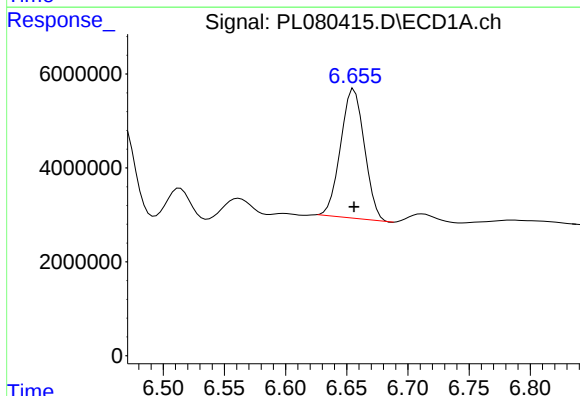


#27 Chlordane-5

R.T.: 6.656 min
Delta R.T.: 0.000 min
Response: 37393004
Conc: 500.00 ng/ml

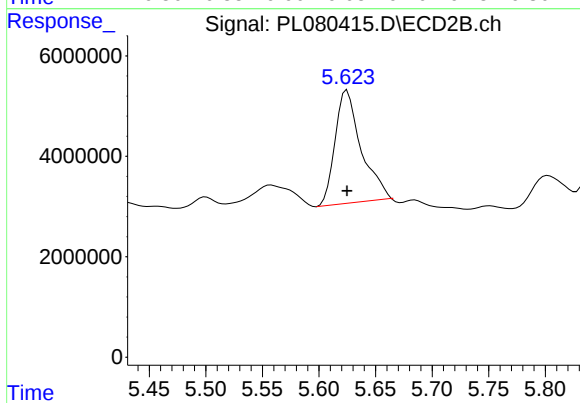

#27 Chlordane-5


R.T.: 5.625 min
Delta R.T.: 0.000 min
Response: 36077954
Conc: 500.00 ng/ml

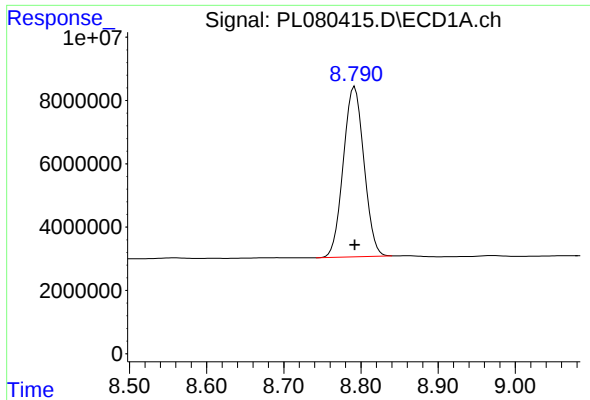

#28 Decachlorobiphenyl

R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 99894251
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

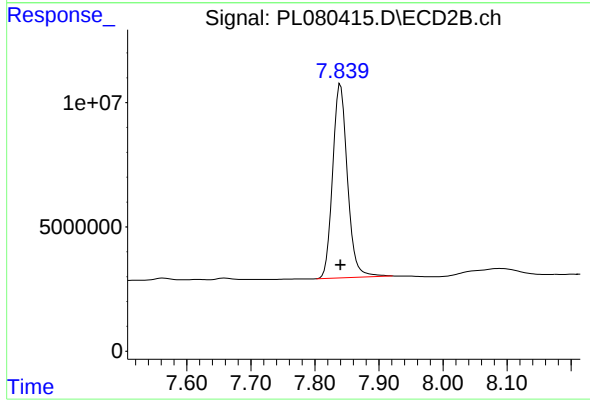

#28 Decachlorobiphenyl

R.T.: 7.840 min
Delta R.T.: 0.000 min
Response: 125285812
Conc: 50.00 ng/ml