

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012023\
 Data File : PL080416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2023 16:31
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 16:53:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 20 16:52:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.689	51788595	66356227	24.290	23.510
28)	SA Decachlor...	8.790	7.839	48277541	62220637	24.164	24.831
Target Compounds							
23)	Chlordane-1	4.500	3.687	20933212	20045408	234.390	241.112
24)	Chlordane-2	5.026	4.264	23944009	22663186	248.160	247.087
25)	Chlordane-3	5.731	4.894	82008109	63440222	236.298	236.116
26)	Chlordane-4	5.814	4.957	106.2E6	64851087	239.868	234.771
27)	Chlordane-5	6.655	5.625	17771529	17724951	237.632	245.648


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012023\
Data File : PL080416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2023 16:31
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 16:53:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Fri Jan 20 16:52:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

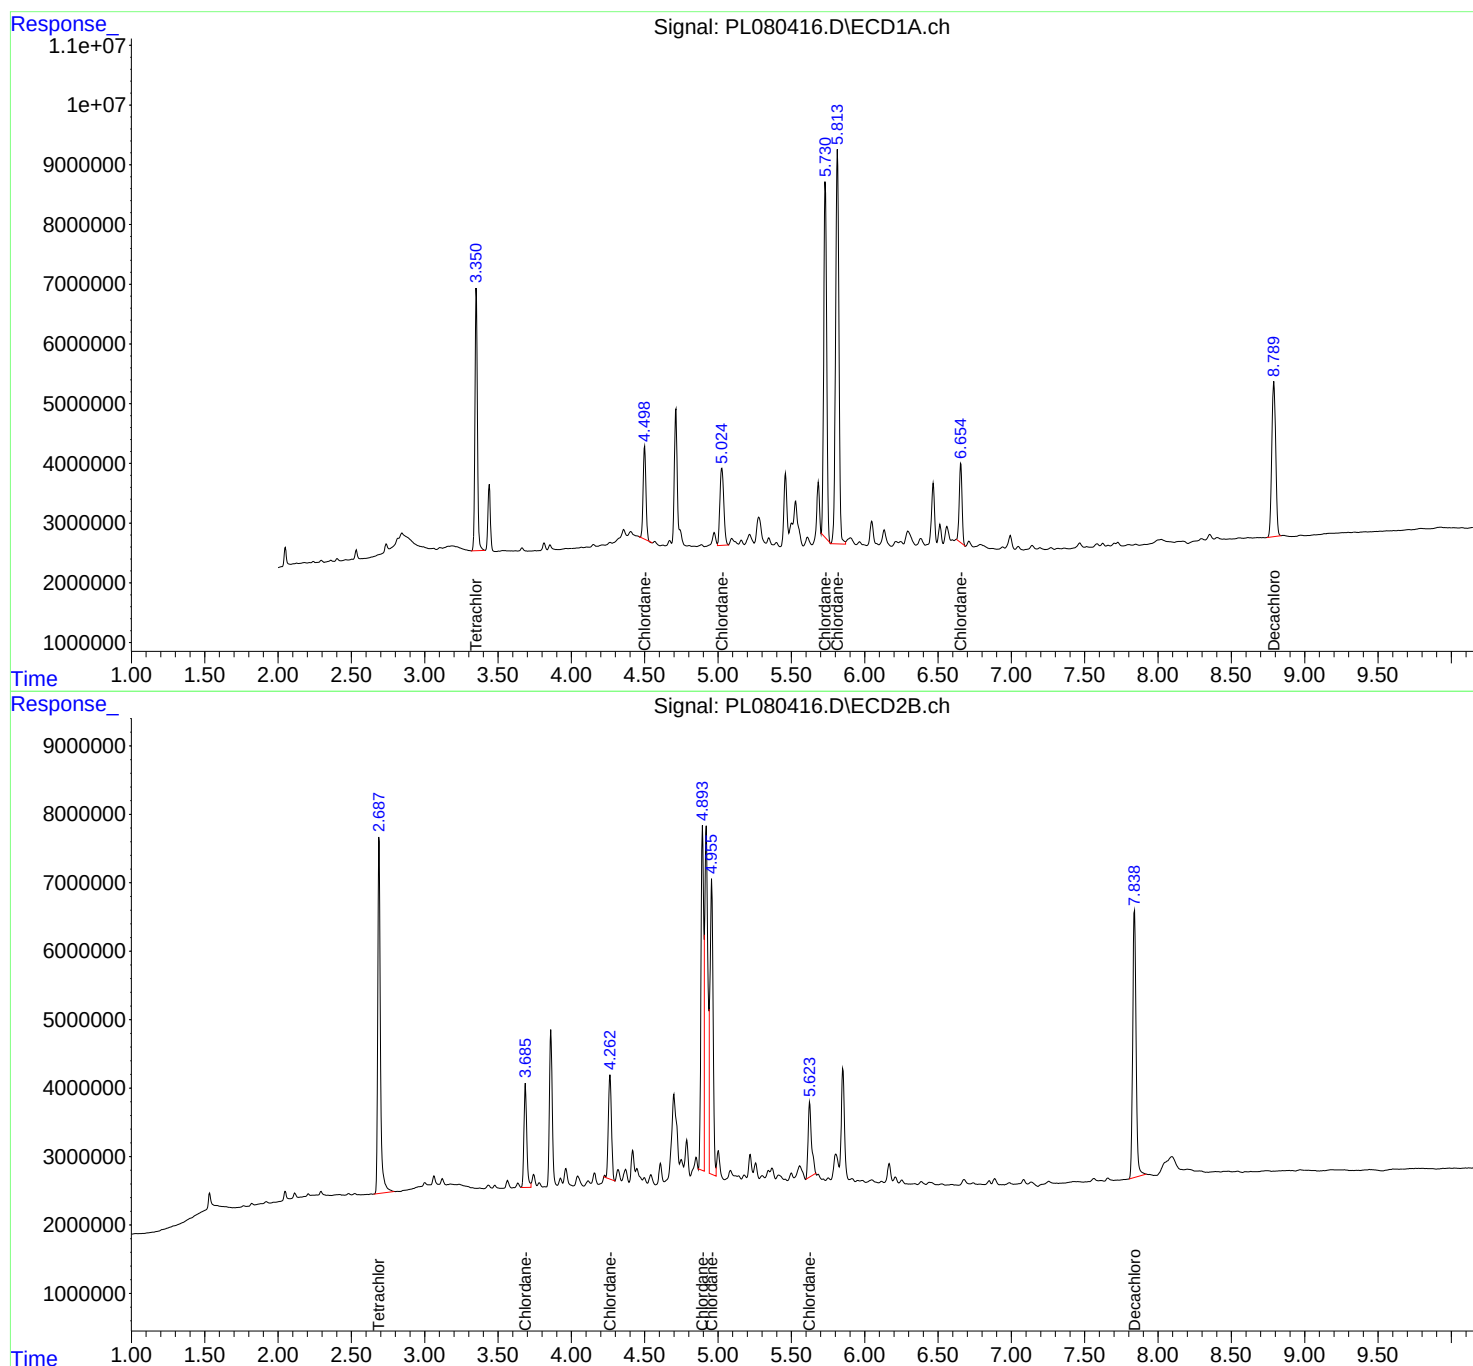


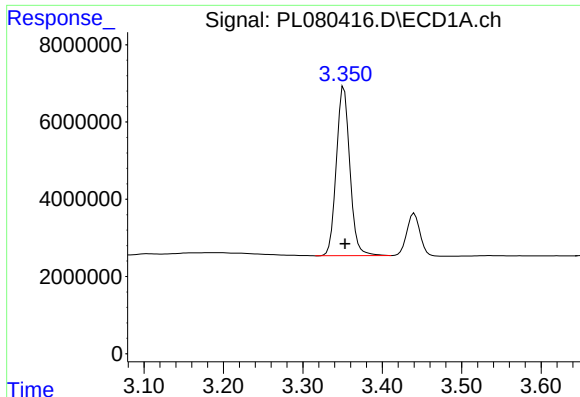

#1 Tetrachloro-m-xylene


R.T.: 3.352 min
Delta R.T.: -0.001 min
Response: 51788595
Conc: 24.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

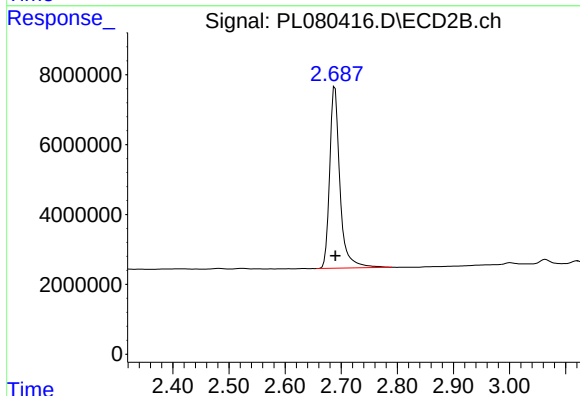


#1 Tetrachloro-m-xylene

R.T.: 2.689 min
Delta R.T.: 0.000 min
Response: 66356227
Conc: 23.51 ng/ml

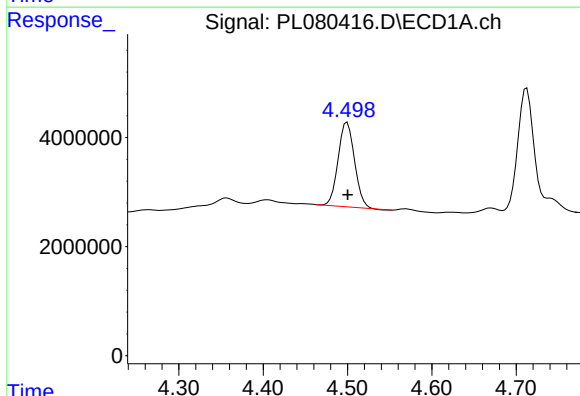


#23 Chlordane-1

R.T.: 4.500 min
Delta R.T.: 0.000 min
Response: 20933212
Conc: 234.39 ng/ml

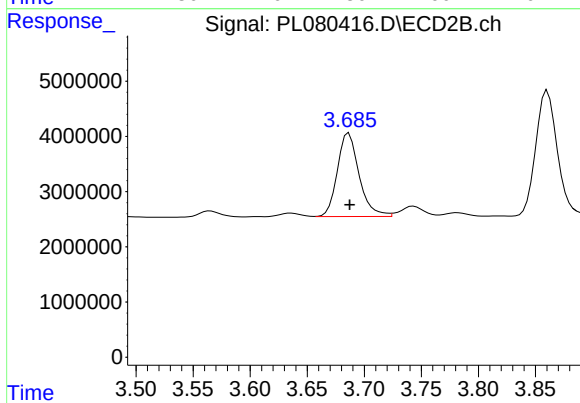

#23 Chlordane-1


R.T.: 3.687 min
Delta R.T.: 0.000 min
Response: 20045408
Conc: 241.11 ng/ml

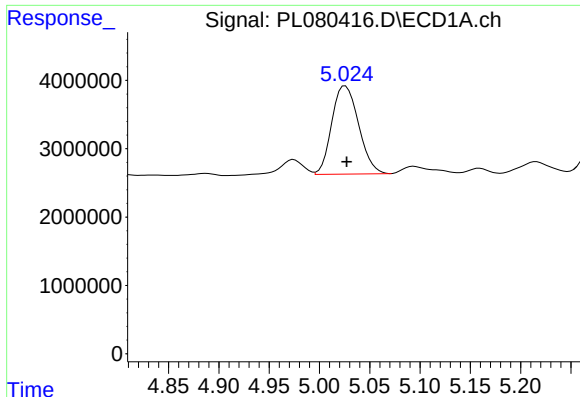

#24 Chlordane-2


R.T.: 5.026 min
Delta R.T.: -0.002 min
Response: 23944009
Conc: 248.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

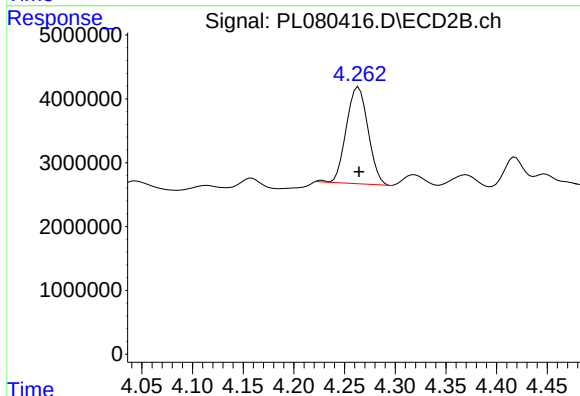


#24 Chlordane-2

R.T.: 4.264 min
Delta R.T.: 0.000 min
Response: 22663186
Conc: 247.09 ng/ml

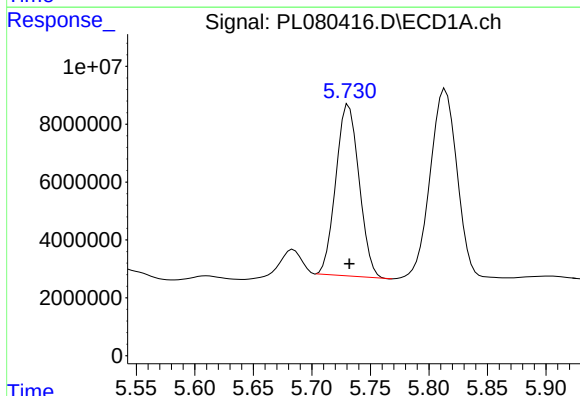


#25 Chlordane-3

R.T.: 5.731 min
Delta R.T.: 0.000 min
Response: 82008109
Conc: 236.30 ng/ml

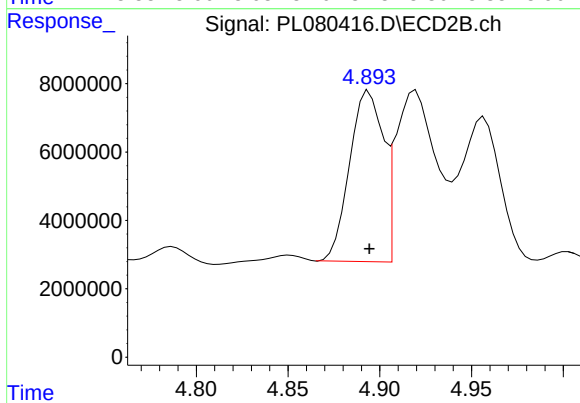

#25 Chlordane-3


R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 63440222
Conc: 236.12 ng/ml

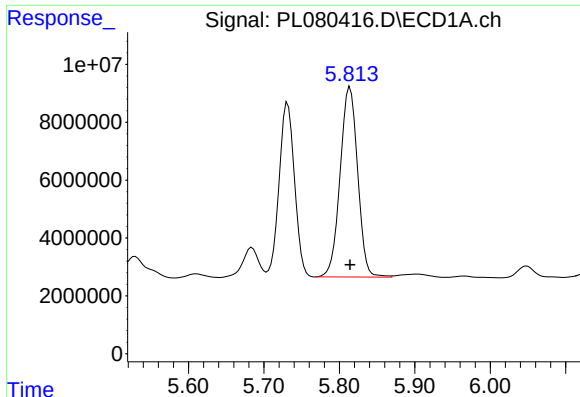

#26 Chlordane-4


R.T.: 5.814 min
Delta R.T.: 0.000 min
Response: 106241503
Conc: 239.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

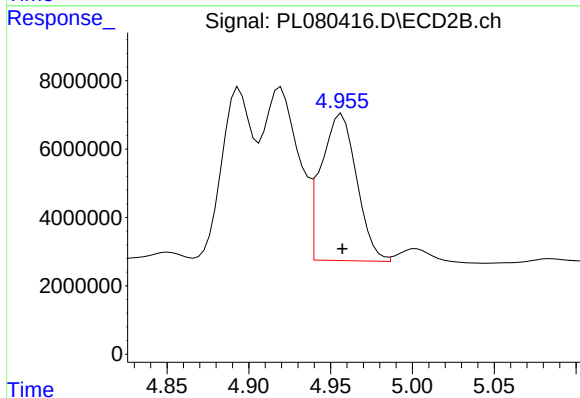


#26 Chlordane-4

R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 64851087
Conc: 234.77 ng/ml

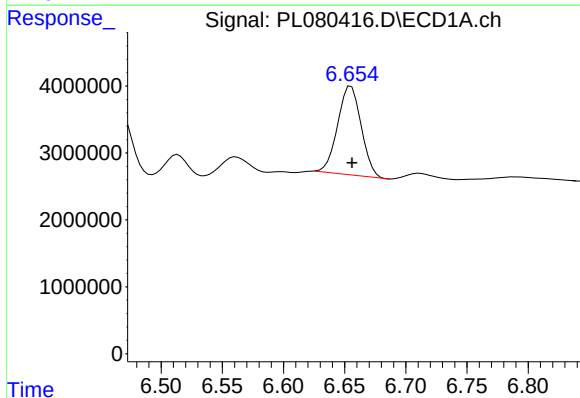


#27 Chlordane-5

R.T.: 6.655 min
Delta R.T.: 0.000 min
Response: 17771529
Conc: 237.63 ng/ml

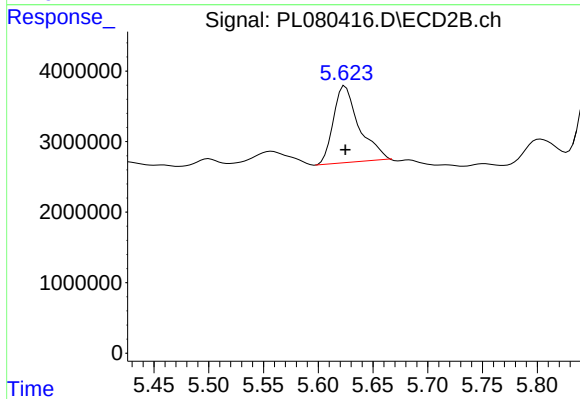

#27 Chlordane-5


R.T.: 5.625 min
Delta R.T.: 0.000 min
Response: 17724951
Conc: 245.65 ng/ml

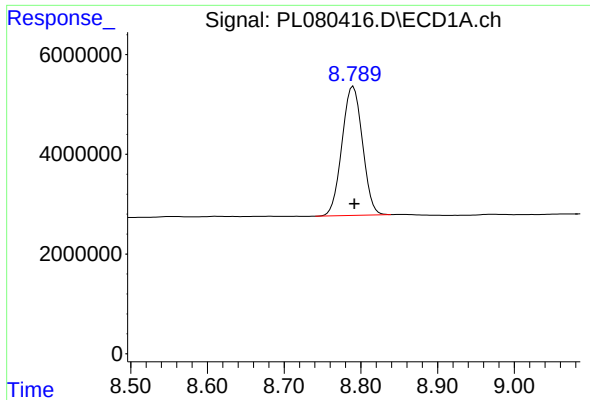

#28 Decachlorobiphenyl

R.T.: 8.790 min
Delta R.T.: -0.002 min
Response: 48277541
Conc: 24.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

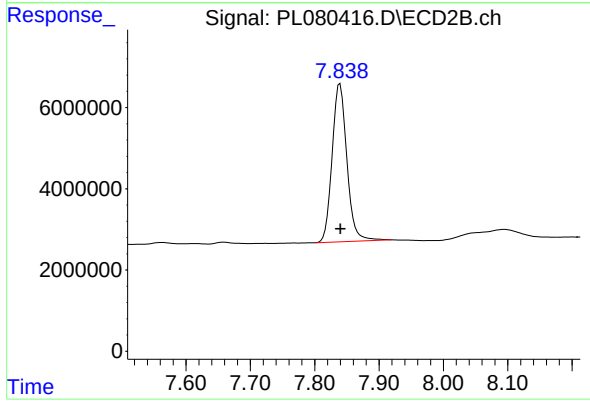

#28 Decachlorobiphenyl

R.T.: 7.839 min
Delta R.T.: 0.000 min
Response: 62220637
Conc: 24.83 ng/ml