

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012023\
 Data File : PL080414.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2023 16:04
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 16:53:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 20 16:52:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.352	2.689	158.1E6	205.5E6	74.167	72.800
28)	SA Decachlor...	8.791	7.840	124.4E6	171.6E6	62.269	68.495
Target Compounds							
23)	Chlordane-1	4.500	3.687	66049986	61556535	739.564	740.421
24)	Chlordane-2	5.026	4.264	70306853	66129865	728.672	720.985
25)	Chlordane-3	5.732	4.895	259.0E6	206.8E6	746.210	769.537
26)	Chlordane-4	5.814	4.957	326.3E6	210.7E6	736.717	762.827
27)	Chlordane-5	6.657	5.625	54722831	54420116	731.726	754.202


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012023\
Data File : PL080414.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2023 16:04
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 16:53:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Fri Jan 20 16:52:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

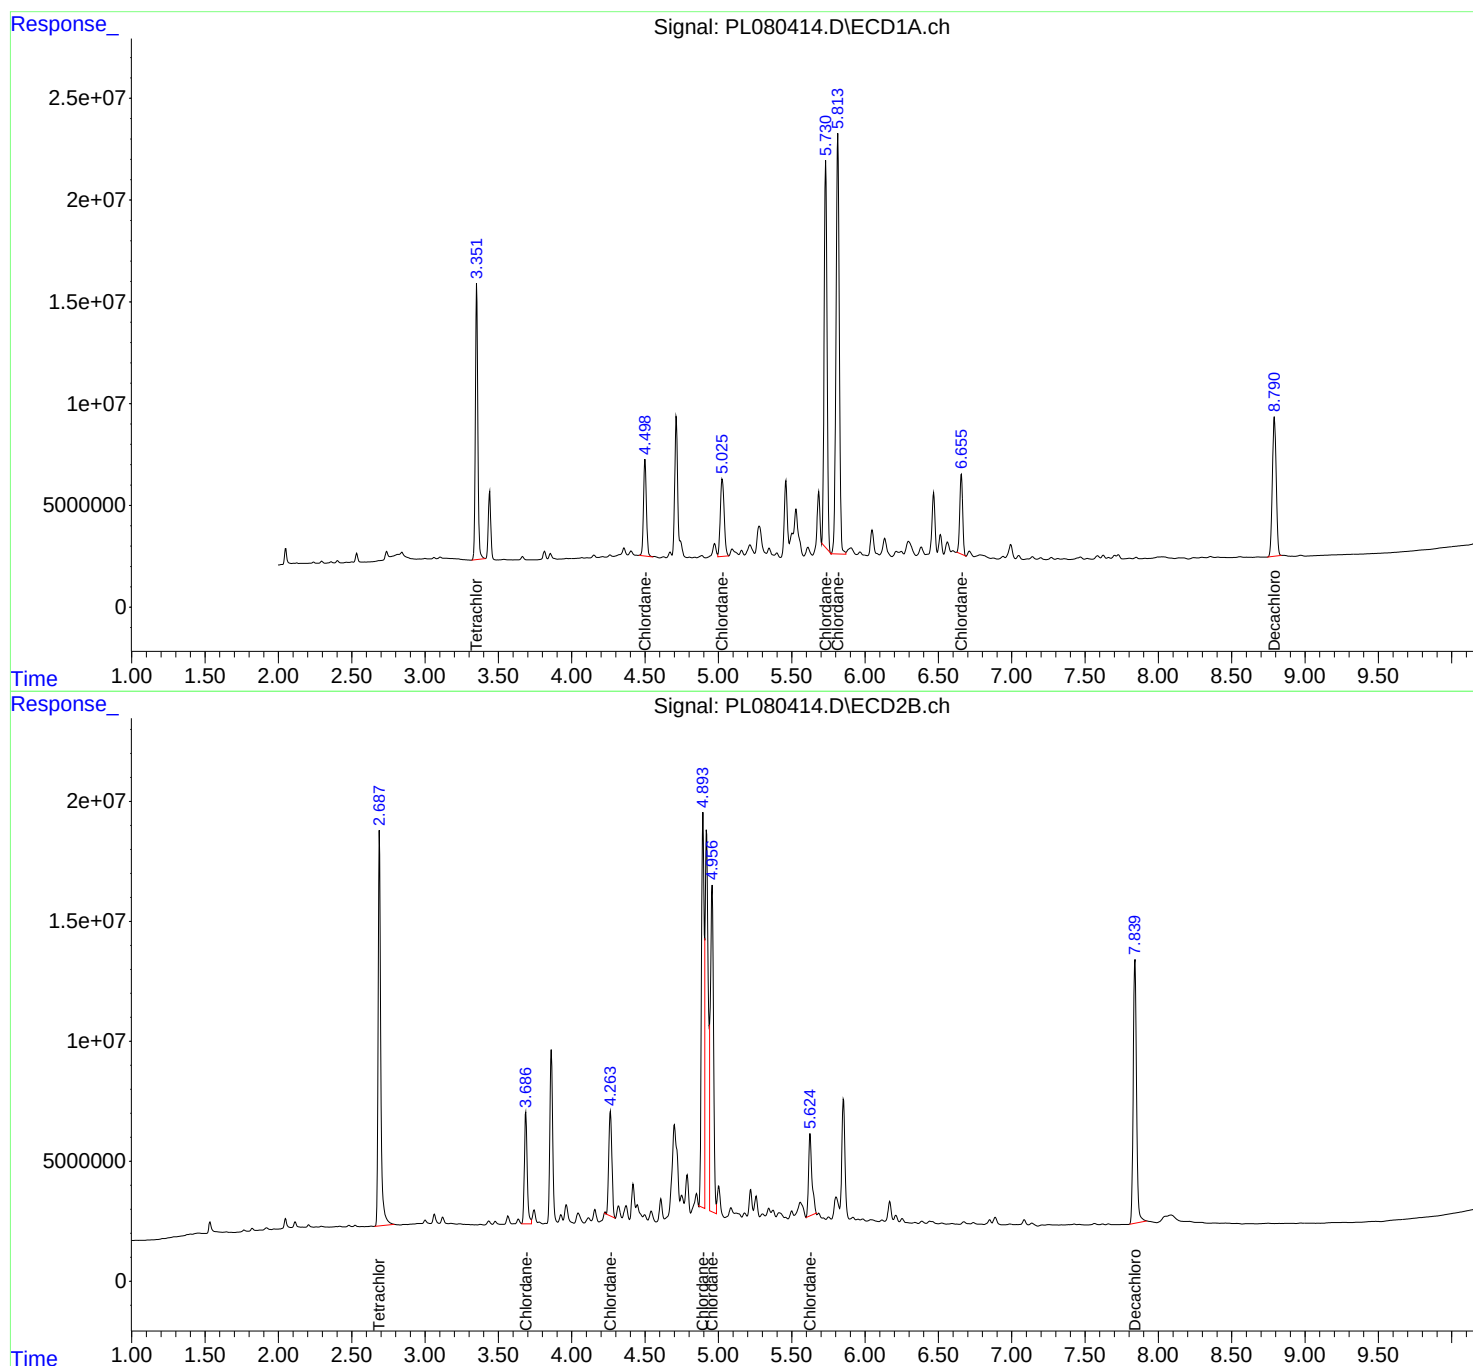


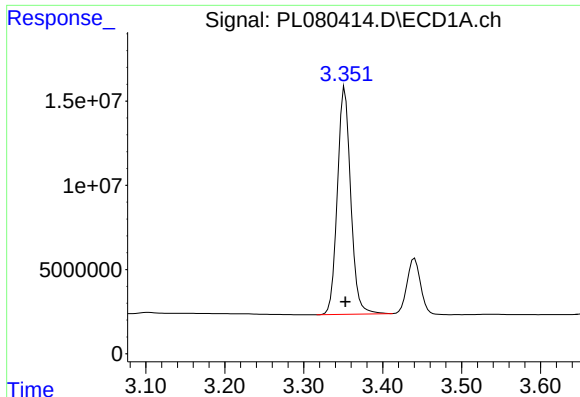

#1 Tetrachloro-m-xylene


R.T.: 3.352 min
Delta R.T.: 0.000 min
Response: 158132647
Conc: 74.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

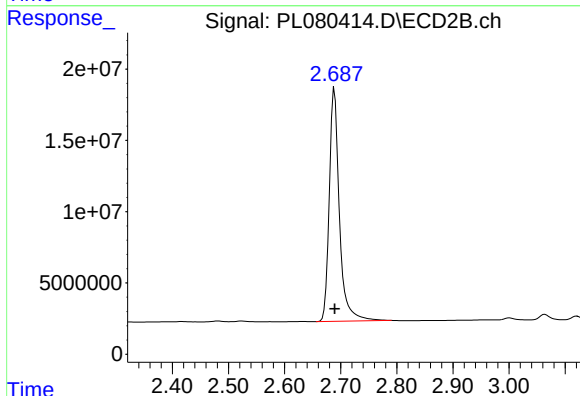


#1 Tetrachloro-m-xylene

R.T.: 2.689 min
Delta R.T.: 0.000 min
Response: 205474854
Conc: 72.80 ng/ml

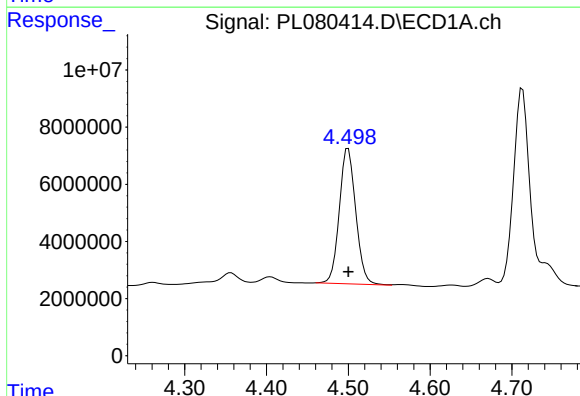


#23 Chlordane-1

R.T.: 4.500 min
Delta R.T.: 0.000 min
Response: 66049986
Conc: 739.56 ng/ml

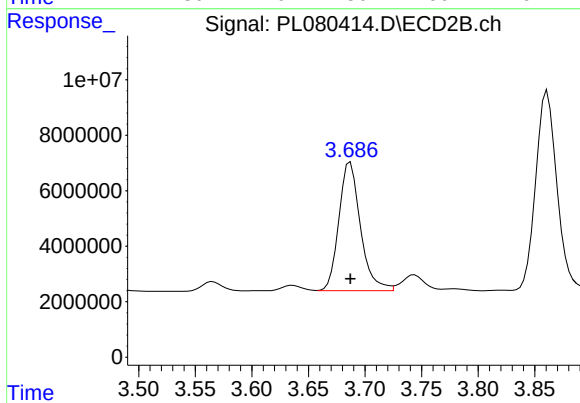

#23 Chlordane-1


R.T.: 3.687 min
Delta R.T.: 0.000 min
Response: 61556535
Conc: 740.42 ng/ml

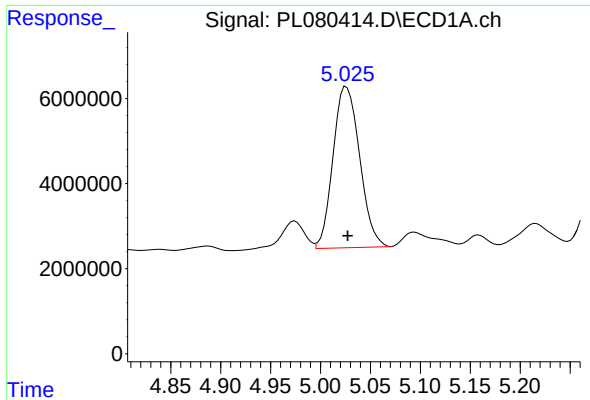

#24 Chlordane-2


R.T.: 5.026 min
Delta R.T.: -0.001 min
Response: 70306853
Conc: 728.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

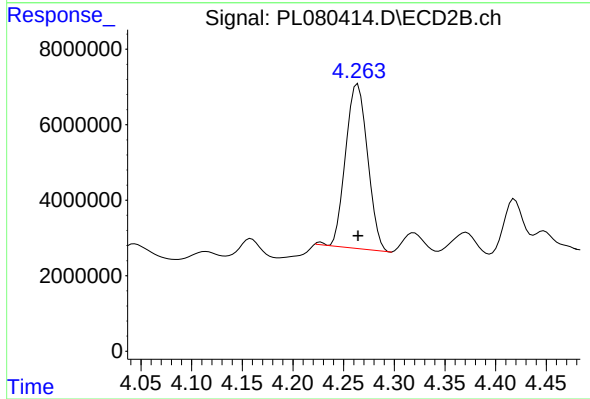


#24 Chlordane-2

R.T.: 4.264 min
Delta R.T.: 0.000 min
Response: 66129865
Conc: 720.99 ng/ml

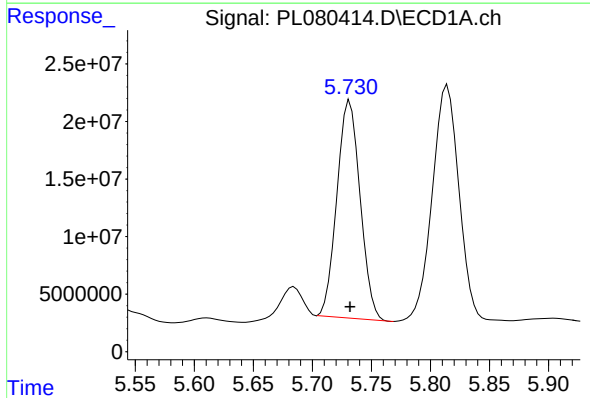


#25 Chlordane-3

R.T.: 5.732 min
Delta R.T.: 0.000 min
Response: 258974943
Conc: 746.21 ng/ml

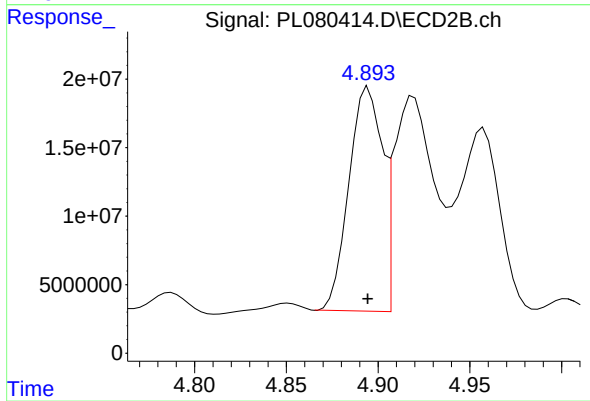

#25 Chlordane-3


R.T.: 4.895 min
Delta R.T.: 0.000 min
Response: 206761063
Conc: 769.54 ng/ml

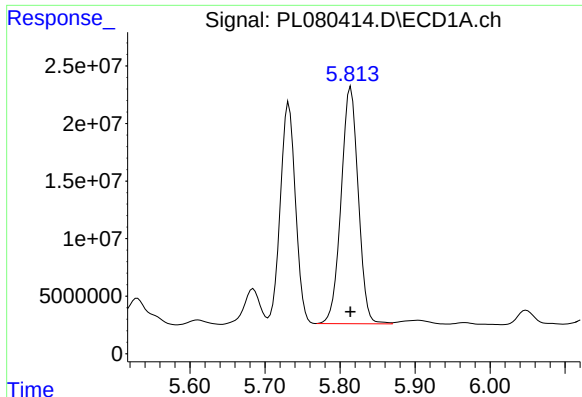

#26 Chlordane-4


R.T.: 5.814 min
Delta R.T.: 0.000 min
Response: 326304136
Conc: 736.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

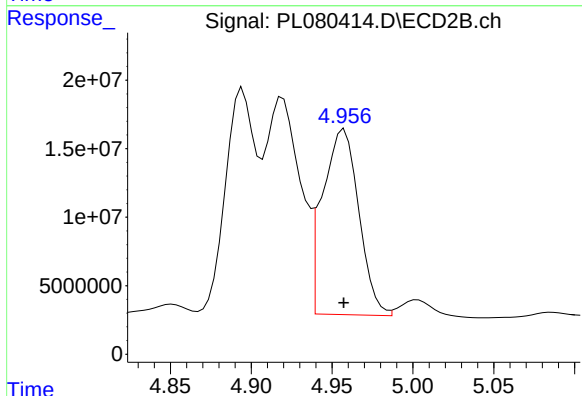


#26 Chlordane-4

R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 210716329
Conc: 762.83 ng/ml

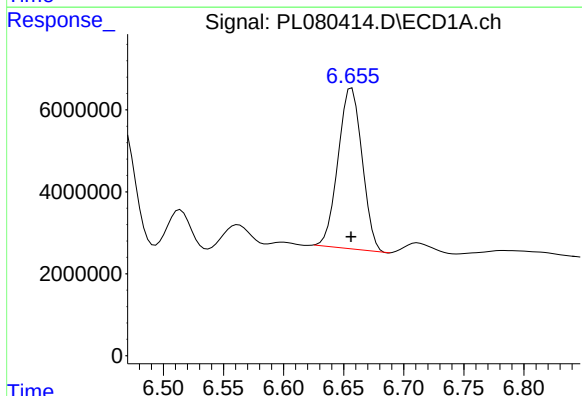


#27 Chlordane-5

R.T.: 6.657 min
Delta R.T.: 0.000 min
Response: 54722831
Conc: 731.73 ng/ml

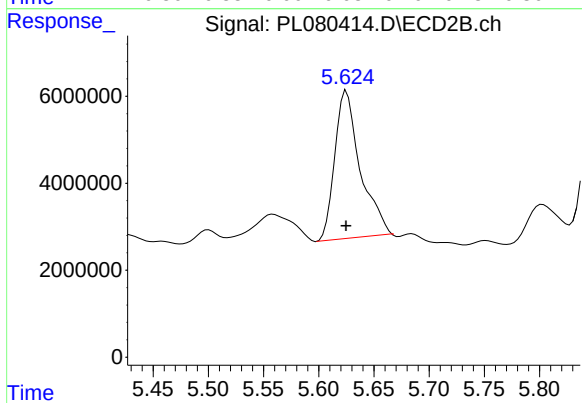

#27 Chlordane-5


R.T.: 5.625 min
Delta R.T.: 0.000 min
Response: 54420116
Conc: 754.20 ng/ml

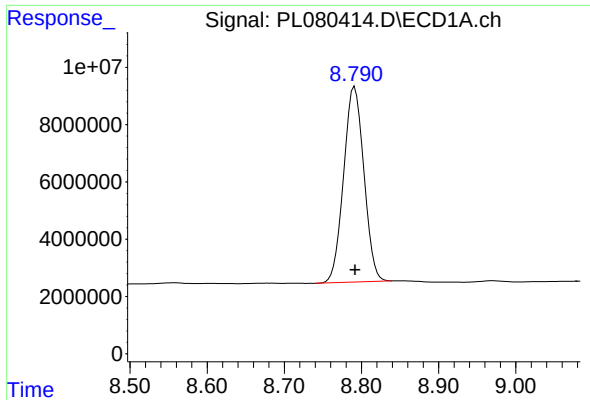

#28 Decachlorobiphenyl

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 124406944
Conc: 62.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

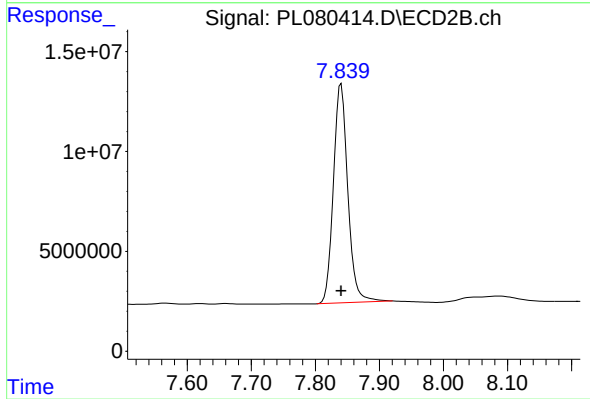

#28 Decachlorobiphenyl

R.T.: 7.840 min
Delta R.T.: 0.000 min
Response: 171629598
Conc: 68.50 ng/ml