

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012023\
 Data File : PL080424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2023 18:37
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL012023CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 23:57:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:55:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.351	2.689	107.8E6	138.9E6	51.539	51.511
28)	SA Decachlor...	8.788	7.838	87300597	118.5E6	47.759	48.528
Target Compounds							
23)	Chlordane-1	4.499	3.686	45135118	42034961	529.883	516.229
24)	Chlordane-2	5.026	4.263	49295336	46601630	511.100	516.888
25)	Chlordane-3	5.731	4.894	175.2E6	136.5E6	518.581	517.708
26)	Chlordane-4	5.813	4.957	223.1E6	138.7E6	517.138	515.053
27)	Chlordane-5	6.655	5.625	37315066	37544445	529.806	527.639



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012023\
Data File : PL080424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2023 18:37
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL012023CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 23:57:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:55:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

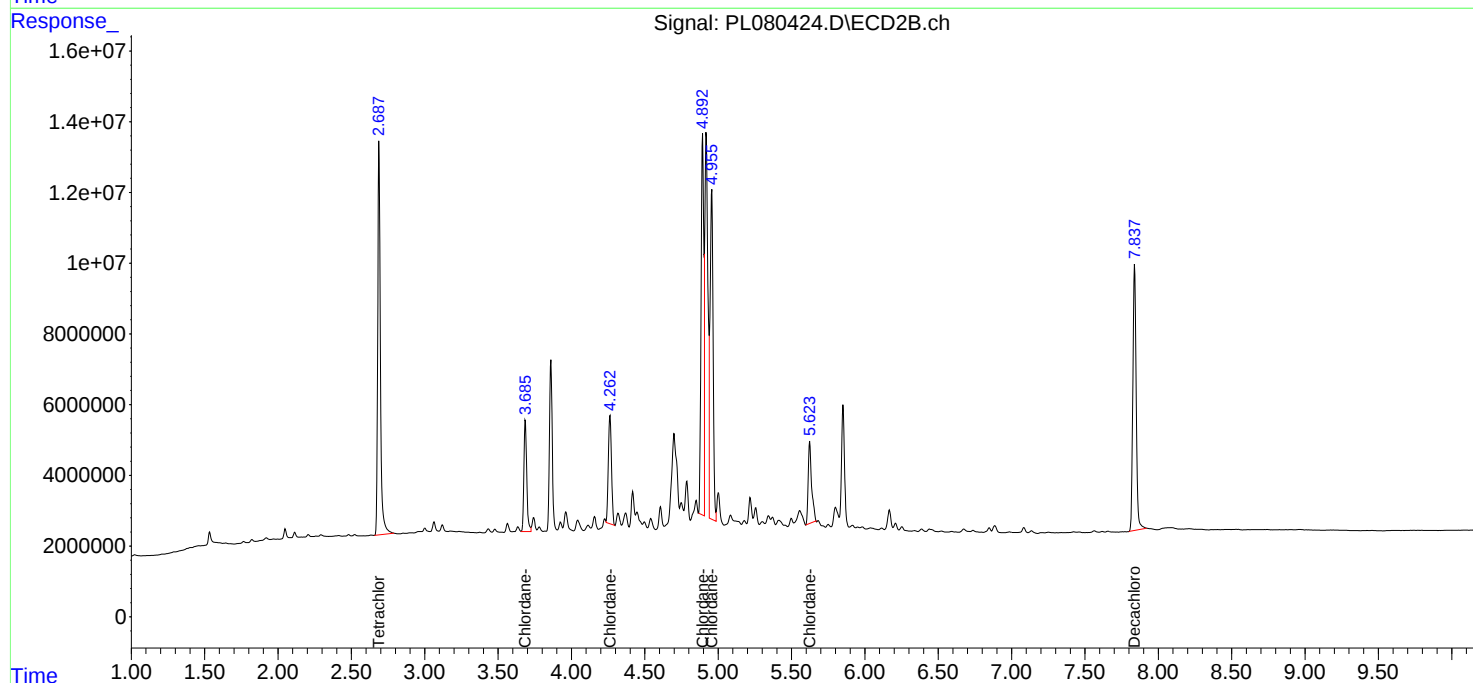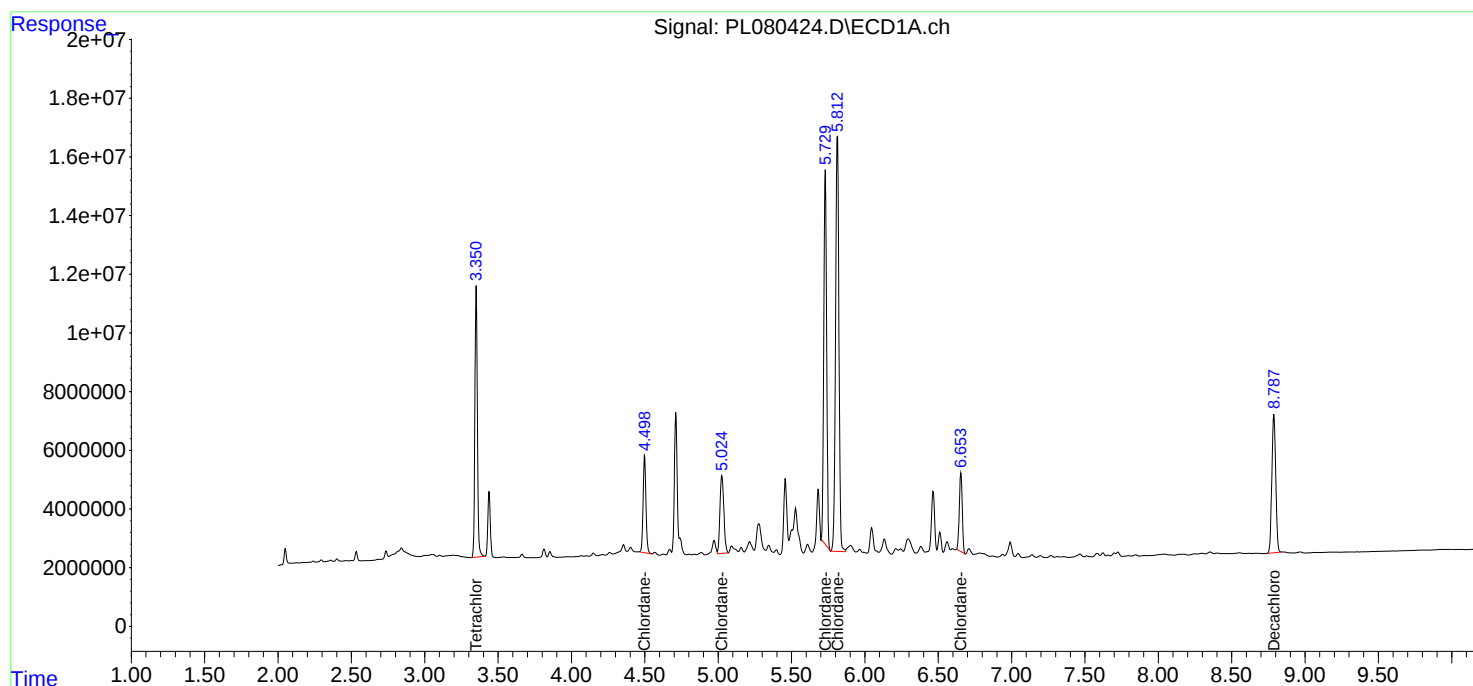


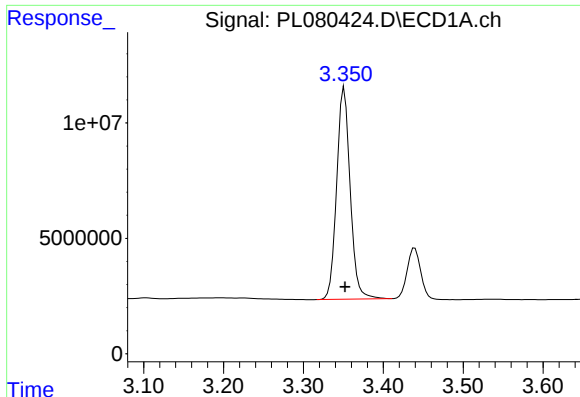

#1 Tetrachloro-m-xylene


R.T.: 3.351 min
Delta R.T.: 0.000 min
Response: 107826259
Conc: 51.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL012023CHLOR

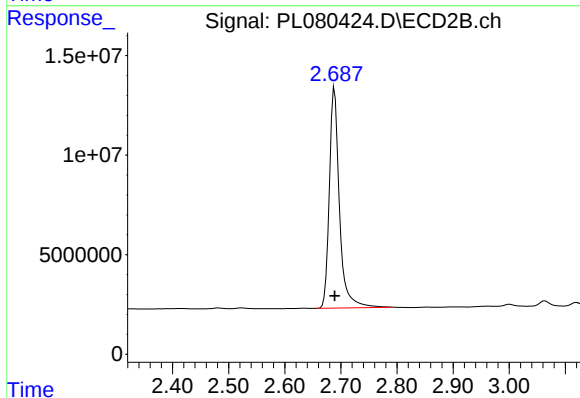


#1 Tetrachloro-m-xylene

R.T.: 2.689 min
Delta R.T.: 0.000 min
Response: 138913990
Conc: 51.51 ng/ml

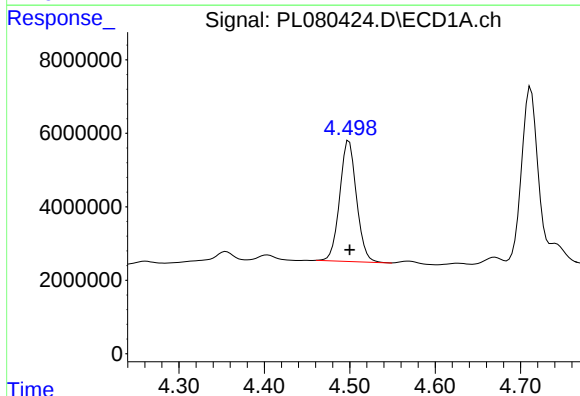


#23 Chlordane-1

R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 45135118
Conc: 529.88 ng/ml

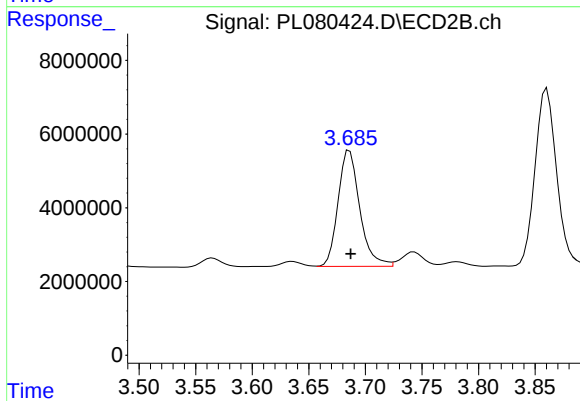

#23 Chlordane-1


R.T.: 3.686 min
Delta R.T.: 0.000 min
Response: 42034961
Conc: 516.23 ng/ml

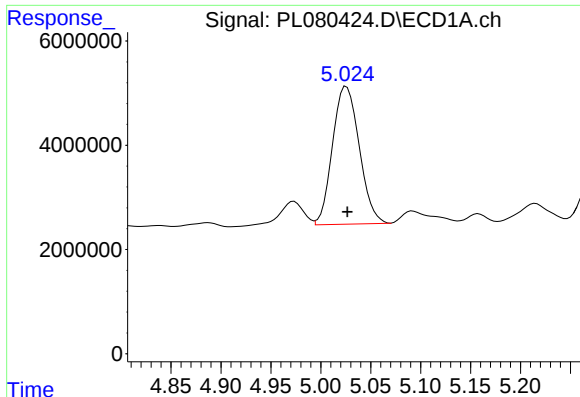

#24 Chlordane-2


R.T.: 5.026 min
Delta R.T.: 0.000 min
Response: 49295336
Conc: 511.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL012023CHLOR

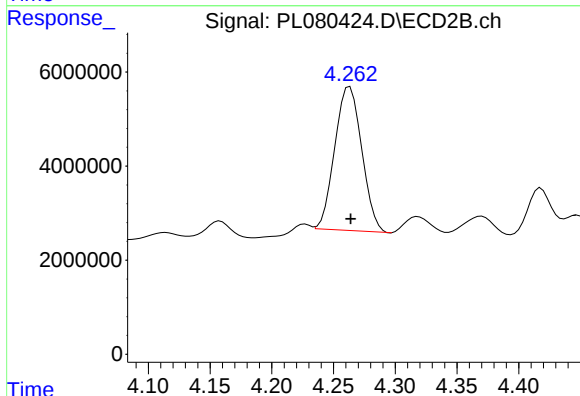


#24 Chlordane-2

R.T.: 4.263 min
Delta R.T.: 0.000 min
Response: 46601630
Conc: 516.89 ng/ml

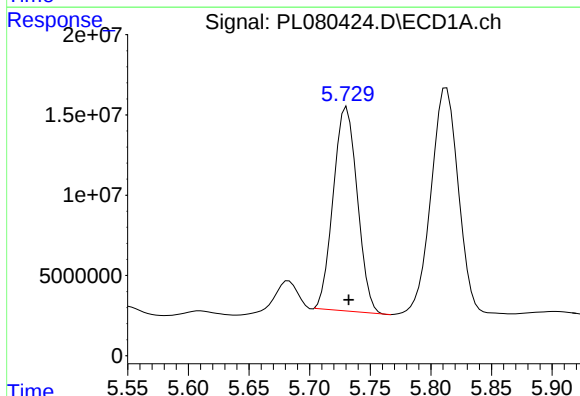


#25 Chlordane-3

R.T.: 5.731 min
Delta R.T.: -0.002 min
Response: 175234280
Conc: 518.58 ng/ml

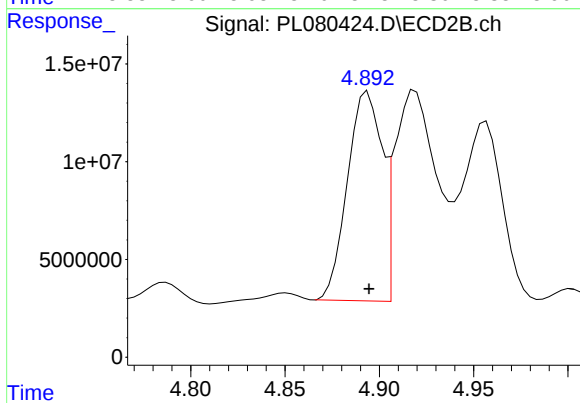

#25 Chlordane-3


R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 136542982
Conc: 517.71 ng/ml

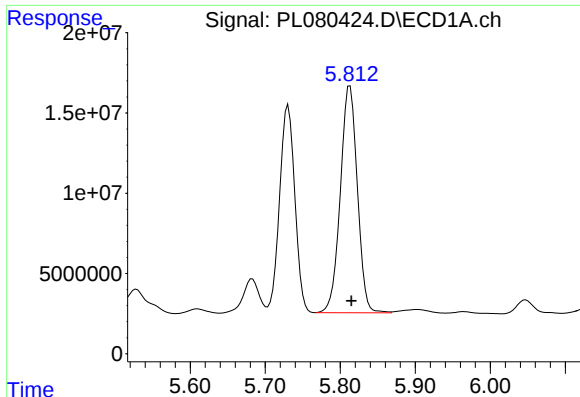

#26 Chlordane-4


R.T.: 5.813 min
Delta R.T.: -0.002 min
Response: 223101134
Conc: 517.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL012023CHLOR

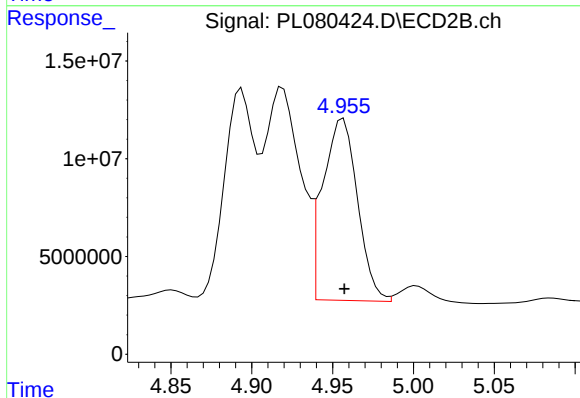


#26 Chlordane-4

R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 138702765
Conc: 515.05 ng/ml

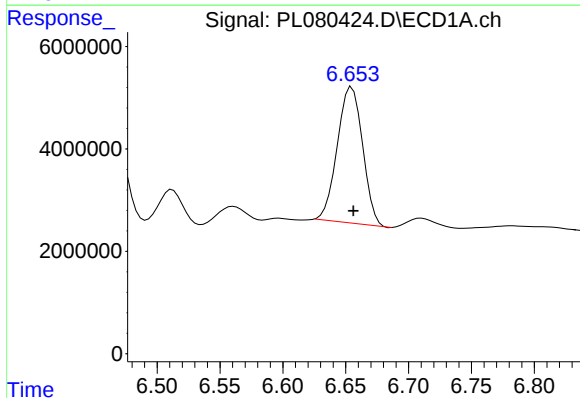


#27 Chlordane-5

R.T.: 6.655 min
Delta R.T.: -0.001 min
Response: 37315066
Conc: 529.81 ng/ml

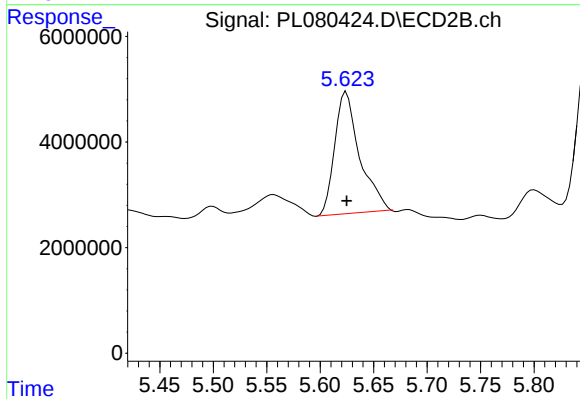

#27 Chlordane-5


R.T.: 5.625 min
Delta R.T.: 0.000 min
Response: 37544445
Conc: 527.64 ng/ml

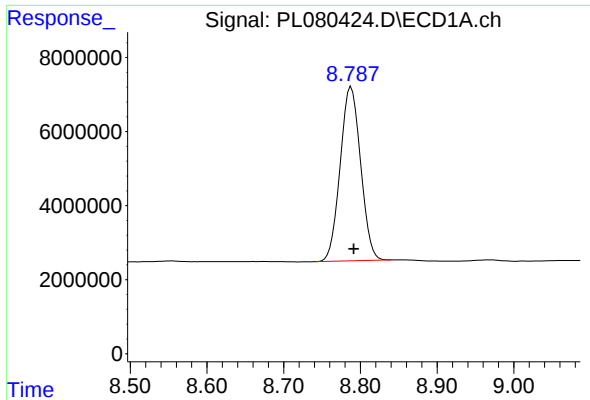

#28 Decachlorobiphenyl

R.T.: 8.788 min
Delta R.T.: -0.003 min
Response: 87300597
Conc: 47.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL012023CHLOR

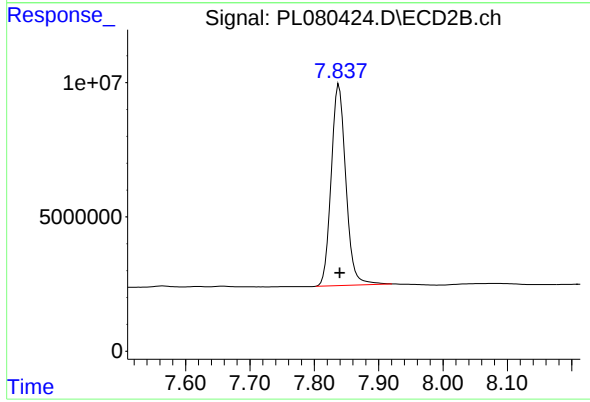

#28 Decachlorobiphenyl

R.T.: 7.838 min
Delta R.T.: -0.001 min
Response: 118547813
Conc: 48.53 ng/ml