

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012120\
 Data File : PL055930.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 11:33
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 01:14:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.489	3.966	204.3E6	62086979	21.313	21.968
28)	SA Decachlor...	8.233	8.951	214.5E6	49624807	20.515	21.661
Target Compounds							
2)	A alpha-BHC	3.923	0.000	6637892	0	0.400	N.D. #
6)	B beta-BHC	4.478f	0.000	1633962	0	0.255	N.D. #
8)	B Heptachlo...	0.000	5.800	0	2251955	N.D.	0.754 #
9)	A Endosulfan I	5.548	0.000	8148699	0	0.628	N.D. #
11)	B alpha-Chl...	5.478	0.000	72977525	0	5.279	N.D. #
14)	MA Endrin	6.044	6.628	5659219	3449060	0.448	1.361 #
19)	B Endosulfa...	6.719f	0.000	1738868	0	0.161	N.D. #
26)	Chlordane-4	5.478	0.000	72977525	0	70.773	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012120\
Data File : PL055930.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 11:33
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 01:14:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

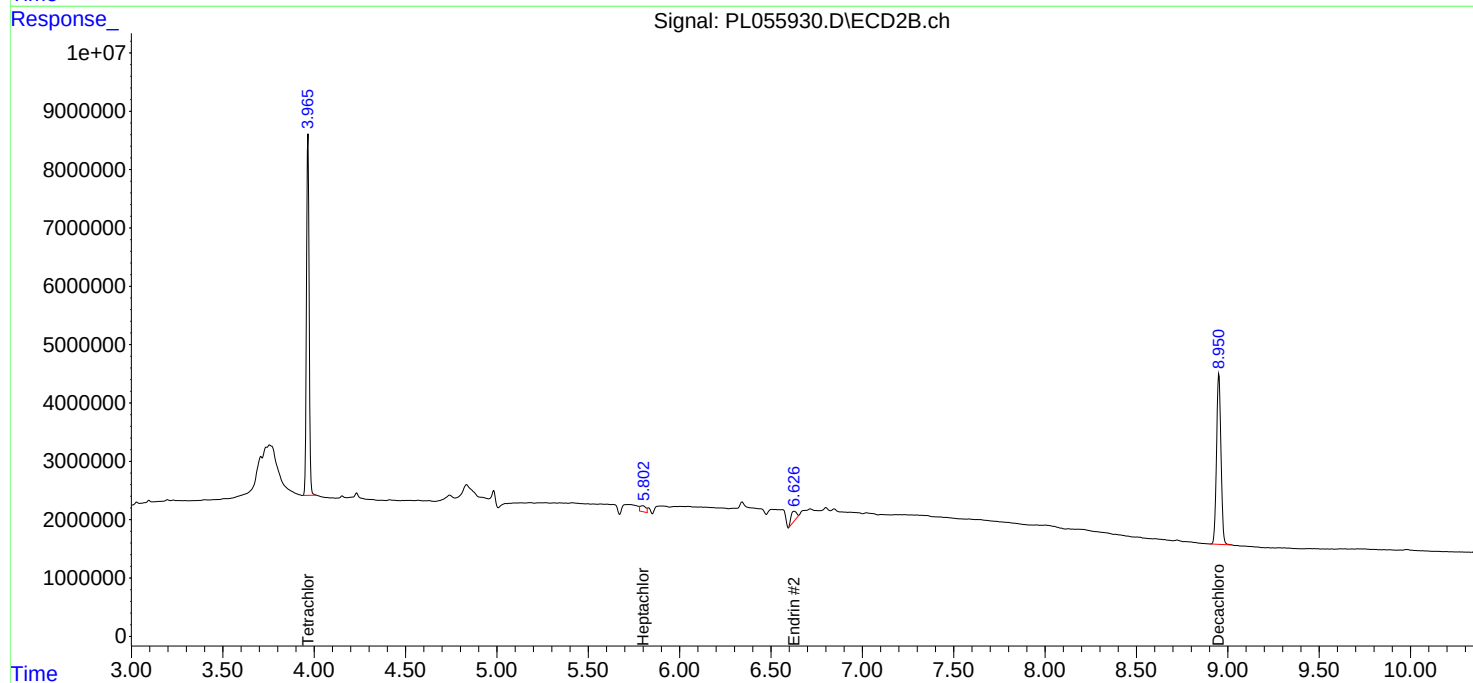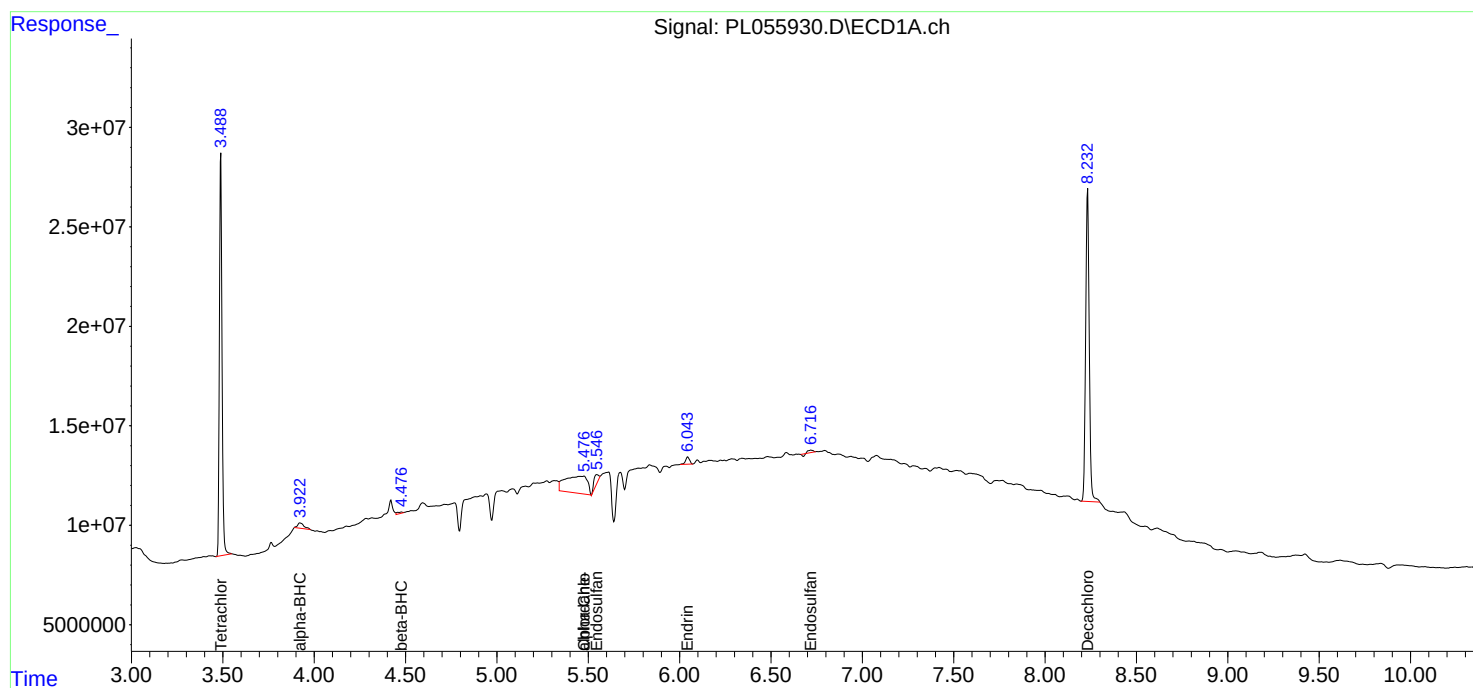


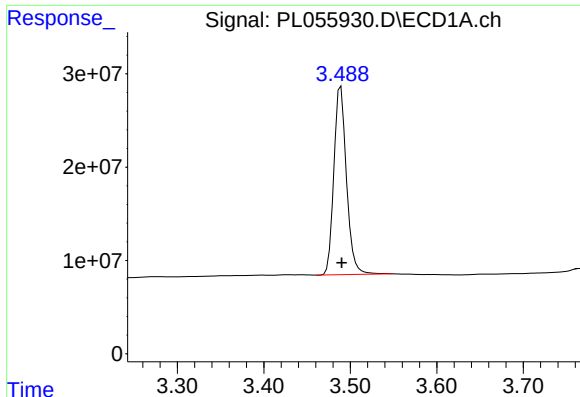

#1 Tetrachloro-m-xylene


R.T.: 3.489 min
Delta R.T.: 0.000 min
Response: 204278635
Conc: 21.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

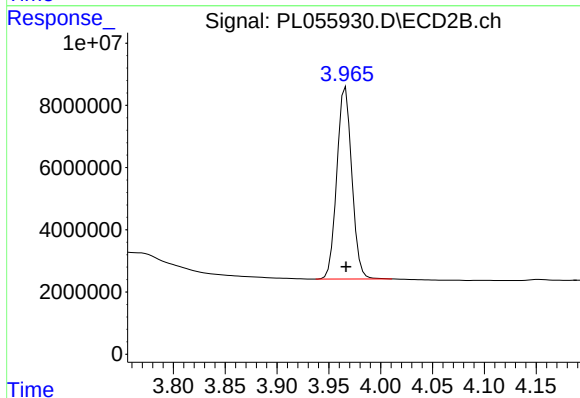


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 62086979
Conc: 21.97 ng/ml

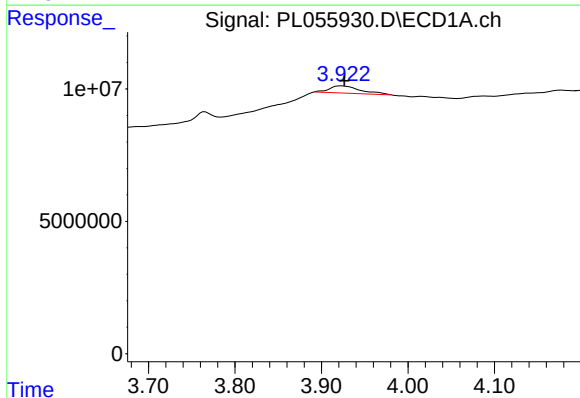


#2 alpha-BHC

R.T.: 3.923 min
Delta R.T.: -0.004 min
Response: 6637892
Conc: 0.40 ng/ml

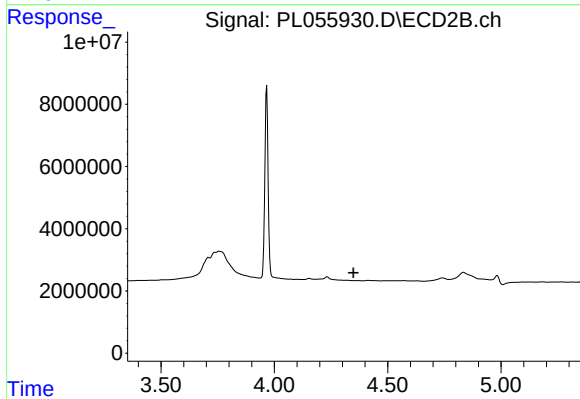

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.350 min
Response: 0
Conc: N.D.

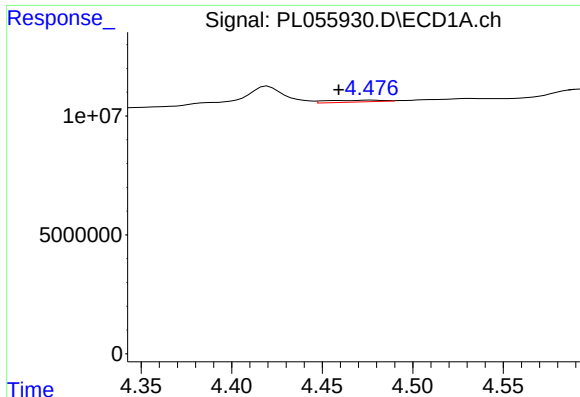

#6 beta-BHC


R.T.: 4.478 min
Delta R.T.: 0.019 min
Response: 1633962
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

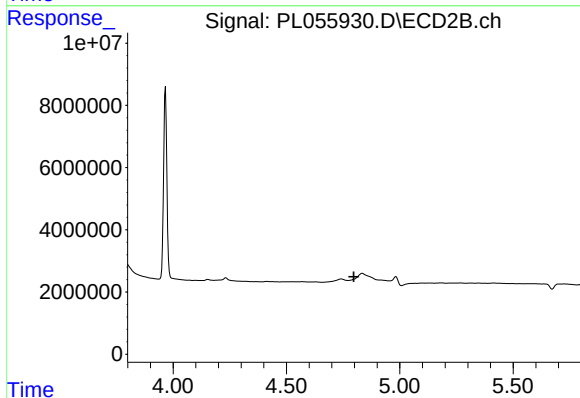


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.798 min
Response: 0
Conc: N.D.

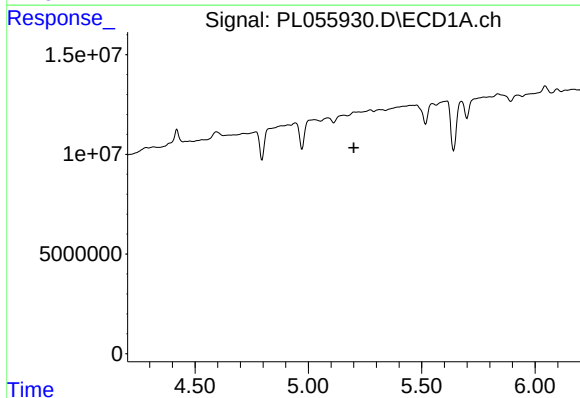


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.201 min
Response: 0
Conc: N.D.

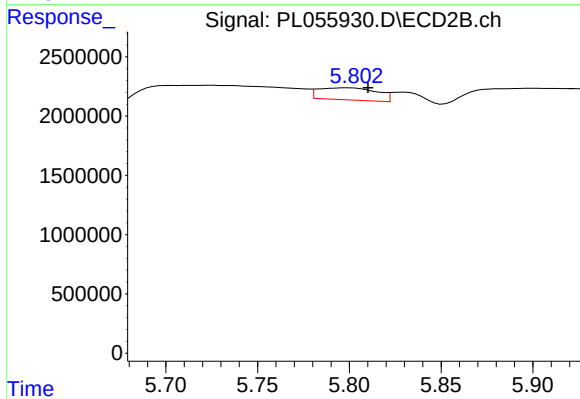

#8 Heptachlor epoxide


R.T.: 5.800 min
Delta R.T.: -0.011 min
Response: 2251955
Conc: 0.75 ng/ml

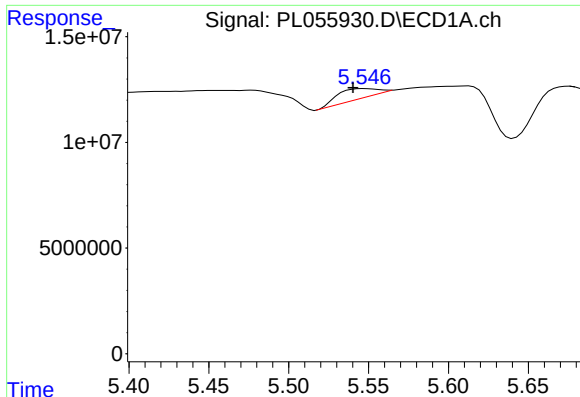

#9 Endosulfan I


R.T.: 5.548 min
Delta R.T.: 0.008 min
Response: 8148699
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

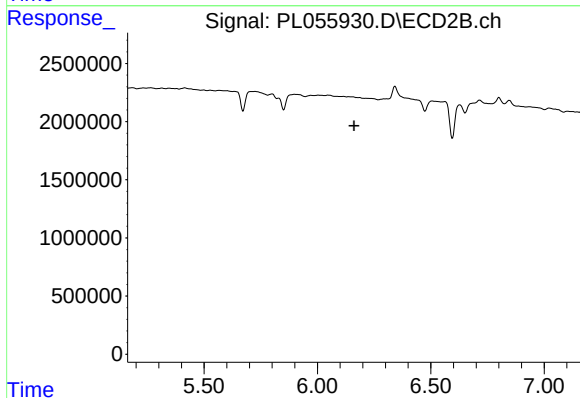


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

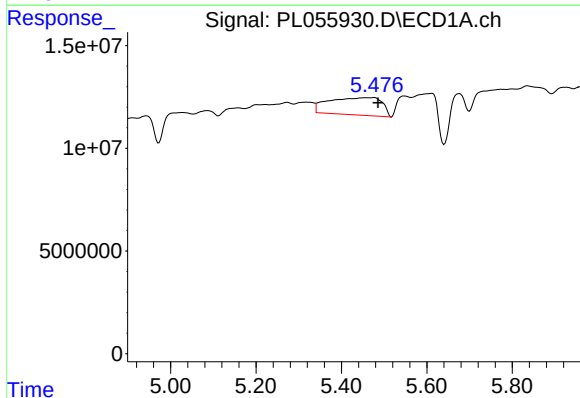


#11 alpha-Chlordane

R.T.: 5.478 min
Delta R.T.: -0.009 min
Response: 72977525
Conc: 5.28 ng/ml

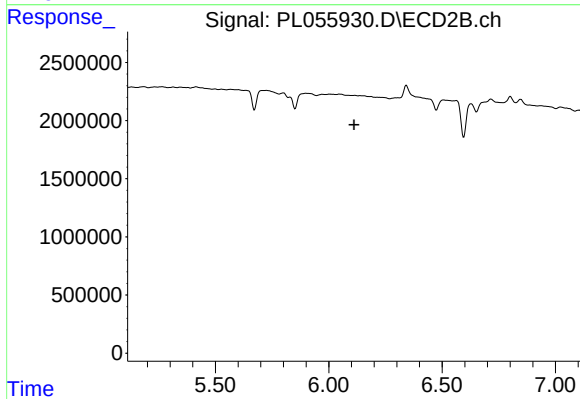

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

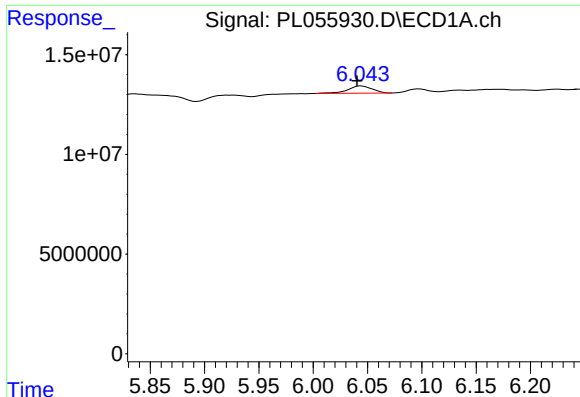

#14 Endrin


R.T.: 6.044 min
Delta R.T.: 0.004 min
Response: 5659219
Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

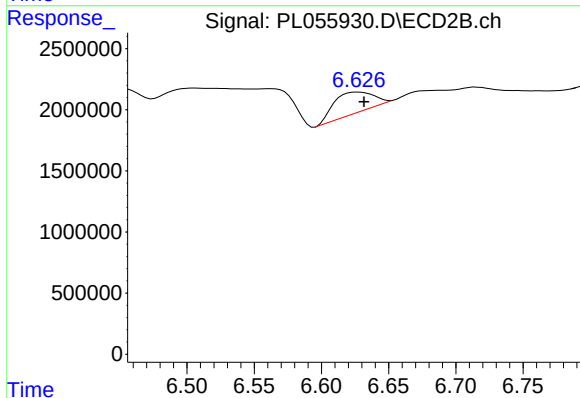


#14 Endrin

R.T.: 6.628 min
Delta R.T.: -0.004 min
Response: 3449060
Conc: 1.36 ng/ml

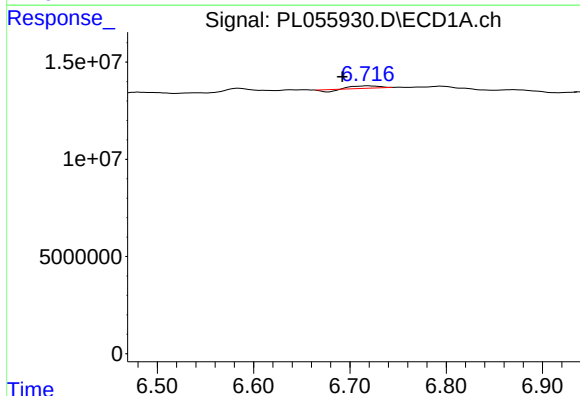


#19 Endosulfan Sulfate

R.T.: 6.719 min
Delta R.T.: 0.027 min
Response: 1738868
Conc: 0.16 ng/ml

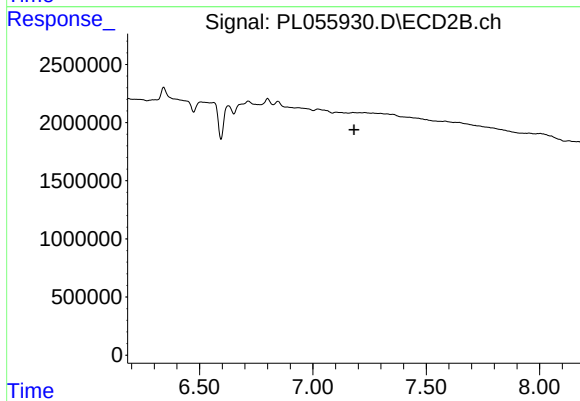

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.182 min
Response: 0
Conc: N.D.

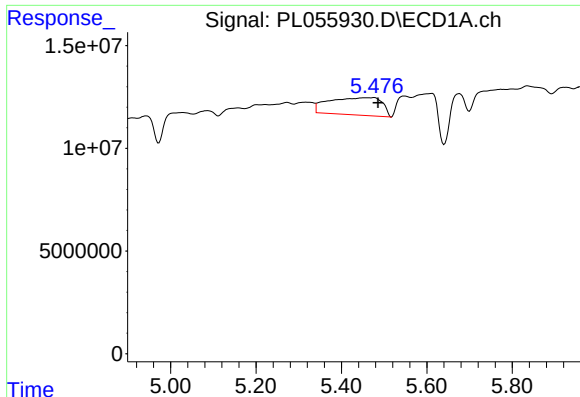

#26 Chlordane-4


R.T.: 5.478 min
Delta R.T.: -0.008 min
Response: 72977525
Conc: 70.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

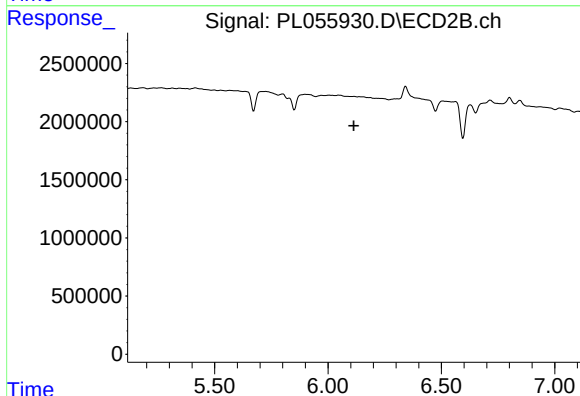


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

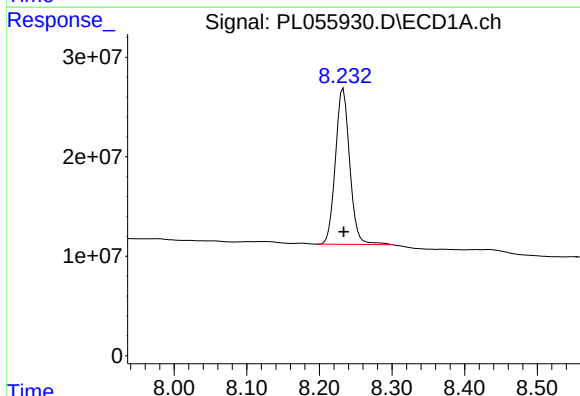

#28 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: 0.000 min
Response: 214501074
Conc: 20.52 ng/ml

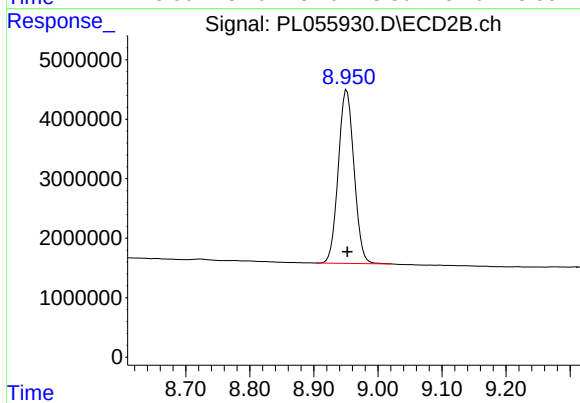

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: 0.000 min
Response: 49624807
Conc: 21.66 ng/ml