

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012120\
 Data File : PL055943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 15:40
 Operator : AJ\MA
 Sample : PB126238BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 01:16:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.492	3.965	215.2E6	65452013	22.451	23.159
28)	SA Decachlor...	8.238	8.954	220.0E6	48891545	21.038	21.341
Target Compounds							
4)	MA Heptachlor	4.515	0.000	3040862	0	0.204	N.D. #
6)	B beta-BHC	4.472	4.826f	1628304	15221421	0.254	9.592 #
9)	A Endosulfan I	5.546	0.000	2390266	0	0.184	N.D. #
10)	B gamma-Chl...	5.423	0.000	18623711	0	1.327	N.D. #
11)	B alpha-Chl...	5.482	0.000	9286451	0	0.672	N.D. #
16)	A 4,4'-DDD	6.175	0.000	3455013	0	0.347	N.D. #
24)	Chlordane-2	4.874	0.000	19819343	0	45.799	N.D. #
25)	Chlordane-3	5.423	0.000	18623711	0	14.955	N.D. #
26)	Chlordane-4	5.482	0.000	9286451	0	9.006	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012120\
Data File : PL055943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 15:40
Operator : AJ\MA
Sample : PB126238BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 01:16:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

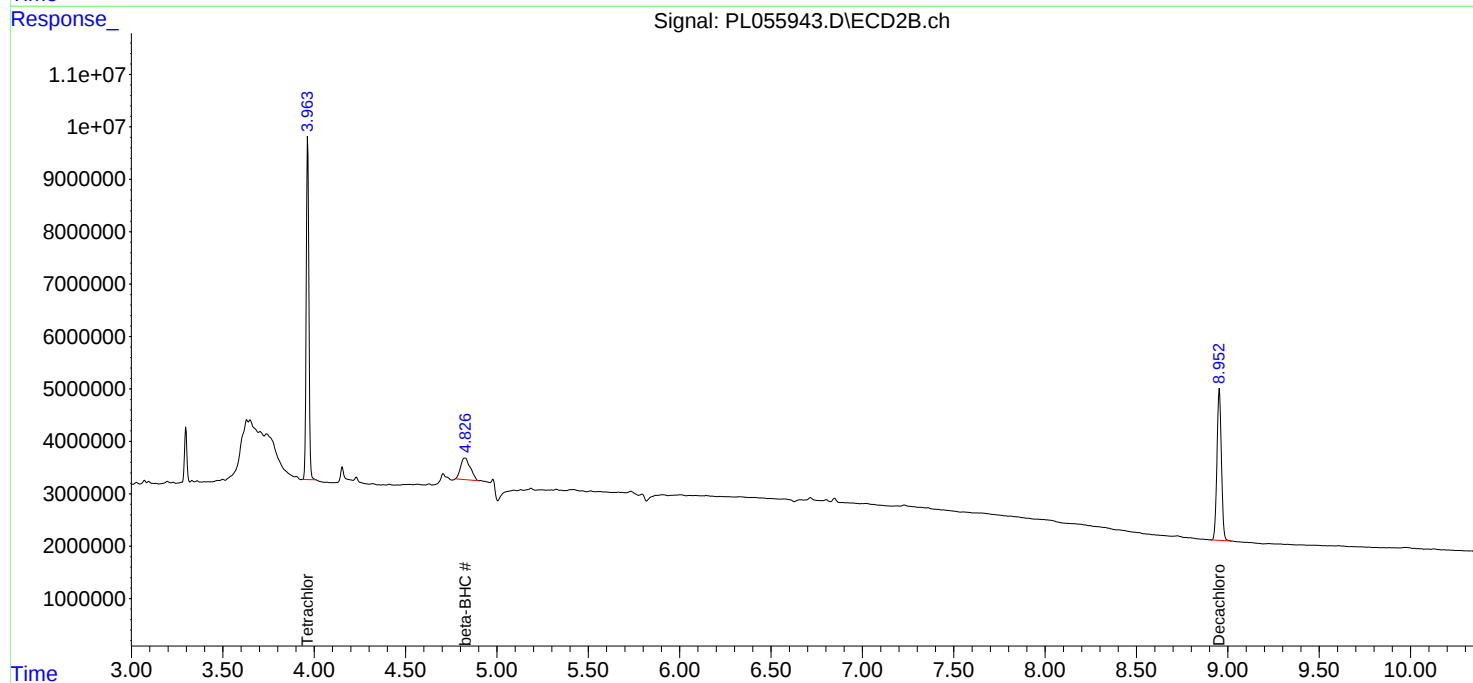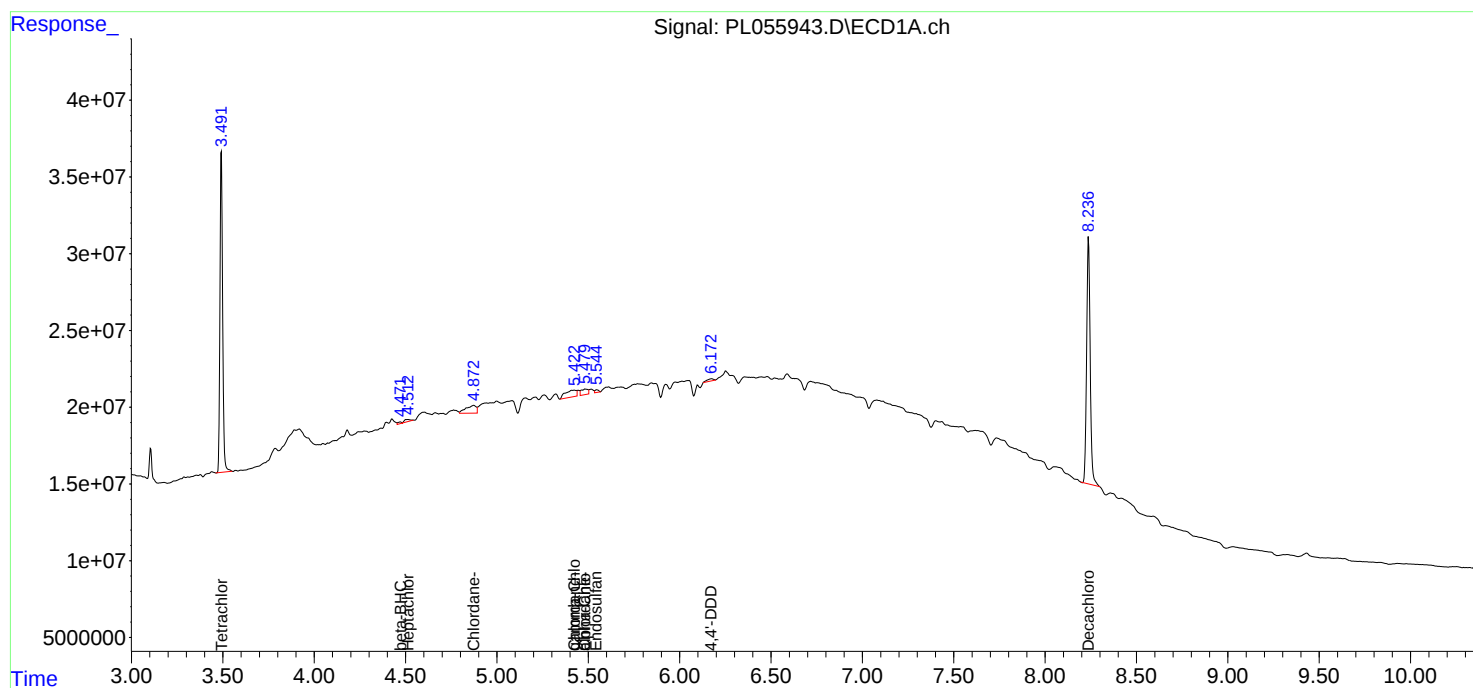


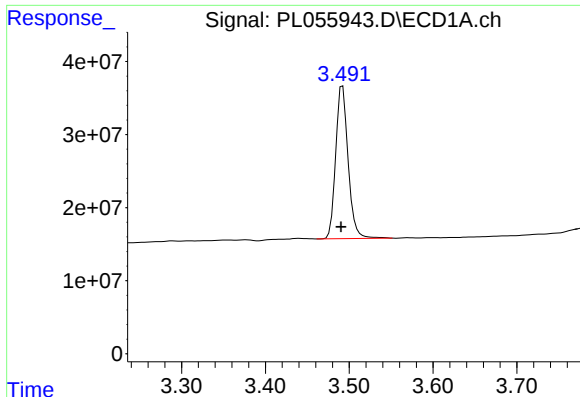

#1 Tetrachloro-m-xylene


R.T.: 3.492 min
Delta R.T.: 0.002 min
Response: 215180796
Conc: 22.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

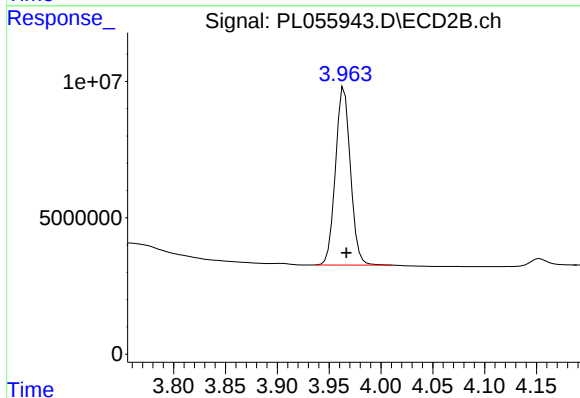


#1 Tetrachloro-m-xylene

R.T.: 3.965 min
Delta R.T.: -0.002 min
Response: 65452013
Conc: 23.16 ng/ml

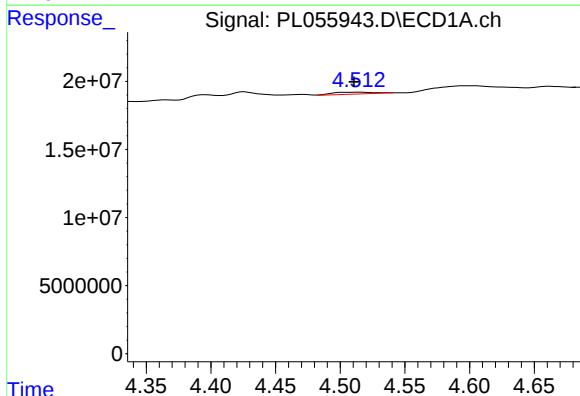


#4 Heptachlor

R.T.: 4.515 min
Delta R.T.: 0.004 min
Response: 3040862
Conc: 0.20 ng/ml

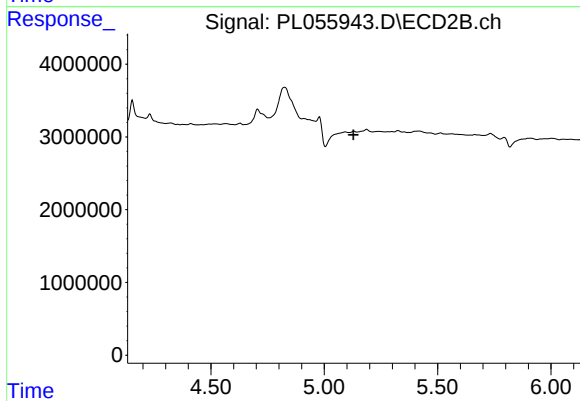

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.129 min
Response: 0
Conc: N.D.

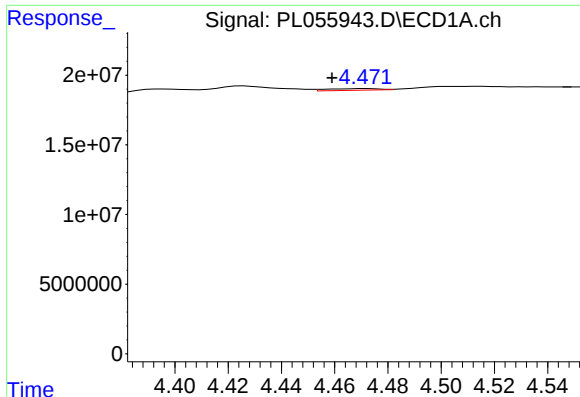

#6 beta-BHC


R.T.: 4.472 min
Delta R.T.: 0.013 min
Response: 1628304
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

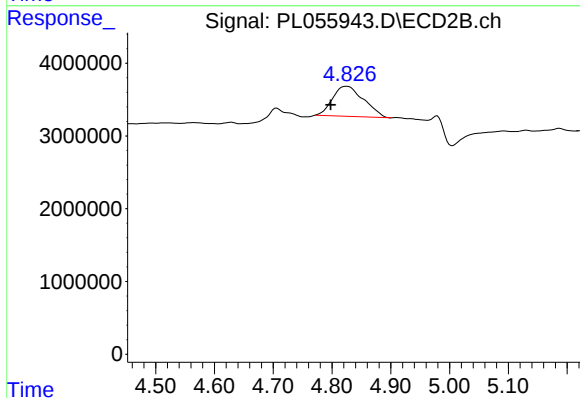


#6 beta-BHC

R.T.: 4.826 min
Delta R.T.: 0.028 min
Response: 15221421
Conc: 9.59 ng/ml

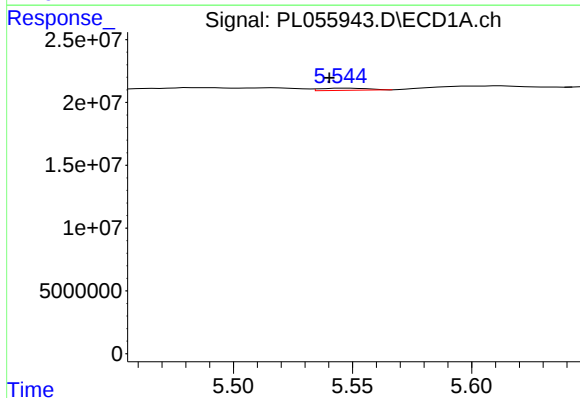


#9 Endosulfan I

R.T.: 5.546 min
Delta R.T.: 0.006 min
Response: 2390266
Conc: 0.18 ng/ml

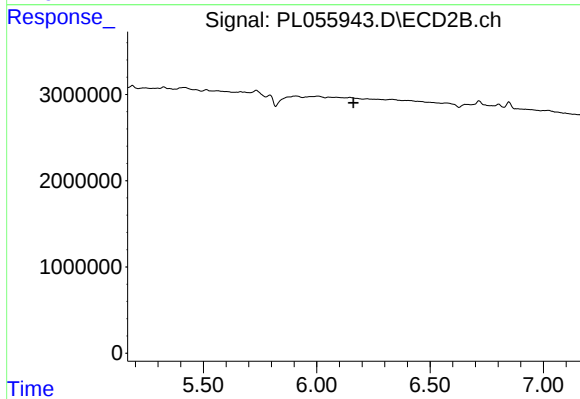

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.162 min
Response: 0
Conc: N.D.

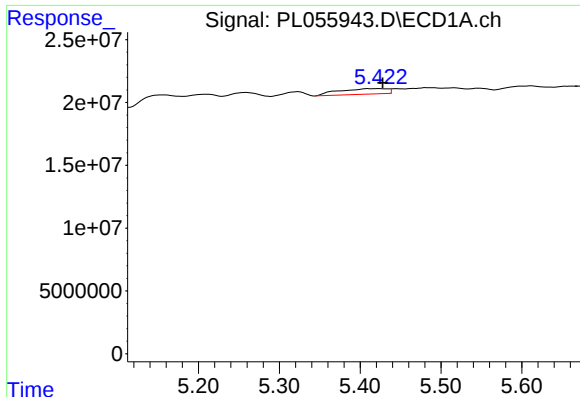

#10 gamma-Chlordane


R.T.: 5.423 min
Delta R.T.: -0.004 min
Response: 18623711
Conc: 1.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

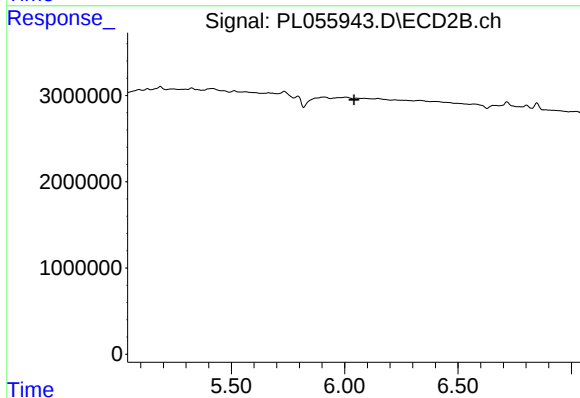


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.041 min
Response: 0
Conc: N.D.

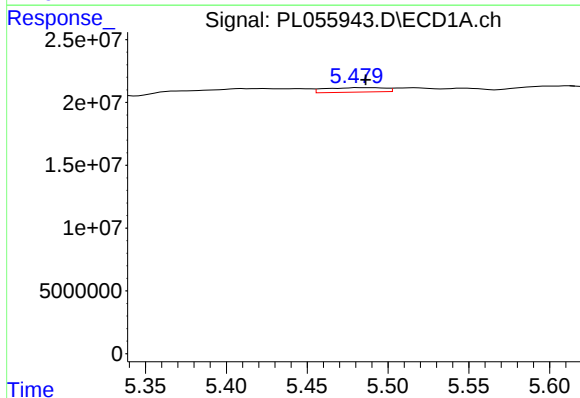


#11 alpha-Chlordane

R.T.: 5.482 min
Delta R.T.: -0.004 min
Response: 9286451
Conc: 0.67 ng/ml

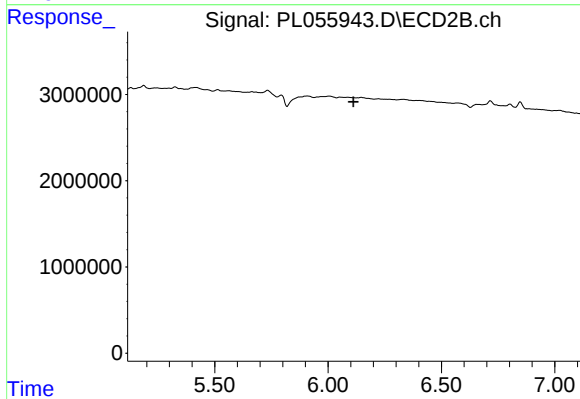

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

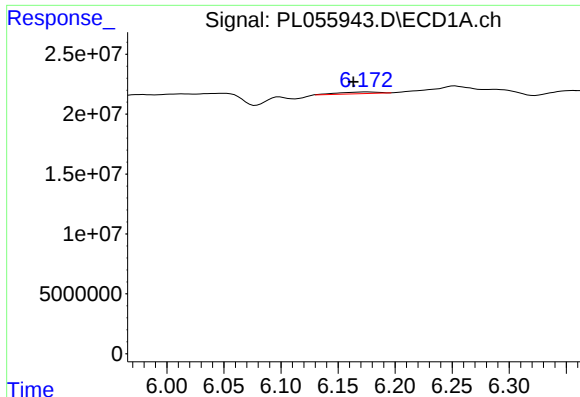

#16 4,4'-DDD


R.T.: 6.175 min
Delta R.T.: 0.011 min
Response: 3455013
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

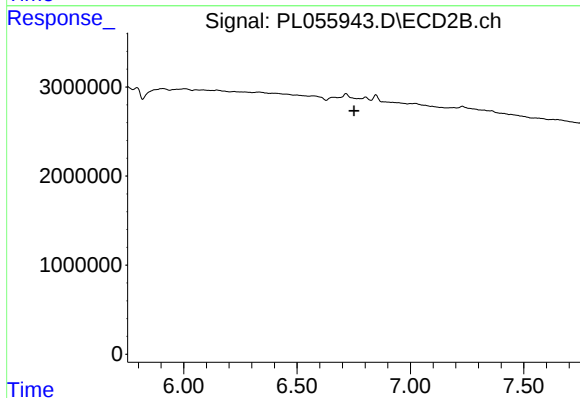


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.752 min
Response: 0
Conc: N.D.

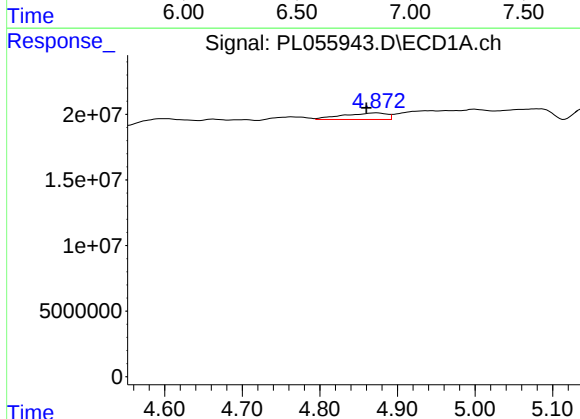


#24 Chlordane-2

R.T.: 4.874 min
Delta R.T.: 0.014 min
Response: 19819343
Conc: 45.80 ng/ml

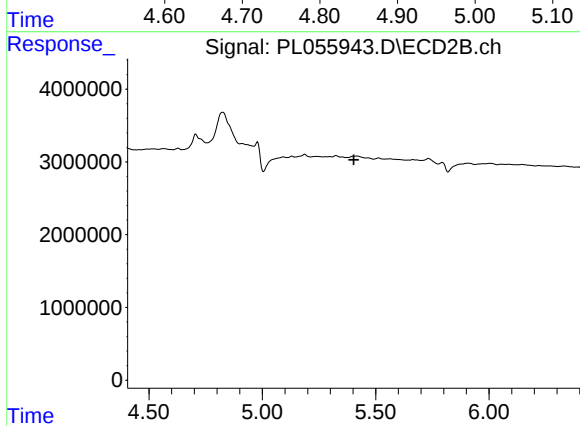

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.403 min
Response: 0
Conc: N.D.

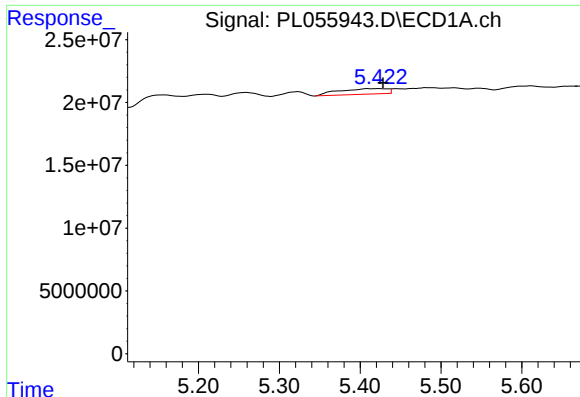

#25 Chlordane-3


R.T.: 5.423 min
Delta R.T.: -0.005 min
Response: 18623711
Conc: 14.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

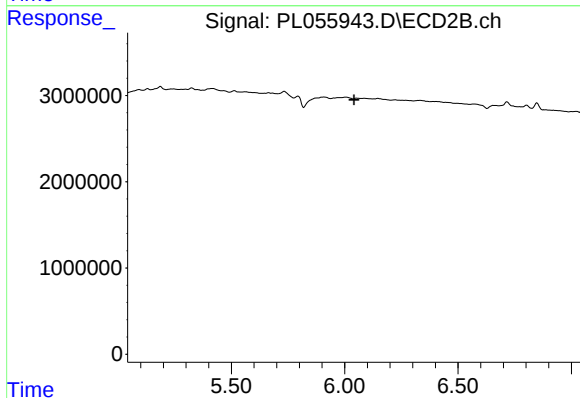


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.041 min
Response: 0
Conc: N.D.

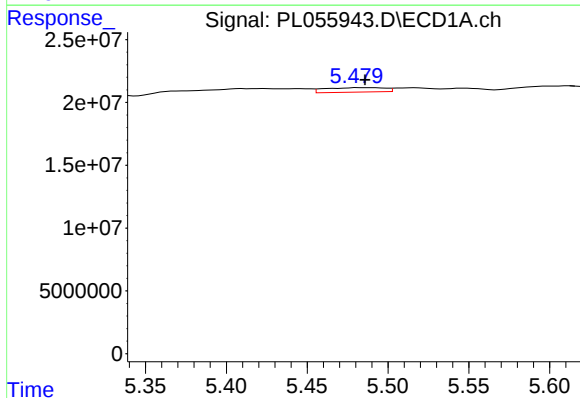


#26 Chlordane-4

R.T.: 5.482 min
Delta R.T.: -0.004 min
Response: 9286451
Conc: 9.01 ng/ml

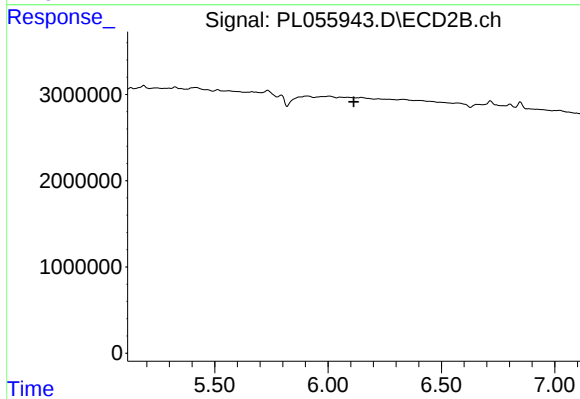

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

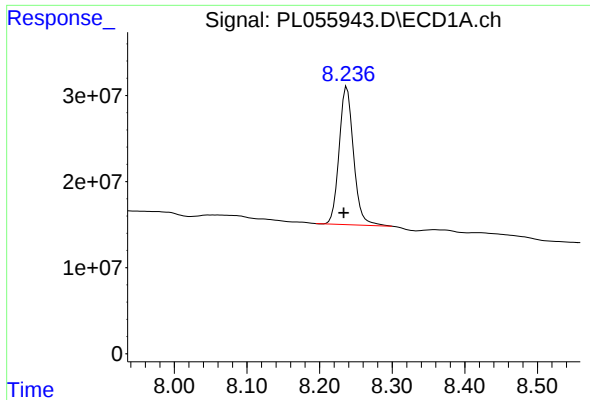

#28 Decachlorobiphenyl

R.T.: 8.238 min
Delta R.T.: 0.004 min
Response: 219969552
Conc: 21.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

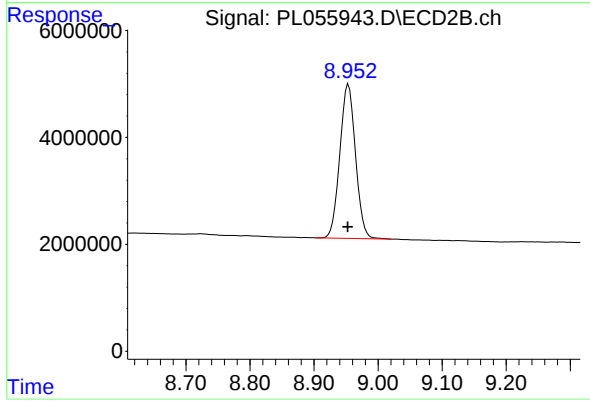

#28 Decachlorobiphenyl

R.T.: 8.954 min
Delta R.T.: 0.001 min
Response: 48891545
Conc: 21.34 ng/ml