

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012120\
 Data File : PL055950.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 17:19
 Operator : AJ\MA
 Sample : PB126245TB
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 01:17:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	3.966	188.6E6	61629898	19.681	21.806
28)	SA Decachlor...	8.233	8.951	240.5E6	55752874	23.003	24.336
Target Compounds							
4)	MA Heptachlor	4.512	0.000	2283976	0	0.153	N.D. #
6)	B beta-BHC	4.460	0.000	2628111	0	0.410	N.D. #
9)	A Endosulfan I	5.549	0.000	1305050	0	0.101	N.D. #
10)	B gamma-Chl...	5.429	0.000	16873726	0	1.203	N.D. #
11)	B alpha-Chl...	5.484	0.000	11636641	0	0.842	N.D. #
19)	B Endosulfa...	6.703	0.000	1157619	0	0.107	N.D. #
23)	Chlordane-1	4.389f	0.000	6429598	0	17.536	N.D. #
24)	Chlordane-2	4.879f	0.000	10829637	0	25.025	N.D. #
25)	Chlordane-3	5.429	0.000	16873726	0	13.550	N.D. #
26)	Chlordane-4	5.484	0.000	11636641	0	11.285	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012120\
Data File : PL055950.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 17:19
Operator : AJ\MA
Sample : PB126245TB
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 01:17:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

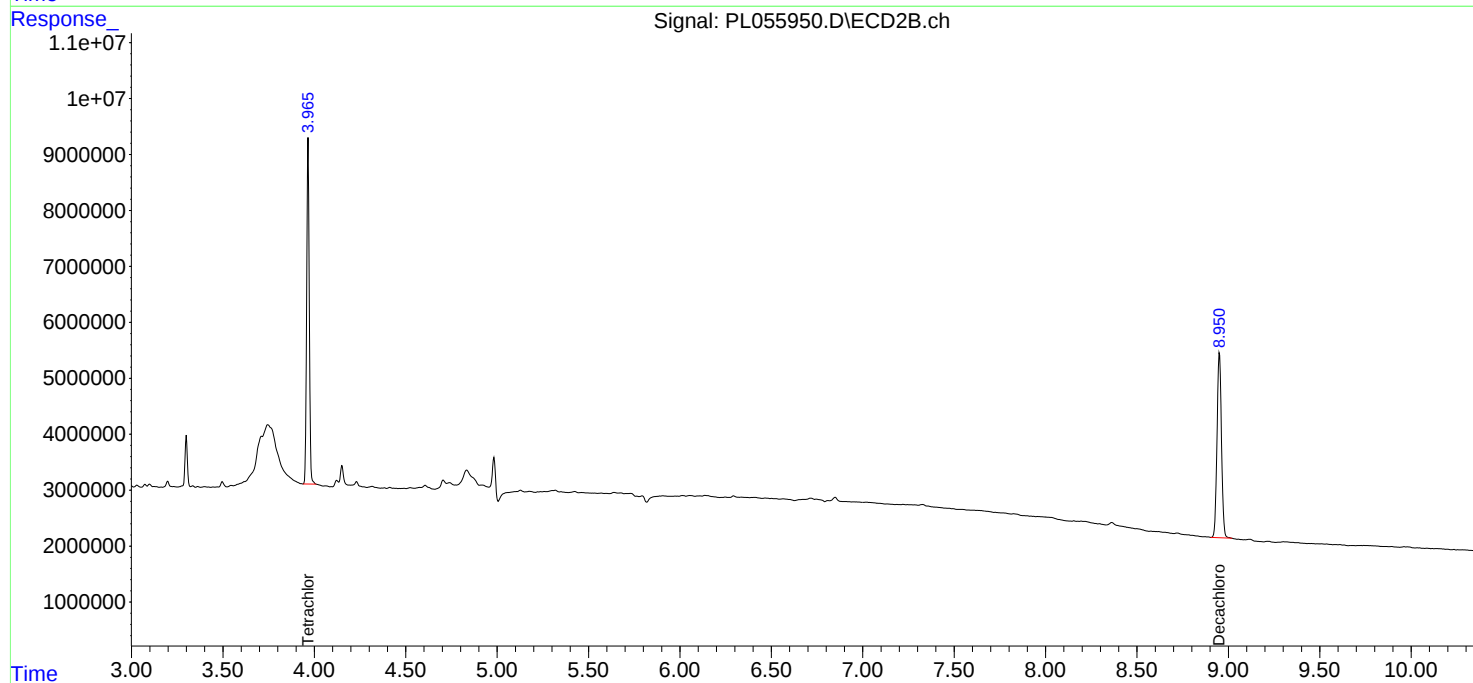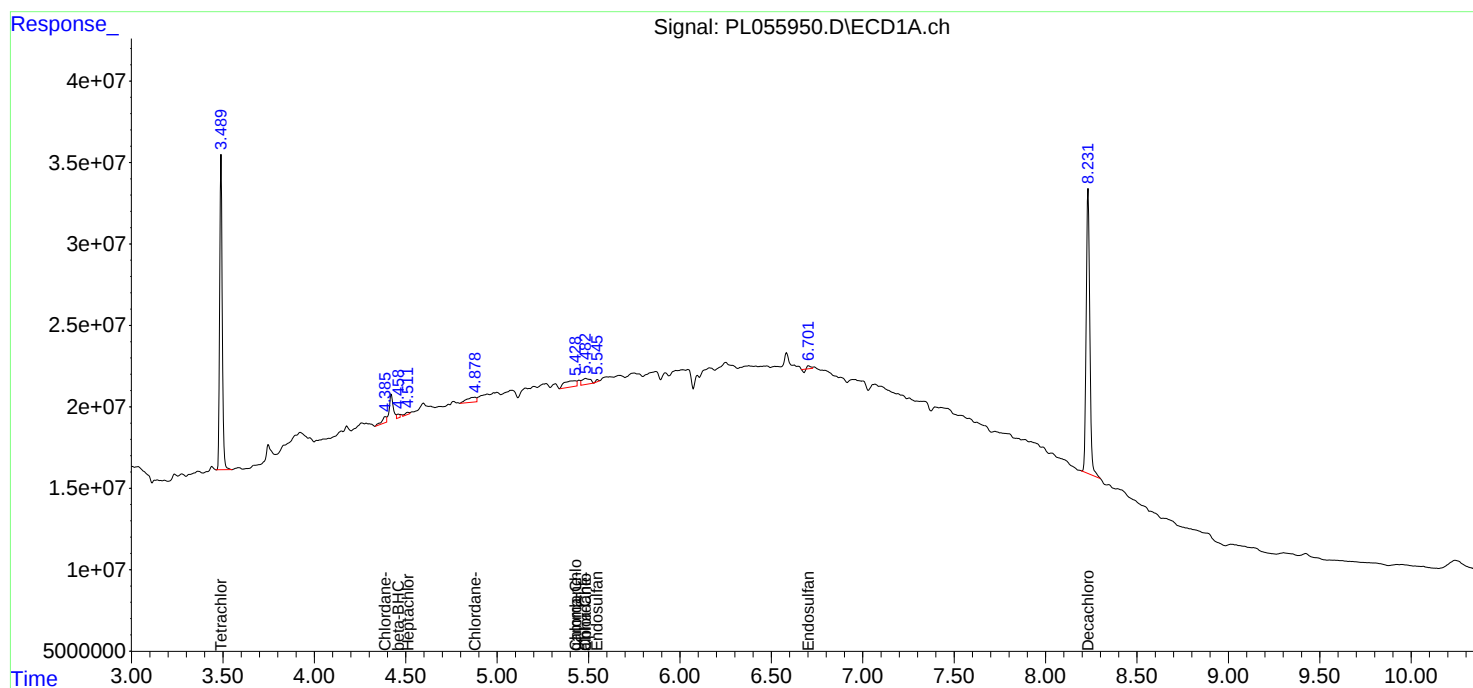


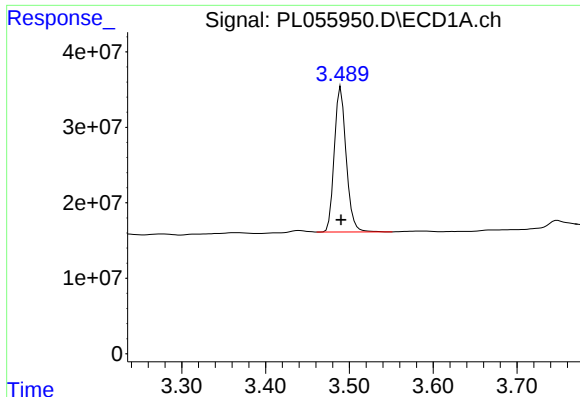

#1 Tetrachloro-m-xylene


R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 188630969
Conc: 19.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

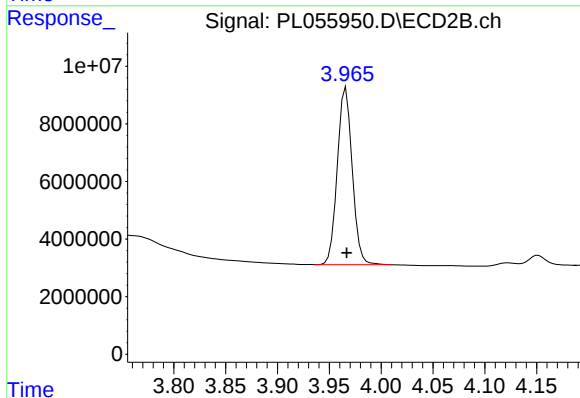


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 61629898
Conc: 21.81 ng/ml

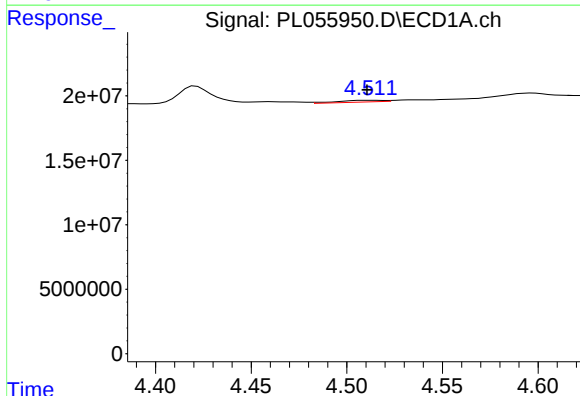


#4 Heptachlor

R.T.: 4.512 min
Delta R.T.: 0.002 min
Response: 2283976
Conc: 0.15 ng/ml

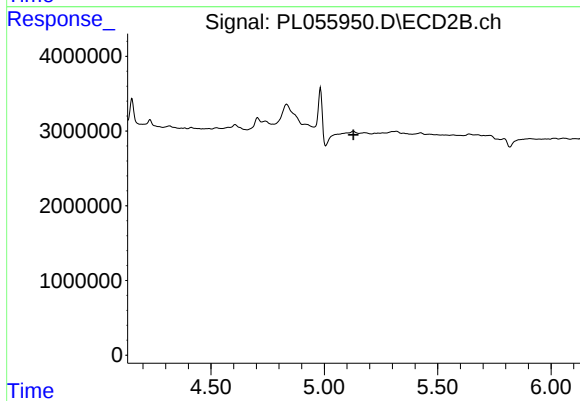

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.129 min
Response: 0
Conc: N.D.

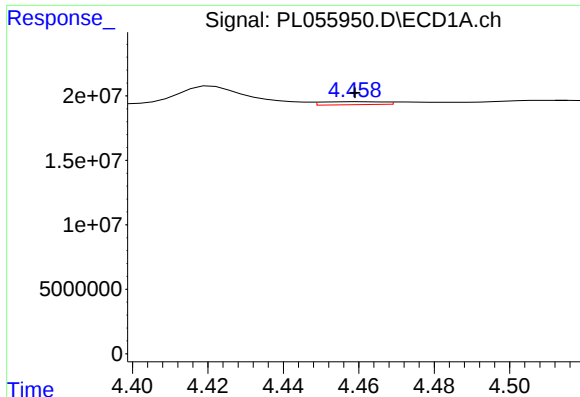

#6 beta-BHC


R.T.: 4.460 min
Delta R.T.: 0.000 min
Response: 2628111
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

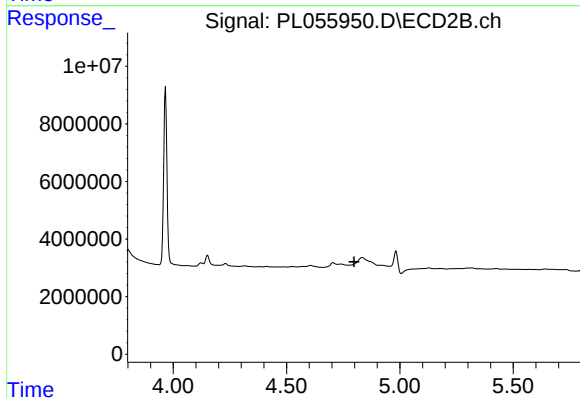


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.798 min
Response: 0
Conc: N.D.

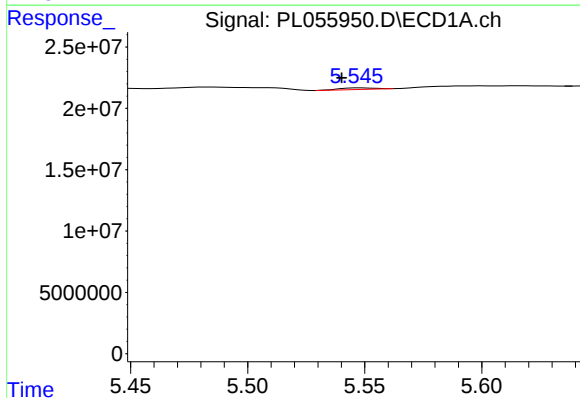


#9 Endosulfan I

R.T.: 5.549 min
Delta R.T.: 0.008 min
Response: 1305050
Conc: 0.10 ng/ml

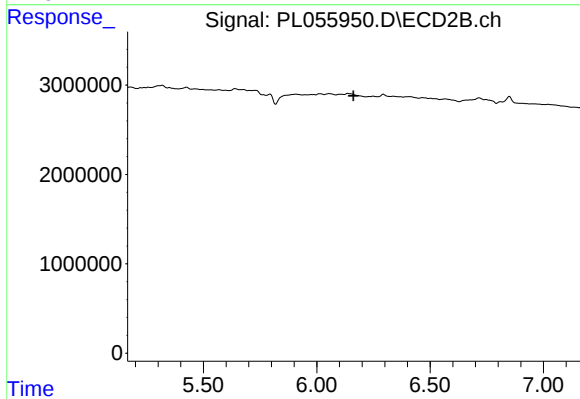

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

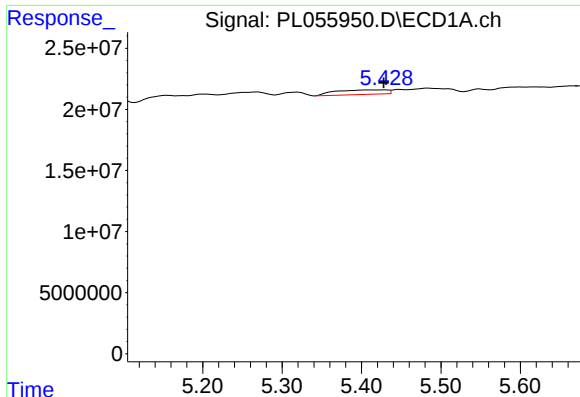

#10 gamma-Chlordane


R.T.: 5.429 min
Delta R.T.: 0.001 min
Response: 16873726
Conc: 1.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

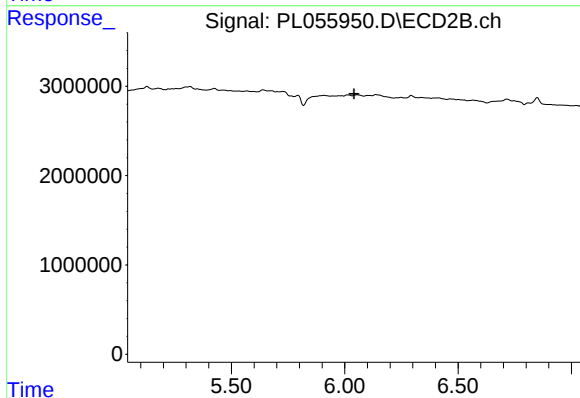


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.041 min
Response: 0
Conc: N.D.

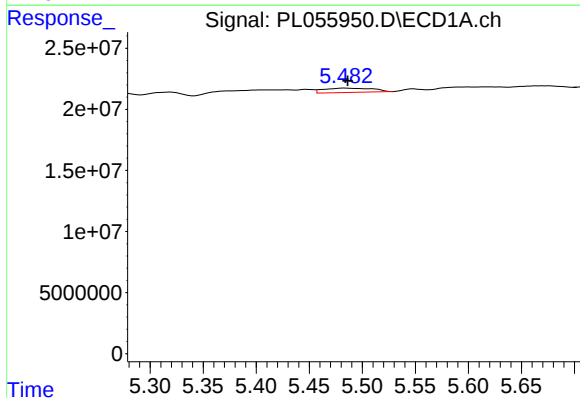


#11 alpha-Chlordane

R.T.: 5.484 min
Delta R.T.: -0.002 min
Response: 11636641
Conc: 0.84 ng/ml

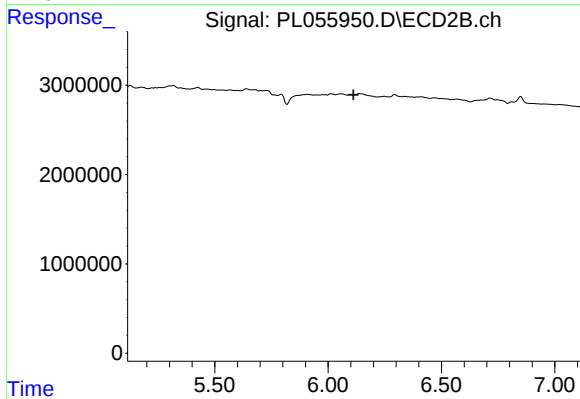

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

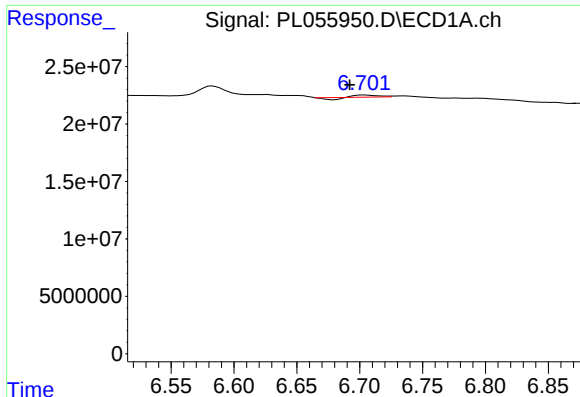

#19 Endosulfan Sulfate


R.T.: 6.703 min
Delta R.T.: 0.011 min
Response: 1157619
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

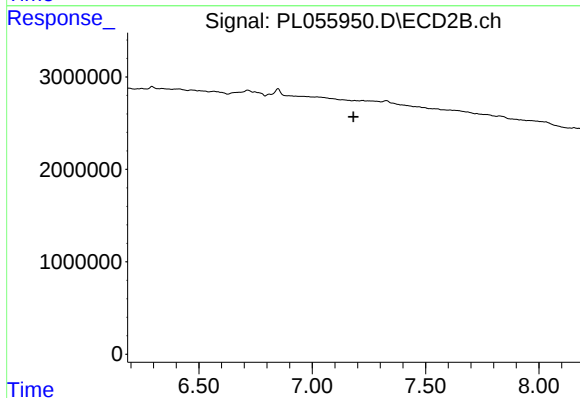


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

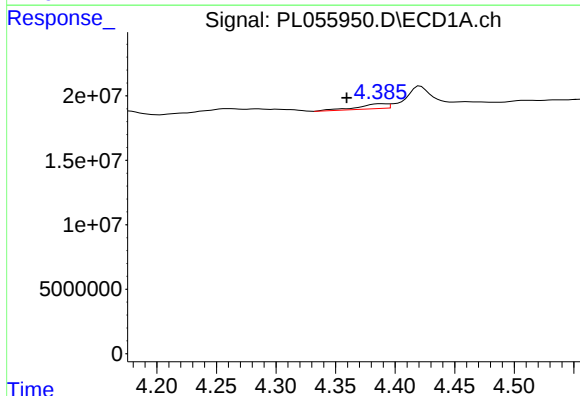


#23 Chlordane-1

R.T.: 4.389 min
Delta R.T.: 0.029 min
Response: 6429598
Conc: 17.54 ng/ml

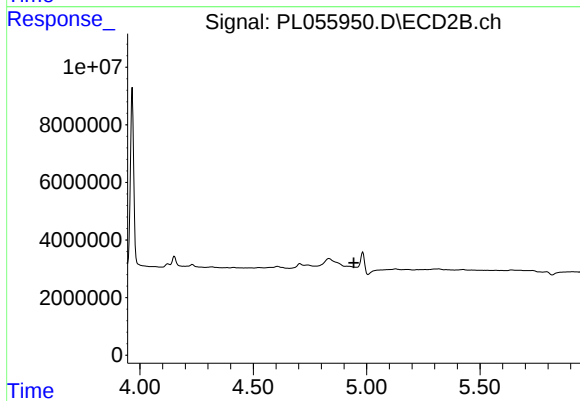

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.943 min
Response: 0
Conc: N.D.

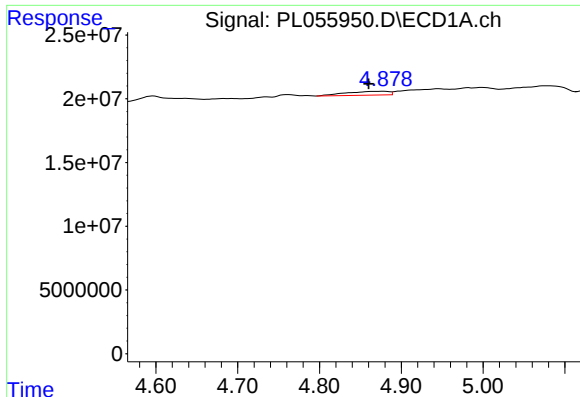

#24 Chlordane-2


R.T.: 4.879 min
Delta R.T.: 0.019 min
Response: 10829637
Conc: 25.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

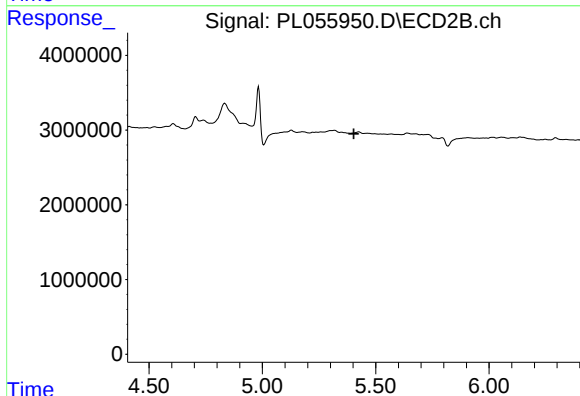


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.403 min
Response: 0
Conc: N.D.

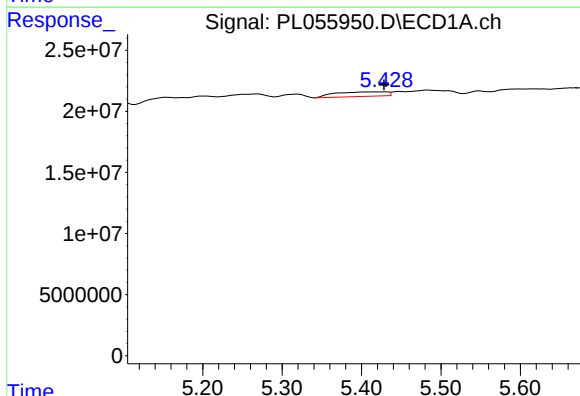


#25 Chlordane-3

R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 16873726
Conc: 13.55 ng/ml

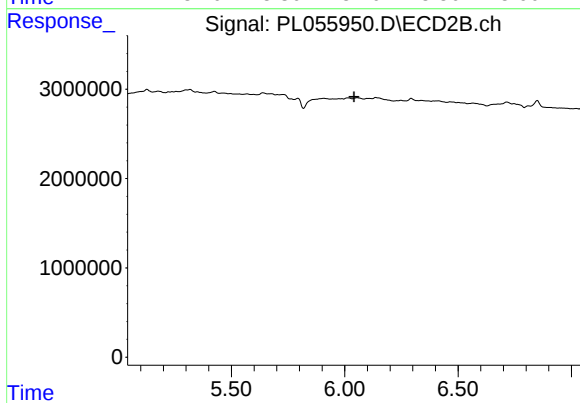

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.041 min
Response: 0
Conc: N.D.

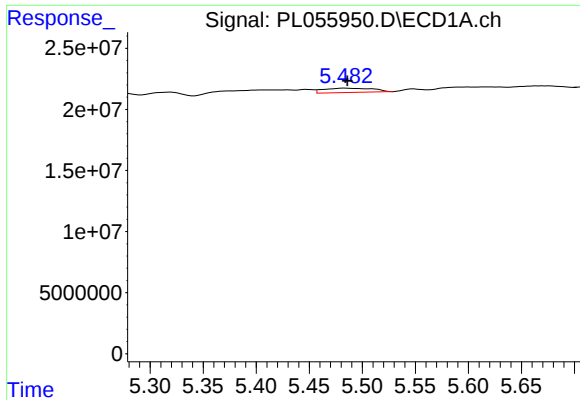

#26 Chlordane-4


R.T.: 5.484 min
Delta R.T.: -0.002 min
Response: 11636641
Conc: 11.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

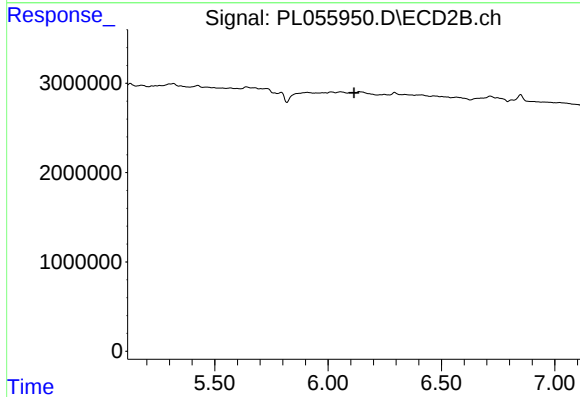


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

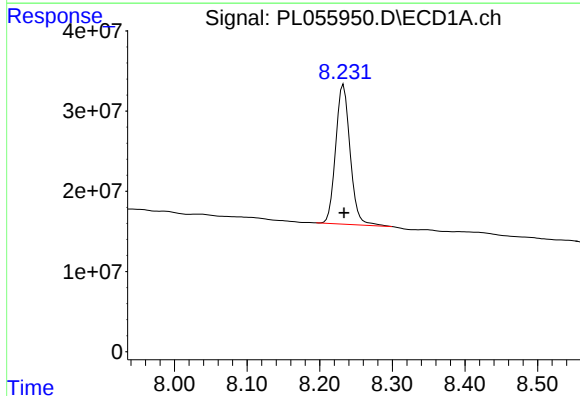

#28 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: 0.000 min
Response: 240512062
Conc: 23.00 ng/ml

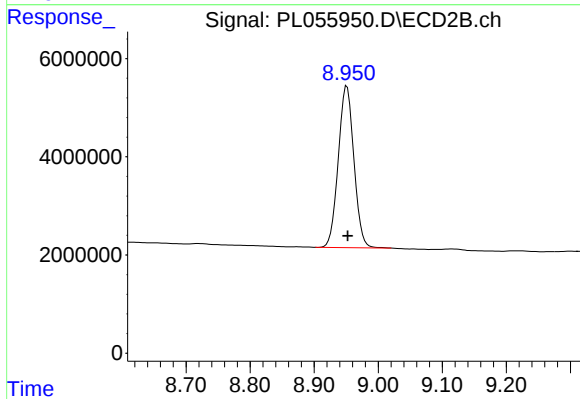

#28 Decachlorobiphenyl

R.T.: 8.951 min
Delta R.T.: -0.001 min
Response: 55752874
Conc: 24.34 ng/ml