

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012120\
 Data File : PL055959.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 19:27
 Operator : AJ\MA
 Sample : L1175-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 01:19:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	3.967	177.9E6	55226824	18.563	19.541
28)	SA Decachlor...	8.233	8.953	214.1E6	47798433	20.477	20.864
Target Compounds							
6)	B beta-BHC	4.469	0.000	2077583	0	0.324	N.D. #
9)	A Endosulfan I	5.544	0.000	2730085	0	0.210	N.D. #
10)	B gamma-Chl...	5.420	0.000	30889476	0	2.202	N.D. #
11)	B alpha-Chl...	5.482	6.108	13822215	5938593	1.000	1.923 #
16)	A 4,4'-DDD	6.171	0.000	1551639	0	0.156	N.D. #
24)	Chlordane-2	4.875f	0.000	11937057	0	27.584	N.D. #
25)	Chlordane-3	5.420	0.000	30889476	0	24.805	N.D. #
26)	Chlordane-4	5.482	6.108	13822215	5938593	13.405	12.651



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012120\
Data File : PL055959.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 19:27
Operator : AJ\MA
Sample : L1175-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 01:19:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

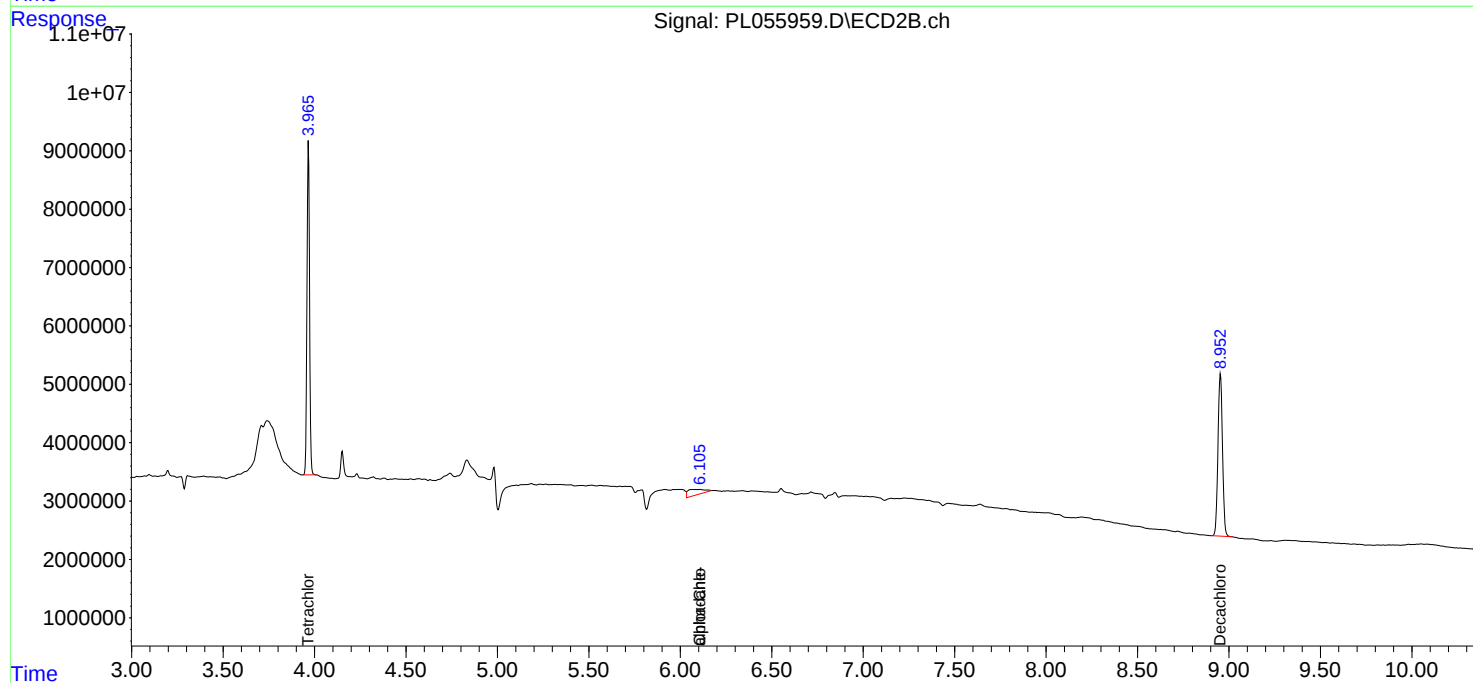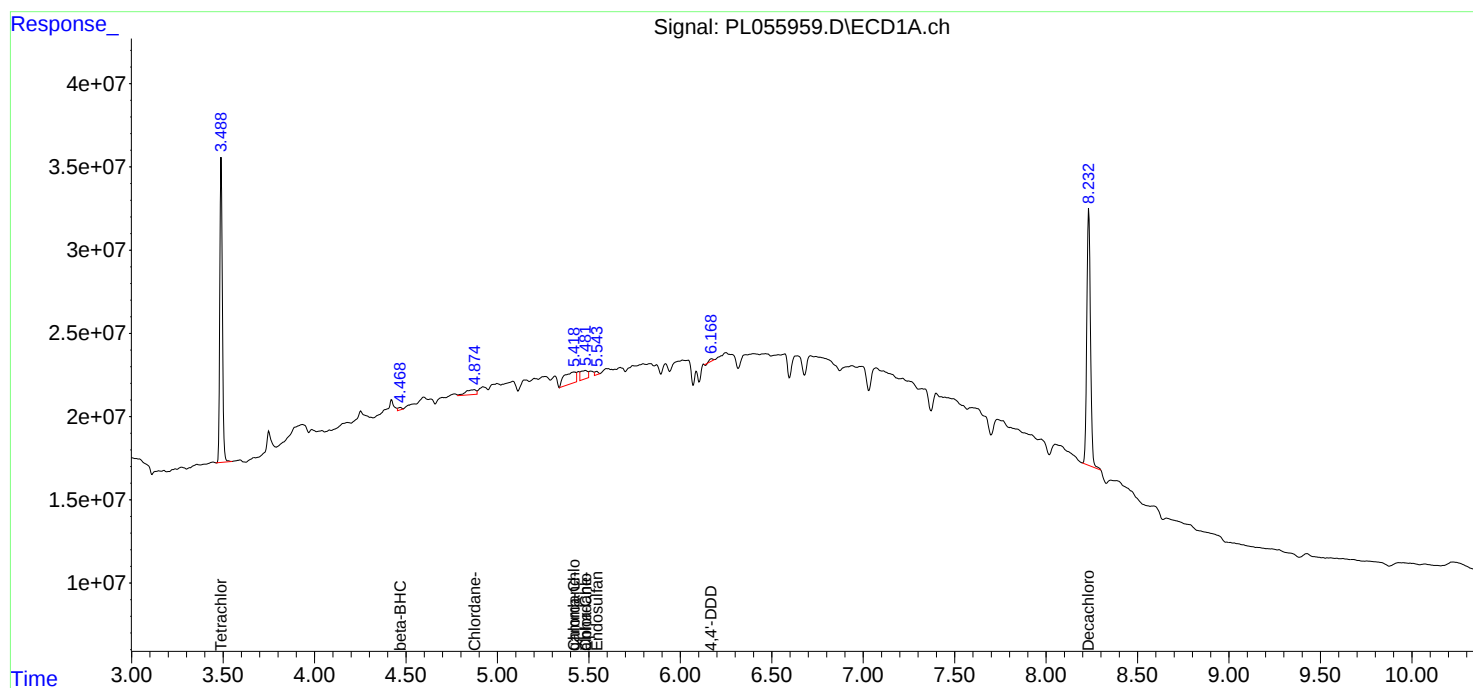


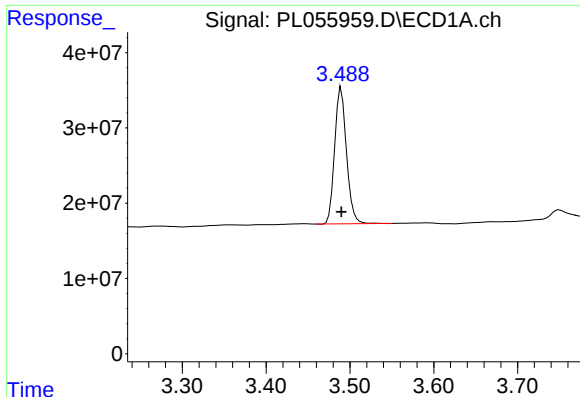

#1 Tetrachloro-m-xylene


R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 177911977
Conc: 18.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

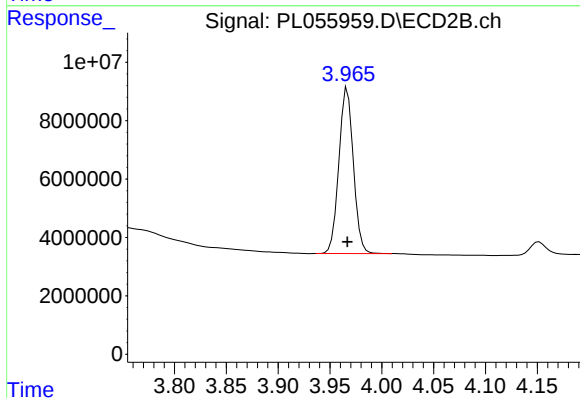


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 55226824
Conc: 19.54 ng/ml

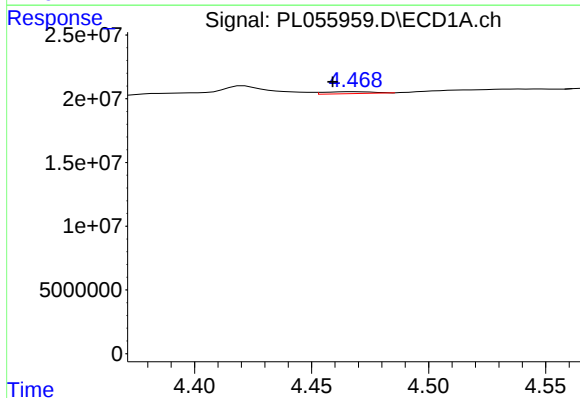


#6 beta-BHC

R.T.: 4.469 min
Delta R.T.: 0.010 min
Response: 2077583
Conc: 0.32 ng/ml

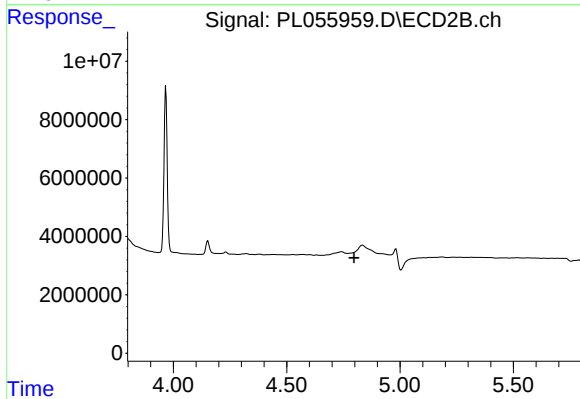

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.798 min
Response: 0
Conc: N.D.

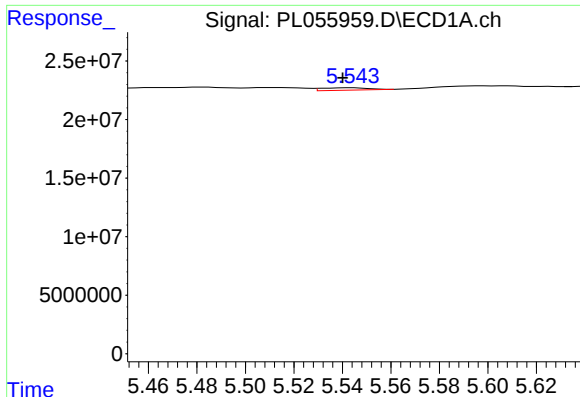

#9 Endosulfan I


R.T.: 5.544 min
Delta R.T.: 0.004 min
Response: 2730085
Conc: 0.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

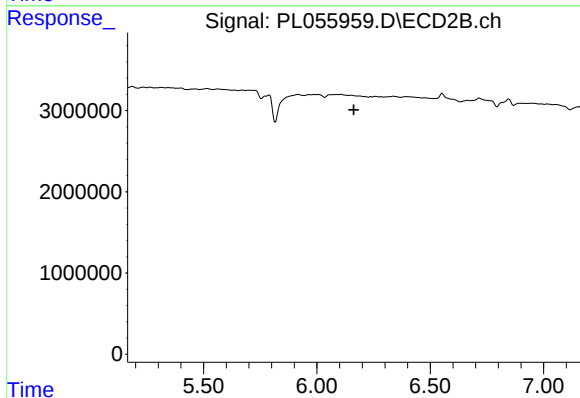


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

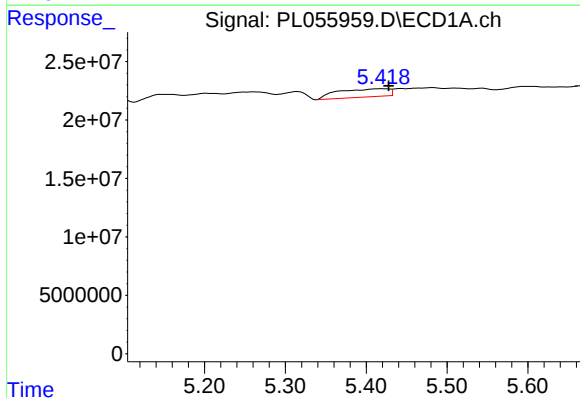


#10 gamma-Chlordane

R.T.: 5.420 min
Delta R.T.: -0.008 min
Response: 30889476
Conc: 2.20 ng/ml

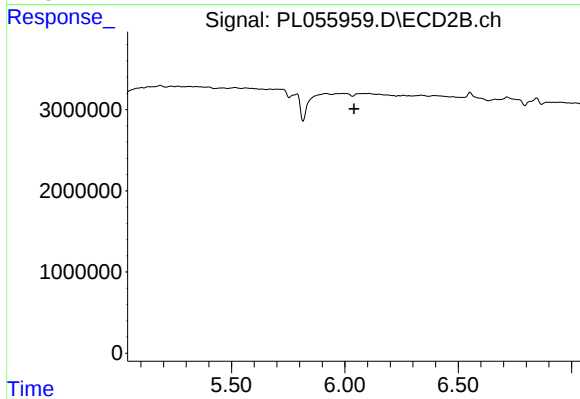

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.041 min
Response: 0
Conc: N.D.

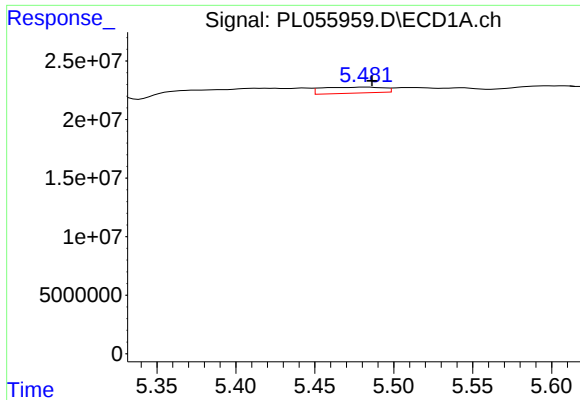

#11 alpha-Chlordane


R.T.: 5.482 min
Delta R.T.: -0.004 min
Response: 13822215
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

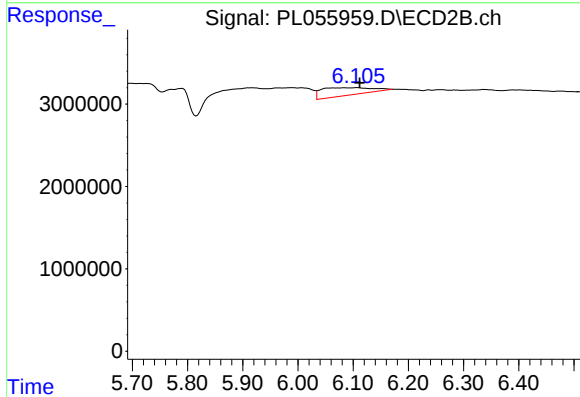


#11 alpha-Chlordane

R.T.: 6.108 min
Delta R.T.: -0.004 min
Response: 5938593
Conc: 1.92 ng/ml

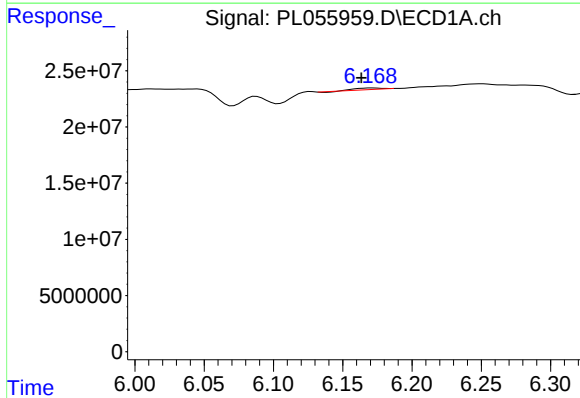


#16 4,4'-DDD

R.T.: 6.171 min
Delta R.T.: 0.008 min
Response: 1551639
Conc: 0.16 ng/ml

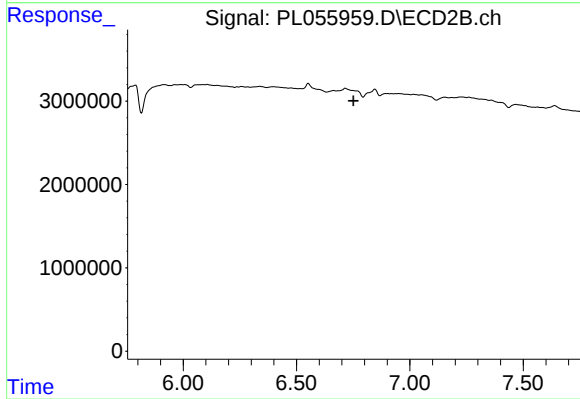

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.752 min
Response: 0
Conc: N.D.

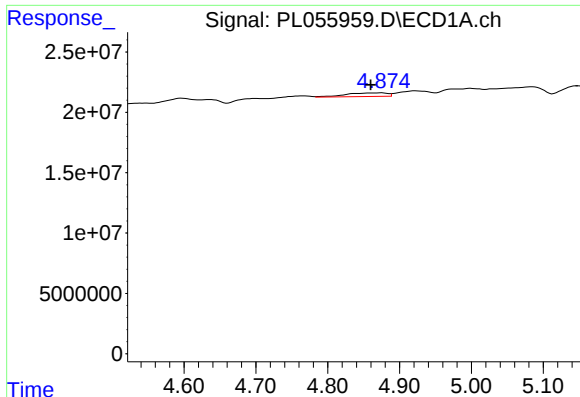

#24 Chlordane-2


R.T.: 4.875 min
Delta R.T.: 0.015 min
Response: 11937057
Conc: 27.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

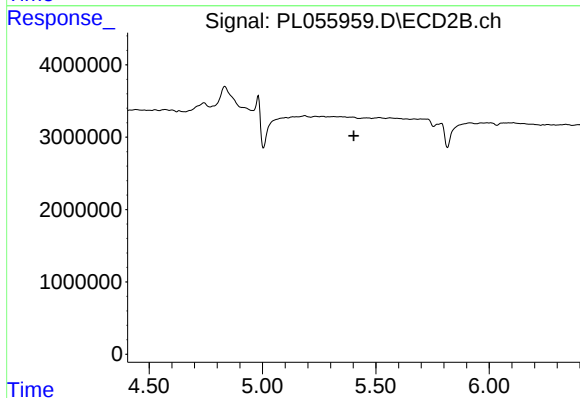


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.403 min
Response: 0
Conc: N.D.

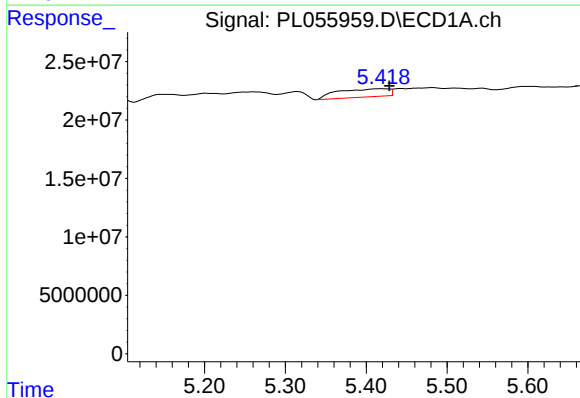


#25 Chlordane-3

R.T.: 5.420 min
Delta R.T.: -0.009 min
Response: 30889476
Conc: 24.81 ng/ml

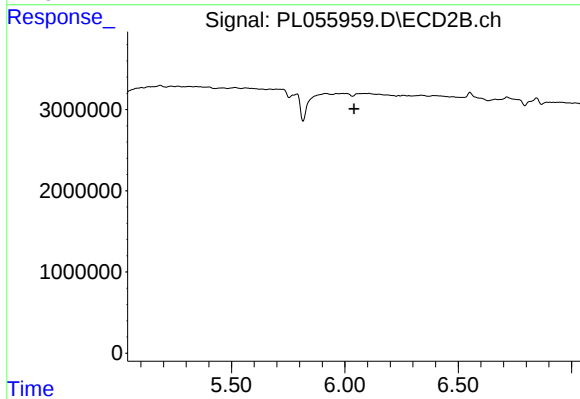

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.041 min
Response: 0
Conc: N.D.

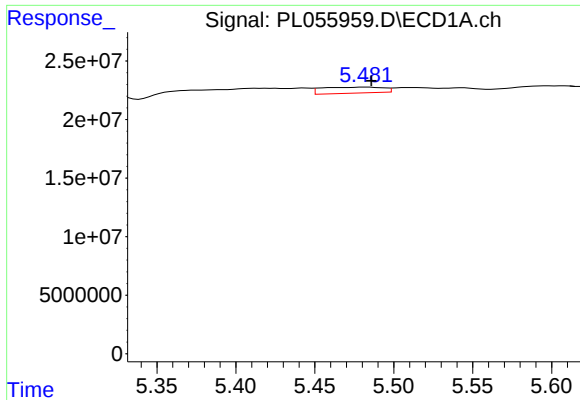

#26 Chlordane-4


R.T.: 5.482 min
Delta R.T.: -0.004 min
Response: 13822215
Conc: 13.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

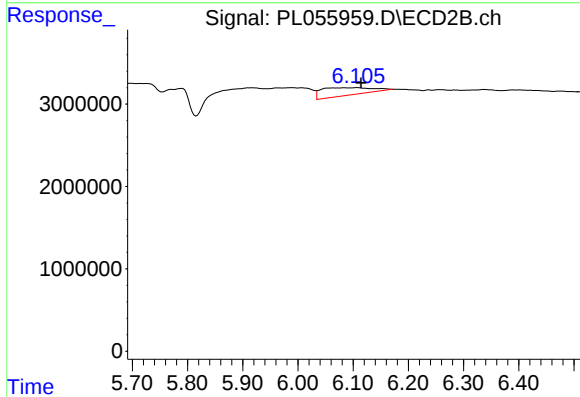


#26 Chlordane-4

R.T.: 6.108 min
Delta R.T.: -0.006 min
Response: 5938593
Conc: 12.65 ng/ml

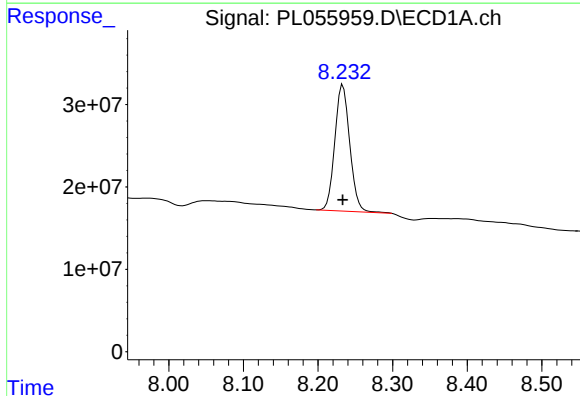

#28 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: 0.000 min
Response: 214100678
Conc: 20.48 ng/ml

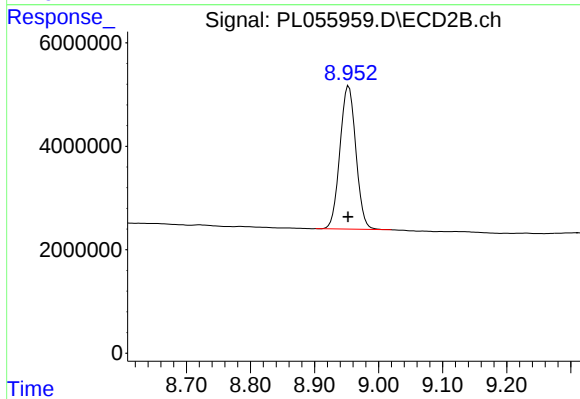

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: 0.001 min
Response: 47798433
Conc: 20.86 ng/ml