

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012120\
 Data File : PL055965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 20:51
 Operator : AJ\MA
 Sample : PB126232BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 01:20:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	3.967	189.1E6	58515108	19.732	20.704
28)	SA Decachlor...	8.233	8.952	218.8E6	48848813	20.924	21.322
Target Compounds							
2)	A alpha-BHC	3.924	0.000	11028913	0	0.665	N.D. #
6)	B beta-BHC	4.464	0.000	1768354	0	0.276	N.D. #
9)	A Endosulfan I	5.535	0.000	4979505	0	0.384	N.D. #
10)	B gamma-Chl...	5.417	0.000	8076653	0	0.576	N.D. #
11)	B alpha-Chl...	5.476	0.000	5622707	0	0.407	N.D. #
25)	Chlordane-3	5.417	0.000	8076653	0	6.486	N.D. #
26)	Chlordane-4	5.476	0.000	5622707	0	5.453	N.D. #
27)	Chlordane-5	6.351f	0.000	1571238	0	4.017	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012120\
Data File : PL055965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 20:51
Operator : AJ\MA
Sample : PB126232BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 01:20:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

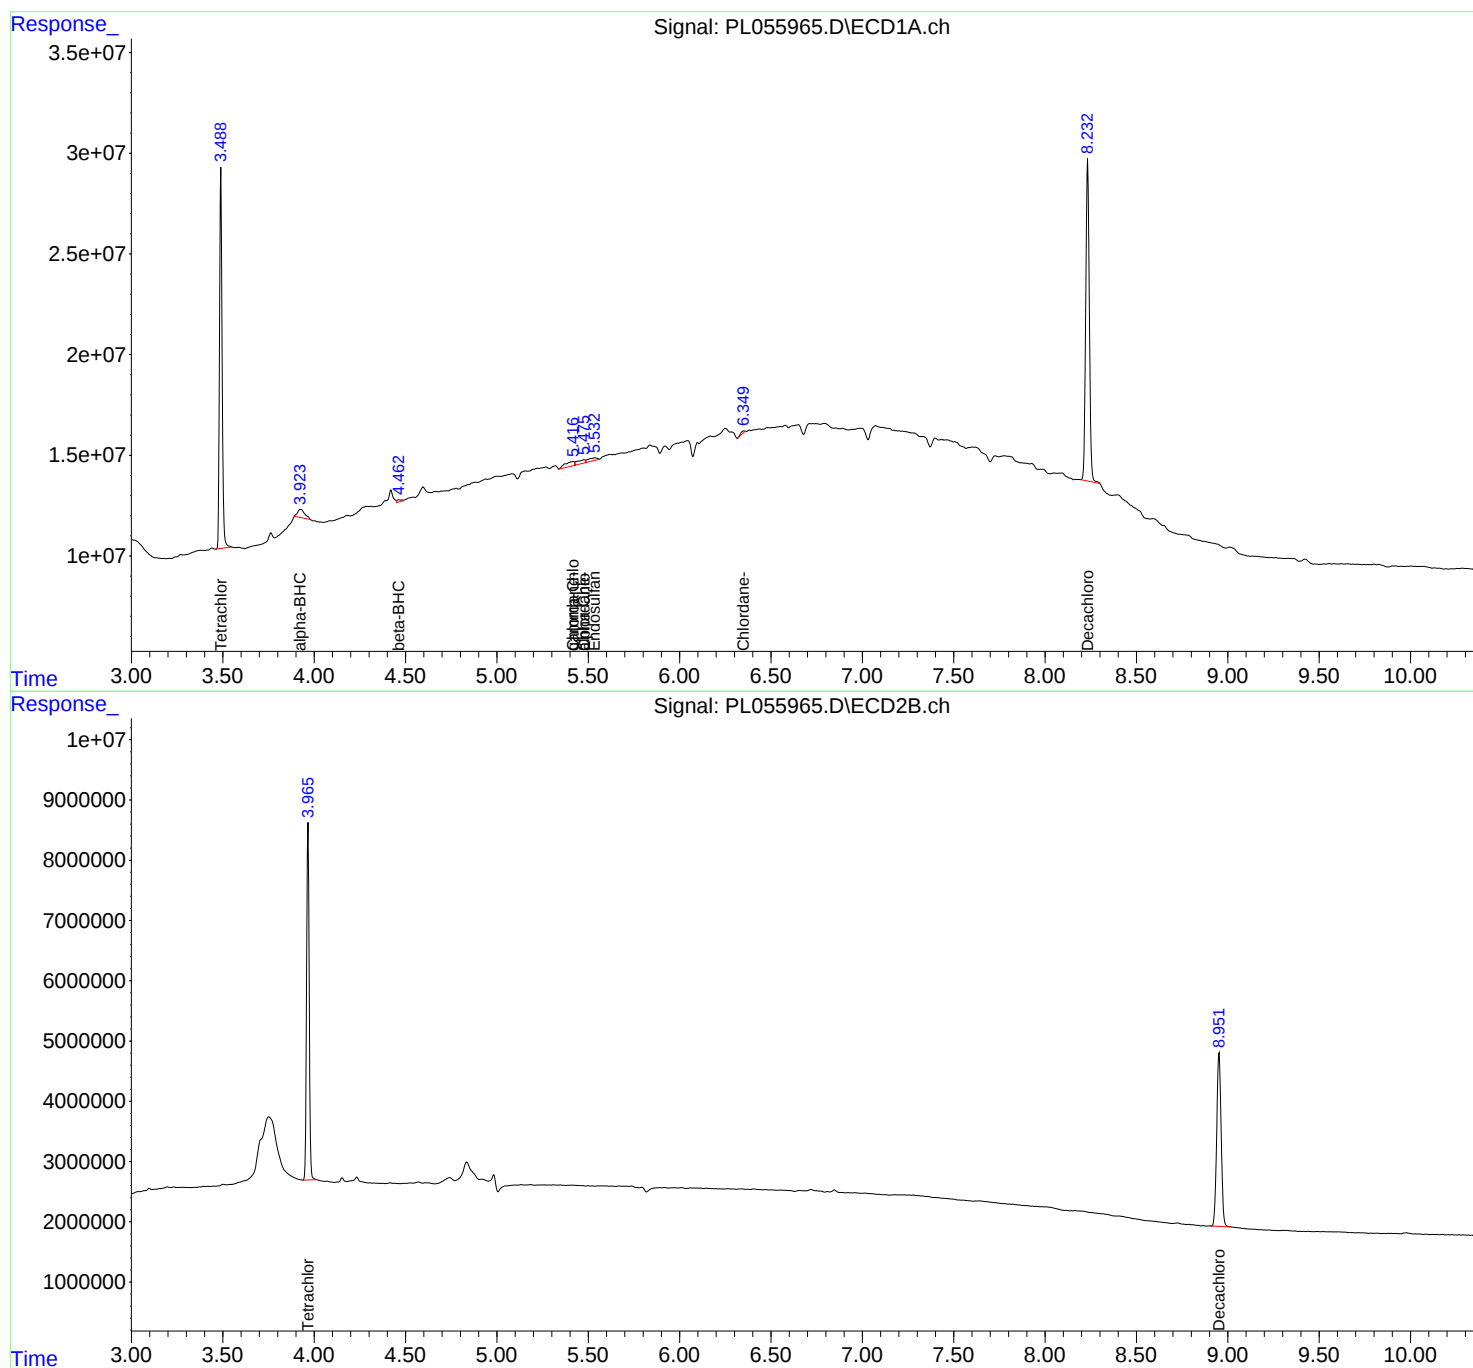


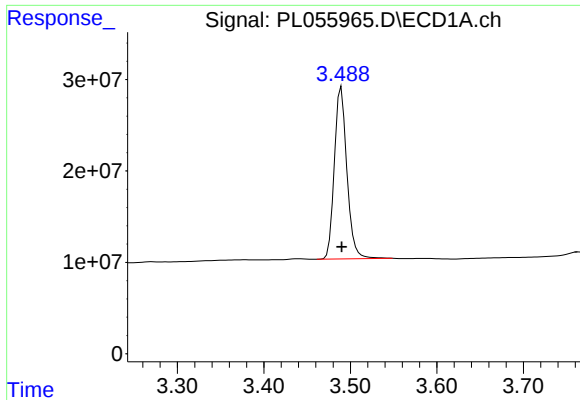

#1 Tetrachloro-m-xylene


R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 189121849
Conc: 19.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

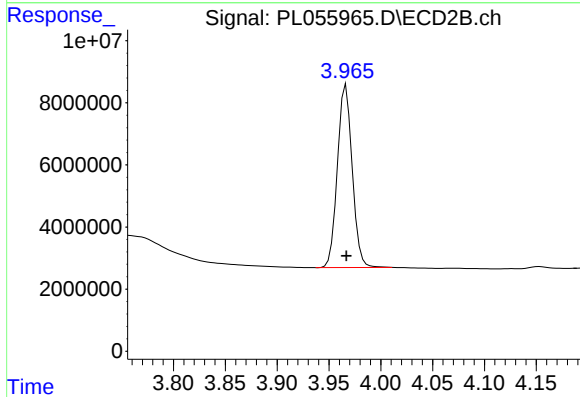


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 58515108
Conc: 20.70 ng/ml

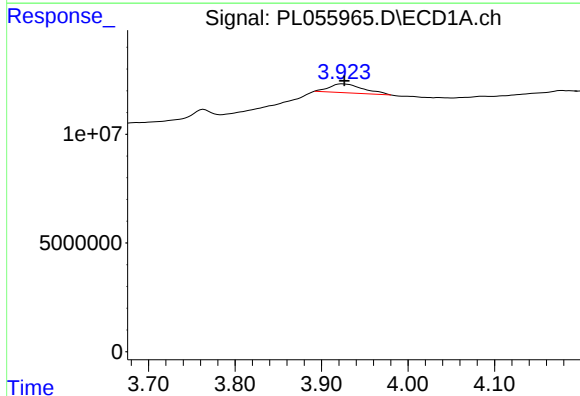


#2 alpha-BHC

R.T.: 3.924 min
Delta R.T.: -0.002 min
Response: 11028913
Conc: 0.66 ng/ml

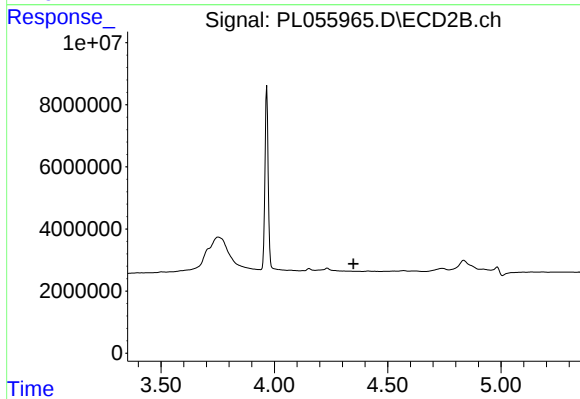

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.350 min
Response: 0
Conc: N.D.

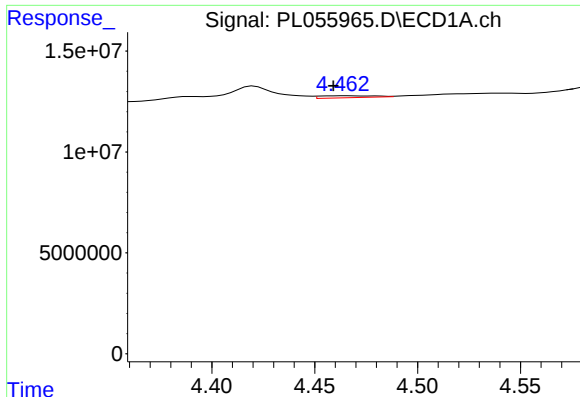

#6 beta-BHC


R.T.: 4.464 min
Delta R.T.: 0.005 min
Response: 1768354
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

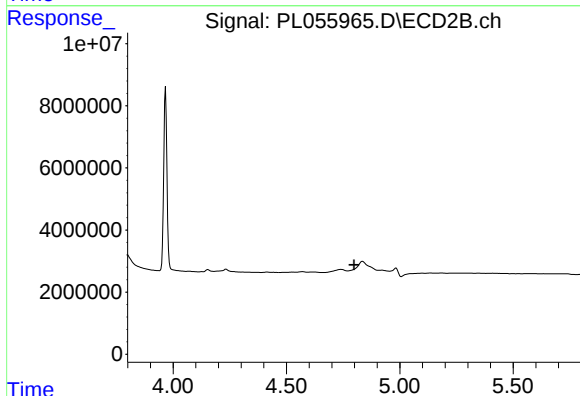


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.798 min
Response: 0
Conc: N.D.

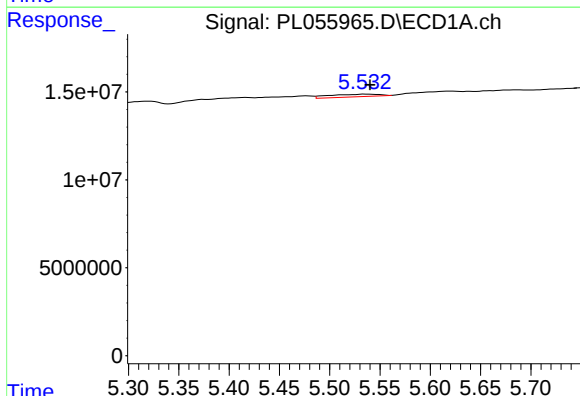


#9 Endosulfan I

R.T.: 5.535 min
Delta R.T.: -0.005 min
Response: 4979505
Conc: 0.38 ng/ml

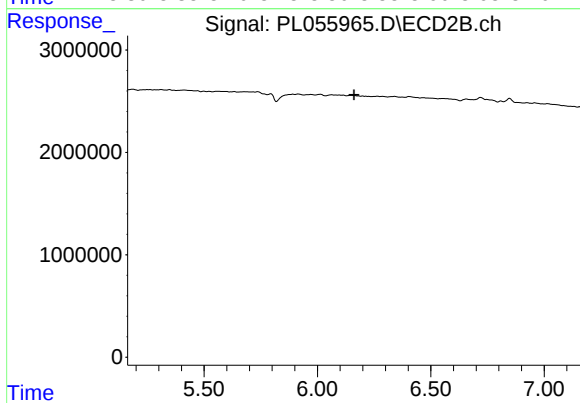

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

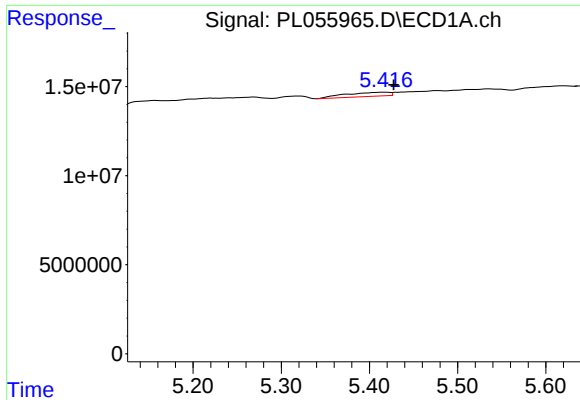

#10 gamma-Chlordane


R.T.: 5.417 min
Delta R.T.: -0.010 min
Response: 8076653
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

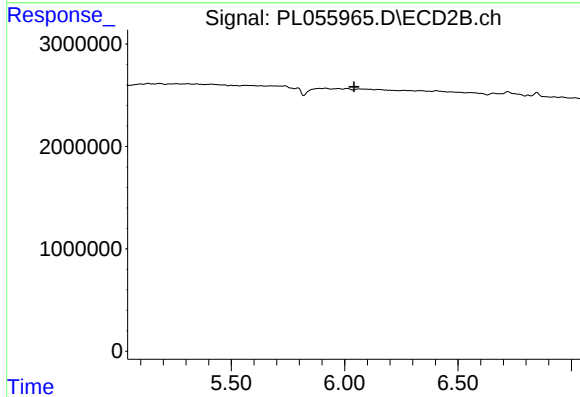


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.041 min
Response: 0
Conc: N.D.

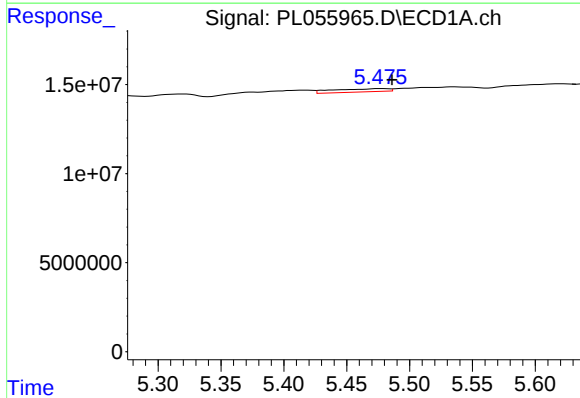


#11 alpha-Chlordane

R.T.: 5.476 min
Delta R.T.: -0.010 min
Response: 5622707
Conc: 0.41 ng/ml

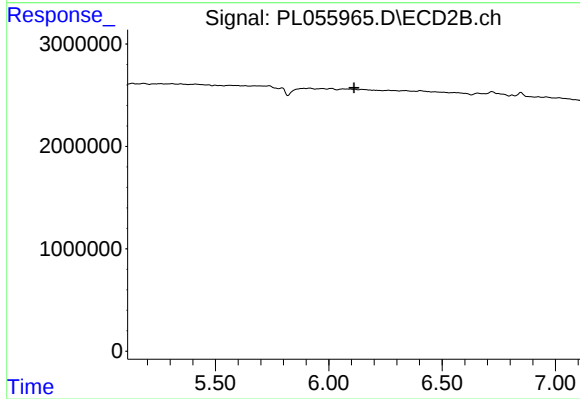

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

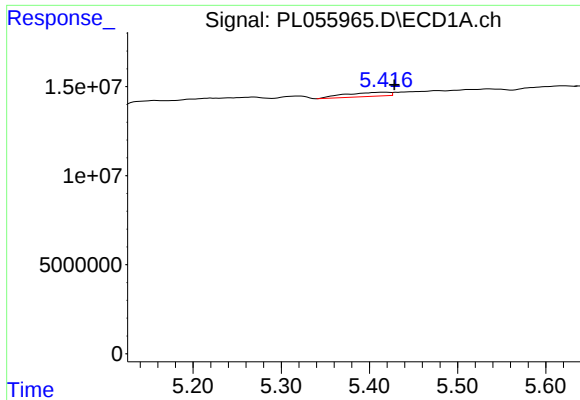

#25 Chlordane-3


R.T.: 5.417 min
Delta R.T.: -0.011 min
Response: 8076653
Conc: 6.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

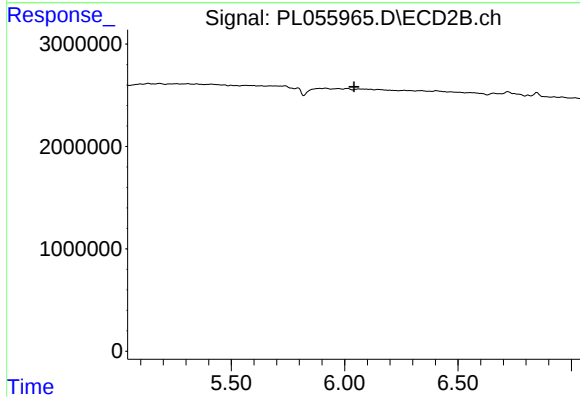


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.041 min
Response: 0
Conc: N.D.

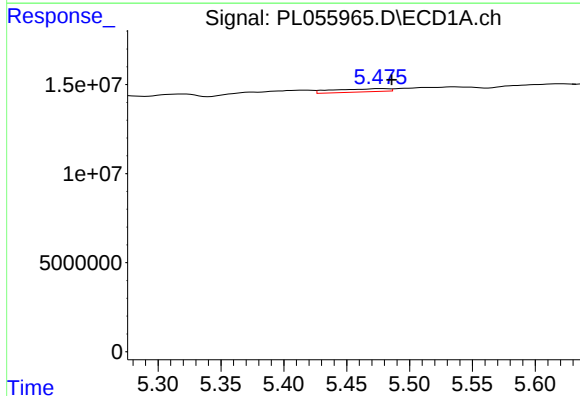


#26 Chlordane-4

R.T.: 5.476 min
Delta R.T.: -0.010 min
Response: 5622707
Conc: 5.45 ng/ml

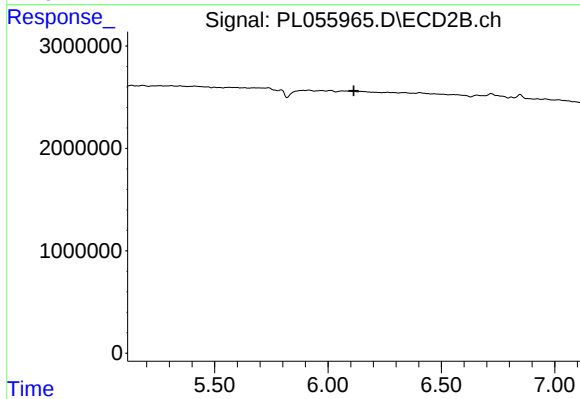

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.114 min
Response: 0
Conc: N.D.

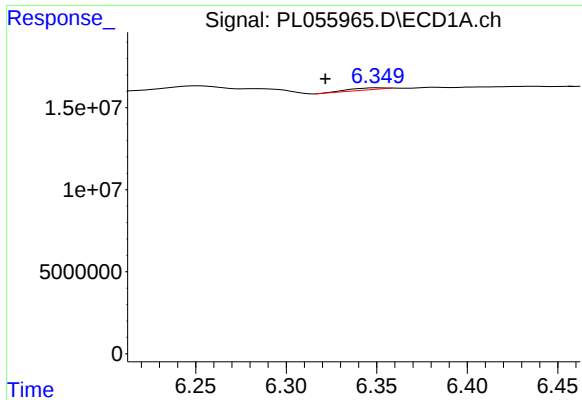

#27 Chlordane-5


R.T.: 6.351 min
Delta R.T.: 0.029 min
Response: 1571238
Conc: 4.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

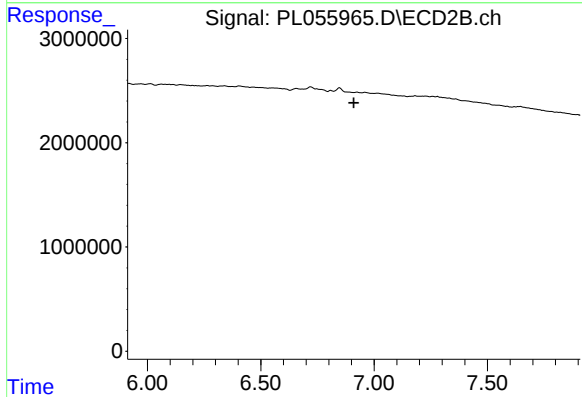


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.910 min
Response: 0
Conc: N.D.

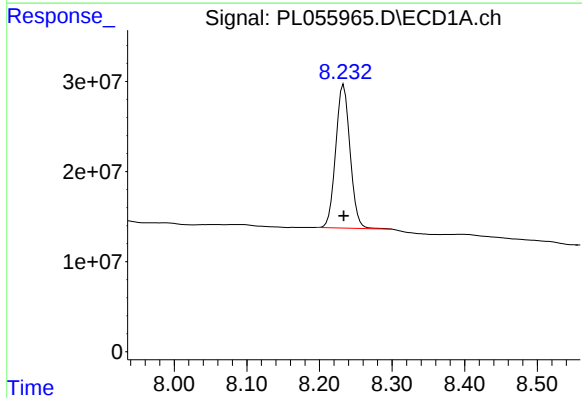

#28 Decachlorobiphenyl

R.T.: 8.233 min
Delta R.T.: 0.000 min
Response: 218771859
Conc: 20.92 ng/ml

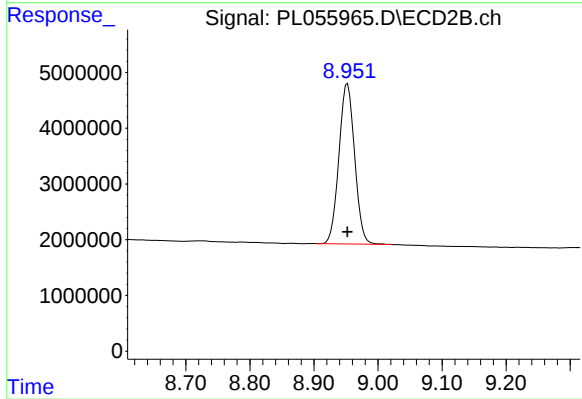

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: 0.000 min
Response: 48848813
Conc: 21.32 ng/ml