

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012120\
 Data File : PL055954.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 18:16
 Operator : AJ\MA
 Sample : L1004-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BU-03-012020

Manual Integrations
 APPROVED

Ankita
 1/22/2020 11:00:10 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 01:18:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 02:21:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	3.967	198.4E6	62939986	20.702	22.270
28)	SA Decachlor...	8.232	8.952	201.5E6	47364492	19.277m	20.674

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012120\
Data File : PL055954.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 18:16
Operator : AJ\MA
Sample : L1004-15
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BU-03-012020


Manual Integrations
APPROVED

Ankita
1/22/2020 11:00:10 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 01:18:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012020.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 02:21:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

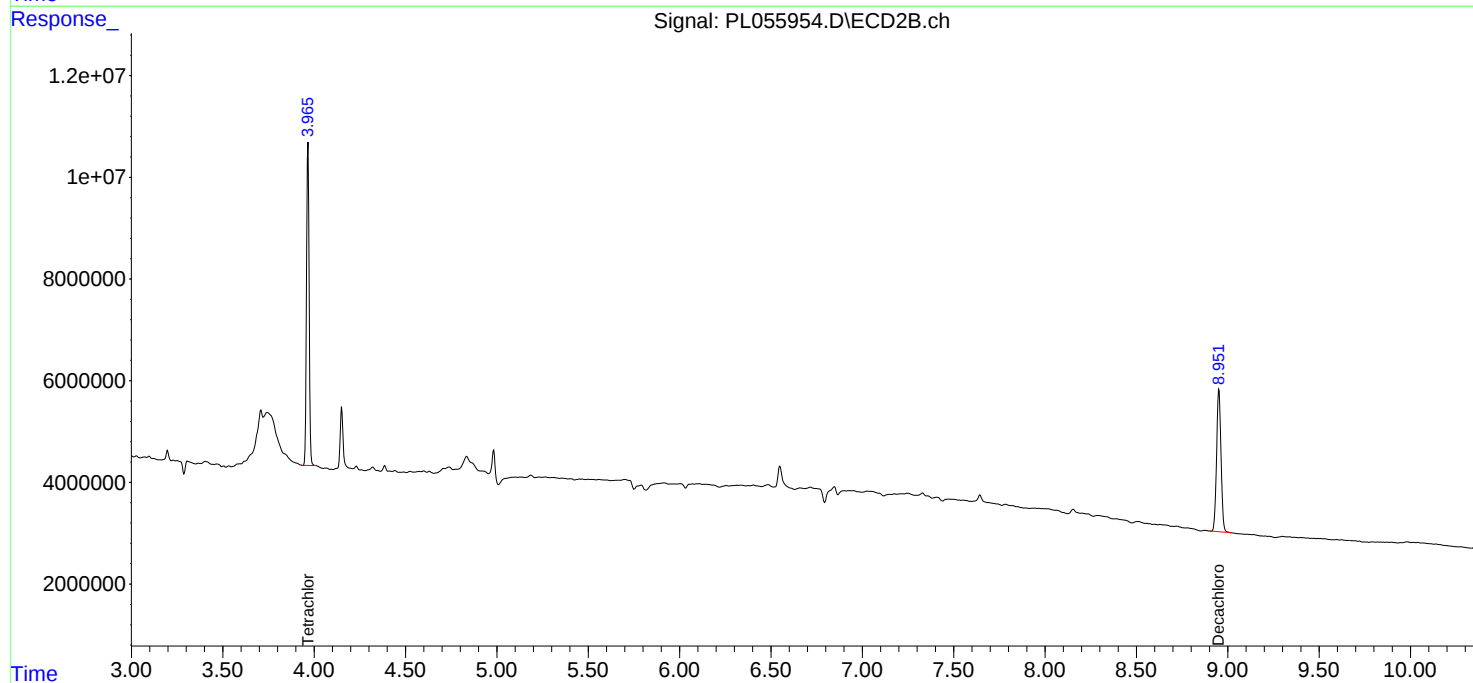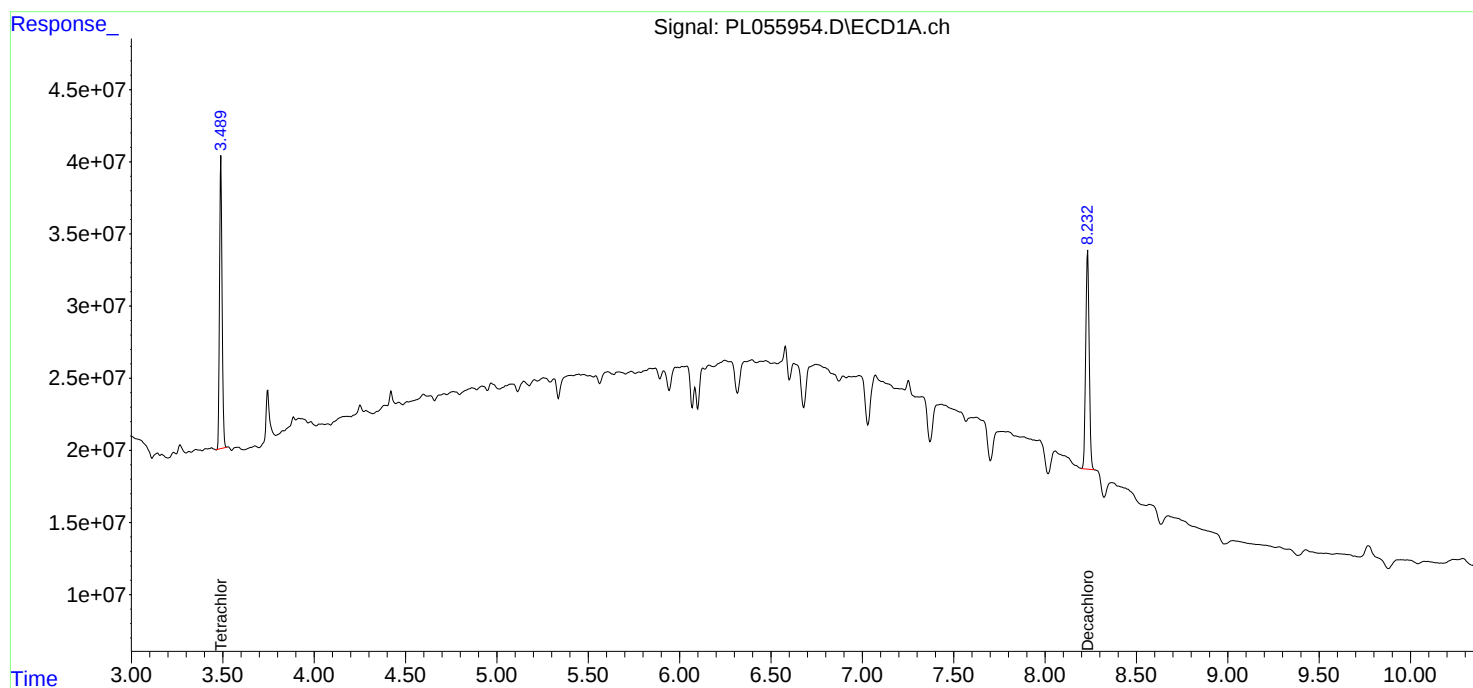

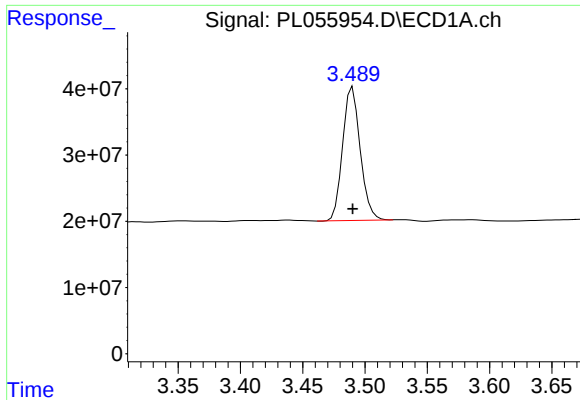


#1 Tetrachloro-m-xylene

R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 198420492
Conc: 20.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
BU-03-012020


Manual Integrations
APPROVED

Ankita
1/22/2020 11:00:10 AM

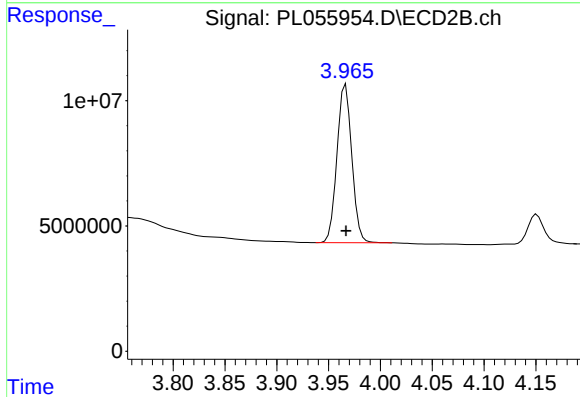


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 62939986
Conc: 22.27 ng/ml

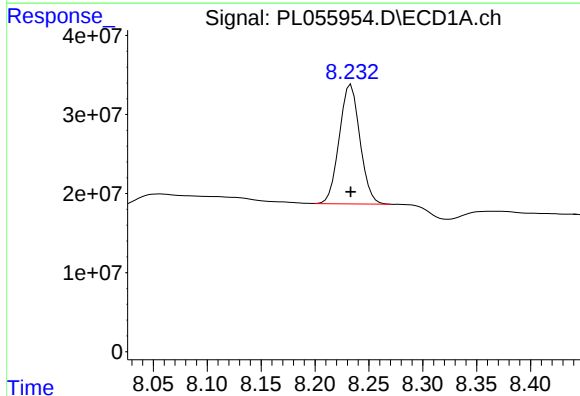

#28 Decachlorobiphenyl

R.T.: 8.232 min
Delta R.T.: -0.001 min
Response: 201549388
Conc: 19.28 ng/ml m

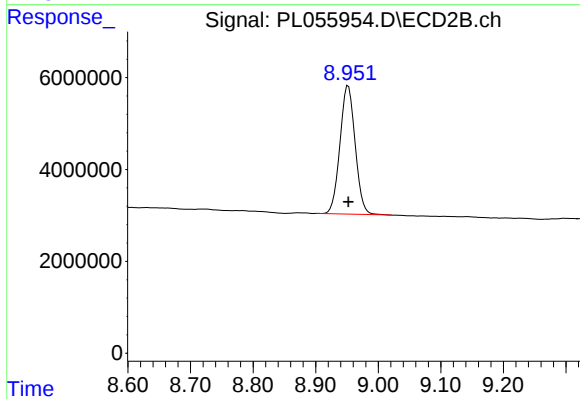

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: 0.000 min
Response: 47364492
Conc: 20.67 ng/ml